


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101218\
 Data File : VW006021.D
 Acq On : 11 Oct 2018 09:49
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W100818S.M
 Title : SW846 8260
 Last Update : Tue Oct 09 02:14:04 2018

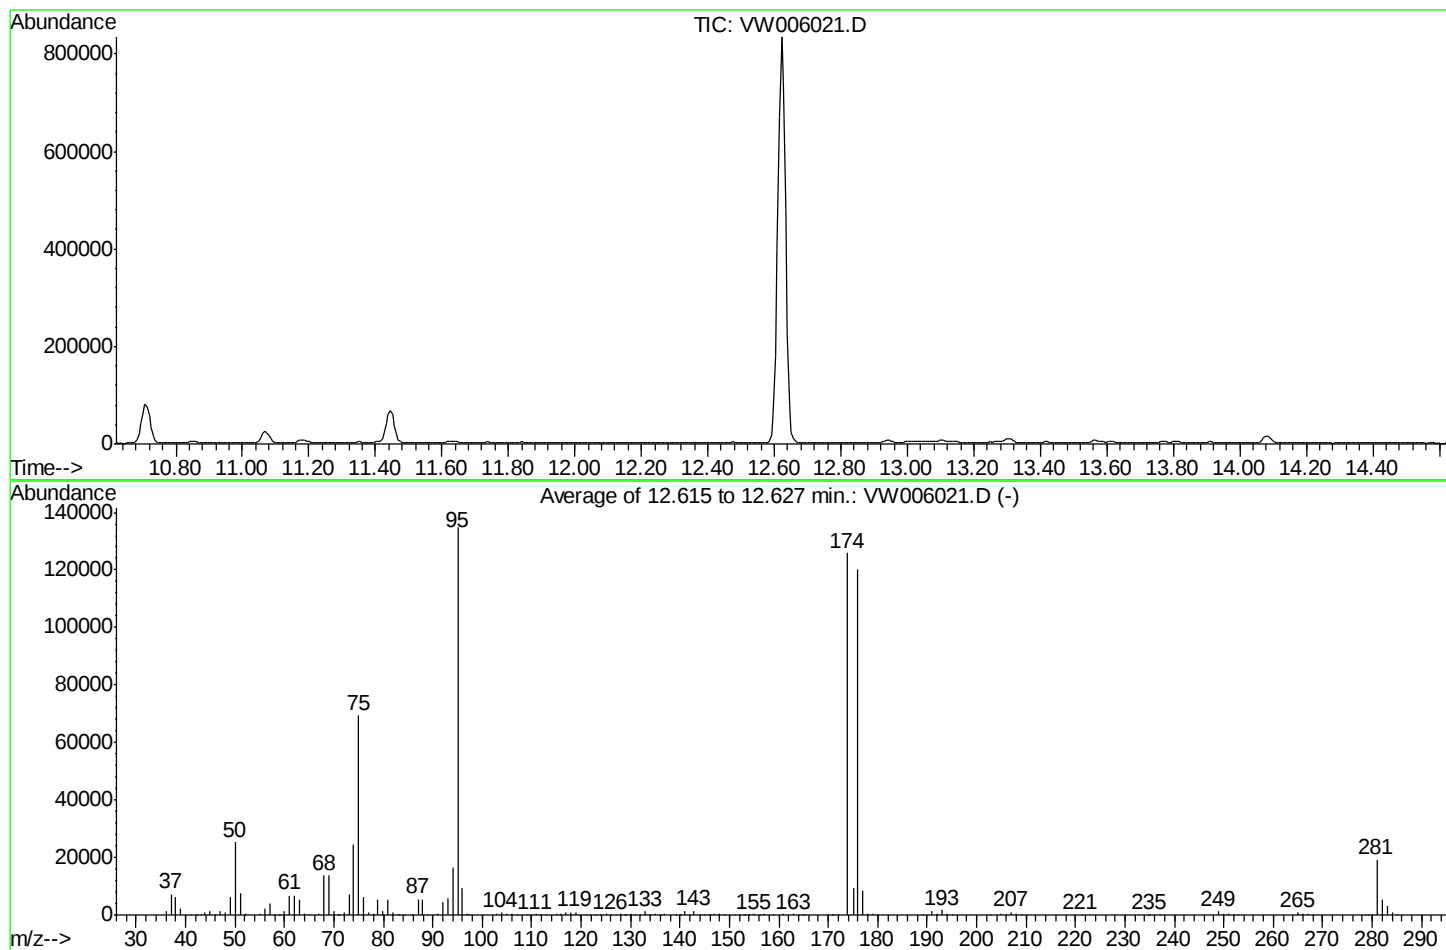

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	25194	PASS
75	95	30	60	51.4	69322	PASS
95	95	100	100	100.0	134819	PASS
96	95	5	9	6.8	9185	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	93.4	125885	PASS
175	174	5	9	7.5	9443	PASS
176	174	95	101	95.4	120112	PASS
177	176	5	9	7.0	8361	PASS