

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101220\
 Data File : VW016876.D
 Acq On : 12 Oct 2020 11:31
 Operator : SY/VA
 Sample : L4209-12
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK02

Manual Integrations
 APPROVED

MMDadoda
 10/13/2020 1:51:17 PM

Quant Time: Oct 13 07:00:30 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 13 06:53:04 2020
 Response via : Initial Calibration

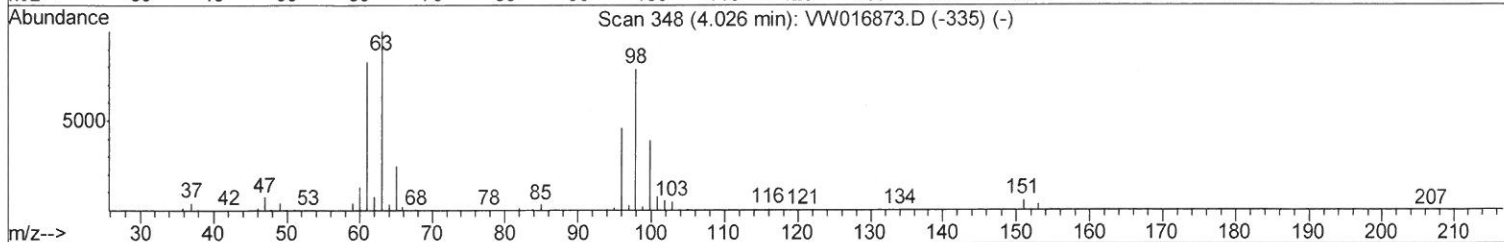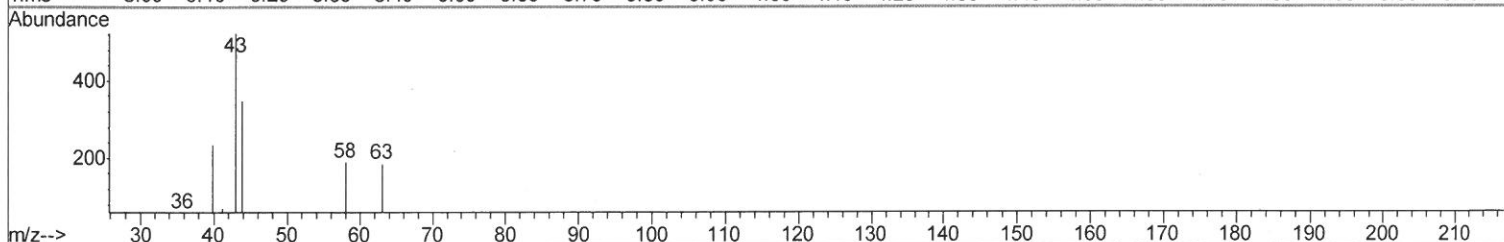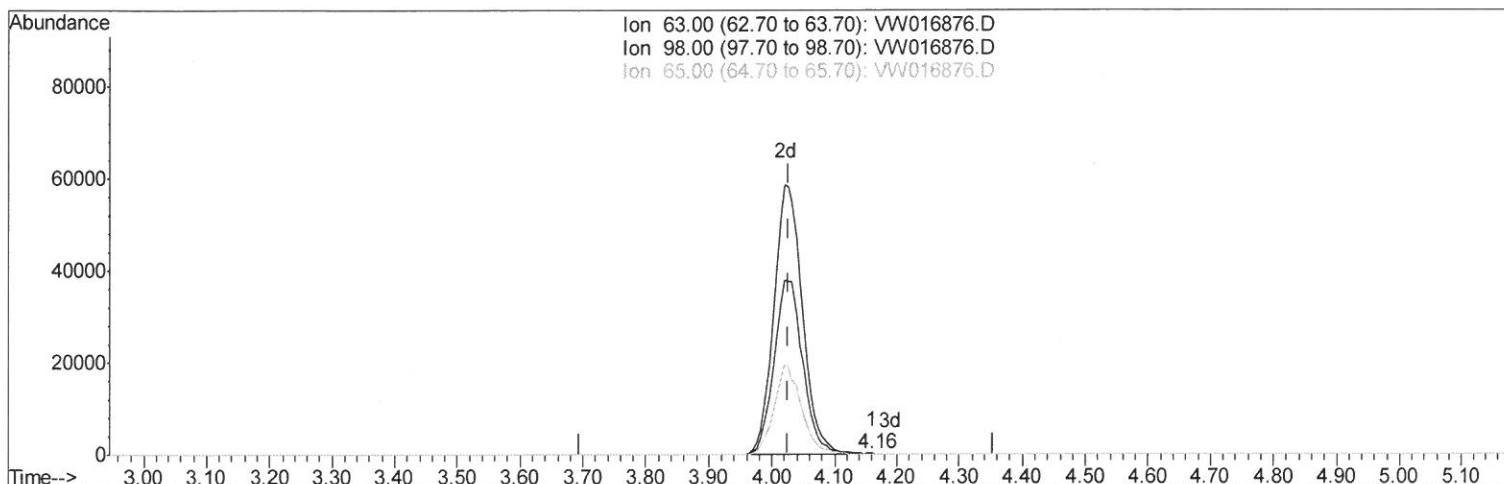

TIC: VW016876.D

(10) 1,1-Dichloroethene-d2 (S)

4.160min (+0.134) 0.02ug/L

response 208

Ion	Exp%	Act%
63.00	100	100
98.00	85.80	62.02
65.00	22.50	25.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101220\
Data File : VW016876.D
Acq On : 12 Oct 2020 11:31
Operator : SY/VA
Sample : L4209-12
Misc : 5.02G/10ML/MSVOA W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK02

Manual Integrations
APPROVED

MMDadoda
10/13/2020 1:51:17 PM

Quant Time: Oct 13 07:00:30 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 13 06:53:04 2020
Response via : Initial Calibration

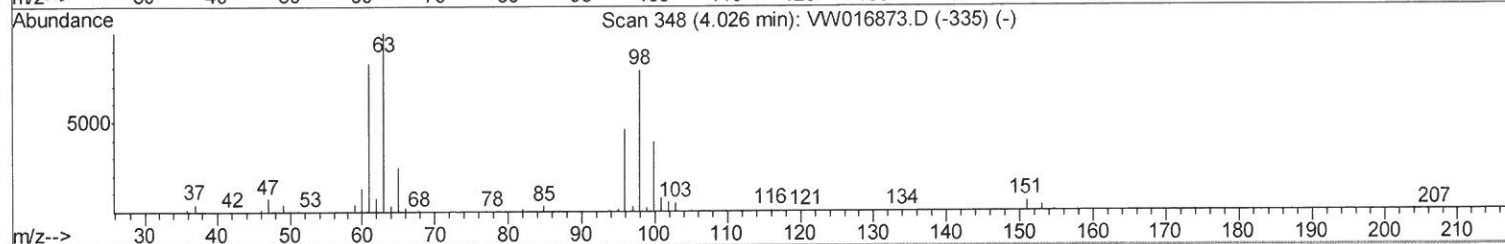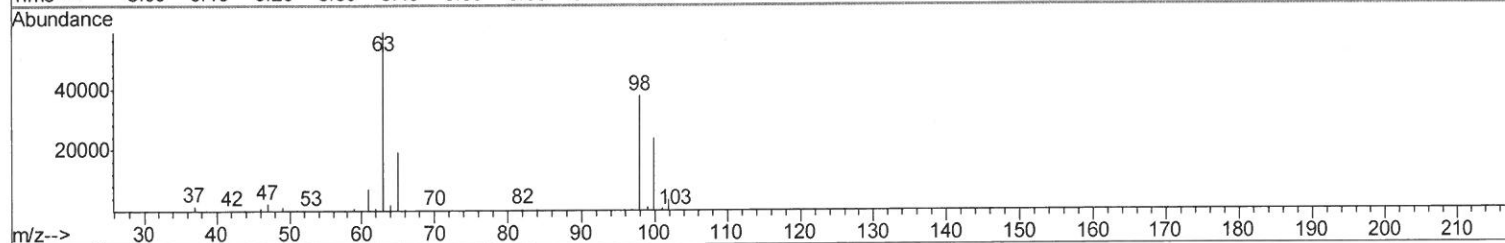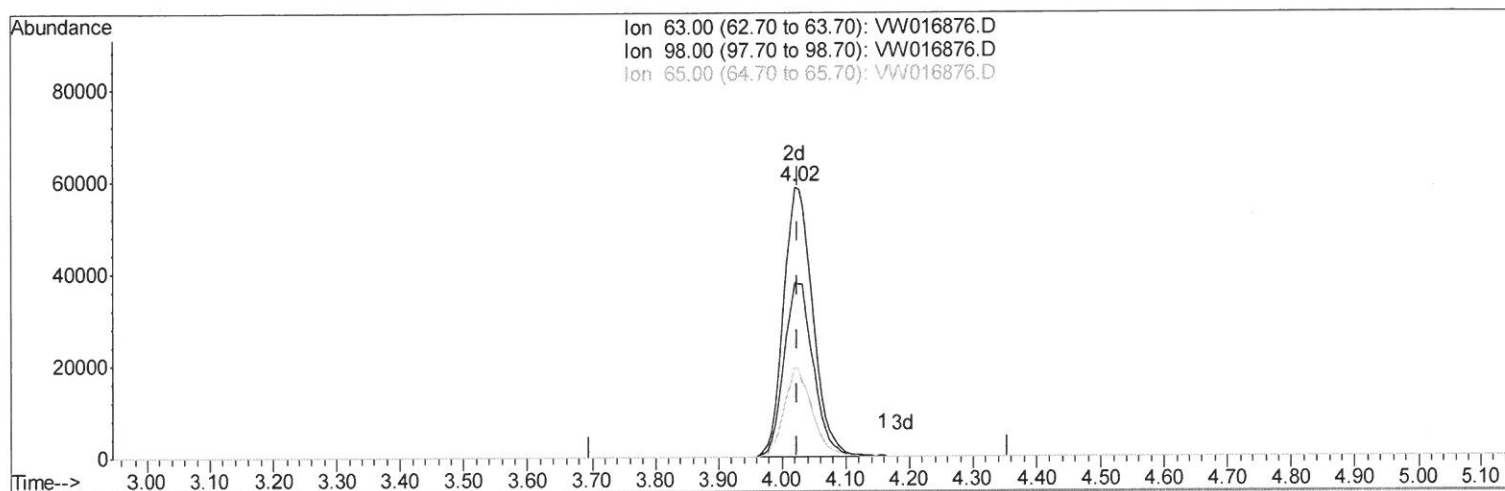

TIC: VW016876.D

(10) 1,1-Dichloroethene-d2 (S)

4.019min (-0.006) 16.36ug/L m

response 185887

Ion	Exp%	Act%
63.00	100	100
98.00	85.80	0.07#
65.00	22.50	0.03#
0.00	0.00	0.00

10/09/2020

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101220\
 Data File : VW016876.D
 Acq On : 12 Oct 2020 11:31
 Operator : SY/VA
 Sample : L4209-12
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VHBLK02

Manual Integrations
APPROVED

MMDadoda
 10/13/2020 1:51:17 PM

Quant Time: Oct 13 07:00:30 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 13 06:53:04 2020
 Response via : Initial Calibration

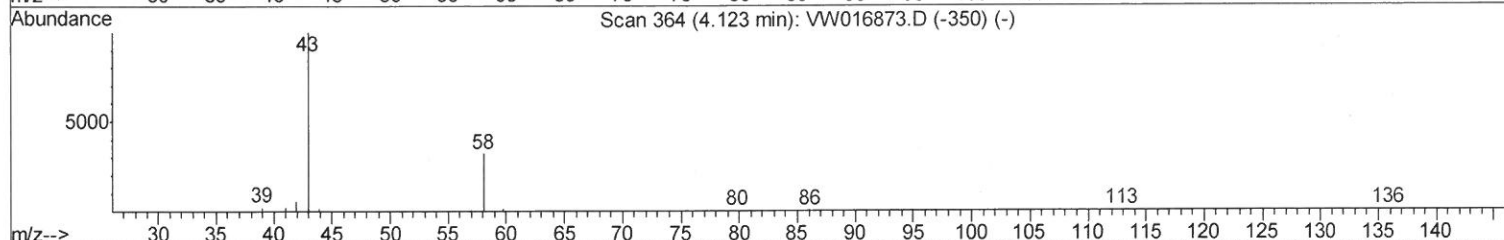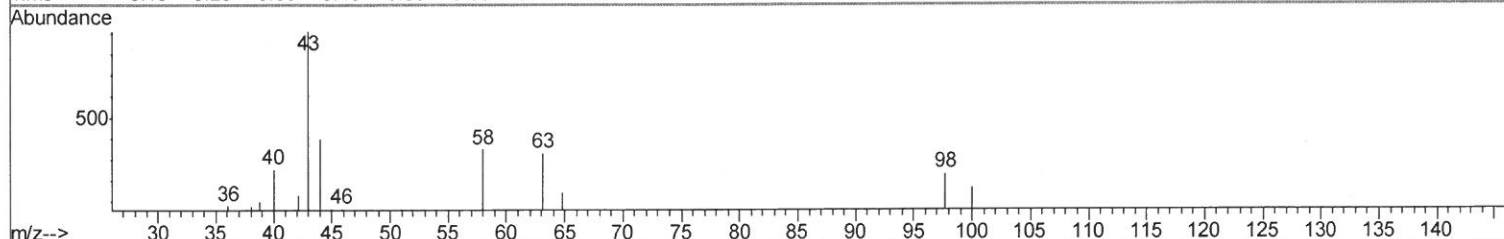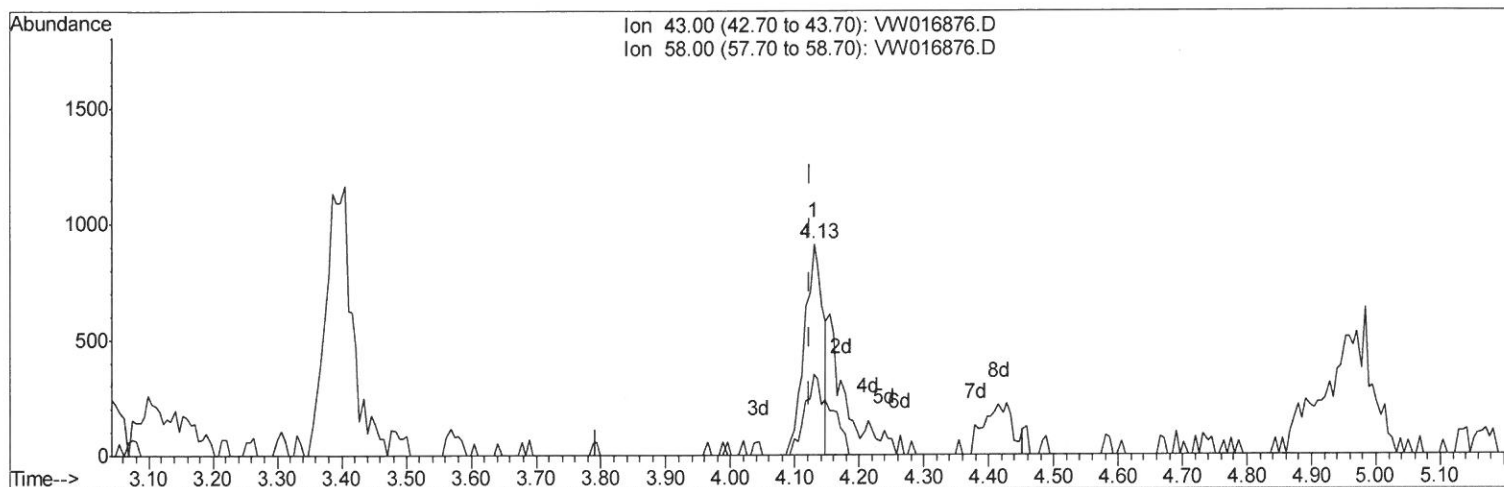

TIC: VW016876.D

(13) Acetone (T)

4.129min (+0.006) 2.02ug/L

response 1856

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	44.29
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101220\
Data File : VW016876.D
Acq On : 12 Oct 2020 11:31
Operator : SY/VA
Sample : L4209-12
Misc : 5.02G/10ML/MSVOA W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK02

Manual Integrations
APPROVED

MMDadoda
10/13/2020 1:51:17 PM

Quant Time: Oct 13 07:00:30 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 13 06:53:04 2020
Response via : Initial Calibration

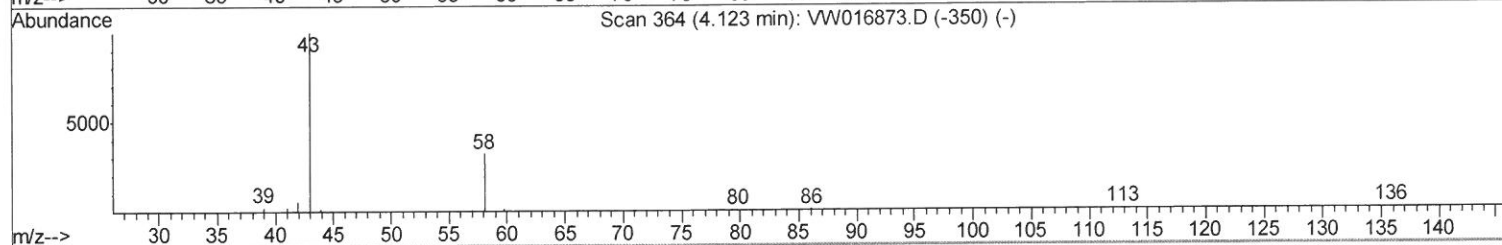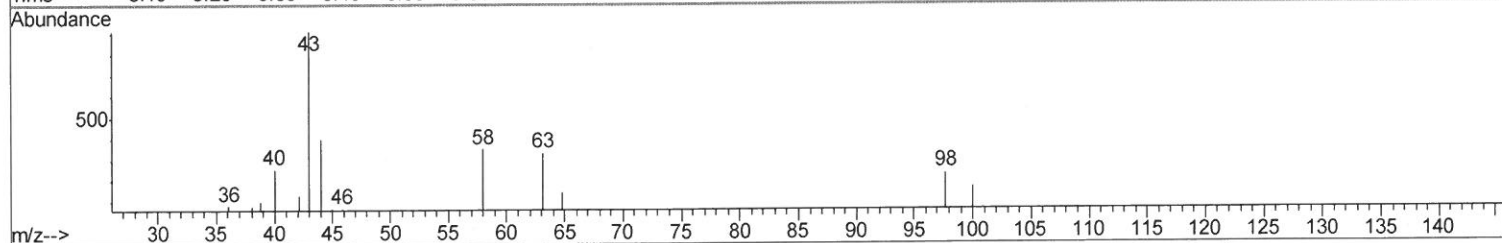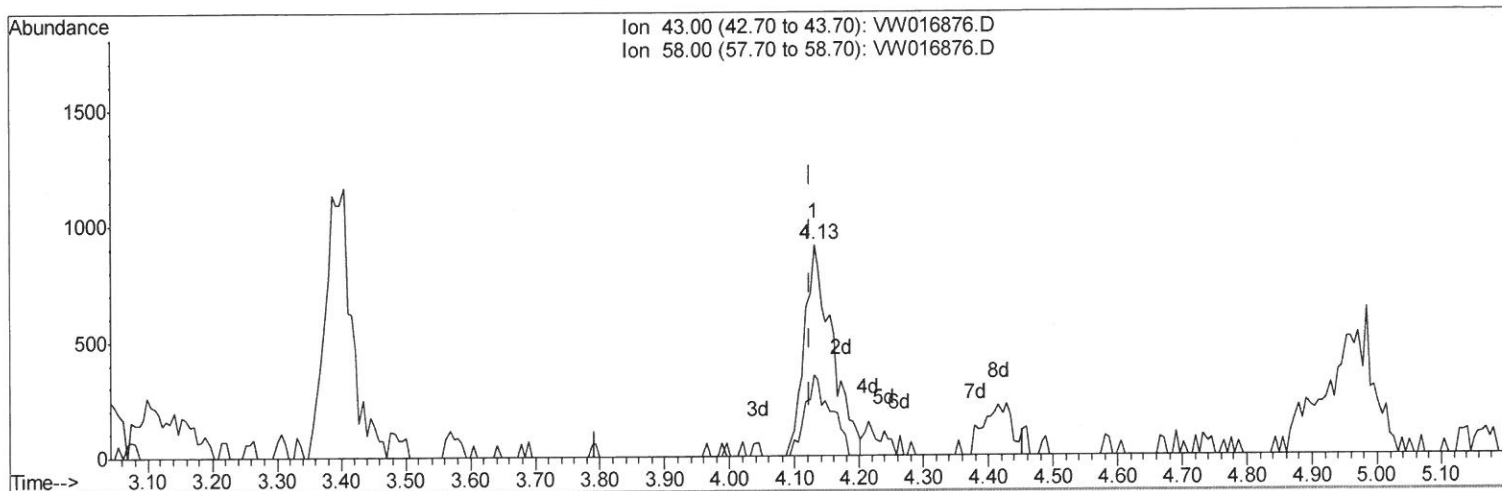

TIC: VW016876.D

(13) Acetone (T)

4.129min (+0.006) 3.00ug/L m

10/19/2021

response 2755

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	29.84
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101220\
 Data File : VW016876.D
 Acq On : 12 Oct 2020 11:31
 Operator : SY/VA
 Sample : L4209-12
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK02

Manual Integrations
 APPROVED

MMDadoda
 10/13/2020 1:51:17 PM

Quant Time: Oct 13 07:14:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 13 06:53:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	542322	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	488382	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	235167	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	122127	22.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.32%
7) Chloroethane-d5	2.89	69	101610	22.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.56%
10) 1,1-Dichloroethene-d2	4.02	63	185887m	16.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.44%
20) 2-Butanone-d5	7.08	46	65430	53.99	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.98%
24) Chloroform-d	7.65	84	264952	23.15	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.60%
26) 1,2-Dichloroethane-d4	8.31	65	134217	24.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.12%
29) Benzene-d6	8.28	84	538359	24.27	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.08%
33) 1,2-Dichloropropane-d6	9.27	67	149532	25.09	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.36%
37) Toluene-d8	10.32	98	501745	23.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.88%
38) trans-1,3-Dichloropropene-	10.58	79	63947	24.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.28%
39) 2-Hexanone-d5	10.93	63	52855	57.34	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.68%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	126600	26.29	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.16%
61) 1,2-Dichlorobenzene-d4	13.85	152	192923	25.86	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.44%

Target Compounds

13) Acetone	4.13	43	2755m	3.004	ug/L	92
16) Methylene chloride	4.92	84	13513	1.805	ug/L	87
43) 4-Methyl-2-pentanone	10.22	43	2480	0.831	ug/L #	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101220\
Data File : VW016876.D
Acq On : 12 Oct 2020 11:31
Operator : SY/VA
Sample : L4209-12
Misc : 5.02G/10ML/MSVOA W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK02

Manual Integrations
APPROVED

MMDadoda
10/13/2020 1:51:17 PM

Quant Time: Oct 13 07:14:48 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 13 06:53:04 2020
Response via : Initial Calibration

