


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW101220\
 Data File : VW016872.D
 Acq On : 12 Oct 2020 09:16
 Operator : SY/VA
 Sample : BFB12
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB12

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Title : VOC Analysis
 Last Update : Tue Oct 13 06:53:04 2020

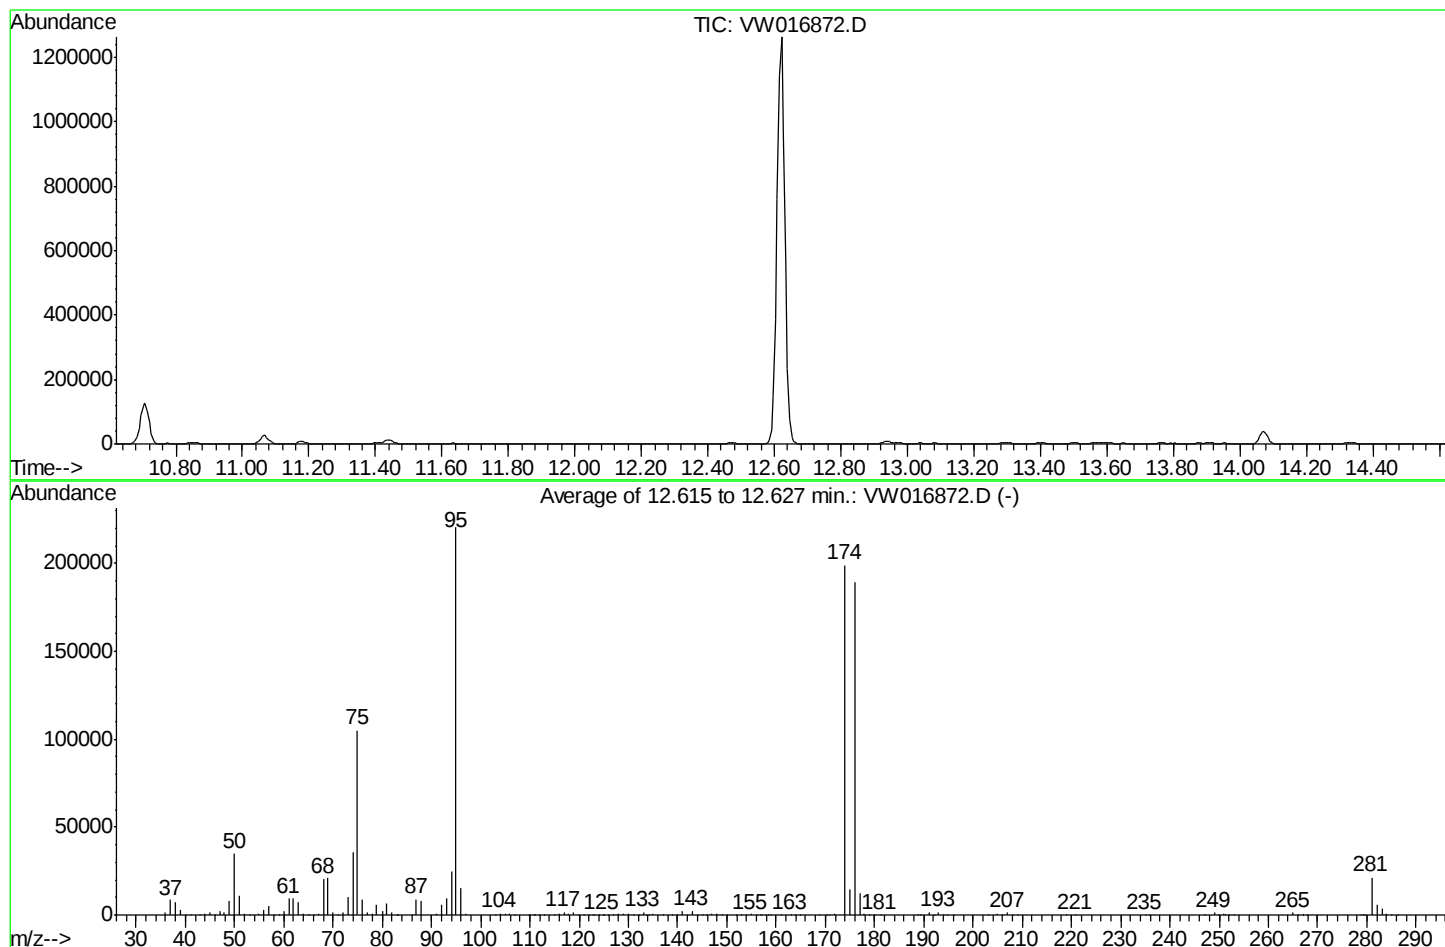

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	34952	PASS
75	95	30	80	47.7	105221	PASS
95	95	100	100	100.0	220565	PASS
96	95	5	9	6.9	15168	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.2	198933	PASS
175	174	5	9	7.4	14748	PASS
176	174	95	101	95.1	189248	PASS
177	176	5	9	6.6	12397	PASS

m/z	Abundance
36.00	1549.0
37.00	9027.0
38.00	8052.0
39.00	2795.0
40.00	278.0
41.20	97.0
43.00	141.0
44.10	1288.0
45.00	2003.0
47.00	2329.0
47.90	1247.0
49.00	8525.0
50.00	37296.0
51.00	12437.0
52.10	382.0
53.10	71.0
55.00	511.0
56.00	2795.0
57.00	5280.0
57.90	208.0
59.10	393.0
60.00	2189.0
61.00	9886.0
62.00	9887.0
63.00	7155.0
64.00	810.0
65.10	473.0
66.00	51.0
67.00	488.0
68.00	21424.0
69.00	22680.0
70.00	1576.0
71.00	92.0
71.90	1028.0
73.00	11557.0
74.00	37792.0
75.00	110808.0
76.00	9694.0
77.10	1372.0
77.90	819.0
78.90	6268.0
79.90	1674.0
80.90	6876.0
81.90	1322.0
83.00	155.0
87.00	8670.0
88.00	8882.0
91.00	833.0
92.00	6404.0
93.00	10027.0
94.00	25248.0
95.00	225856.0
96.00	16163.0
97.00	422.0
102.90	460.0
103.90	1247.0
105.00	497.0
105.80	844.0
106.90	263.0
109.70	264.0
110.70	328.0
111.10	297.0
111.90	364.0
112.90	194.0
115.00	411.0
116.00	909.0
117.00	1569.0
117.90	989.0
118.90	1609.0
120.00	129.0
121.00	97.0
121.90	77.0
122.60	60.0
124.10	163.0
124.80	963.0
125.80	278.0
127.00	70.0
127.80	613.0
128.90	449.0
129.90	751.0
130.90	398.0
132.10	74.0
133.00	2408.0
134.20	379.0
134.90	676.0
136.90	275.0
138.90	91.0
139.90	195.0
141.00	2013.0
141.90	298.0
142.90	2292.0
143.90	125.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

145.00	394.0
145.70	300.0
146.90	405.0
147.80	425.0
149.00	308.0
149.90	243.0
151.80	114.0
152.80	201.0
153.90	177.0
155.00	616.0
155.90	96.0
156.90	330.0
157.70	67.0
159.00	345.0
160.90	406.0
163.00	408.0
164.90	313.0
168.70	62.0
170.90	176.0
171.90	996.0
174.00	186816.0
175.00	13003.0
175.90	170176.0
176.90	12328.0
177.90	590.0
178.90	557.0
179.80	152.0
181.10	86.0
188.90	246.0
191.00	2191.0
192.00	418.0
193.00	3106.0
193.90	451.0
194.90	420.0
196.10	66.0
203.00	319.0
204.90	745.0
207.00	2216.0
207.90	323.0
209.00	220.0
219.00	132.0
220.80	97.0
235.00	254.0
235.70	80.0
247.00	63.0
249.00	2136.0
250.00	575.0
250.90	980.0
252.00	206.0
253.10	129.0
265.00	1870.0
266.10	546.0
266.90	451.0
267.90	184.0
278.80	90.0
279.20	129.0
281.00	31176.0
282.10	8781.0
283.10	5619.0
284.10	1113.0
285.00	441.0
286.20	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

m/z	Abundance
36.00	1725.0
37.00	9646.0
38.00	8328.0
39.00	3304.0
39.90	347.0
41.10	70.0
43.00	204.0
44.00	1441.0
45.00	1674.0
46.00	179.0
47.00	2438.0
48.00	1336.0
49.00	9470.0
50.00	39432.0
51.00	12003.0
52.00	593.0
53.00	60.0
55.00	663.0
56.00	3440.0
57.00	6122.0
58.00	226.0
59.00	241.0
60.00	2148.0
61.00	10274.0
62.00	10445.0
63.00	8036.0
64.00	799.0
65.00	390.0
66.10	57.0
66.90	642.0
68.00	23208.0
69.00	23304.0
69.90	1793.0
71.10	197.0
72.00	1295.0
73.00	11009.0
74.00	39808.0
75.00	116728.0
76.00	9746.0
76.90	1383.0
77.90	944.0
78.90	6530.0
79.90	2200.0
80.90	6589.0
81.90	1815.0
83.20	215.0
86.00	505.0
86.90	10405.0
88.00	9063.0
90.80	827.0
92.00	6938.0
93.00	11052.0
94.00	28248.0
95.00	249792.0
96.00	16912.0
97.00	571.0
102.90	380.0
103.90	1042.0
105.00	353.0
105.90	948.0
107.00	188.0
109.90	227.0
111.10	239.0
111.80	207.0
112.90	203.0
114.90	476.0
115.90	822.0
116.90	1700.0
117.90	1151.0
118.90	1487.0
119.80	52.0
121.00	83.0
123.90	199.0
125.10	492.0
125.90	275.0
127.00	98.0
127.90	889.0
129.00	475.0
129.90	979.0
131.00	415.0
133.00	1549.0
133.70	355.0
134.90	529.0
136.90	326.0
138.80	78.0
140.90	2519.0
143.00	2699.0
143.90	173.0
144.90	392.0
145.80	442.0
146.80	464.0
147.90	711.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

149.00	324.0
149.90	284.0
151.90	165.0
152.90	241.0
153.80	207.0
154.90	528.0
156.00	233.0
157.10	514.0
157.80	112.0
158.30	105.0
159.00	231.0
160.90	398.0
163.00	215.0
163.70	82.0
165.00	179.0
170.20	87.0
170.80	141.0
172.00	779.0
173.90	231040.0
175.00	16680.0
175.90	210944.0
176.90	13813.0
178.00	340.0
178.90	410.0
180.00	60.0
189.10	154.0
191.00	1530.0
192.10	339.0
193.00	1704.0
193.90	297.0
194.70	194.0
203.00	223.0
205.00	328.0
206.00	136.0
207.00	1078.0
208.00	235.0
209.00	240.0
220.90	104.0
235.00	234.0
249.10	1515.0
249.90	369.0
250.90	821.0
252.00	183.0
264.90	1395.0
265.90	386.0
267.10	374.0
267.90	65.0
279.40	111.0
281.10	22144.0
282.10	5732.0
283.00	3234.0
284.00	592.0
285.00	204.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

m/z	Abundance
36.00	1151.0
37.00	7445.0
38.00	5873.0
39.10	2428.0
39.90	237.0
41.10	54.0
42.90	100.0
43.90	1064.0
45.00	1354.0
46.00	132.0
47.10	1831.0
48.00	944.0
49.00	6411.0
50.00	28128.0
51.00	8992.0
52.00	459.0
52.90	68.0
54.90	444.0
56.00	2384.0
57.00	4210.0
57.90	256.0
58.90	116.0
60.10	1903.0
61.00	7747.0
62.00	7655.0
63.00	5757.0
64.10	550.0
65.00	280.0
66.00	57.0
66.90	416.0
68.00	16640.0
69.00	16760.0
70.00	1310.0
72.00	1088.0
73.00	8474.0
74.00	29296.0
75.00	88128.0
76.00	7460.0
77.00	1116.0
78.00	646.0
78.90	5154.0
80.00	1698.0
80.90	5325.0
81.90	1242.0
83.00	190.0
85.80	299.0
86.90	7819.0
87.90	7088.0
90.90	691.0
92.00	5038.0
93.00	7811.0
94.00	21944.0
95.00	186048.0
96.00	12429.0
97.10	350.0
102.90	164.0
103.90	766.0
104.80	368.0
105.90	817.0
106.90	208.0
110.00	176.0
111.00	258.0
111.80	156.0
112.80	266.0
114.80	271.0
115.80	715.0
117.00	1314.0
117.90	779.0
118.90	1086.0
123.00	51.0
123.90	155.0
124.80	181.0
125.70	133.0
127.00	58.0
127.90	637.0
129.00	390.0
129.90	748.0
131.00	268.0
132.20	68.0
133.00	440.0
133.80	303.0
134.90	371.0
137.00	421.0
139.80	152.0
140.90	1947.0
141.90	234.0
143.00	2233.0
144.00	128.0
145.00	237.0
145.80	335.0
147.00	316.0
147.80	385.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

149.00	132.0
149.90	348.0
152.00	77.0
152.90	182.0
154.00	127.0
154.90	518.0
155.90	153.0
156.90	301.0
158.20	59.0
158.90	236.0
160.80	253.0
163.00	138.0
164.90	130.0
168.80	61.0
170.20	77.0
170.70	78.0
171.90	702.0
173.90	178944.0
175.00	14562.0
175.90	186624.0
177.00	11051.0
177.80	275.0
179.00	122.0
188.70	87.0
189.20	60.0
191.00	502.0
191.90	126.0
193.00	728.0
194.00	128.0
194.80	99.0
203.00	104.0
204.90	109.0
205.10	108.0
207.10	604.0
207.90	71.0
235.00	107.0
248.90	618.0
250.00	208.0
251.10	216.0
251.90	80.0
265.10	580.0
265.80	133.0
267.10	185.0
279.50	97.0
281.10	10844.0
282.10	2378.0
283.00	1595.0
283.90	299.0
284.20	238.0
285.10	74.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

Scan 1749 (12.566 min): VW016872.D
BFB12

m/z	Abundance
40.00	184.0
41.10	70.0
43.10	55.0
43.90	322.0
169.00	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12