
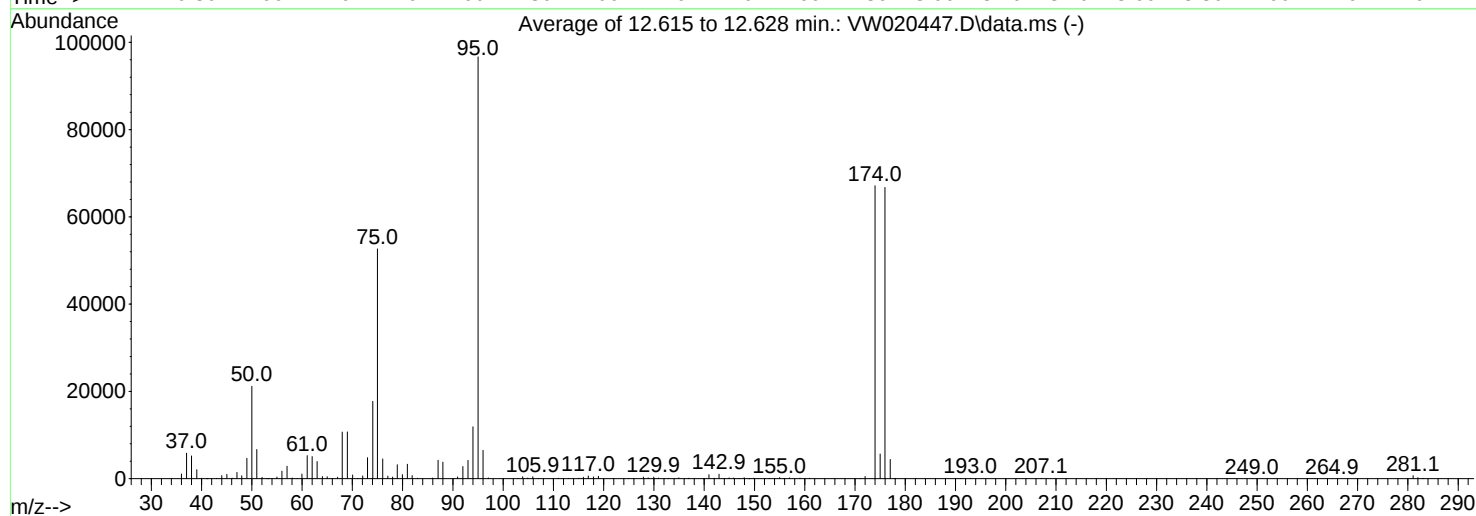


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101221\
Data File : VW020447.D
Acq On : 12 Oct 2021 07:58
Operator : SY/VA
Sample : BFB450
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB450

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Title : SFAM01.0
Last Update : Wed Oct 13 02:22:35 2021

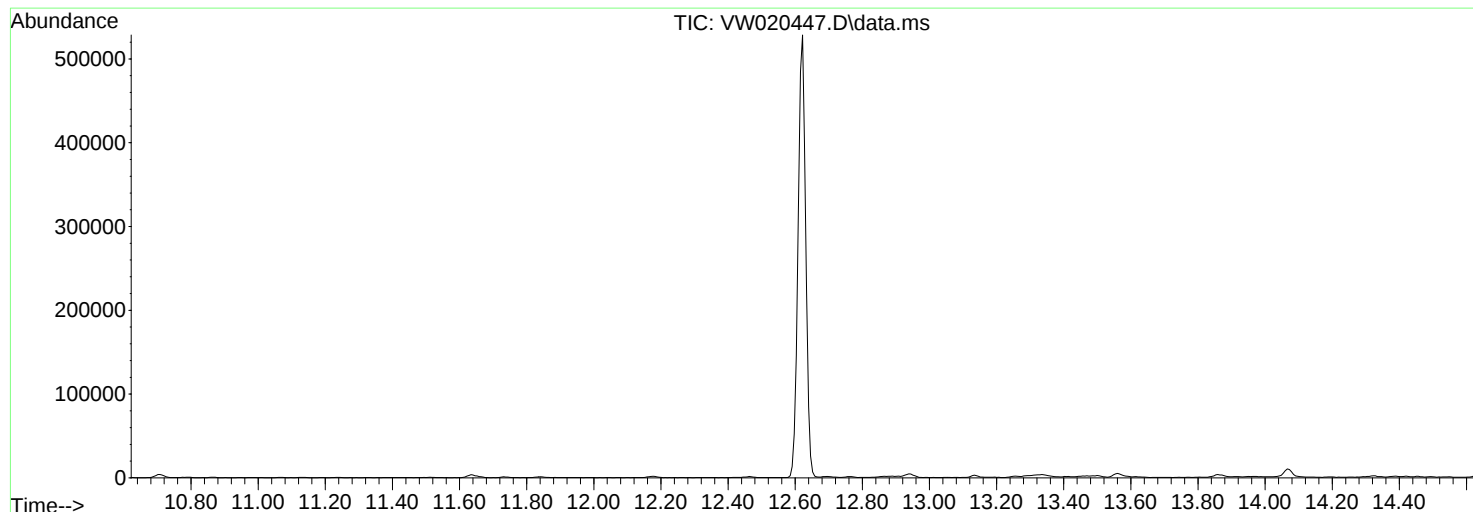

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	21171	PASS
75	95	30	80	54.5	52672	PASS
95	95	100	100	100.0	96680	PASS
96	95	5	9	6.7	6484	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.5	67168	PASS
175	174	5	9	8.4	5657	PASS
176	174	95	105	99.4	66755	PASS
177	176	5	10	6.6	4413	PASS

m/z	Abundance
40.00	104.0
41.10	56.0
44.00	174.0
57.00	67.0
141.10	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

m/z	Abundance
36.00	1250.0
37.00	6581.0
38.00	5785.0
39.00	2303.0
40.10	197.0
41.10	51.0
42.90	91.0
44.00	956.0
45.00	1000.0
46.10	134.0
47.10	1565.0
48.00	745.0
49.00	5226.0
50.00	22912.0
51.00	7243.0
52.10	305.0
52.90	77.0
55.00	392.0
56.00	1893.0
57.00	3258.0
58.00	123.0
59.00	63.0
60.00	1055.0
61.00	5774.0
62.00	5720.0
63.00	4374.0
64.00	543.0
65.00	580.0
66.00	59.0
67.10	350.0
68.00	11247.0
69.00	11626.0
70.10	930.0
71.00	50.0
72.00	670.0
73.00	5210.0
74.00	18472.0
75.00	55200.0
76.10	5178.0
77.10	512.0
78.00	358.0
78.90	3265.0
79.90	1011.0
80.90	3678.0
81.90	759.0
83.00	142.0
85.90	199.0
87.10	4083.0
88.00	3995.0
91.00	381.0
92.00	2920.0
93.00	4365.0
94.00	12725.0
95.00	100360.0
96.00	7064.0
97.00	219.0
102.90	77.0
103.90	474.0
104.80	161.0
105.90	503.0
107.00	98.0
111.00	113.0
111.90	77.0
113.00	96.0
115.00	121.0
115.90	317.0
116.90	710.0
118.00	387.0
118.90	638.0
124.90	84.0
125.90	71.0
127.90	389.0
128.90	188.0
130.00	380.0
130.90	136.0
132.90	114.0
134.90	158.0
136.80	165.0
140.90	1105.0
142.00	132.0
143.00	1044.0
144.00	66.0
144.90	230.0
145.80	156.0
146.90	78.0
148.00	263.0
148.90	55.0
149.80	83.0
152.80	83.0
155.00	275.0
155.80	51.0
156.90	152.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

159.00	122.0
161.00	113.0
171.10	115.0
172.10	601.0
174.00	64680.0
175.00	5317.0
175.90	63048.0
177.00	3966.0
177.90	131.0
191.00	99.0
193.00	131.0
207.10	90.0
249.00	101.0
264.90	83.0
281.00	1094.0
282.10	303.0
282.90	128.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

m/z	Abundance
36.00	1240.0
37.00	6513.0
38.00	5697.0
39.00	2274.0
39.90	235.0
41.10	81.0
43.00	107.0
44.10	938.0
45.00	1112.0
46.10	128.0
47.00	1622.0
48.00	776.0
49.00	5159.0
50.00	23320.0
51.00	7222.0
52.00	318.0
52.90	70.0
55.00	440.0
56.00	1940.0
57.00	3158.0
58.00	202.0
60.00	1255.0
61.00	5974.0
62.00	5372.0
63.00	4360.0
64.10	496.0
65.00	413.0
65.90	57.0
67.00	354.0
68.00	11766.0
69.00	11966.0
70.00	936.0
71.10	67.0
72.00	679.0
73.00	5449.0
74.10	19856.0
75.00	59448.0
76.10	4753.0
77.00	662.0
78.00	418.0
78.90	3694.0
80.00	975.0
81.00	3669.0
81.90	768.0
82.90	129.0
85.90	157.0
87.00	4941.0
88.00	4144.0
90.90	519.0
92.00	3123.0
93.00	4643.0
94.00	13300.0
95.00	110016.0
96.00	7373.0
97.10	242.0
103.00	71.0
103.90	510.0
104.90	164.0
105.90	476.0
107.00	110.0
109.90	126.0
111.00	120.0
111.90	58.0
112.90	111.0
115.00	162.0
115.90	444.0
117.00	680.0
117.90	453.0
119.00	589.0
127.90	410.0
128.90	202.0
129.90	404.0
130.90	142.0
133.00	74.0
135.00	180.0
137.00	235.0
141.00	1044.0
141.90	129.0
142.90	1203.0
143.90	80.0
145.00	217.0
145.90	131.0
147.00	81.0
147.90	263.0
149.80	127.0
152.00	58.0
152.90	75.0
154.00	87.0
155.00	272.0
157.00	228.0
159.10	153.0
161.00	135.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

172.00	499.0
174.00	75856.0
175.00	6304.0
176.00	74832.0
177.00	4953.0
178.10	155.0
191.00	68.0
193.00	73.0
207.10	90.0
249.00	70.0
265.00	89.0
281.10	729.0
282.00	202.0
283.10	129.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

m/z	Abundance
36.00	744.0
37.00	4364.0
38.00	4149.0
39.10	1621.0
40.00	233.0
41.00	74.0
42.90	82.0
44.00	752.0
45.10	827.0
46.10	71.0
47.00	1090.0
48.00	479.0
49.00	3648.0
50.00	17280.0
51.00	5550.0
52.00	227.0
53.20	53.0
55.00	271.0
56.00	1317.0
57.00	2385.0
58.10	123.0
59.90	839.0
61.00	4055.0
62.00	4047.0
63.00	3044.0
64.00	394.0
65.00	288.0
65.90	64.0
67.00	259.0
68.00	8964.0
69.00	8577.0
70.00	705.0
71.10	53.0
72.10	512.0
73.00	3754.0
74.00	14835.0
75.00	43368.0
76.00	3572.0
77.00	554.0
78.00	307.0
79.00	2577.0
80.00	730.0
80.90	2611.0
81.90	531.0
83.00	94.0
85.90	108.0
87.00	3678.0
88.00	3224.0
90.90	351.0
92.00	2357.0
93.00	3533.0
94.00	9610.0
95.00	79664.0
96.00	5014.0
97.10	140.0
102.90	61.0
103.90	376.0
105.00	142.0
105.90	391.0
106.90	74.0
109.80	52.0
110.90	78.0
112.90	62.0
115.10	103.0
116.00	264.0
116.90	504.0
117.90	329.0
118.90	460.0
128.00	263.0
128.70	129.0
130.00	301.0
130.90	120.0
134.90	206.0
136.90	156.0
139.80	58.0
140.90	865.0
141.90	112.0
142.90	823.0
143.90	77.0
145.00	114.0
145.90	132.0
147.90	178.0
149.90	78.0
152.10	54.0
153.00	59.0
154.90	175.0
157.00	135.0
159.00	61.0
160.80	96.0
171.90	470.0
174.00	60968.0
175.00	5351.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450

176.00	62384.0
177.00	4321.0
178.10	115.0
193.10	61.0
206.90	51.0
281.00	292.0
281.90	131.0

Instrument :
MSVOA_W
ClientSampleId :
BFB450