

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101222\
 Data File : VW024870.D
 Acq On : 12 Oct 2022 13:45
 Operator : SY/VA
 Sample : VW1012SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK423

Quant Time: Oct 12 23:20:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 23:18:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	467683	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	427293	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	200682	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	123585	22.398	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.600%
7) Chloroethane-d5	2.885	69	71311	22.074	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.280%
11) 1,1-Dichloroethene-d2	4.019	63	204422	17.040	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.160%
21) 2-Butanone-d5	7.086	46	75250	43.043	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.080%
24) Chloroform-d	7.647	84	296302	22.462	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.840%
26) 1,2-Dichloroethane-d4	8.305	65	159369	23.084	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.320%
32) Benzene-d6	8.275	84	626655	23.387	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.560%
36) 1,2-Dichloropropane-d6	9.274	67	191578	23.311	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.240%
41) Toluene-d8	10.323	98	558115	23.207	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.840%
43) trans-1,3-Dichloroprop...	10.573	79	70494	22.617	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.480%
47) 2-Hexanone-d5	10.920	63	59432	43.134	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.260%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	138871	21.668	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.680%
66) 1,2-Dichlorobenzene-d4	13.847	152	169886	23.165	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.680%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	5950	0.568	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101222\
Data File : VW024870.D
Acq On : 12 Oct 2022 13:45
Operator : SY/VA
Sample : VW1012SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK423

Quant Time: Oct 12 23:20:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 23:18:51 2022
Response via : Initial Calibration

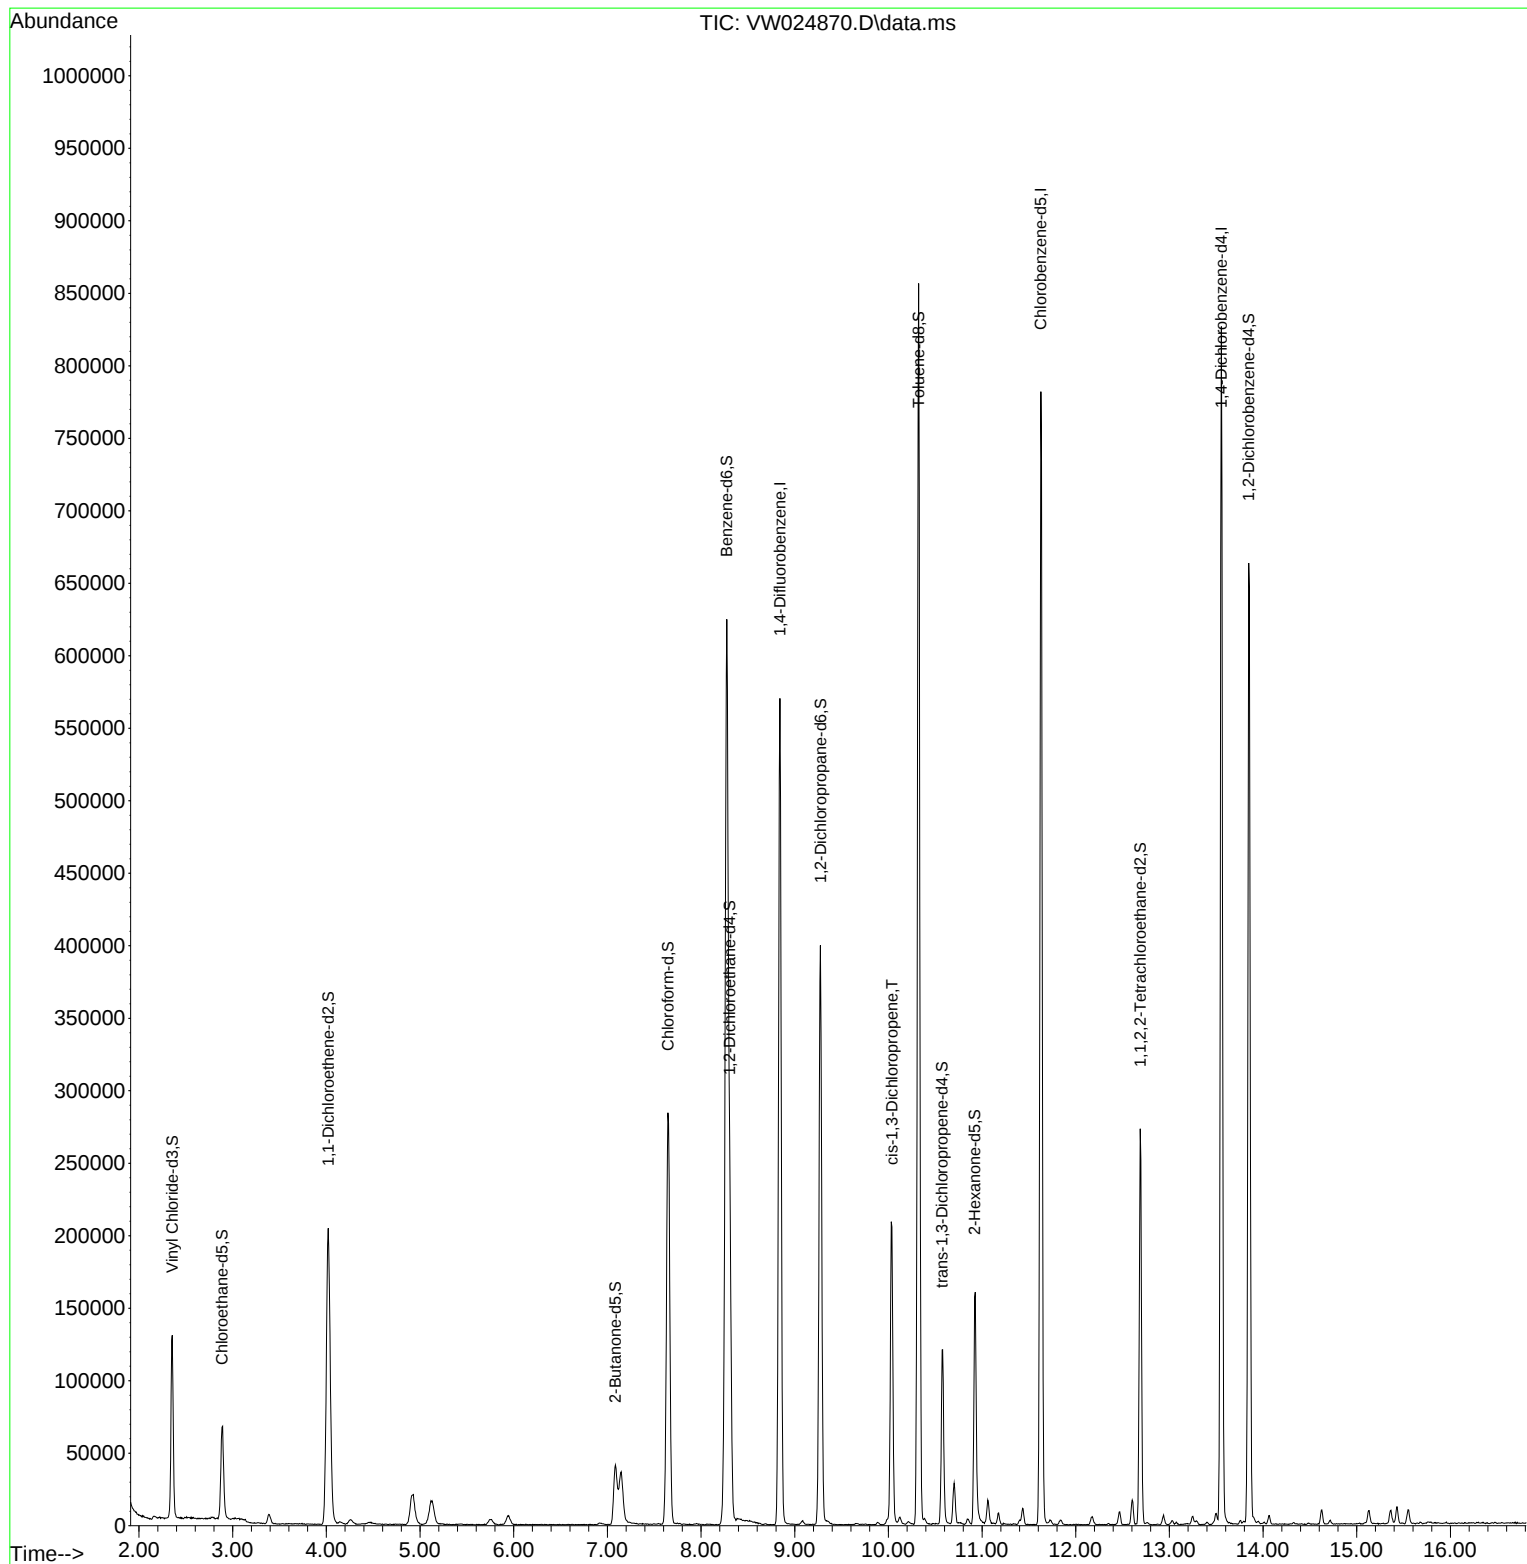

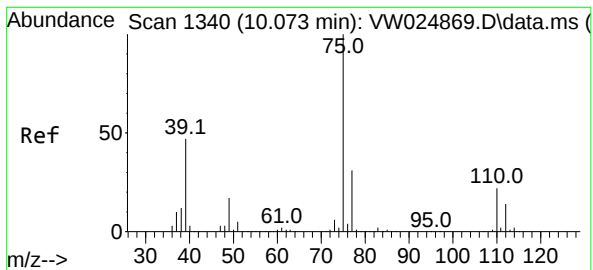

#39
 cis-1,3-Dichloropropene
 Concen: 0.568 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW024870.D
 Acq: 12 Oct 2022 13:45

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK423

Tgt Ion: 75 Resp: 5950
 Ion Ratio Lower Upper
 75 100
 77 47.2 21.9 40.7#

