

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101222\
 Data File : VW024872.D
 Acq On : 12 Oct 2022 14:45
 Operator : SY/VA
 Sample : N5049-12RE
 Misc : 5.96g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP8

Quant Time: Oct 12 23:20:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 23:18:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	530265	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	440066	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	158833	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	106672	17.051	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.200%
7) Chloroethane-d5	2.891	69	73817	20.153	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.600%
11) 1,1-Dichloroethene-d2	4.019	63	173394	12.748	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	51.000%
21) 2-Butanone-d5	7.086	46	44897	22.650	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	45.300%
24) Chloroform-d	7.647	84	329899	22.057	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.240%
26) 1,2-Dichloroethane-d4	8.427	65	210	0.027	ug/L	0.12
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.120%#
32) Benzene-d6	8.275	84	615096	22.290	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.160%
36) 1,2-Dichloropropane-d6	9.274	67	213587	25.235	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.960%
41) Toluene-d8	10.323	98	488278	19.714	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.840%
43) trans-1,3-Dichloroprop...	10.579	79	36829	11.473	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	45.880%
47) 2-Hexanone-d5	10.926	63	26010	18.329	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	36.660%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	162642	24.640	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.560%
66) 1,2-Dichlorobenzene-d4	13.847	152	120310	20.727	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.920%
Target Compounds					Qvalue	
13) Acetone	4.141	43	10003	7.212	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101222\
Data File : VW024872.D
Acq On : 12 Oct 2022 14:45
Operator : SY/VA
Sample : N5049-12RE
Misc : 5.96g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BP8

Quant Time: Oct 12 23:20:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 23:18:51 2022
Response via : Initial Calibration

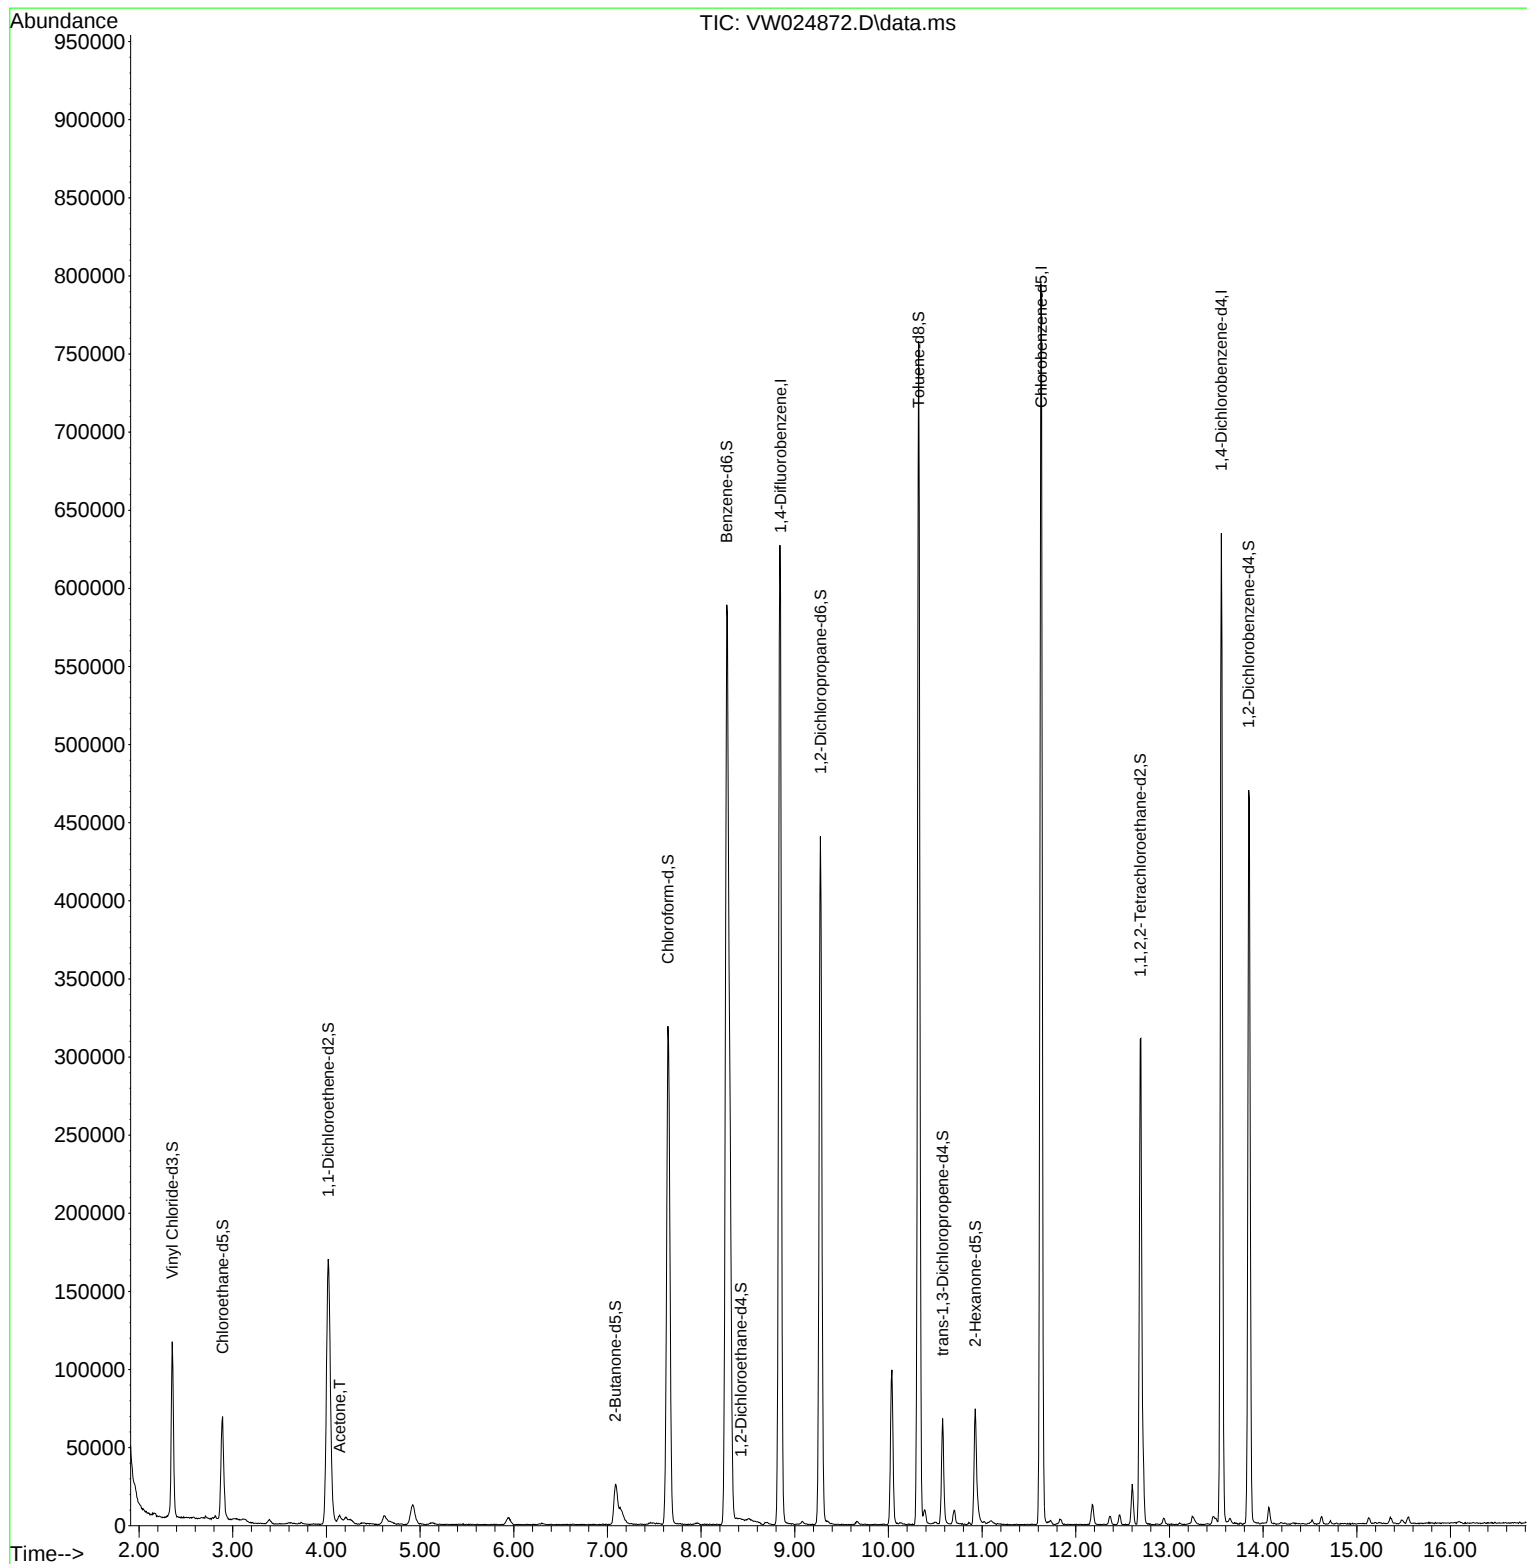

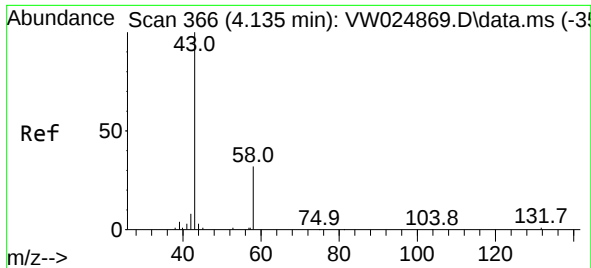

#13
 Acetone
 Concen: 7.212 ug/L
 RT: 4.141 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW024872.D
 Acq: 12 Oct 2022 14:45

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BP8

Tgt Ion: 43 Resp: 10003
 Ion Ratio Lower Upper
 43 100
 58 28.5 0.0 64.2

