

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101222\
 Data File : VW024887.D
 Acq On : 12 Oct 2022 20:47
 Operator : SY/VA
 Sample : N5070-13
 Misc : 6.54g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BS5

Quant Time: Oct 12 23:23:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 23:18:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	589251	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	503746	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	214332	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	112490	16.181	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.720%
7) Chloroethane-d5	2.885	69	72036	17.698	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.800%
11) 1,1-Dichloroethene-d2	4.019	63	177851	11.767	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	47.080%
21) 2-Butanone-d5	7.086	46	78381	35.584	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.160%
24) Chloroform-d	7.653	84	344835	20.748	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.000%
26) 1,2-Dichloroethane-d4	8.305	65	197512	22.707	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.840%
32) Benzene-d6	8.274	84	621690	19.681	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.720%
36) 1,2-Dichloropropane-d6	9.274	67	223742	23.093	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.360%
41) Toluene-d8	10.323	98	479183	16.901	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.600%
43) trans-1,3-Dichloroprop...	10.579	79	58527	15.928	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	63.720%
47) 2-Hexanone-d5	10.926	63	37907	23.336	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	46.680%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	205309	27.172	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.680%
66) 1,2-Dichlorobenzene-d4	13.847	152	160603	20.505	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	82.000%
Target Compounds					Qvalue	
34) Trichloroethene	8.841	95	18607	2.156	ug/L	# 7


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101222\
Data File : VW024887.D
Acq On : 12 Oct 2022 20:47
Operator : SY/VA
Sample : N5070-13
Misc : 6.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BS5


Quant Time: Oct 12 23:23:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 23:18:51 2022
Response via : Initial Calibration

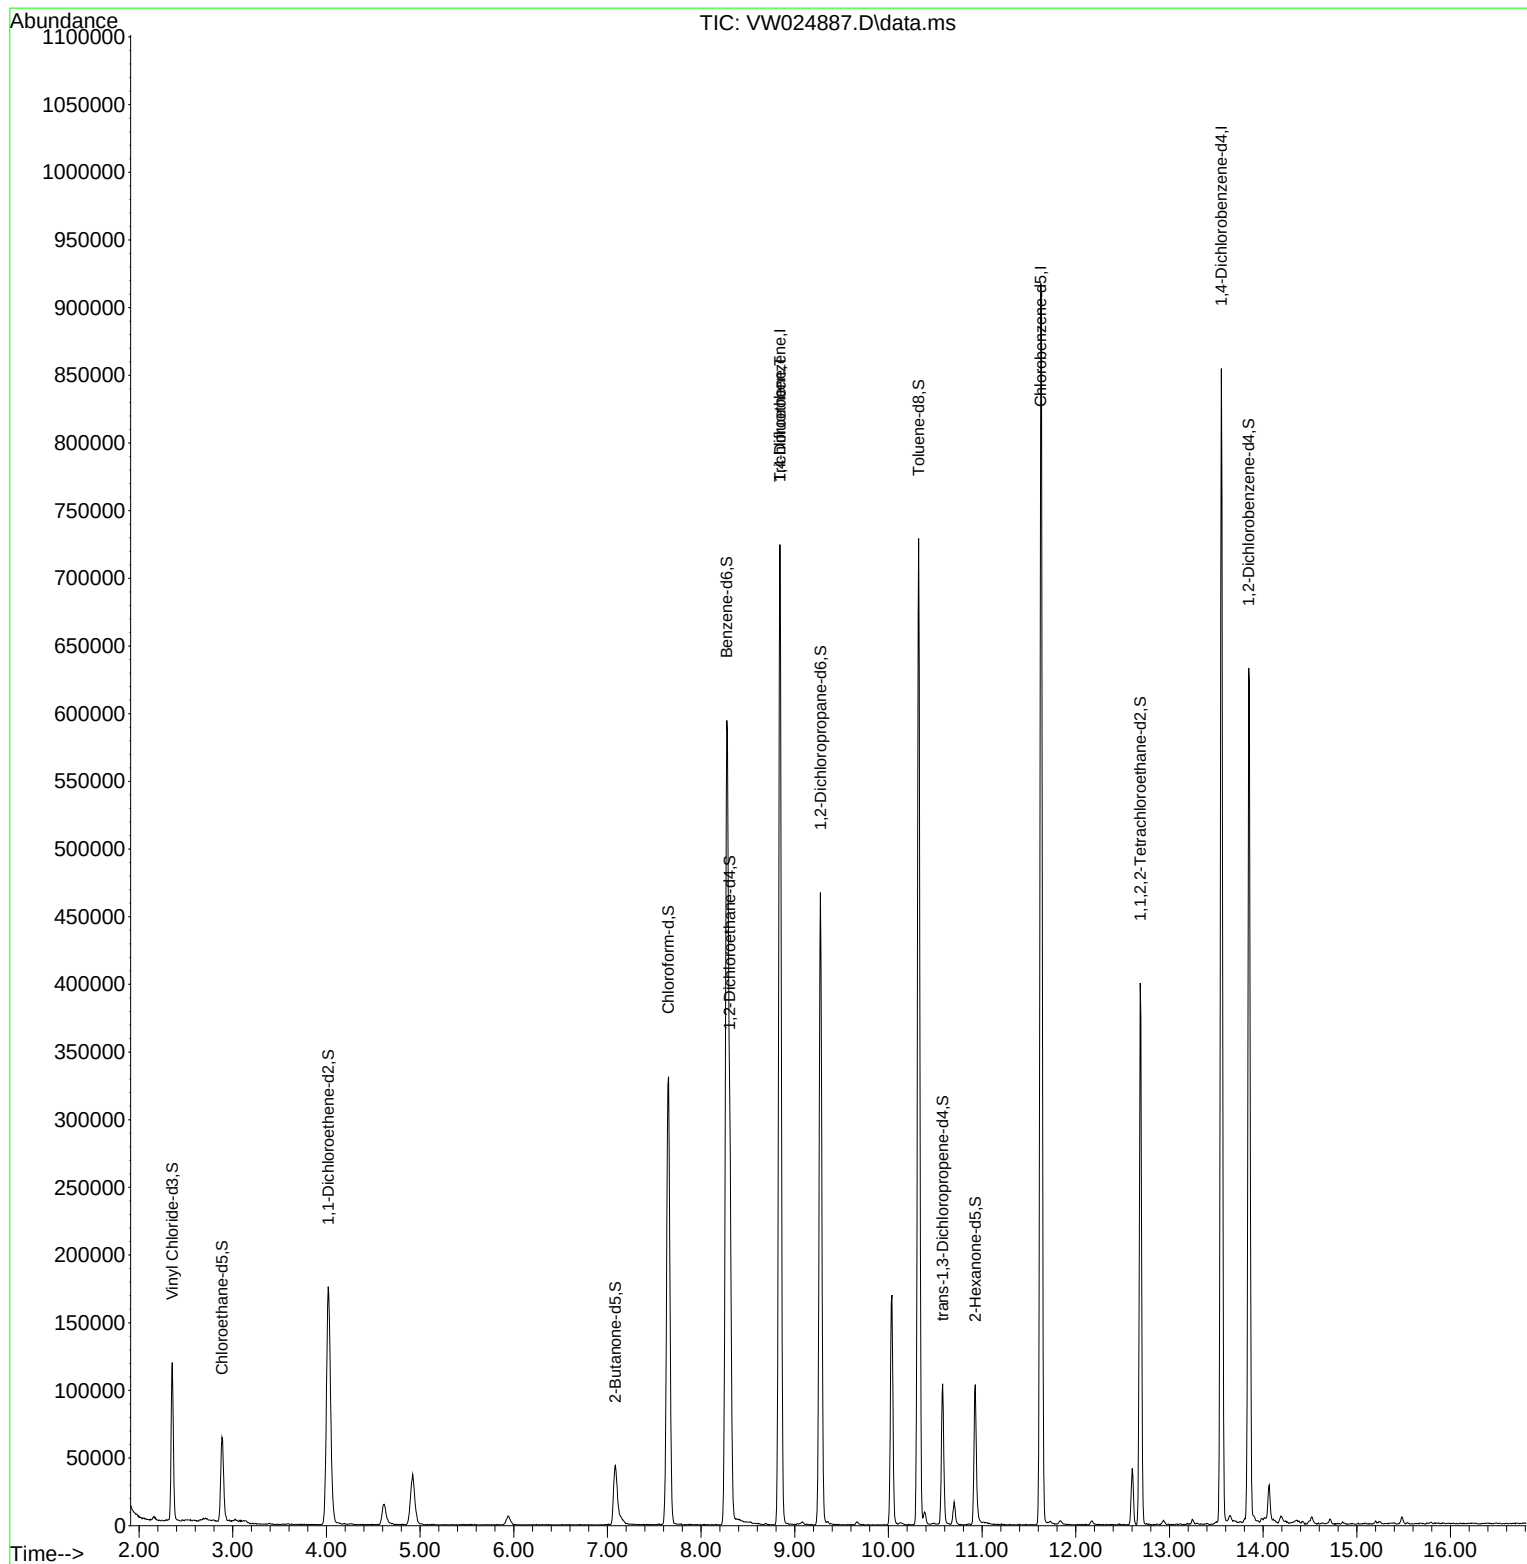

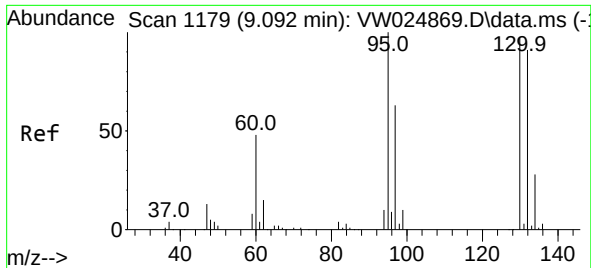

#34
 Trichloroethene
 Concen: 2.156 ug/L
 RT: 8.841 min Scan# 1179
 Delta R.T. -0.250 min
 Lab File: VW024887.D
 Acq: 12 Oct 2022 20:47

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BS5

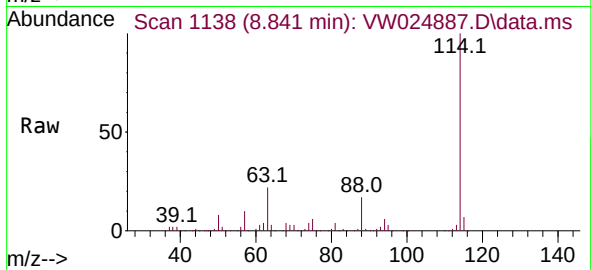

Tgt Ion: 95 Resp: 18607

Ion	Ratio	Lower	Upper
95	100		
97	0.0	44.2	82.0#
132	0.0	62.9	116.7#
130	0.0	66.8	124.0#

