

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101222\
 Data File : VW024891.D
 Acq On : 12 Oct 2022 22:23
 Operator : SY/VA
 Sample : N5064-17RE
 Misc : 7.44g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0BN6RE

Quant Time: Oct 12 23:24:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 12 23:18:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	158275	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	140245	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	51434	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	32730	17.528	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.120%
7) Chloroethane-d5	2.885	69	23161	21.185	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.720%
11) 1,1-Dichloroethene-d2	4.019	63	61961	15.262	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.040%
21) 2-Butanone-d5	7.086	46	41128	69.514	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	139.020%#
24) Chloroform-d	7.647	84	102642	22.992	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.960%
26) 1,2-Dichloroethane-d4	8.305	65	63657	27.246	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.000%
32) Benzene-d6	8.275	84	191731	21.801	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.200%
36) 1,2-Dichloropropane-d6	9.275	67	68679	25.462	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.840%
41) Toluene-d8	10.323	98	150812	19.106	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.440%
43) trans-1,3-Dichloroprop...	10.579	79	22727	22.216	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.880%
47) 2-Hexanone-d5	10.927	63	28313	62.607	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.220%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	65910	31.332	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	125.320%#
66) 1,2-Dichlorobenzene-d4	13.853	152	45254	24.076	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.320%
Target Compounds						
16) Methylene chloride	4.916	84	21928	7.847	ug/L	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101222\
Data File : VW024891.D
Acq On : 12 Oct 2022 22:23
Operator : SY/VA
Sample : N5064-17RE
Misc : 7.44g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BN6RE


Quant Time: Oct 12 23:24:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 12 23:18:51 2022
Response via : Initial Calibration

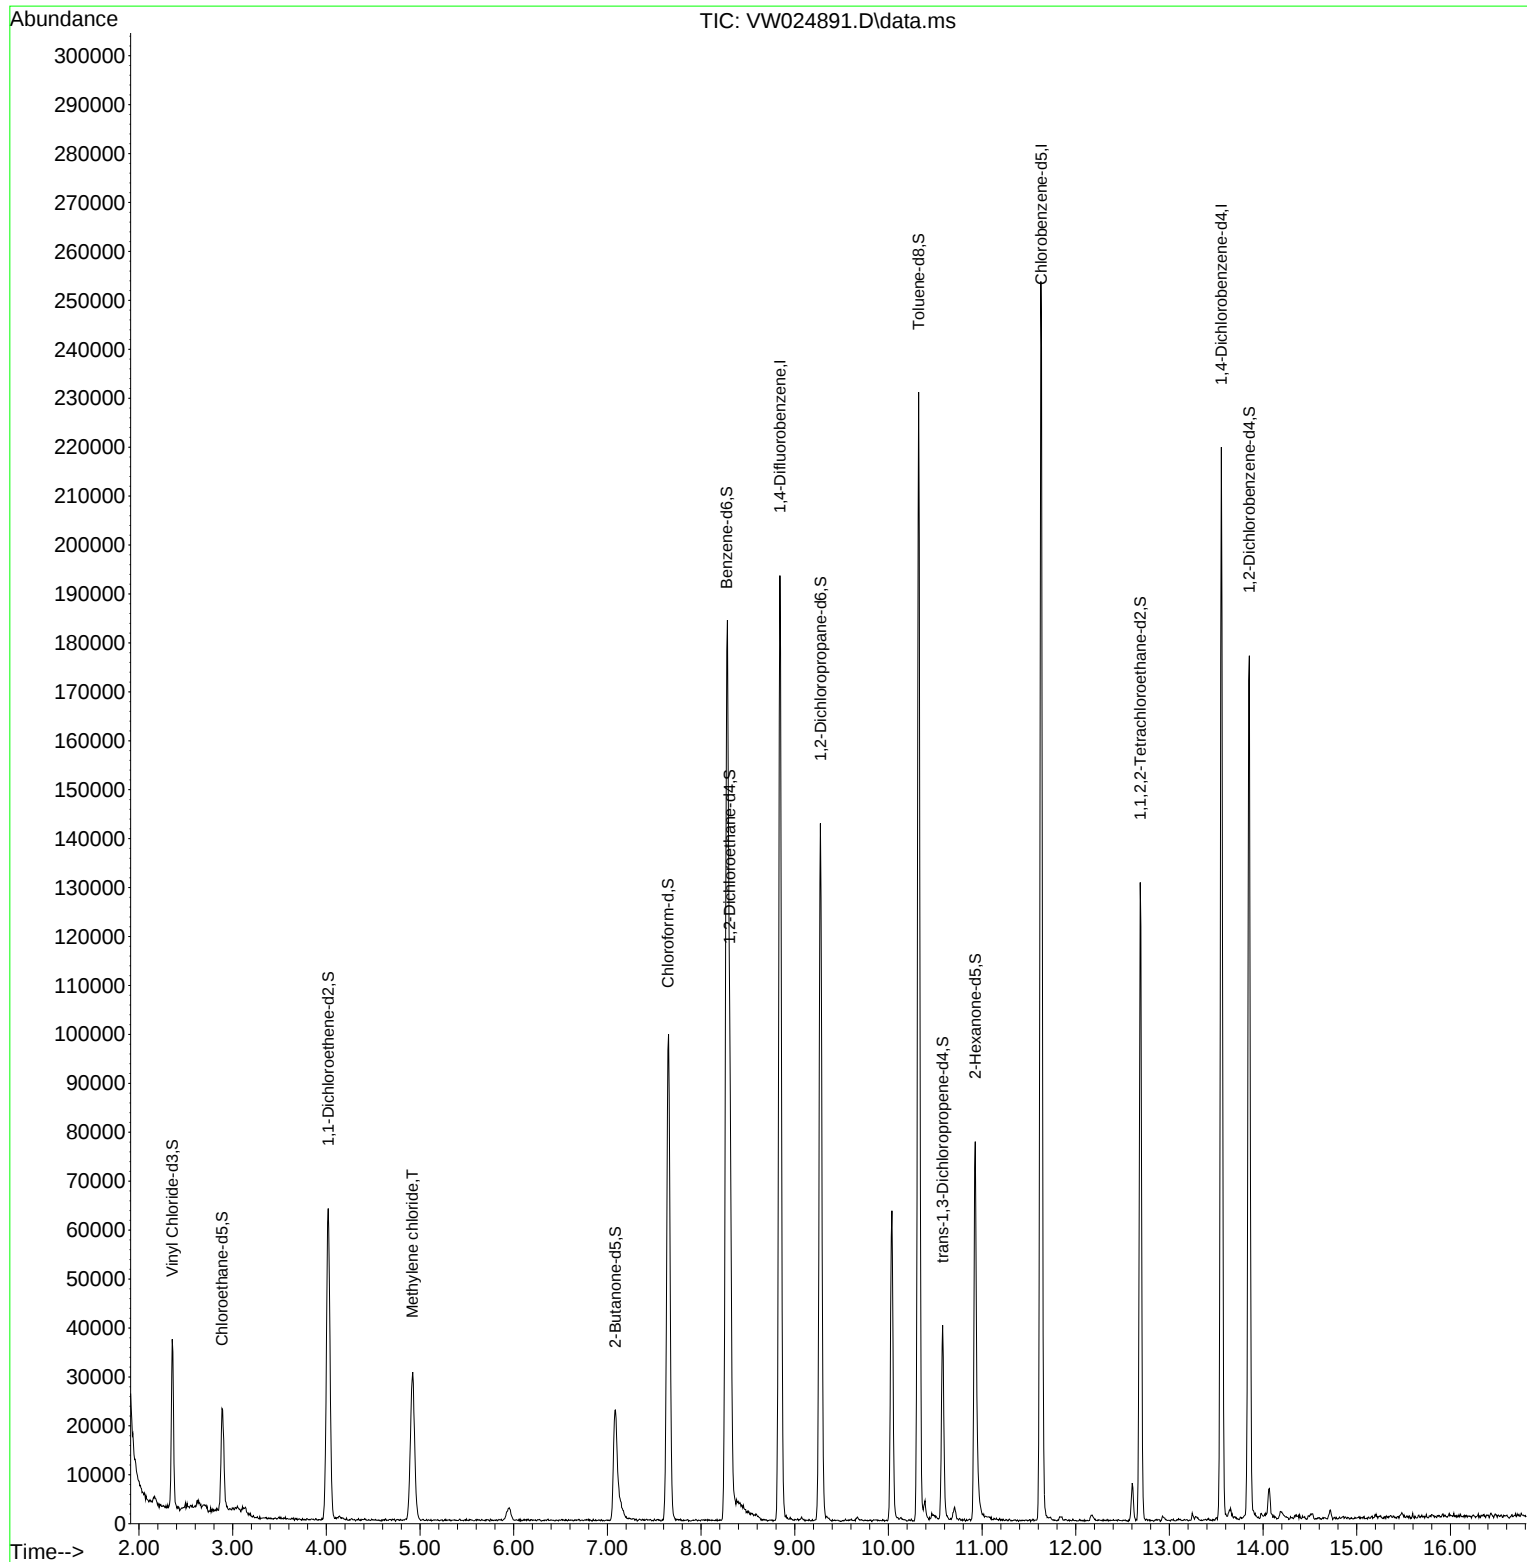

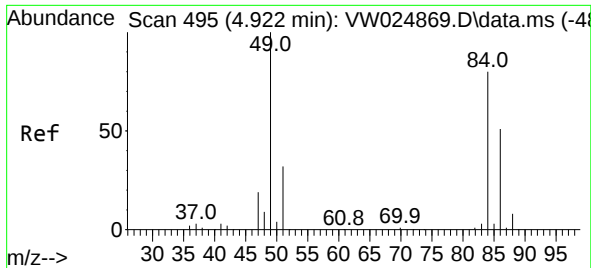

#16
Methylene chloride
Concen: 7.847 ug/L
RT: 4.916 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW024891.D
Acq: 12 Oct 2022 22:23

Instrument :
MSVOA_W
ClientSampleId :
C0BN6RE

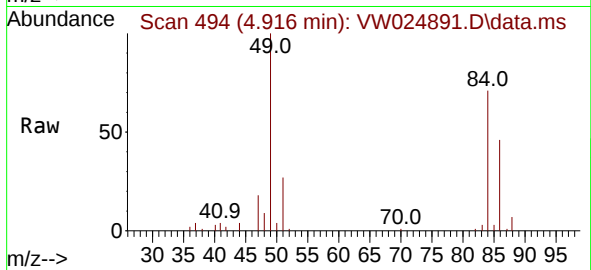

Tgt Ion: 84 Resp: 21928

Ion	Ratio	Lower	Upper
84	100		
86	64.5	45.5	84.5
49	140.6	90.9	168.9

