
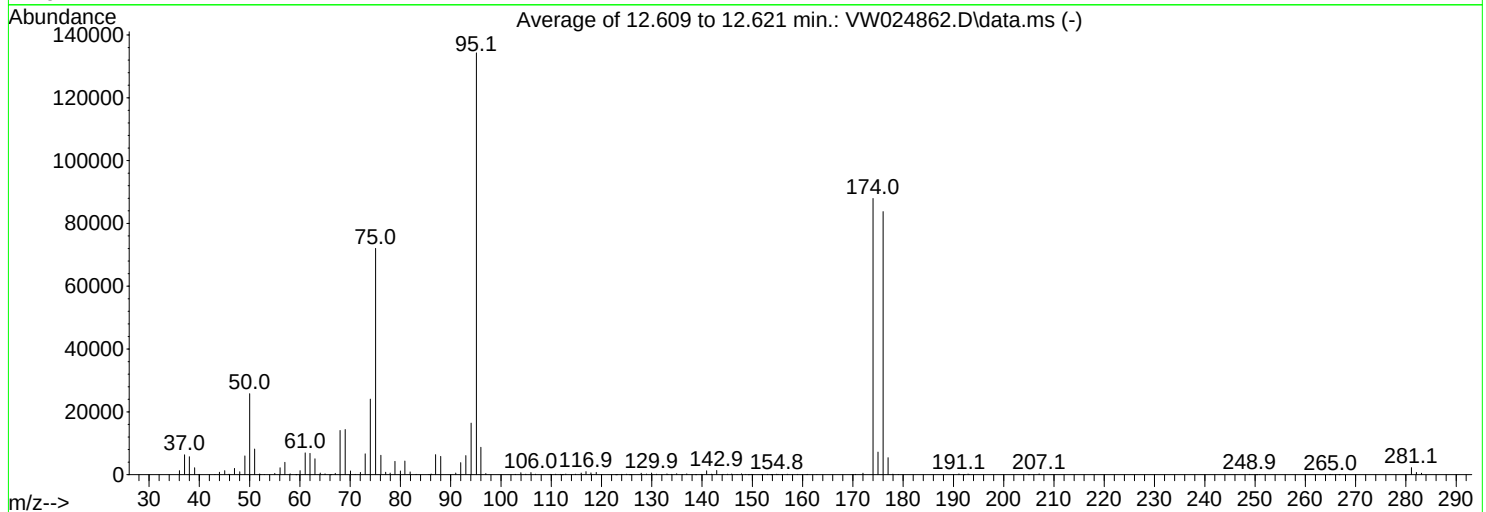


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101222\
Data File : VW024862.D
Acq On : 12 Oct 2022 09:57
Operator : SY/VA
Sample : BFB441
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB441

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101222SMA.M
Title : SFAM01.0
Last Update : Wed Oct 12 23:18:51 2022

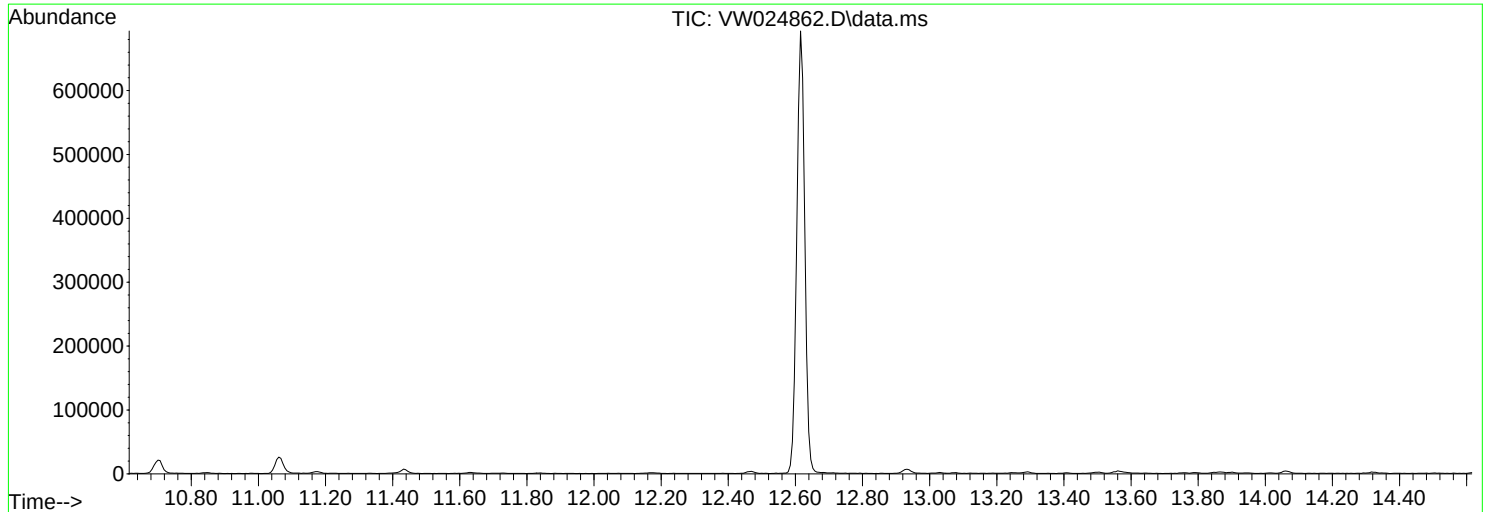

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	25792	PASS
75	95	30	80	53.6	72040	PASS
95	95	100	100	100.0	134325	PASS
96	95	5	9	6.5	8701	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	65.5	87960	PASS
175	174	5	9	8.2	7196	PASS
176	174	95	105	95.2	83755	PASS
177	176	5	10	6.5	5407	PASS

m/z	Abundance
39.90	339.0
41.00	80.0
43.10	100.0
44.00	342.0
57.40	58.0
169.00	74.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

m/z	Abundance
36.00	1254.0
37.10	6044.0
38.00	5574.0
39.10	2123.0
40.00	393.0
43.10	192.0
44.00	1206.0
45.00	1128.0
45.90	209.0
47.00	1825.0
48.00	928.0
49.10	5414.0
50.00	24952.0
51.00	7801.0
52.00	352.0
53.00	74.0
55.10	448.0
56.00	2153.0
57.00	3854.0
58.10	204.0
59.20	93.0
60.00	1327.0
61.00	7121.0
62.00	6265.0
63.00	4607.0
64.10	425.0
65.00	399.0
66.10	67.0
67.20	328.0
68.00	13202.0
69.00	14016.0
70.10	1084.0
71.00	128.0
72.00	703.0
73.00	6199.0
74.00	21392.0
75.00	67448.0
76.10	5857.0
77.10	771.0
78.00	481.0
78.90	3823.0
80.00	1025.0
80.90	3963.0
81.90	876.0
86.20	206.0
87.00	5470.0
88.00	5600.0
91.10	455.0
92.00	3200.0
93.00	5255.0
94.10	14556.0
95.10	125448.0
96.00	8062.0
97.00	318.0
104.00	578.0
105.00	190.0
105.90	553.0
106.90	177.0
109.80	104.0
110.80	143.0
111.80	107.0
112.90	159.0
114.90	154.0
116.00	472.0
116.80	839.0
117.90	685.0
118.90	703.0
122.80	65.0
124.10	77.0
125.00	249.0
125.60	90.0
127.90	285.0
128.90	233.0
129.90	400.0
131.00	210.0
133.00	574.0
134.00	209.0
135.00	250.0
137.00	153.0
139.80	100.0
140.90	1032.0
141.90	146.0
142.90	1012.0
144.10	94.0
145.10	113.0
145.90	177.0
146.90	102.0
147.80	165.0
148.70	144.0
149.80	79.0
153.10	73.0
154.00	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

154.80	211.0
156.90	147.0
159.00	92.0
160.70	96.0
162.90	102.0
170.60	53.0
171.90	405.0
174.00	70760.0
175.00	5734.0
176.00	70424.0
177.00	4689.0
178.00	145.0
179.00	105.0
191.00	345.0
192.10	82.0
192.90	490.0
204.90	65.0
207.00	375.0
248.90	189.0
250.30	56.0
250.90	117.0
264.80	194.0
265.30	186.0
266.00	103.0
266.70	75.0
280.00	118.0
281.20	3397.0
282.10	1107.0
283.10	693.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

m/z	Abundance
36.00	1519.0
37.00	7185.0
38.00	6909.0
39.10	2237.0
40.00	470.0
43.10	171.0
44.00	1159.0
45.00	1326.0
45.90	187.0
47.00	2392.0
48.00	960.0
49.00	6649.0
50.00	28544.0
51.00	9094.0
52.20	296.0
52.90	64.0
54.90	424.0
56.10	2374.0
57.00	4096.0
58.00	300.0
60.10	1484.0
61.10	7376.0
62.00	7722.0
63.00	5671.0
64.00	571.0
65.00	266.0
67.00	523.0
68.00	15829.0
69.00	15483.0
70.00	1364.0
71.00	101.0
72.00	858.0
73.00	7343.0
74.00	27208.0
75.10	81176.0
76.10	6697.0
77.10	773.0
77.90	621.0
78.90	4782.0
80.00	1336.0
80.90	4760.0
81.90	953.0
83.10	193.0
86.00	240.0
87.00	7112.0
88.00	6903.0
91.00	505.0
92.00	4558.0
93.00	6870.0
94.00	18416.0
95.10	147520.0
96.00	9756.0
97.00	432.0
102.80	154.0
103.90	668.0
104.80	168.0
105.90	717.0
107.00	196.0
109.80	162.0
110.90	174.0
111.90	138.0
112.80	237.0
114.80	144.0
115.90	692.0
116.90	1207.0
117.90	607.0
119.00	710.0
124.00	96.0
124.80	107.0
125.90	58.0
127.90	575.0
129.00	244.0
130.00	526.0
130.90	216.0
133.00	231.0
133.90	79.0
135.00	323.0
136.90	296.0
139.90	150.0
140.90	1249.0
141.90	146.0
142.90	1438.0
144.20	92.0
145.00	166.0
145.80	219.0
147.00	82.0
147.90	301.0
148.70	122.0
149.80	165.0
153.00	218.0
153.90	71.0
154.90	292.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

155.90	102.0
156.90	194.0
158.90	188.0
161.00	139.0
162.80	53.0
169.90	51.0
170.50	160.0
172.00	499.0
174.00	95776.0
175.00	8030.0
176.00	91848.0
177.00	5987.0
177.90	150.0
179.10	90.0
191.10	246.0
193.10	320.0
207.10	294.0
248.90	142.0
250.90	111.0
265.00	206.0
266.10	68.0
281.00	2083.0
282.10	738.0
283.10	488.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

m/z	Abundance
36.10	1134.0
37.00	5825.0
38.00	4702.0
39.00	2232.0
40.00	424.0
43.10	125.0
44.00	919.0
45.10	1330.0
46.00	107.0
47.00	1807.0
48.10	877.0
49.00	5816.0
50.00	23880.0
51.00	7625.0
52.00	273.0
52.80	50.0
55.00	295.0
56.10	1980.0
57.00	3811.0
58.10	210.0
60.00	1001.0
61.00	6273.0
62.00	6355.0
63.00	4815.0
64.00	500.0
65.10	160.0
67.00	417.0
68.00	13249.0
69.00	13617.0
70.10	1145.0
71.00	137.0
72.10	647.0
73.00	6343.0
74.00	23552.0
75.00	67496.0
76.10	5952.0
77.00	767.0
78.00	486.0
78.90	4173.0
80.00	1154.0
80.90	4237.0
82.00	734.0
83.10	120.0
85.70	115.0
86.00	116.0
87.00	6498.0
88.00	5002.0
90.90	650.0
92.00	3729.0
93.00	6034.0
94.00	16196.0
95.10	130008.0
96.00	8285.0
97.00	293.0
102.90	103.0
103.90	650.0
105.00	167.0
106.00	650.0
106.80	125.0
109.70	75.0
111.00	105.0
111.80	68.0
112.20	60.0
113.00	163.0
114.90	207.0
115.90	439.0
117.00	903.0
117.90	455.0
118.90	762.0
123.00	77.0
124.00	79.0
125.10	115.0
126.00	67.0
127.90	561.0
129.00	174.0
129.90	553.0
131.00	93.0
133.20	205.0
134.90	315.0
136.10	104.0
136.90	309.0
138.70	86.0
139.80	89.0
140.90	1334.0
141.90	128.0
142.90	1490.0
144.10	74.0
145.10	131.0
146.00	264.0
147.80	315.0
149.20	56.0
149.70	157.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441

150.10	122.0
151.90	51.0
152.90	63.0
153.70	72.0
155.10	336.0
155.90	56.0
157.00	154.0
159.00	120.0
160.90	177.0
169.10	58.0
170.40	64.0
172.10	481.0
174.00	97344.0
175.00	7825.0
176.00	88992.0
177.00	5546.0
177.90	220.0
191.20	128.0
192.90	201.0
207.10	82.0
265.00	62.0
281.10	1258.0
282.20	334.0
283.10	204.0

Instrument :
MSVOA_W
ClientSampleId :
BFB441