

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101223\
 Data File : VW027296.D
 Acq On : 12 Oct 2023 15:17
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 12 21:58:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 12 21:57:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	490846	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	444771	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	232731	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	195808	26.139	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 104.560%			
7) Chloroethane-d5	2.899	69	145325	27.018	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 108.080%			
11) 1,1-Dichloroethene-d2	4.021	65	97271	25.914	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 103.640%			
21) 2-Butanone-d5	7.075	46	125282	50.317	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 100.640%			
24) Chloroform-d	7.648	84	380524	26.011	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 104.040%			
26) 1,2-Dichloroethane-d4	8.307	65	212021	26.979	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 107.920%			
32) Benzene-d6	8.276	84	818243	27.191	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 108.760%			
36) 1,2-Dichloropropane-d6	9.276	67	245185	26.676	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 106.720%			
41) Toluene-d8	10.325	98	726888	26.638	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 106.560%			
43) trans-1,3-Dichloroprop...	10.575	79	111516	26.611	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 106.440%			
47) 2-Hexanone-d5	10.922	63	103587	54.473	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 108.940%			
56) 1,1,2,2-Tetrachloroeth...	12.690	84	185778	27.091	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 108.360%			
66) 1,2-Dichlorobenzene-d4	13.848	152	213975	25.371	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 101.480%			
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	17302	1.926	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101223\
Data File : VW027296.D
Acq On : 12 Oct 2023 15:17
Operator : SY/MD
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 12 21:58:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 12 21:57:41 2023
Response via : Initial Calibration

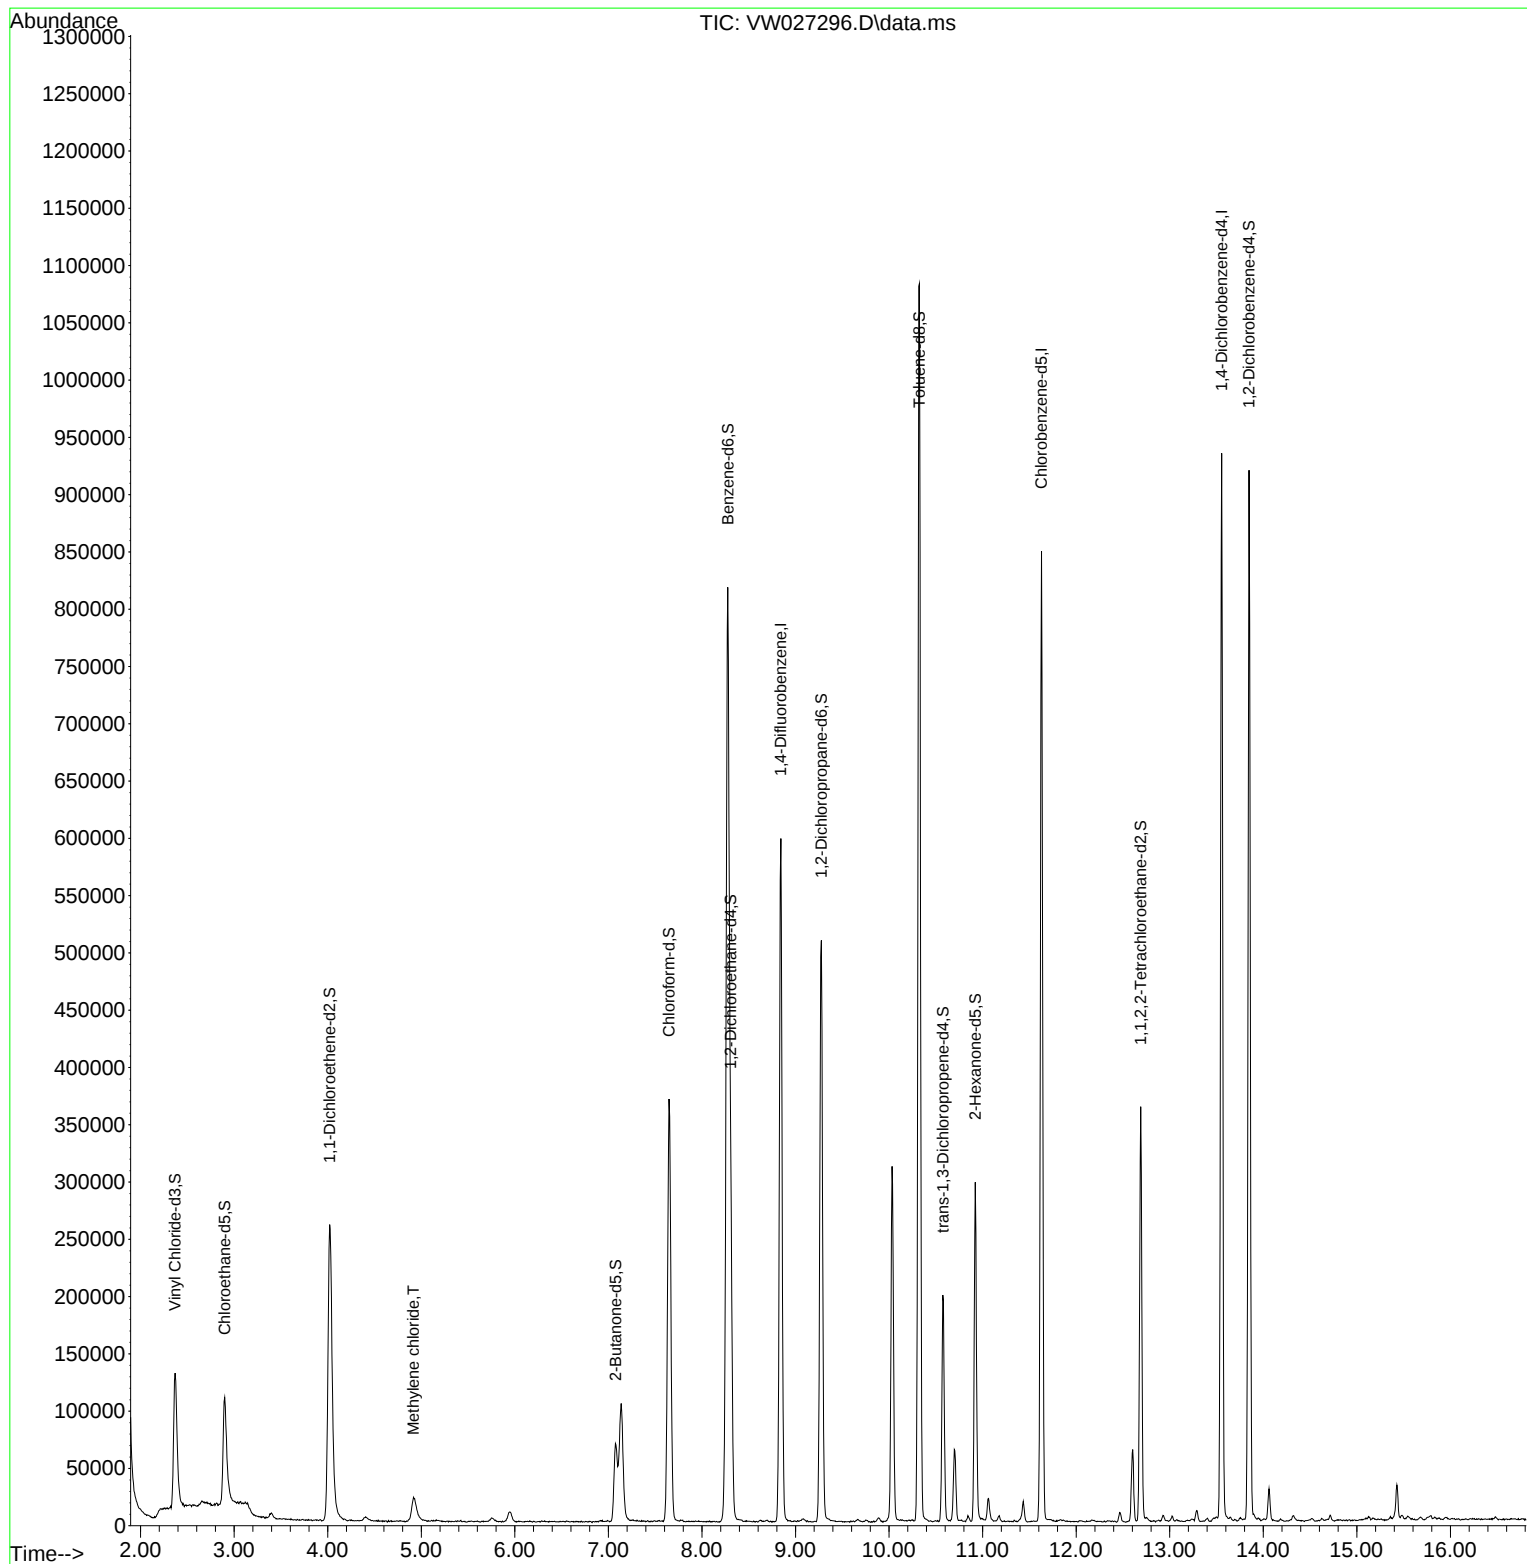

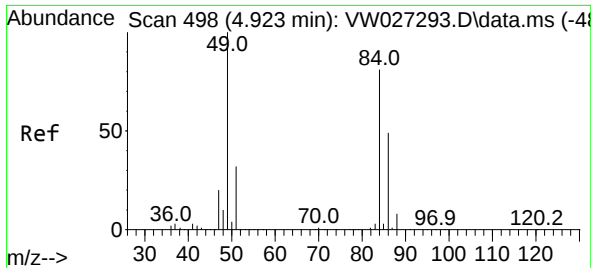

#16
 Methylene chloride
 Concen: 1.926 ug/L
 RT: 4.917 min Scan# 49
 Delta R.T. -0.006 min
 Lab File: VW027296.D
 Acq: 12 Oct 2023 15:17

Instrument :
 MSVOA_W
 ClientSampleId :

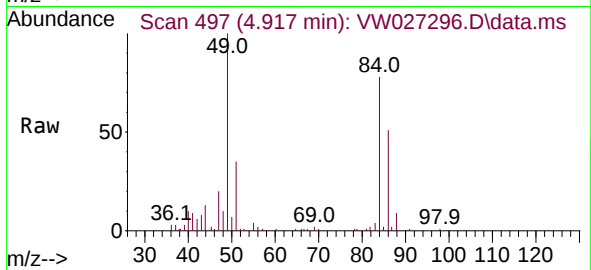

Tgt Ion:	84	Resp:	17302
Ion	Ratio	Lower	Upper
84	100		
86	64.8	41.3	76.7
49	127.8	92.8	172.4

