

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101223\
 Data File : VW027296.D
 Acq On : 12 Oct 2023 15:17
 Operator : SY/MD
 Sample : VIBLK529
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK529

Quant Time: Oct 12 21:58:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 12 21:57:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	490846	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	444771	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	232731	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	195808	26.139	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.560%
7) Chloroethane-d5	2.899	69	145325	27.018	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.080%
11) 1,1-Dichloroethene-d2	4.021	65	97271	25.914	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	103.640%
21) 2-Butanone-d5	7.075	46	125282	50.317	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.640%
24) Chloroform-d	7.648	84	380524	26.011	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.040%
26) 1,2-Dichloroethane-d4	8.307	65	212021	26.979	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.920%
32) Benzene-d6	8.276	84	818243	27.191	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.760%
36) 1,2-Dichloropropane-d6	9.276	67	245185	26.676	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.720%
41) Toluene-d8	10.325	98	726888	26.638	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	106.560%
43) trans-1,3-Dichloroprop...	10.575	79	111516	26.611	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	106.440%
47) 2-Hexanone-d5	10.922	63	103587	54.473	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.940%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	185778	27.091	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.360%
66) 1,2-Dichlorobenzene-d4	13.848	152	213975	25.371	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.480%
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	17302	1.926	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101223\
Data File : VW027296.D
Acq On : 12 Oct 2023 15:17
Operator : SY/MD
Sample : VIBLK529
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK529

Quant Time: Oct 12 21:58:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM101123SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 12 21:57:41 2023
Response via : Initial Calibration

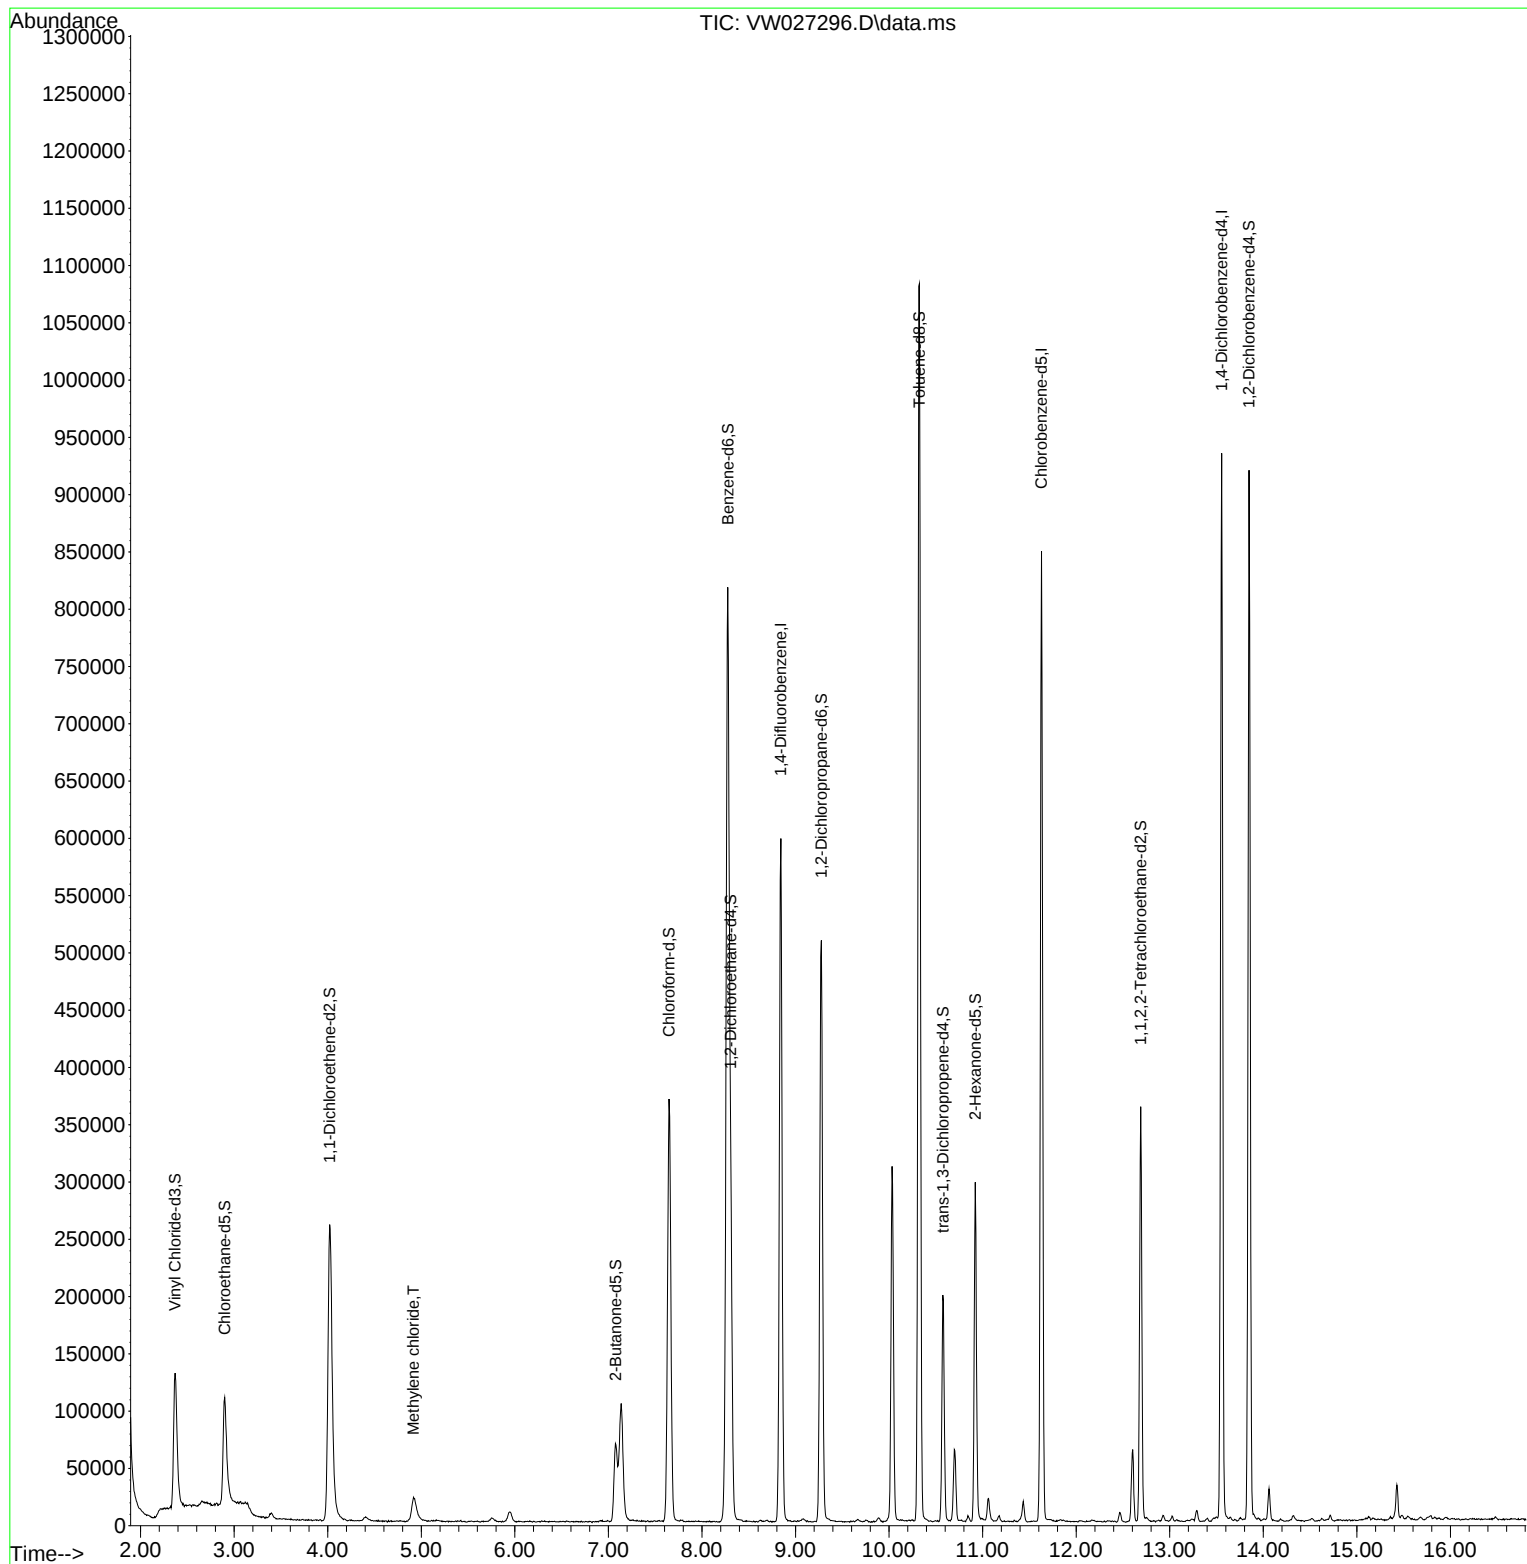

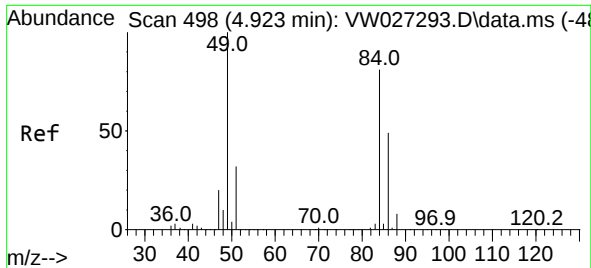

#16
Methylene chloride
Concen: 1.926 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.006 min
Lab File: VW027296.D
Acq: 12 Oct 2023 15:17

Instrument :
MSVOA_W
ClientSampleId :
VIBLK529

Tgt Ion: 84 Resp: 17302
Ion Ratio Lower Upper
84 100
86 64.8 41.3 76.7
49 127.8 92.8 172.4

