

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101419\
 Data File : VW013560.D
 Acq On : 14 Oct 2019 14:04
 Operator : SY/VA
 Sample : K5262-19RE
 Misc : 3.89G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 14 15:32:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 14 15:29:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	261028	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	188275	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	57116	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	47136	15.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.12%
7) Chloroethane-d5	2.89	69	44016	19.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.76%
10) 1,1-Dichloroethene-d2	4.01	63	74949	12.09	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.36%
20) 2-Butanone-d5	7.08	46	34197	38.00	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.00%
24) Chloroform-d	7.65	84	118004	20.81	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.24%
26) 1,2-Dichloroethane-d4	8.31	65	66791	22.74	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.96%
29) Benzene-d6	8.27	84	236821	23.48	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.92%
33) 1,2-Dichloropropane-d6	9.27	67	76469	25.56	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.24%
37) Toluene-d8	10.32	98	184239	19.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.00%
38) trans-1,3-Dichloropropene-	10.58	79	26526	19.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.60%
39) 2-Hexanone-d5	10.92	63	27581	46.08	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.16%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	60295	25.13	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	40464	19.71	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.84%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.55	75	6590	3.591 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101419\
Data File : VW013560.D
Acq On : 14 Oct 2019 14:04
Operator : SY/VA
Sample : K5262-19RE
Misc : 3.89G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 14 15:32:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 14 15:29:36 2019
Response via : Initial Calibration

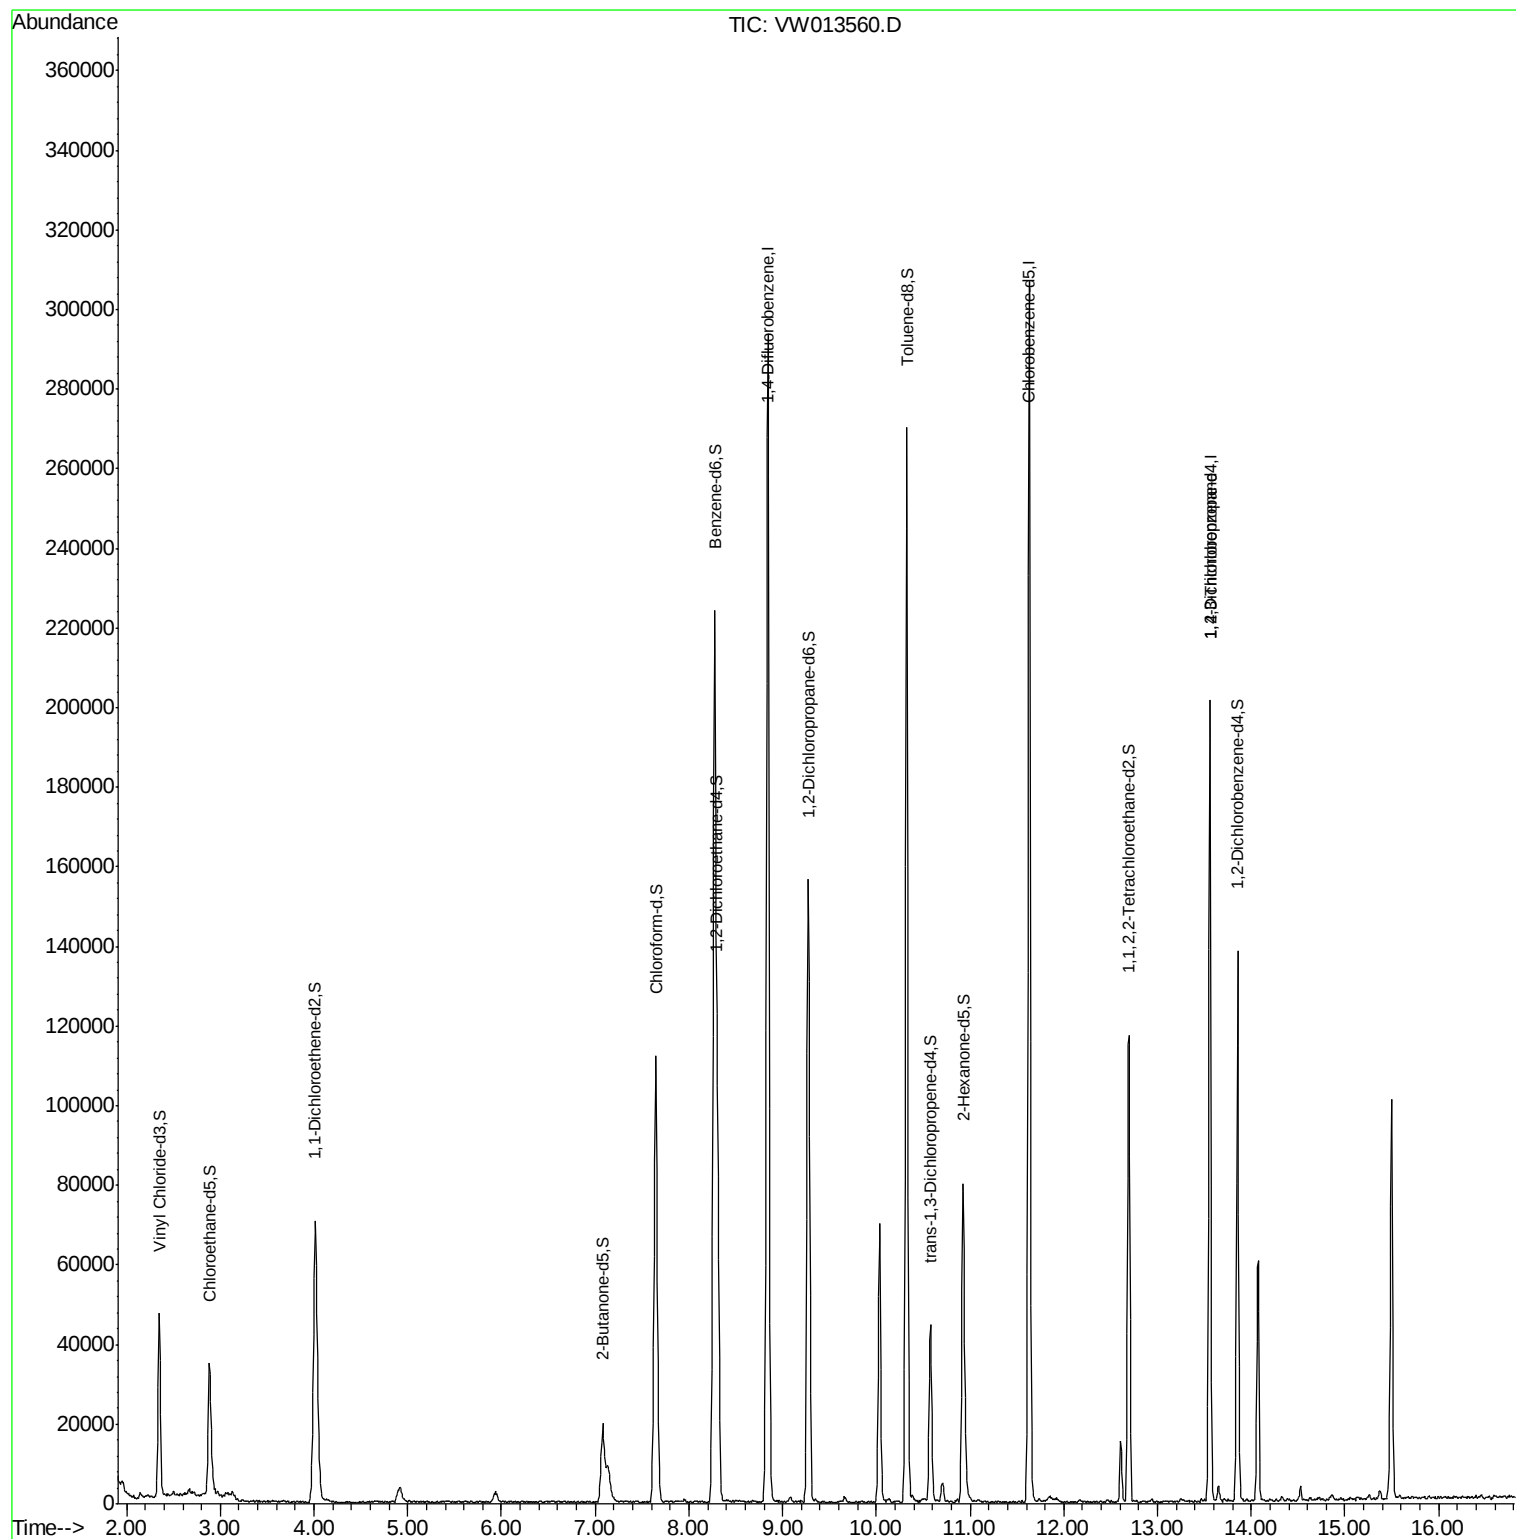

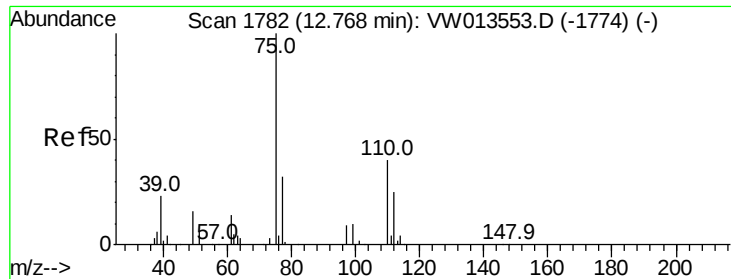

#59

1,2,3-Trichloropropane

Concen: 3.591 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW013560.D

Acq: 14 Oct 2019 14:04

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 6590

Ion Ratio Lower Upper

75 100

77 32.8 25.5 38.3

