

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101419\NOT REVIEWED DATA\
 Data File : VW013563.D
 Acq On : 14 Oct 2019 15:33
 Operator : SY/VA
 Sample : K5354-02
 Misc : 4.21G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 14 18:05:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 14 15:29:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	294878	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	217919	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	70651	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	61287	18.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.64%
7) Chloroethane-d5	2.89	69	57627	22.24	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.96%
10) 1,1-Dichloroethene-d2	4.01	63	96822	13.82	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.28%
20) 2-Butanone-d5	7.07	46	46307	45.55	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.10%
24) Chloroform-d	7.64	84	156474	24.43	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.72%
26) 1,2-Dichloroethane-d4	8.31	65	80803	24.35	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.40%
29) Benzene-d6	8.27	84	306690	26.27	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.08%
33) 1,2-Dichloropropane-d6	9.27	67	101108	29.19	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	116.76%
37) Toluene-d8	10.32	98	251342	22.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.72%
38) trans-1,3-Dichloropropene-	10.58	79	32209	20.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.52%
39) 2-Hexanone-d5	10.93	63	33540	48.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.84%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	71183	25.64	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.56%
61) 1,2-Dichlorobenzene-d4	13.85	152	56367	22.20	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.80%


Target Compounds					Ovalue
40) 1,2-Dichloropropane	9.27	63	10770	3.396 ug/L #	85
59) 1,2,3-Trichloropropane	13.55	75	7080	3.334 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101419\NOT REVIEWED DATA\
Data File : VW013563.D
Acq On : 14 Oct 2019 15:33
Operator : SY/VA
Sample : K5354-02
Misc : 4.21G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 14 18:05:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 14 15:29:36 2019
Response via : Initial Calibration

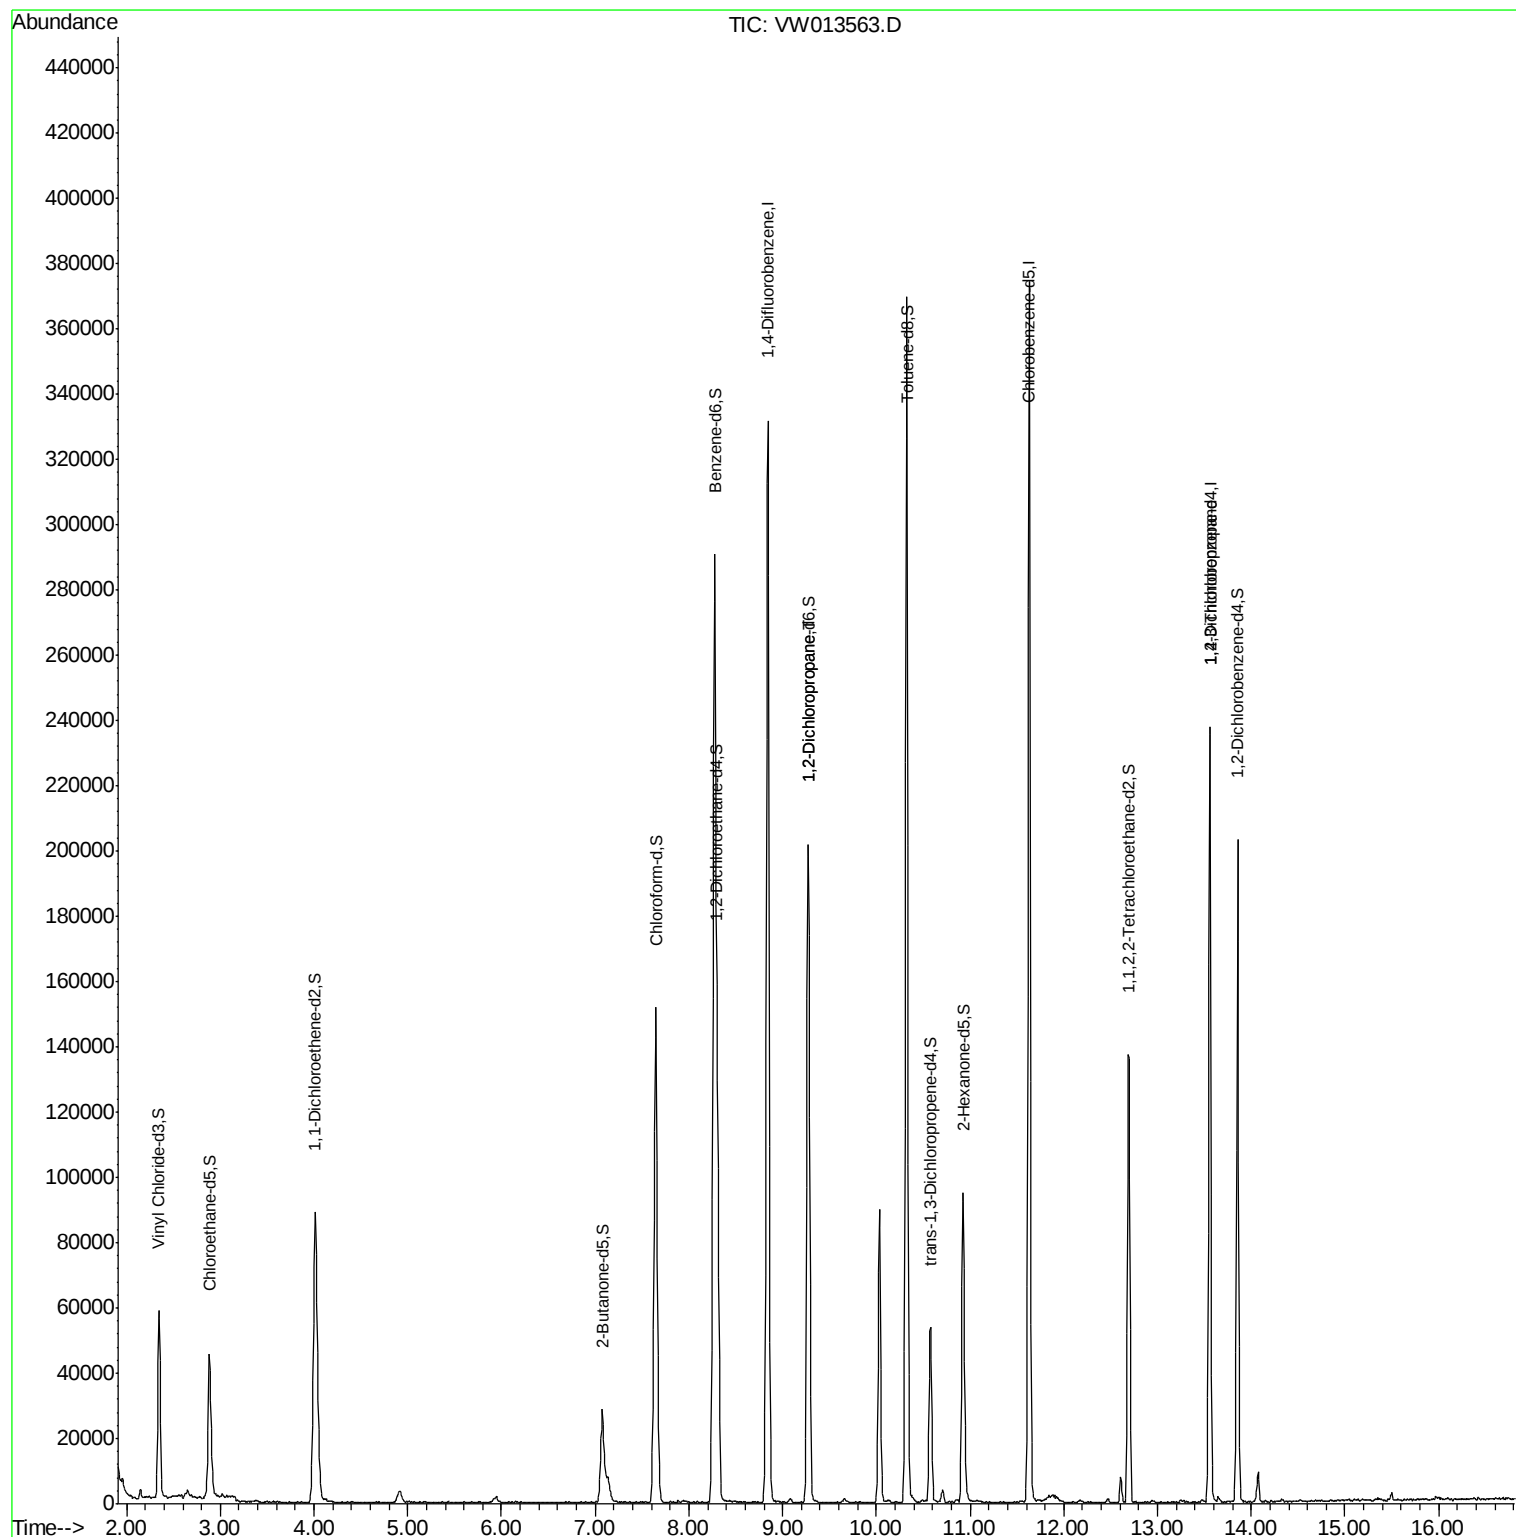

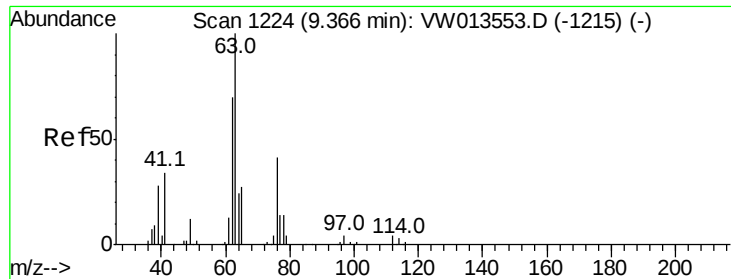

#40

1,2-Dichloropropane

Concen: 3.396 ug/L

RT: 9.27 min Scan# 1209

Delta R.T. -0.09 min

Lab File: VW013563.D

Acq: 14 Oct 2019 15:33

Instrument :

MSVOA_W





ClientSampleId :

Tot Ion: 63 Resp: 10770

Ion Ratio Lower Upper

63 100

112 0.0 3.8 5.8#

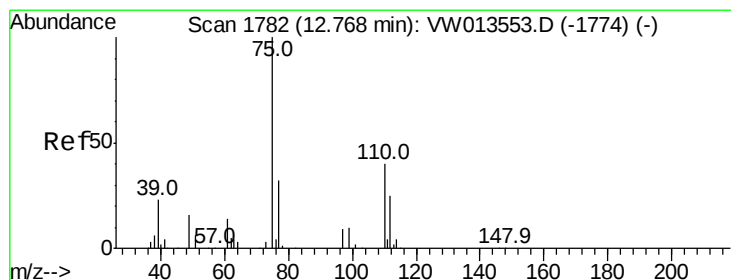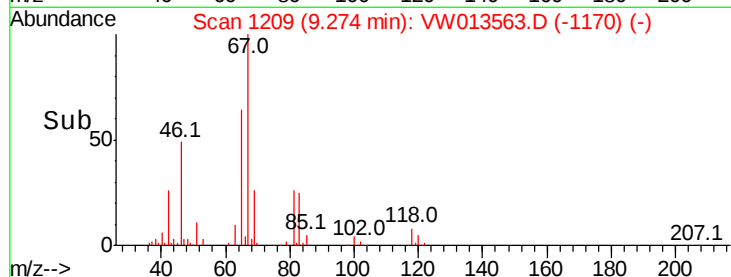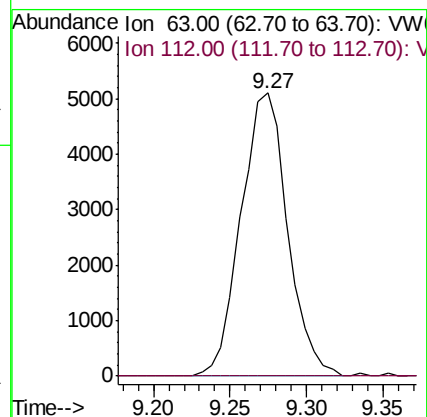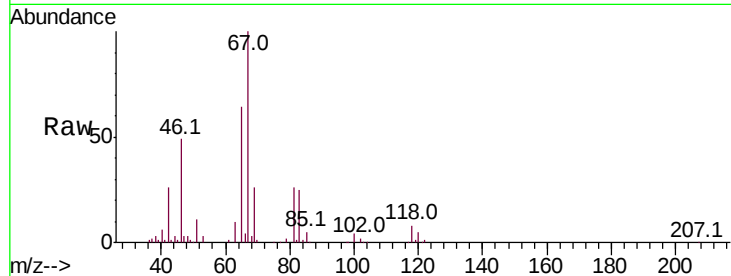

#59

1,2,3-Trichloropropane

Concen: 3.334 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW013563.D

Acq: 14 Oct 2019 15:33

Tgt Ion: 75 Resp: 7080

Ion Ratio Lower Upper

75 100

77 35.2 25.5 38.3

