

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101420\
 Data File : VW016891.D
 Acq On : 13 Oct 2020 11:07
 Operator : SY/VA
 Sample : VW1014SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VBLK27

Manual Integrations
APPROVED

MMDadoda
 10/15/2020 4:54:53 PM

Quant Time: Oct 14 08:42:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 14 08:34:08 2020
 Response via : Initial Calibration

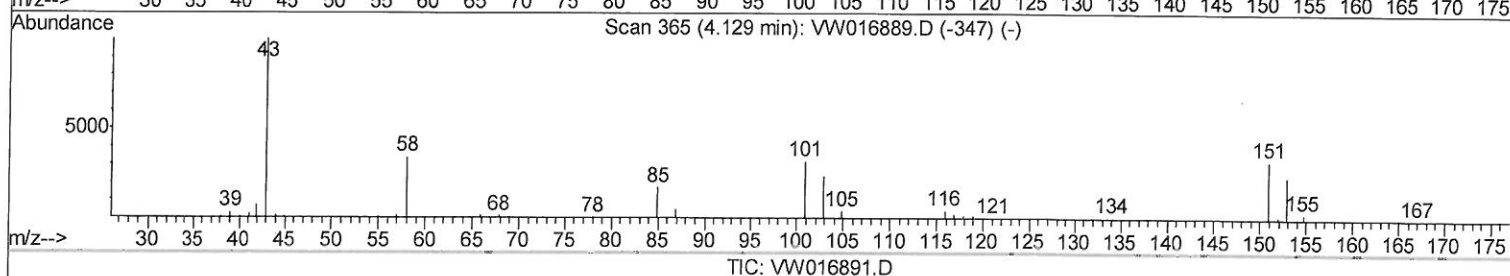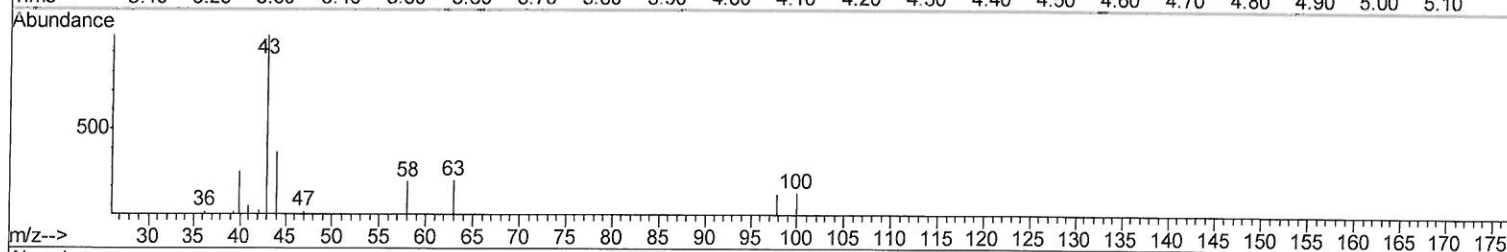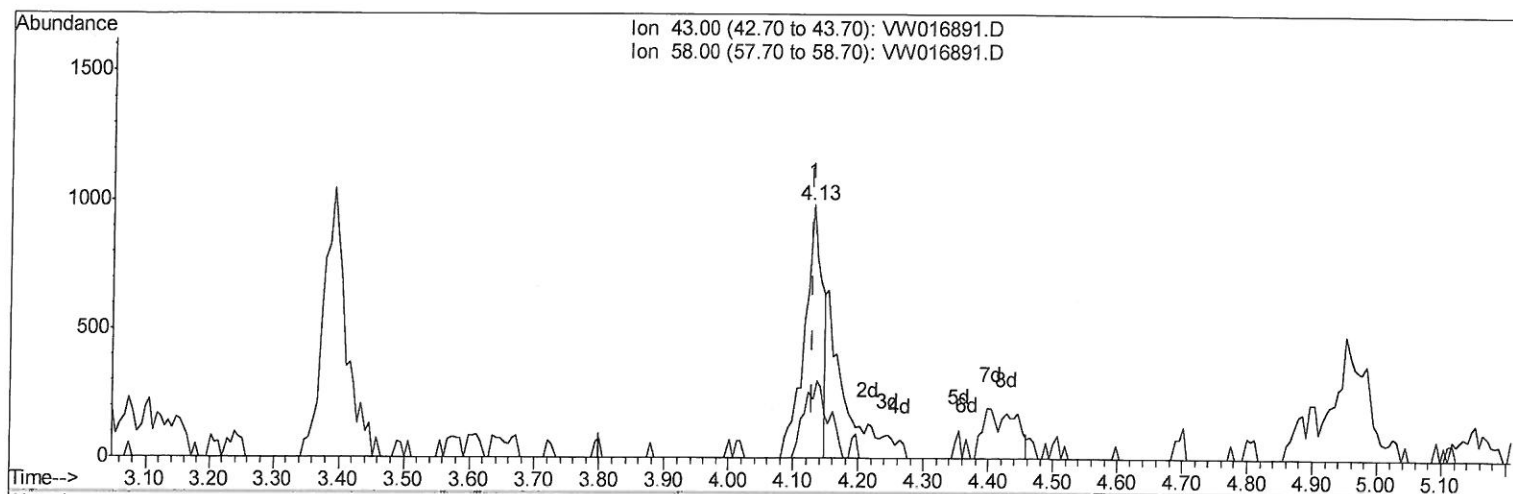

TIC: VW016891.D

(13) Acetone (T)

4.129min (-0.001) 2.02ug/L

response 1884

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	33.81
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101420\
 Data File : VW016891.D
 Acq On : 13 Oct 2020 11:07
 Operator : SY/VA
 Sample : VW1014SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VBLK27

Manual Integrations
APPROVED

MMDadoda
 10/15/2020 4:54:53 PM

Quant Time: Oct 14 08:42:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 14 08:34:08 2020
 Response via : Initial Calibration

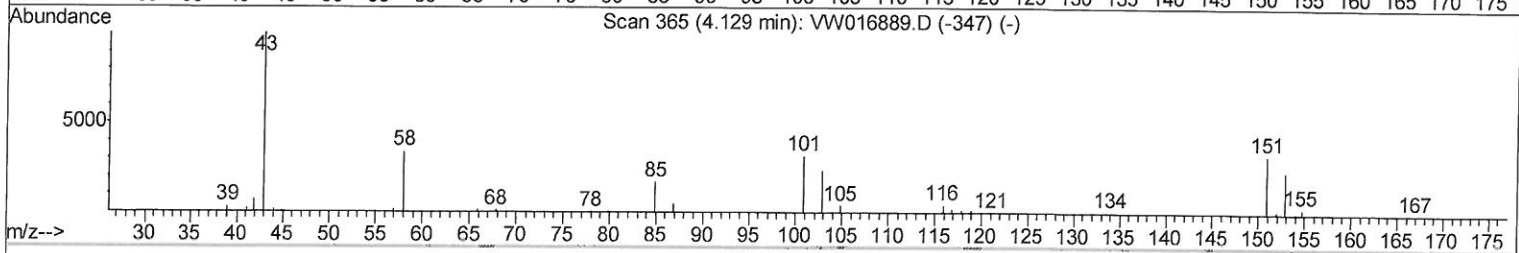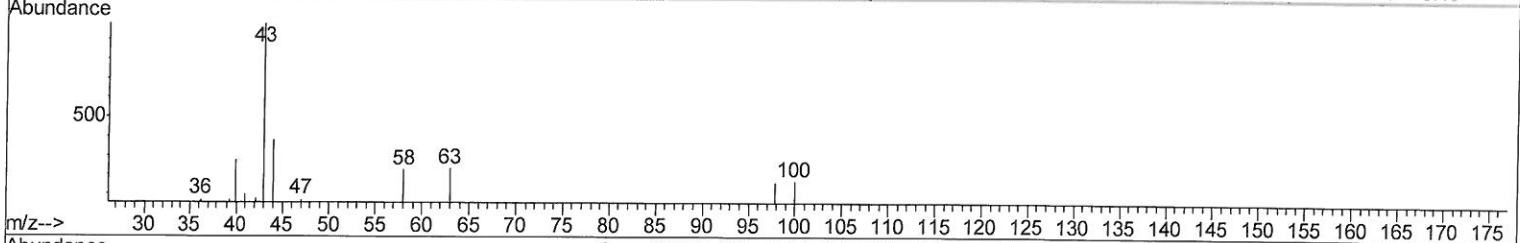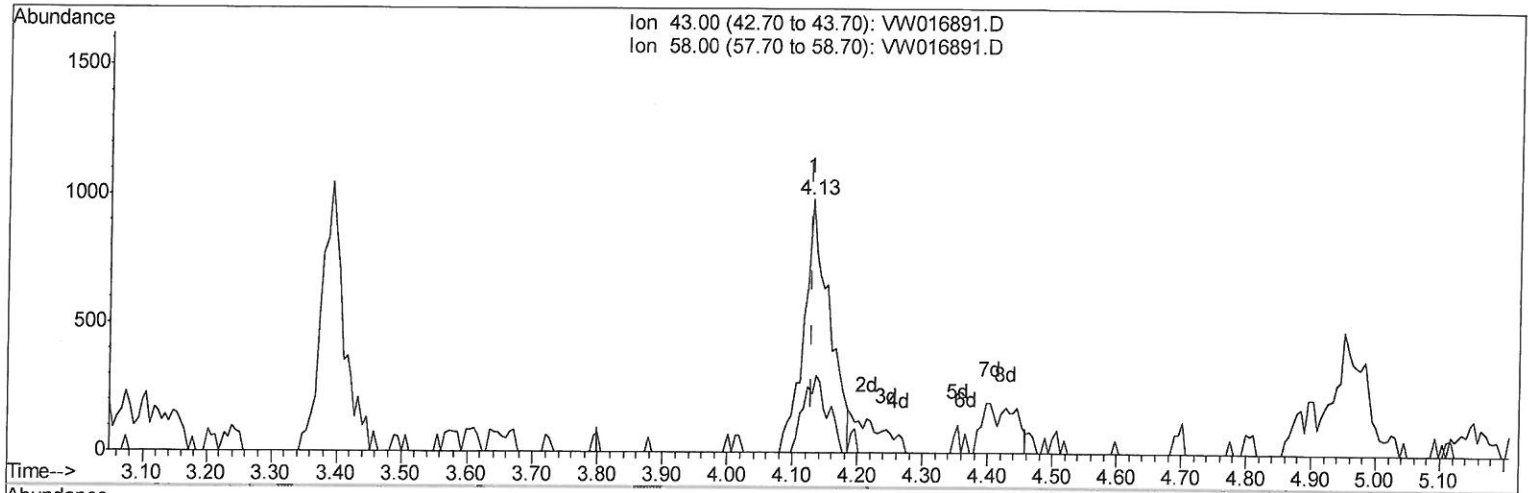

(13) Acetone (T)

4.129min (-0.001) 2.88ug/L m

>10/30/2020

response 2676

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	23.80
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101420\
 Data File : VW016891.D
 Acq On : 13 Oct 2020 11:07
 Operator : SY/VA
 Sample : VW1014SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK27

Manual Integrations
 APPROVED

MMDadoda
 10/15/2020 4:54:53 PM

Quant Time: Oct 14 20:23:36 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 14 08:34:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	550360	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	507163	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	241136	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	125541	23.12	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.48%		
7) Chloroethane-d5	2.89	69	105465	23.16	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.64%		
10) 1,1-Dichloroethene-d2	4.02	63	190145	16.49	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	65.96%		
20) 2-Butanone-d5	7.08	46	64210	52.21	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	104.42%		
24) Chloroform-d	7.65	84	283068	24.37	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	97.48%		
26) 1,2-Dichloroethane-d4	8.30	65	143444	25.57	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	102.28%		
29) Benzene-d6	8.27	84	564468	24.51	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	98.04%		
33) 1,2-Dichloropropane-d6	9.27	67	159135	25.71	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	102.84%		
37) Toluene-d8	10.32	98	537225	24.72	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	98.88%		
38) trans-1,3-Dichloropropene-	10.58	79	65863	24.12	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	96.48%		
39) 2-Hexanone-d5	10.93	63	53149	55.52	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	111.04%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	129477	25.89	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.56%		
61) 1,2-Dichlorobenzene-d4	13.85	152	201803	26.39	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.56%		

Target Compounds

13) Acetone	4.13	43	2676m	2.875	ug/L	Ovalue 90
16) Methylene chloride	4.92	84	12754	1.679	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101420\
Data File : VW016891.D
Acq On : 13 Oct 2020 11:07
Operator : SY/VA
Sample : VW1014SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK27

Manual Integrations
APPROVED

MMDadoda
10/15/2020 4:54:53 PM

Quant Time: Oct 14 20:23:36 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 14 08:34:08 2020
Response via : Initial Calibration

