

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW0101420\
 Data File : VW016893.D
 Acq On : 13 Oct 2020 12:35
 Operator : SY/VA
 Sample : VIBLK10
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VIBLK10

Manual Integrations
APPROVED

MMDadoda
 10/15/2020 4:54:58 PM

Quant Time: Oct 14 08:42:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 14 08:34:08 2020
 Response via : Initial Calibration

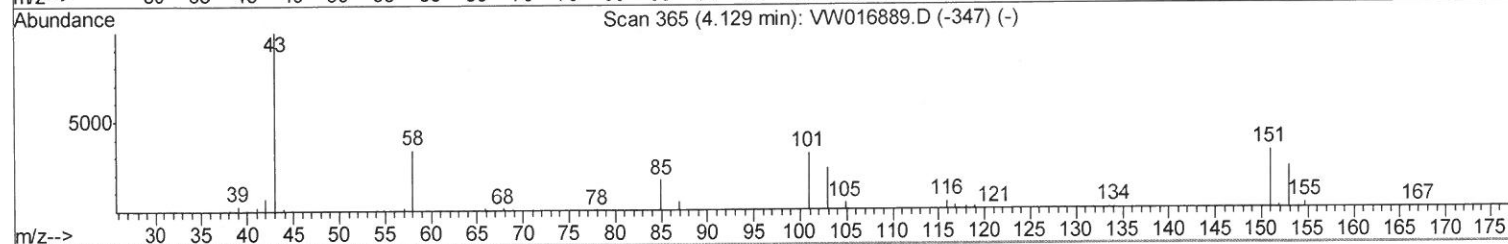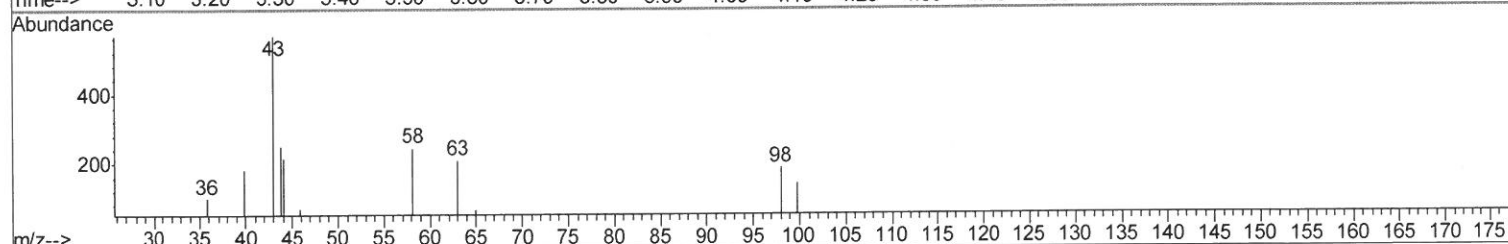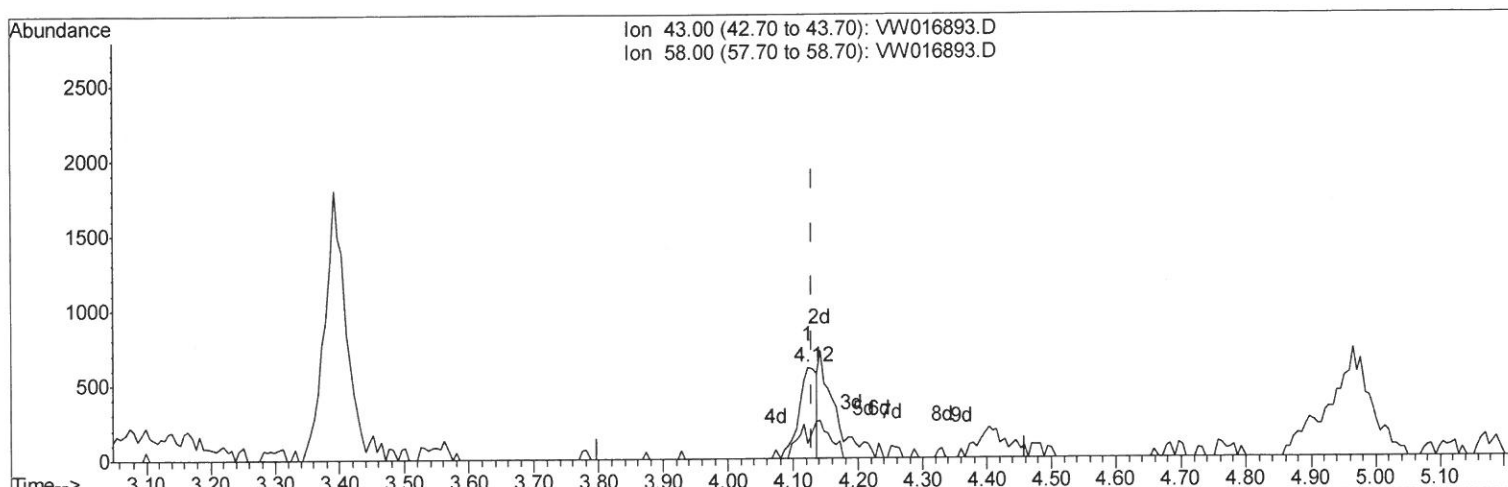

TIC: VW016893.D

(13) Acetone (T)

4.123min (-0.006) 1.22ug/L

response 1147

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	22.23
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101420\
 Data File : VW016893.D
 Acq On : 13 Oct 2020 12:35
 Operator : SY/VA
 Sample : VIBLK10
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK10

Manual Integrations
 APPROVED

MMDadoda
 10/15/2020 4:54:58 PM

Quant Time: Oct 14 08:42:21 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 14 08:34:08 2020
 Response via : Initial Calibration

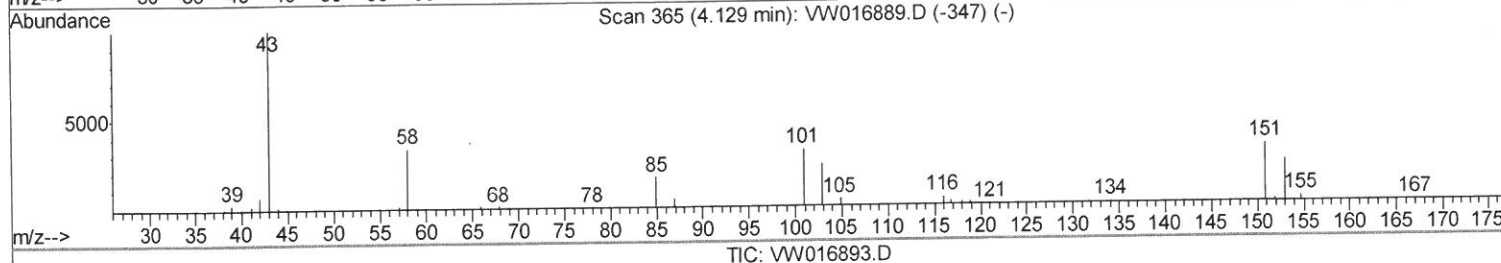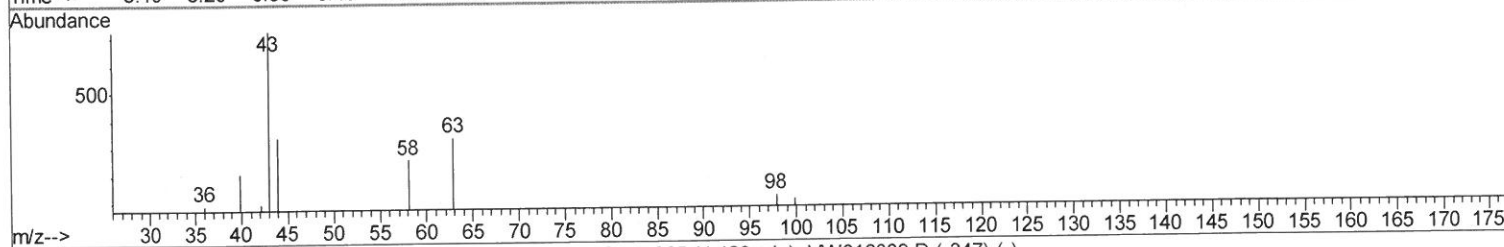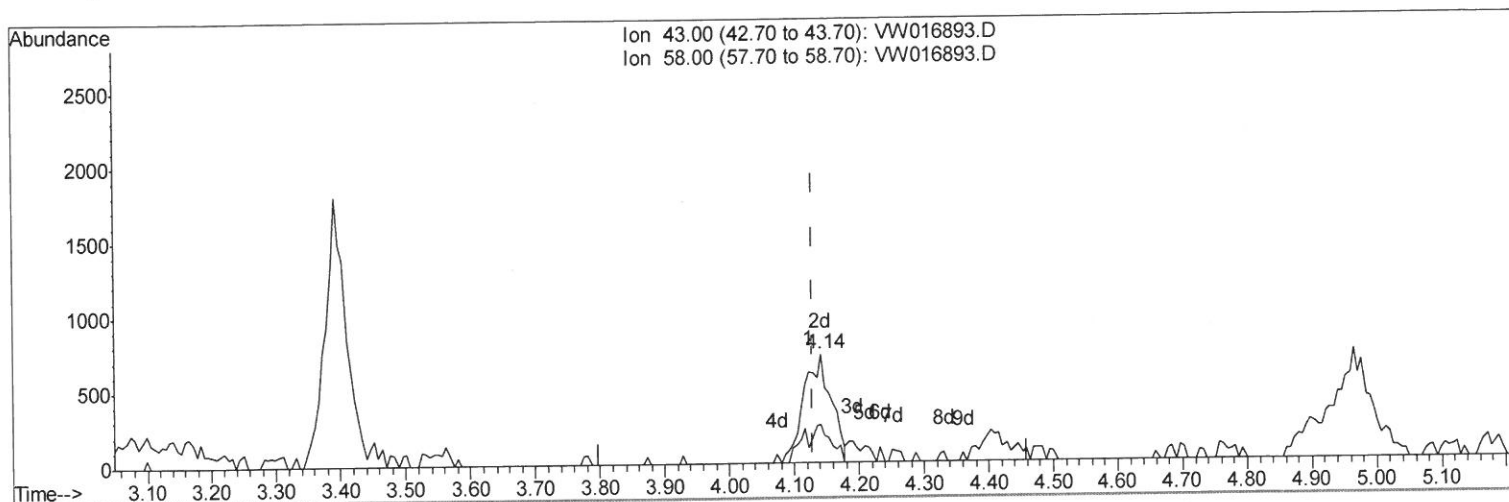

(13) Acetone (T)

4.141min (+0.012) 2.30ug/L m

response 2151

Ion	Exp%	Act%
43.00	100	100
58.00	33.80	11.85
0.00	0.00	0.00
0.00	0.00	0.00

10/19/2020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101420\
Quantitation Report (LSC Reviewed)

Data File : VW016893.D
Acq On : 13 Oct 2020 12:35
Operator : SY/VA
Sample : VIBLK10
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK10

Manual Integrations
APPROVED

MMDadoda
10/15/2020 4:54:58 PM

Quant Time: Oct 14 20:24:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 14 08:34:08 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	553937	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	503852	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	245492	25.00	ug/L	0.00

System Monitoring Compounds						
4) Vinyl Chloride-d3	2.35	65	108559	19.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.48%
7) Chloroethane-d5	2.89	69	90644	19.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.08%
10) 1,1-Dichloroethene-d2	4.03	63	163408	14.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.32%
20) 2-Butanone-d5	7.08	46	62748	50.70	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.40%
24) Chloroform-d	7.65	84	246198	21.06	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.24%
26) 1,2-Dichloroethane-d4	8.31	65	126618	22.43	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.72%
29) Benzene-d6	8.27	84	494961	21.63	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.52%
33) 1,2-Dichloropropane-d6	9.27	67	137721	22.39	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.56%
37) Toluene-d8	10.33	98	466735	21.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.48%
38) trans-1,3-Dichloropropene-	10.58	79	59563	21.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.84%
39) 2-Hexanone-d5	10.93	63	51194	53.83	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.66%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	121010	24.36	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.44%
61) 1,2-Dichlorobenzene-d4	13.85	152	180162	23.14	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.56%

Target Compounds					Qvalue
13) Acetone	4.14	43	2151m	2.296	ug/L
16) Methylene chloride	4.92	84	14032	1.836	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101420\
Quantitation Report (LSC Reviewed)

Data File : VW016893.D
Acq On : 13 Oct 2020 12:35
Operator : SY/VA
Sample : VIBLK10
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK10

Manual Integrations
APPROVED

MMDadoda
10/15/2020 4:54:58 PM

Quant Time: Oct 14 20:24:53 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 14 08:34:08 2020
Response via : Initial Calibration

