


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101421\
 Data File : VW020479.D
 Acq On : 14 Oct 2021 07:07
 Operator : SY/VA
 Sample : BFB452
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB452

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0
 Last Update : Sat Oct 16 06:56:08 2021

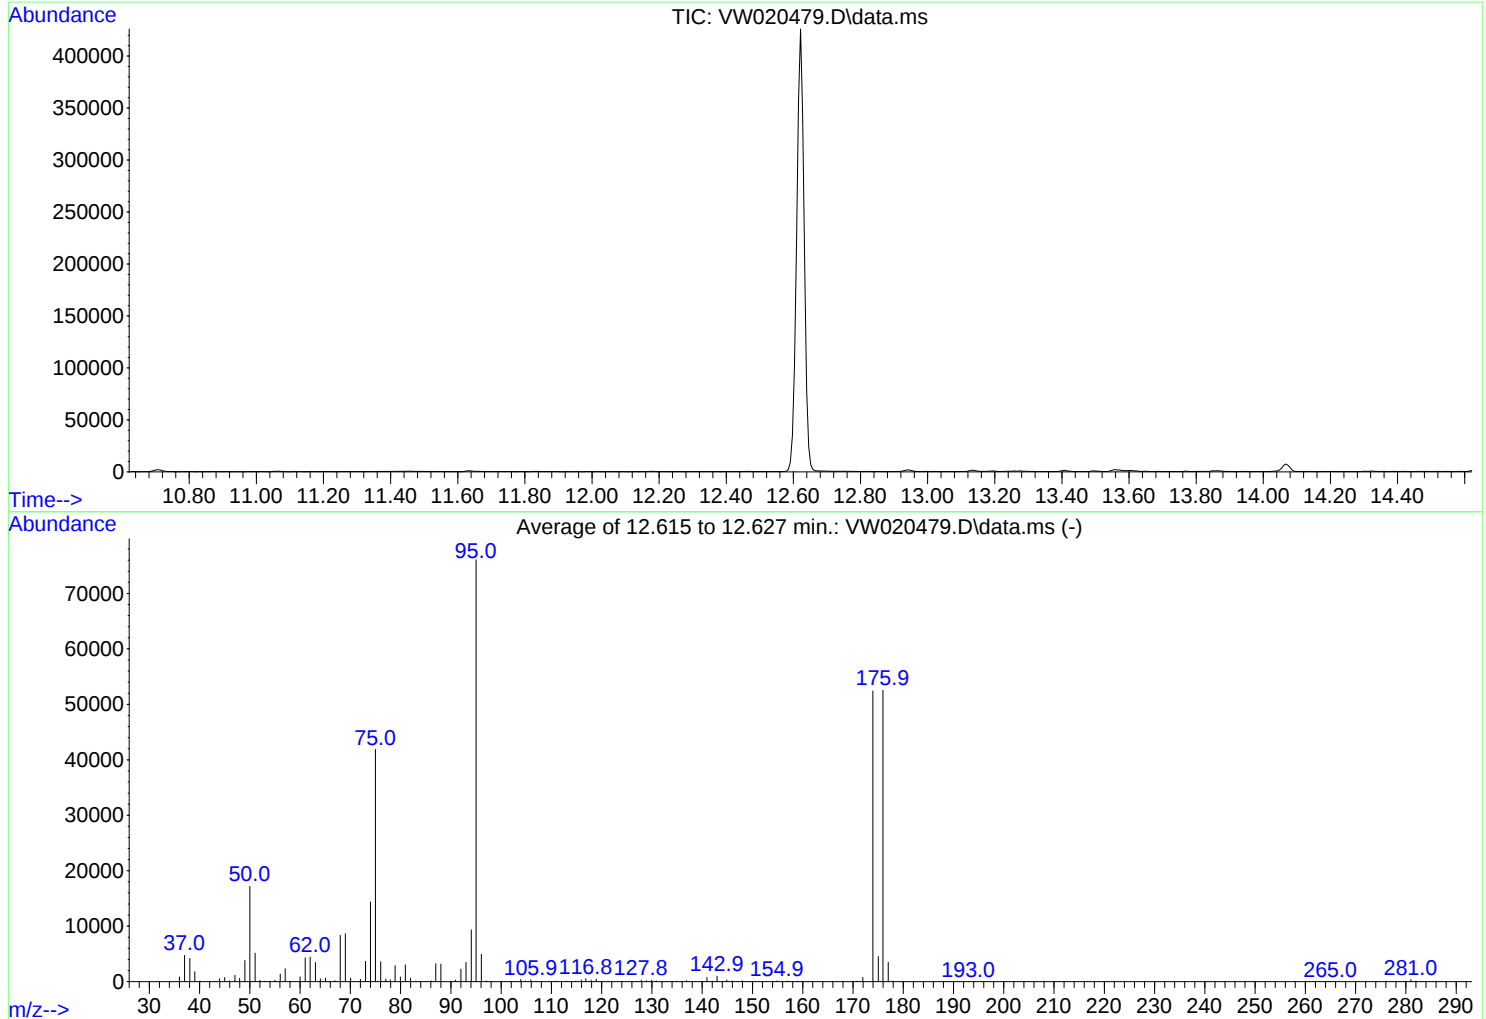

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.6	17170	PASS
75	95	30	80	55.1	41875	PASS
95	95	100	100	100.0	76053	PASS
96	95	5	9	6.5	4919	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.9	52381	PASS
175	174	5	9	8.6	4520	PASS
176	174	95	105	100.3	52547	PASS
177	176	5	10	6.6	3486	PASS

m/z	Abundance
36.00	91.0
40.10	91.0
43.90	127.0

Instrument :
MSVOA_W
ClientSampleId :
BFB452

m/z	Abundance
36.10	932.0
37.00	4944.0
38.10	4494.0
39.00	1802.0
40.10	189.0
44.00	689.0
45.00	850.0
46.10	201.0
47.00	1125.0
48.00	509.0
49.00	4011.0
50.00	17744.0
51.00	5098.0
52.00	239.0
52.90	85.0
54.00	51.0
55.10	271.0
56.00	1265.0
57.10	2329.0
58.10	90.0
60.00	854.0
61.00	4383.0
62.00	4373.0
63.00	3533.0
64.00	560.0
65.00	723.0
66.90	239.0
68.00	8552.0
69.00	8683.0
70.00	643.0
72.10	411.0
73.00	3674.0
74.00	14267.0
75.00	41568.0
76.00	3508.0
77.00	535.0
77.90	303.0
78.90	3039.0
80.00	841.0
80.90	3155.0
81.90	632.0
83.10	75.0
86.00	204.0
87.00	3334.0
88.00	2875.0
91.00	334.0
92.00	2141.0
93.00	3234.0
94.00	9096.0
95.00	72936.0
96.00	4898.0
97.00	122.0
103.90	389.0
104.80	139.0
105.90	293.0
106.90	85.0
110.90	90.0
111.90	68.0
112.90	73.0
115.00	97.0
115.90	253.0
116.80	576.0
117.90	215.0
118.90	538.0
127.80	270.0
128.90	91.0
129.90	251.0
130.80	100.0
132.80	91.0
134.80	115.0
136.90	175.0
140.90	665.0
142.00	95.0
142.90	906.0
144.90	377.0
145.90	146.0
148.00	124.0
149.80	63.0
154.10	52.0
154.90	130.0
156.90	98.0
158.90	96.0
170.80	161.0
172.00	795.0
173.90	45456.0
175.00	4199.0
176.00	42336.0
177.00	3140.0
178.00	102.0
191.10	61.0
193.00	114.0
265.00	60.0

Instrument :
MSVOA_W
ClientSampleId :
BFB452

281.00	448.0
282.00	241.0
283.10	119.0

Instrument :
MSVOA_W
ClientSampleId :
BFB452

m/z	Abundance
36.00	1017.0
37.00	5349.0
38.00	4666.0
39.10	1944.0
40.20	164.0
43.00	61.0
44.00	704.0
45.00	870.0
45.90	169.0
47.10	1311.0
48.00	715.0
49.00	4294.0
50.00	19208.0
51.00	6031.0
52.00	240.0
53.00	101.0
54.90	275.0
56.00	1554.0
57.00	2751.0
58.00	105.0
60.00	971.0
61.00	4827.0
62.00	5094.0
63.10	3842.0
64.00	510.0
65.00	651.0
66.00	72.0
66.90	238.0
68.00	9475.0
69.00	9697.0
70.10	855.0
71.90	500.0
73.00	4066.0
74.00	16134.0
75.00	46824.0
76.10	4248.0
77.10	549.0
78.00	405.0
78.90	3296.0
79.90	900.0
81.00	3395.0
81.90	735.0
83.10	105.0
86.00	134.0
87.00	3561.0
88.00	3823.0
90.90	287.0
92.00	2453.0
93.00	3978.0
94.10	10635.0
95.00	85808.0
96.10	5445.0
97.10	125.0
103.90	372.0
104.90	128.0
105.90	395.0
107.00	80.0
110.00	58.0
110.90	107.0
111.90	72.0
113.00	85.0
114.80	102.0
115.90	316.0
116.90	655.0
117.90	341.0
118.90	468.0
127.90	308.0
128.90	153.0
129.90	306.0
130.80	118.0
135.00	154.0
136.90	197.0
141.00	850.0
141.90	77.0
142.90	1089.0
144.00	65.0
144.90	329.0
146.00	125.0
148.00	216.0
150.00	68.0
154.90	175.0
157.00	121.0
158.90	102.0
161.00	74.0
170.80	128.0
172.00	915.0
174.00	60888.0
175.10	5048.0
175.90	61624.0
177.00	3793.0
177.90	132.0
281.00	429.0

Instrument :
MSVOA_W
ClientSampleId :
BFB452

282.00
283.10

132.0
72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB452

m/z	Abundance
36.00	826.0
37.00	3938.0
38.00	3385.0
39.10	1671.0
40.00	195.0
43.00	55.0
44.00	563.0
45.00	581.0
45.90	118.0
47.10	1003.0
47.90	556.0
49.00	3119.0
50.00	14558.0
51.10	4260.0
52.00	201.0
53.00	82.0
55.00	219.0
56.10	1287.0
57.00	1916.0
58.00	88.0
60.00	754.0
61.00	3654.0
62.00	3802.0
63.00	3044.0
64.10	427.0
65.10	509.0
65.90	66.0
67.10	227.0
68.00	7065.0
69.00	7554.0
70.00	470.0
72.00	413.0
73.00	3232.0
74.00	12710.0
75.00	37232.0
76.00	2967.0
77.00	349.0
78.00	249.0
78.90	2330.0
80.00	777.0
81.00	2505.0
82.00	515.0
83.00	99.0
86.10	123.0
87.00	2827.0
88.00	2789.0
90.80	253.0
92.00	2208.0
93.00	3160.0
94.00	8313.0
95.00	69416.0
96.00	4413.0
97.00	109.0
103.90	368.0
104.80	100.0
105.90	288.0
106.90	76.0
109.90	54.0
110.90	63.0
112.00	65.0
113.00	75.0
114.80	74.0
116.00	314.0
116.90	451.0
117.90	287.0
118.90	419.0
127.90	294.0
129.00	159.0
129.90	258.0
130.90	137.0
134.90	151.0
136.80	115.0
141.00	747.0
142.10	90.0
143.00	926.0
144.00	60.0
145.00	138.0
145.90	140.0
147.90	187.0
150.00	115.0
154.90	168.0
156.90	94.0
159.00	69.0
161.10	66.0
171.90	603.0
174.00	50800.0
175.00	4314.0
176.00	53680.0
177.00	3526.0
178.00	132.0
281.10	241.0

Instrument :
MSVOA_W
ClientSampleId :
BFB452