



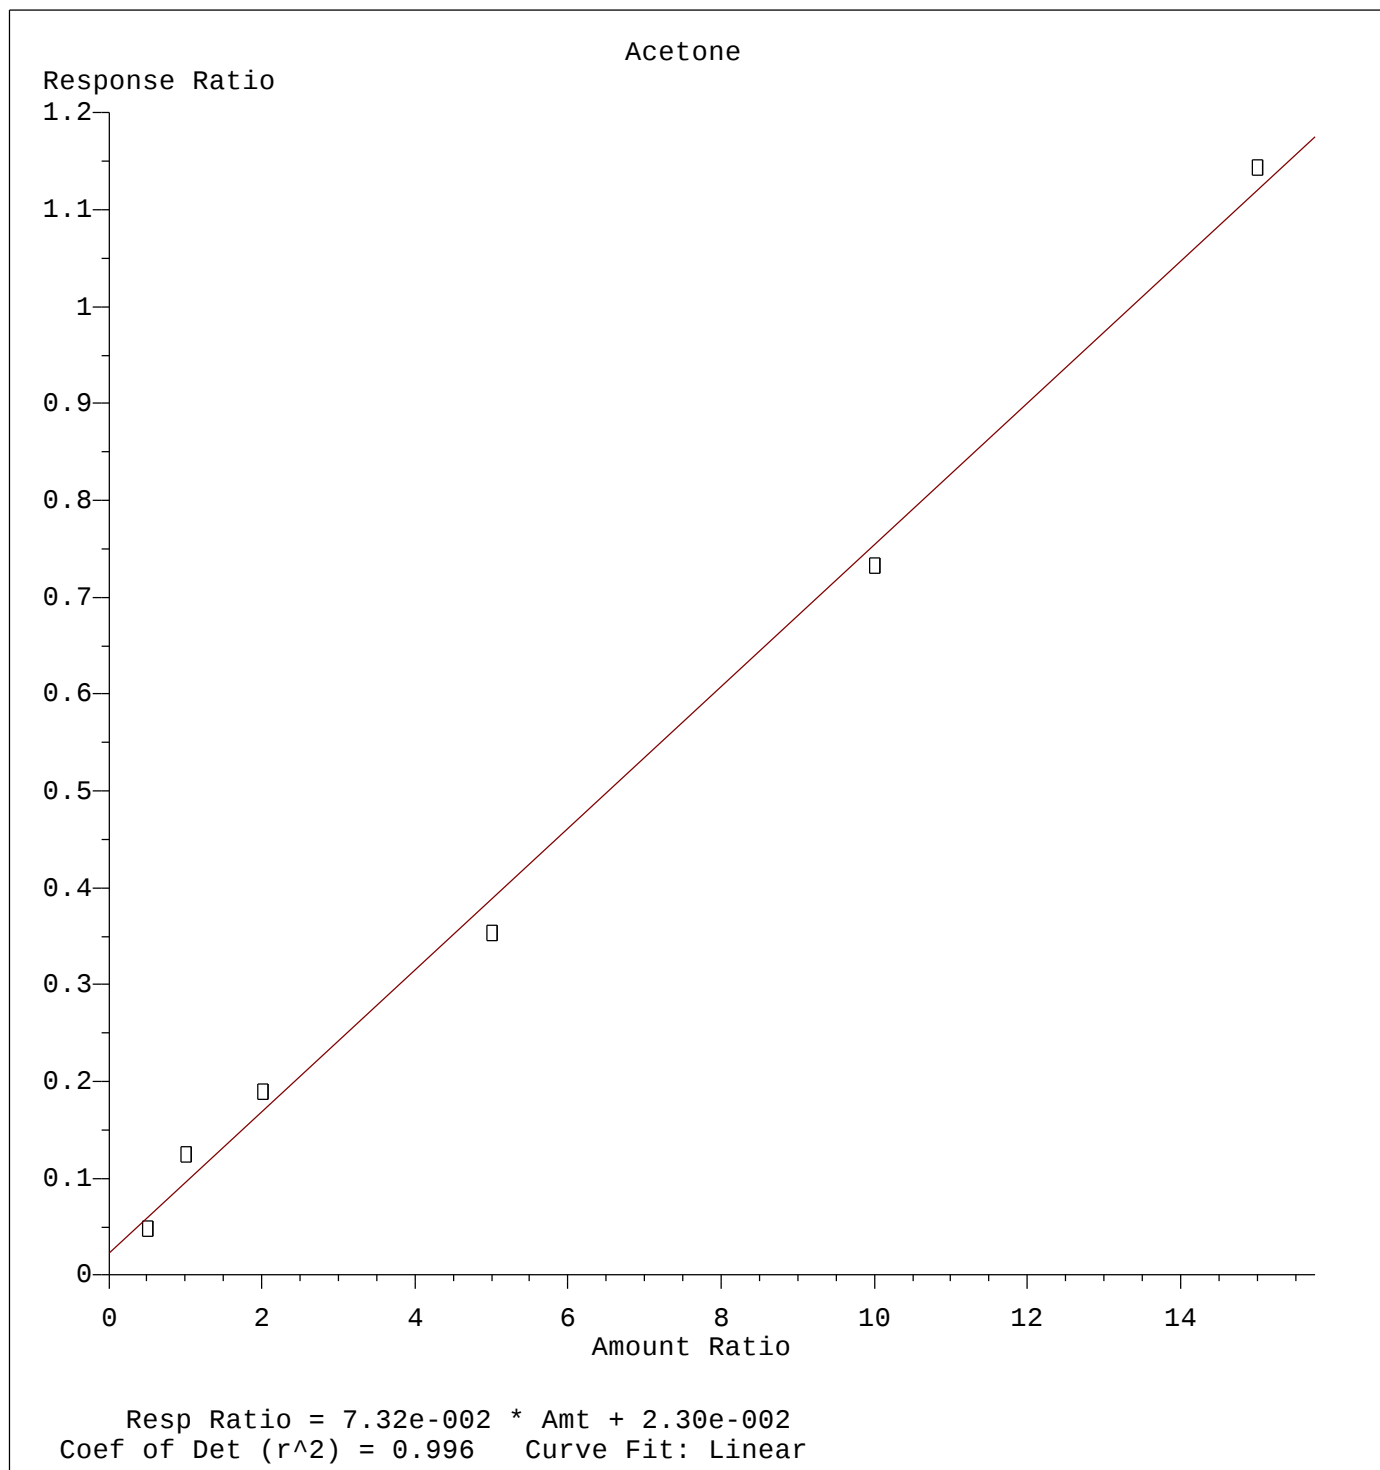

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Calibration Table Last Updated: Tue Oct 16 13:56:35 2018

Methylene Chloride

Response Ratio

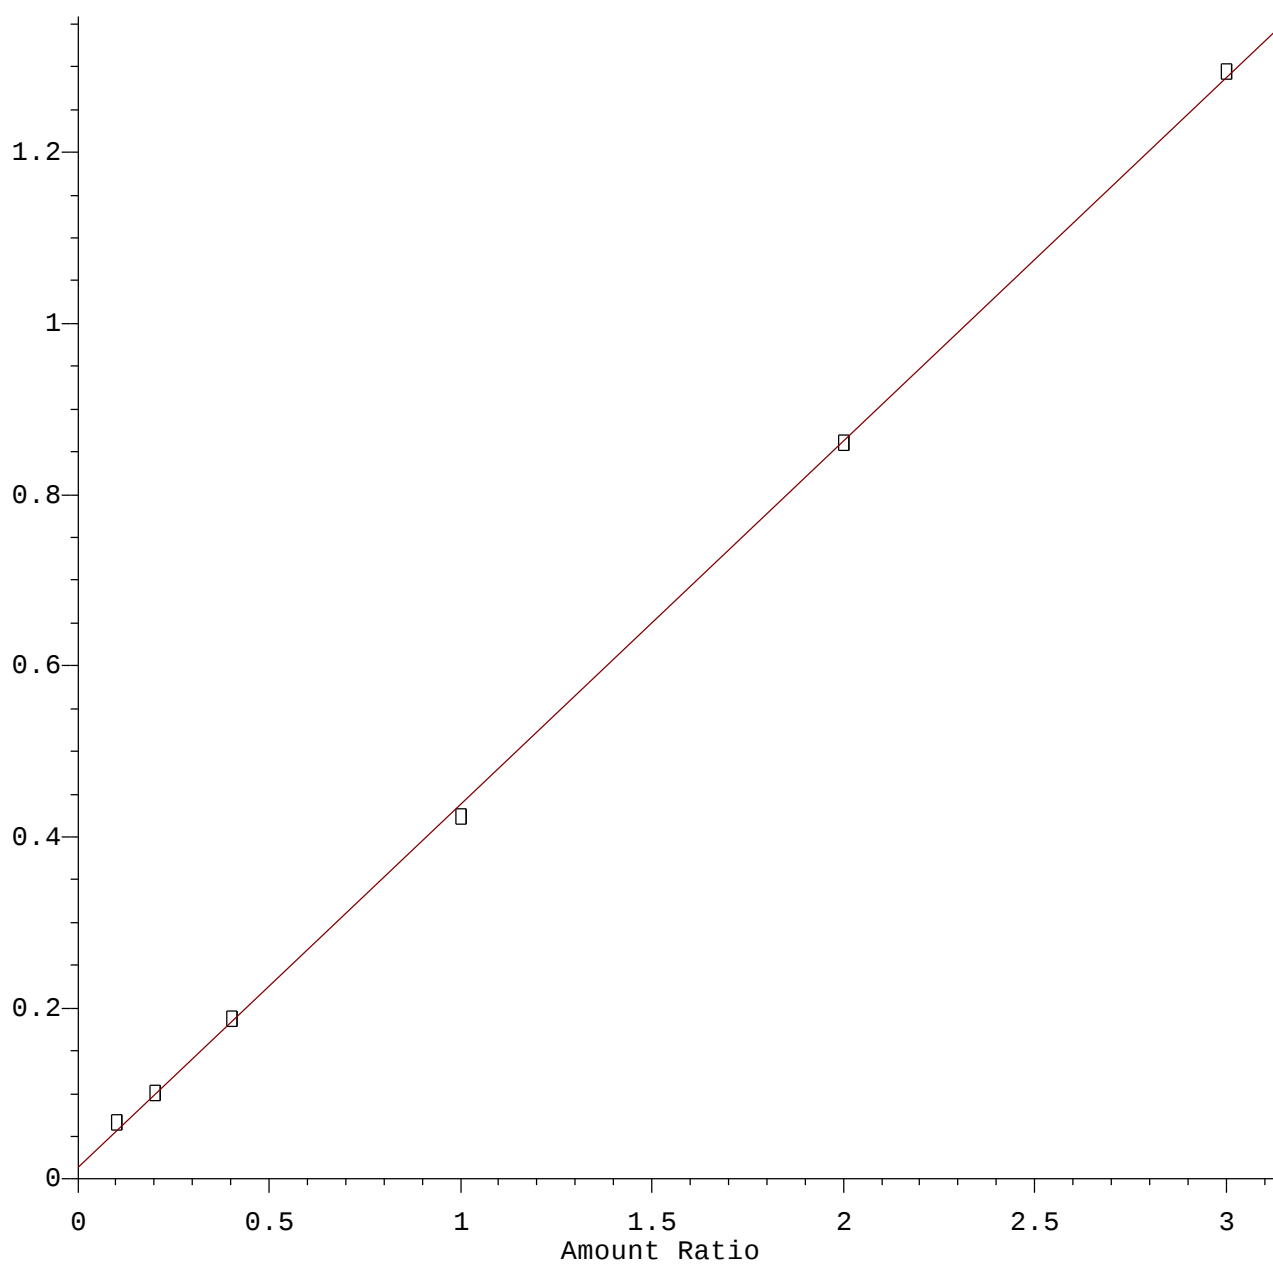

Resp Ratio = $4.24 \times 10^{-1} \times \text{Amt} + 1.43 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Calibration Table Last Updated: Tue Oct 16 13:56:35 2018