


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101518\
Data File : VW006061.D
Acq On : 15 Oct 2018 14:49
Operator : VA/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Title : SW846 8260
Last Update : Tue Oct 16 05:36:33 2018

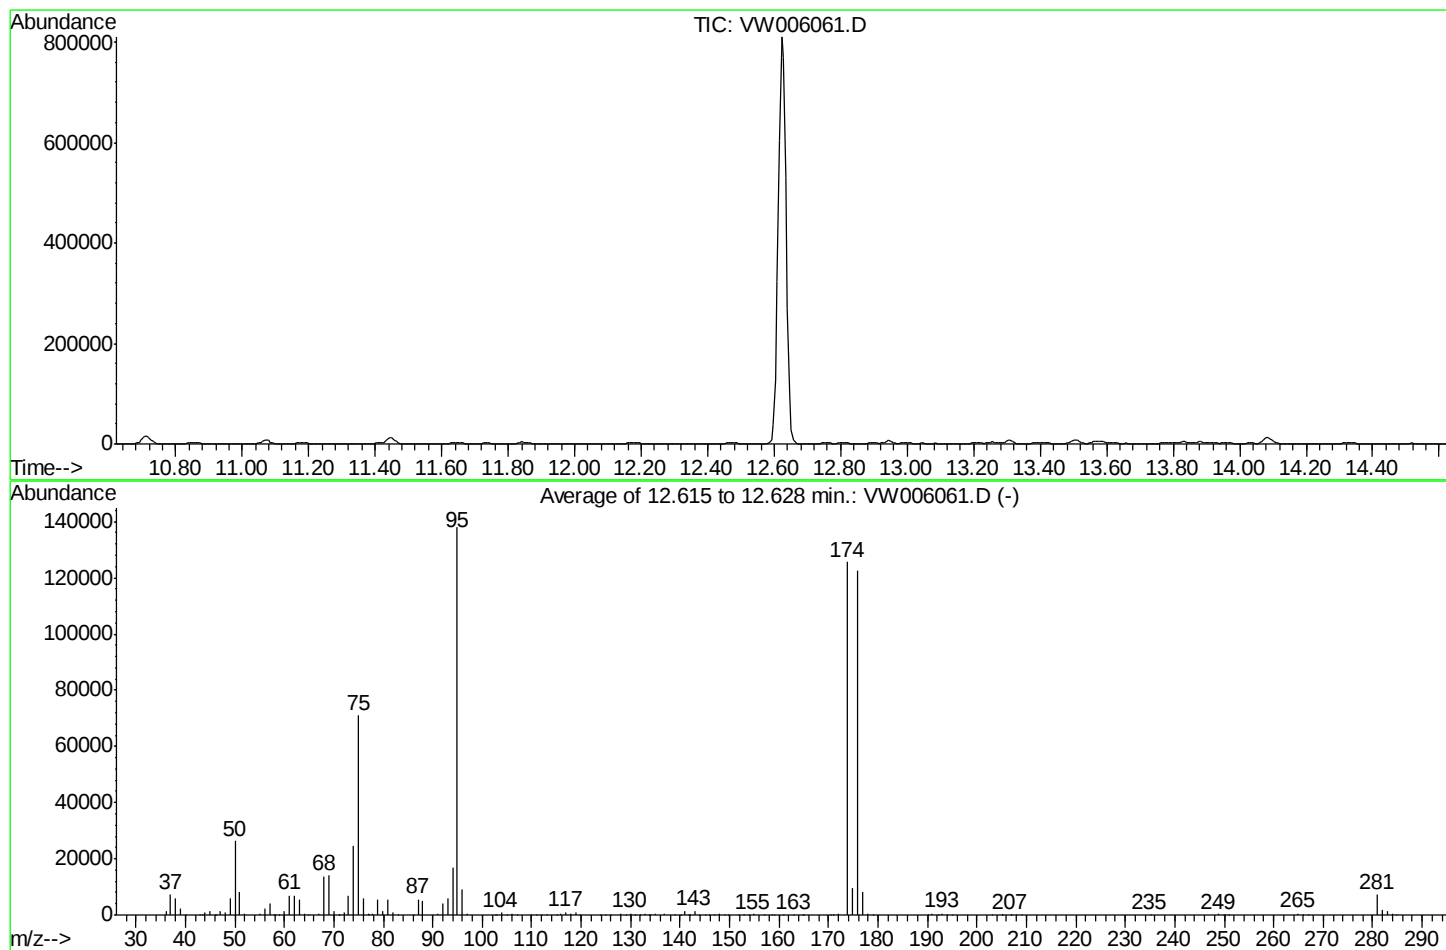

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	26253	PASS
75	95	30	60	51.5	71053	PASS
95	95	100	100	100.0	137968	PASS
96	95	5	9	6.8	9334	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.0	125552	PASS
175	174	5	9	7.7	9618	PASS
176	174	95	101	97.8	122754	PASS
177	176	5	9	6.6	8088	PASS