

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW016901.D
 Data File : VW016901.D
 Acq On : 14 Oct 2020 13:36
 Operator : SY/VA
 Sample : L4382-11
 Misc : 5.53G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3X9

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:36:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 08:29:28 2020
 Response via : Initial Calibration

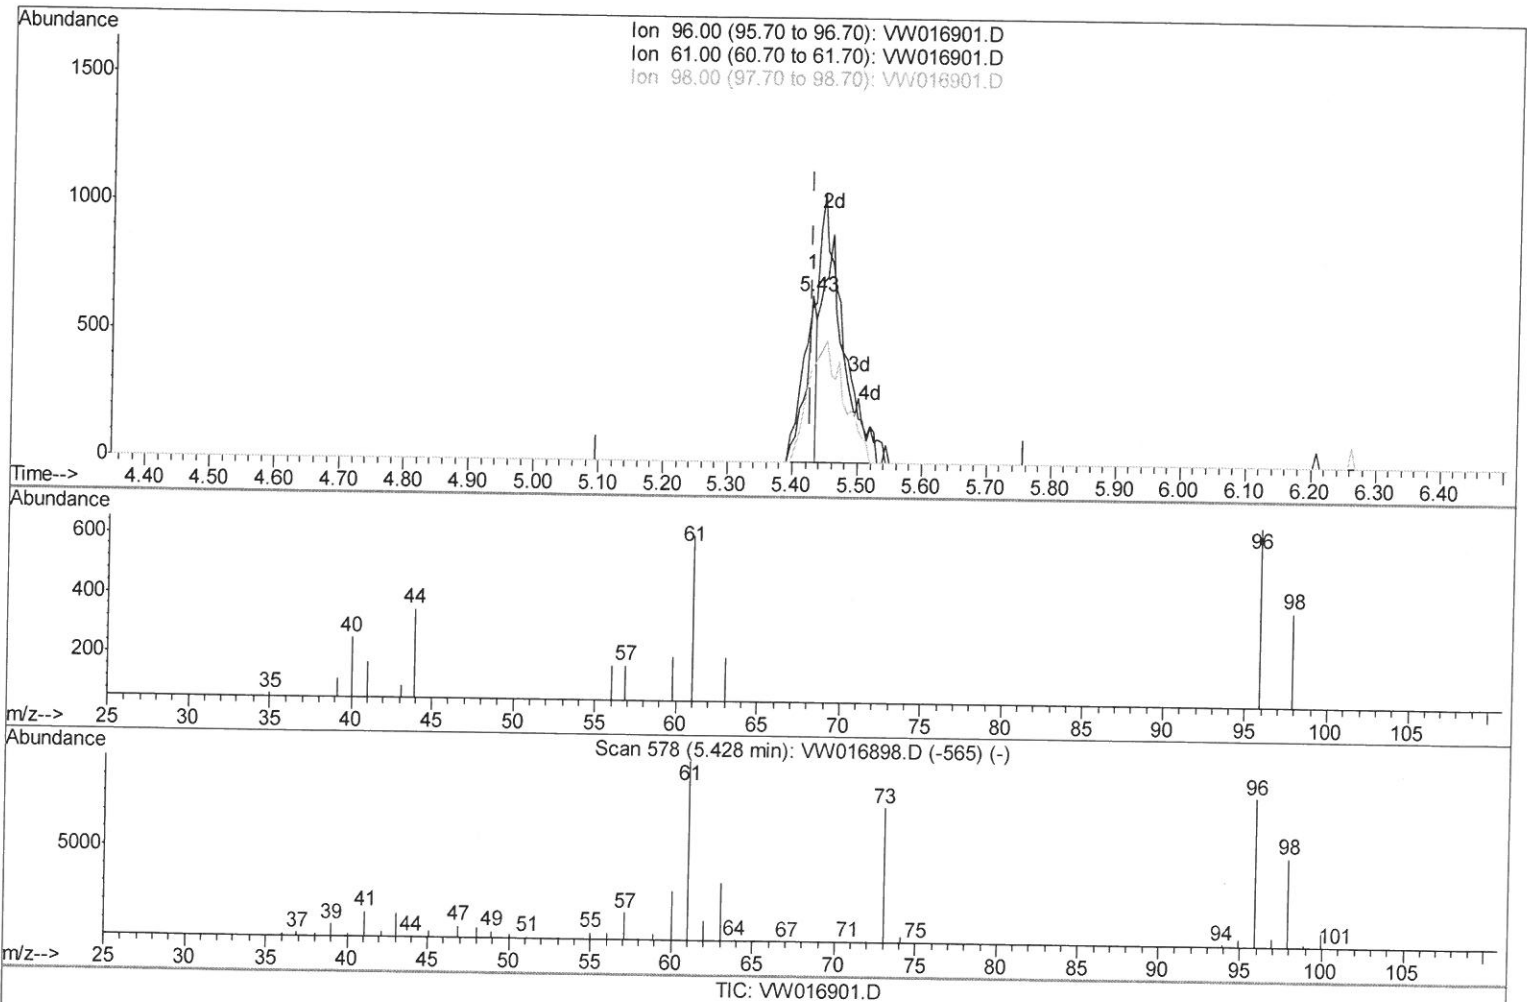

(18) trans-1,2-Dichloroethene (T)

5.427min (-0.000) 0.30ug/L

response 778

Ion	Exp%	Act%
96.00	100	100
61.00	117.90	93.10
98.00	61.90	56.90
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
 Data File : VW016901.D
 Acq On : 14 Oct 2020 13:36
 Operator : SY/VA
 Sample : L4382-11
 Misc : 5.53G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG3X9

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:36:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 08:29:28 2020
 Response via : Initial Calibration

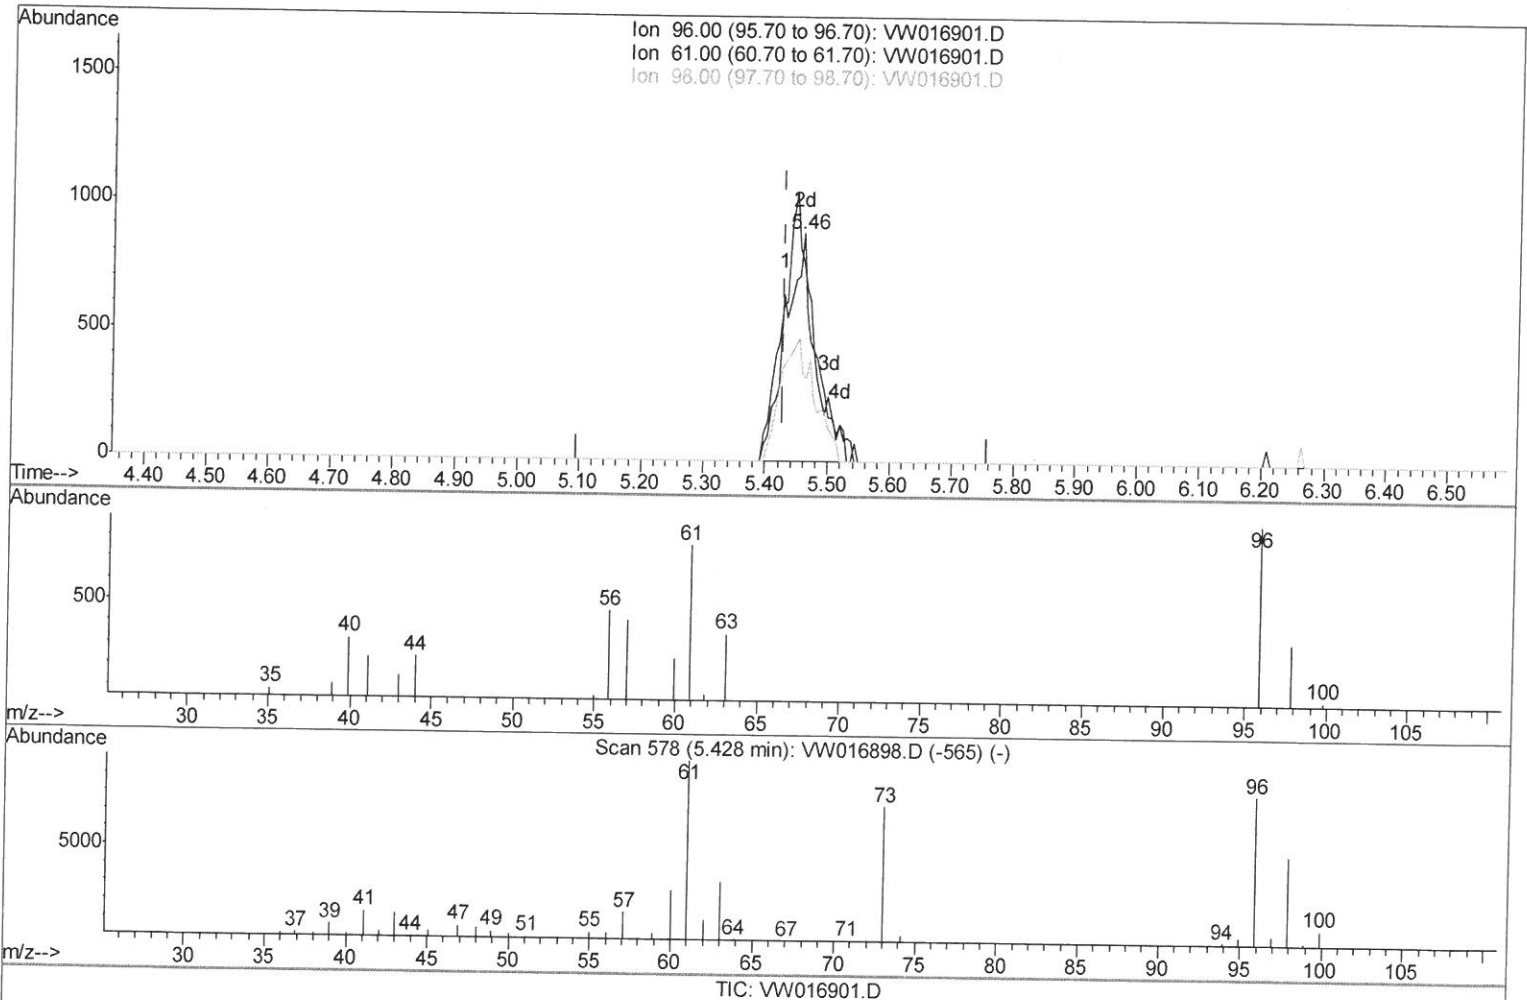

(18) trans-1,2-Dichloroethene (T)

5.458min (+0.030) 1.16ug/L m) 10/19/2020

response 2982

Ion	Exp%	Act%
96.00	100	100
61.00	117.90	87.99
98.00	61.90	38.27#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
 Data File : VW016901.D
 Acq On : 14 Oct 2020 13:36
 Operator : SY/VA
 Sample : L4382-11
 Misc : 5.53G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BG3X9

Manual Integrations
APPROVED

MMDadoda
 10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:36:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 08:29:28 2020
 Response via : Initial Calibration

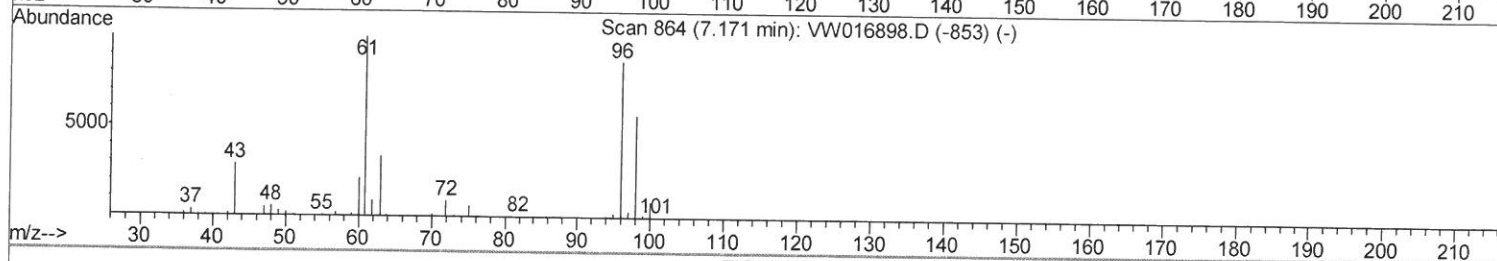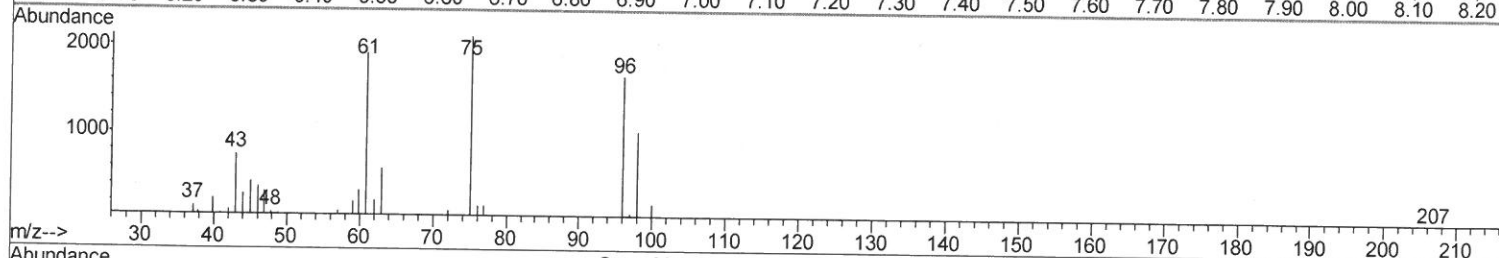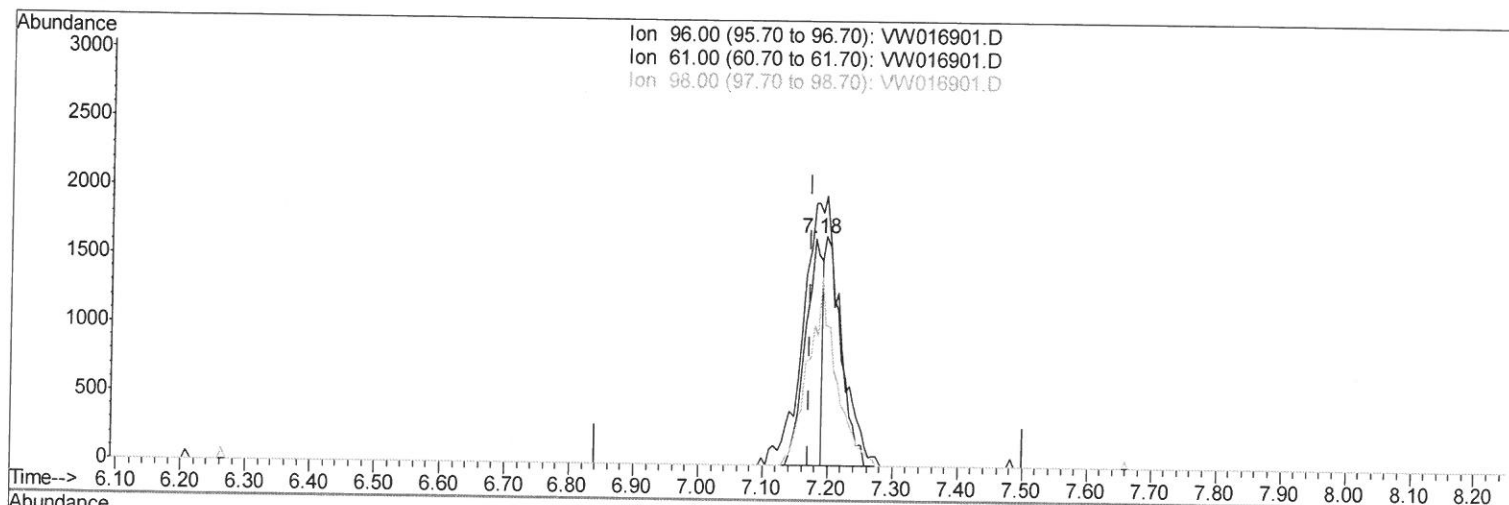

TIC: VW016901.D

(22) cis-1,2-Dichloroethene (T)

7.177min (+0.006) 1.17ug/L

response 3069

Ion	Exp%	Act%
96.00	100	100
61.00	108.60	115.56
98.00	61.00	61.86
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
 Data File : VW016901.D
 Acq On : 14 Oct 2020 13:36
 Operator : SY/VA
 Sample : L4382-11
 Misc : 5.53G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3X9

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:36:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 08:29:28 2020
 Response via : Initial Calibration

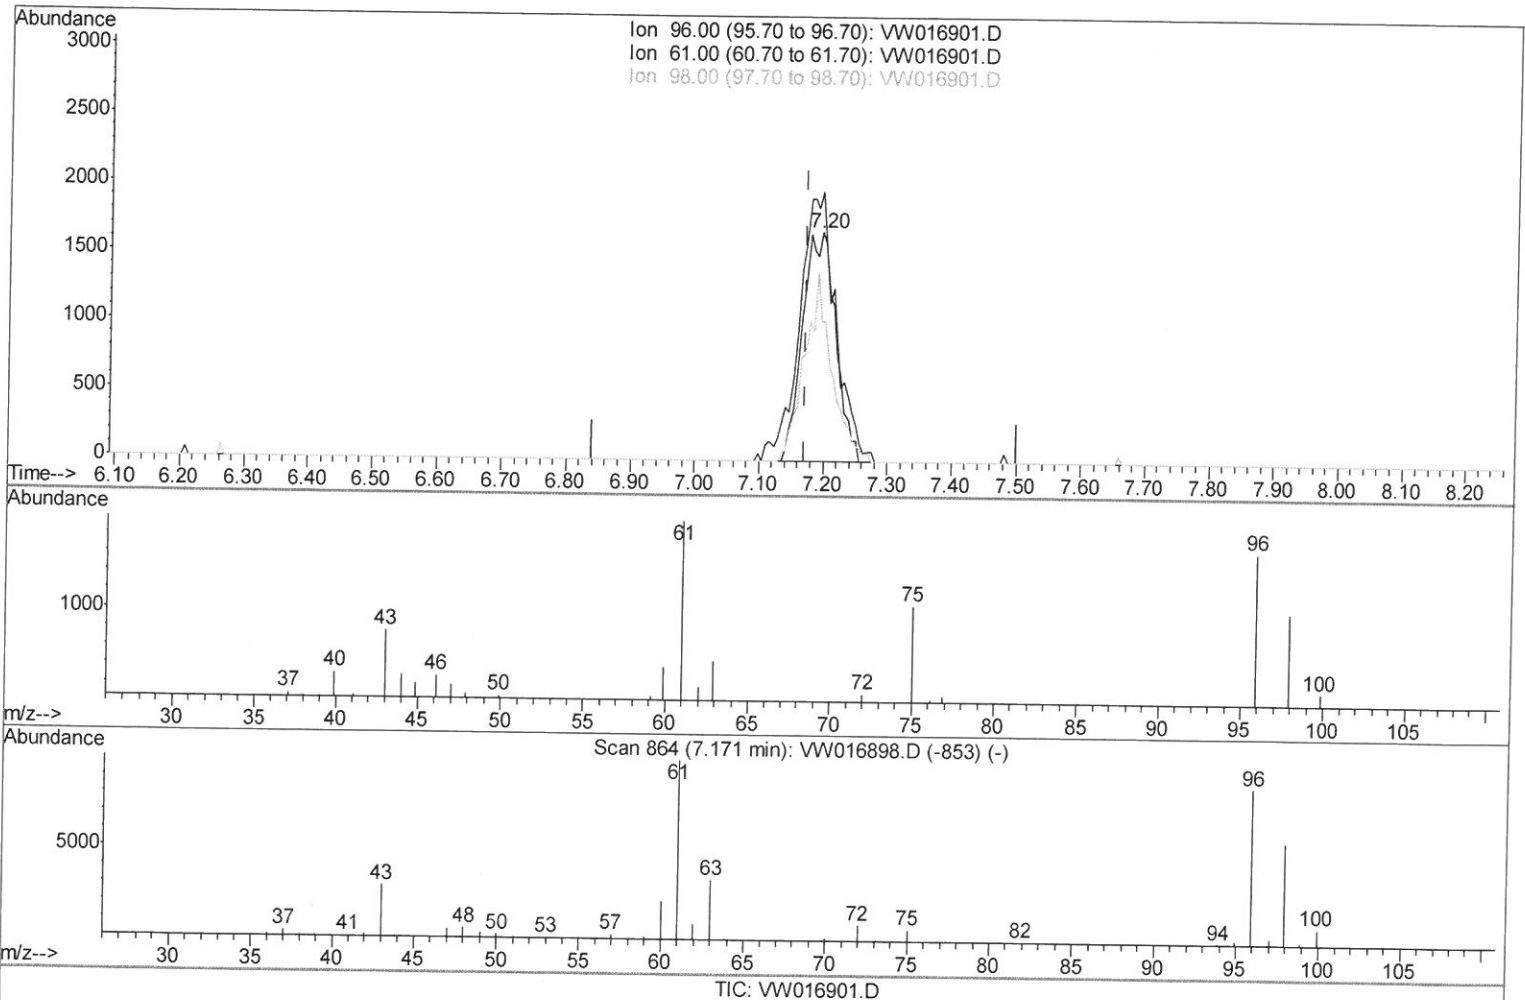

(22) cis-1,2-Dichloroethene (T)

7.195min (+0.024) 2.28ug/L m

response 5982

Ion	Exp%	Act%
96.00	100	100
61.00	108.60	117.75
98.00	61.00	61.75
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
 Data File : VW016901.D
 Acq On : 14 Oct 2020 13:36
 Operator : SY/VA
 Sample : L4382-11
 Misc : 5.53G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BG3X9

Manual Integrations
APPROVED

MMDadoda
 10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:36:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 08:29:28 2020
 Response via : Initial Calibration

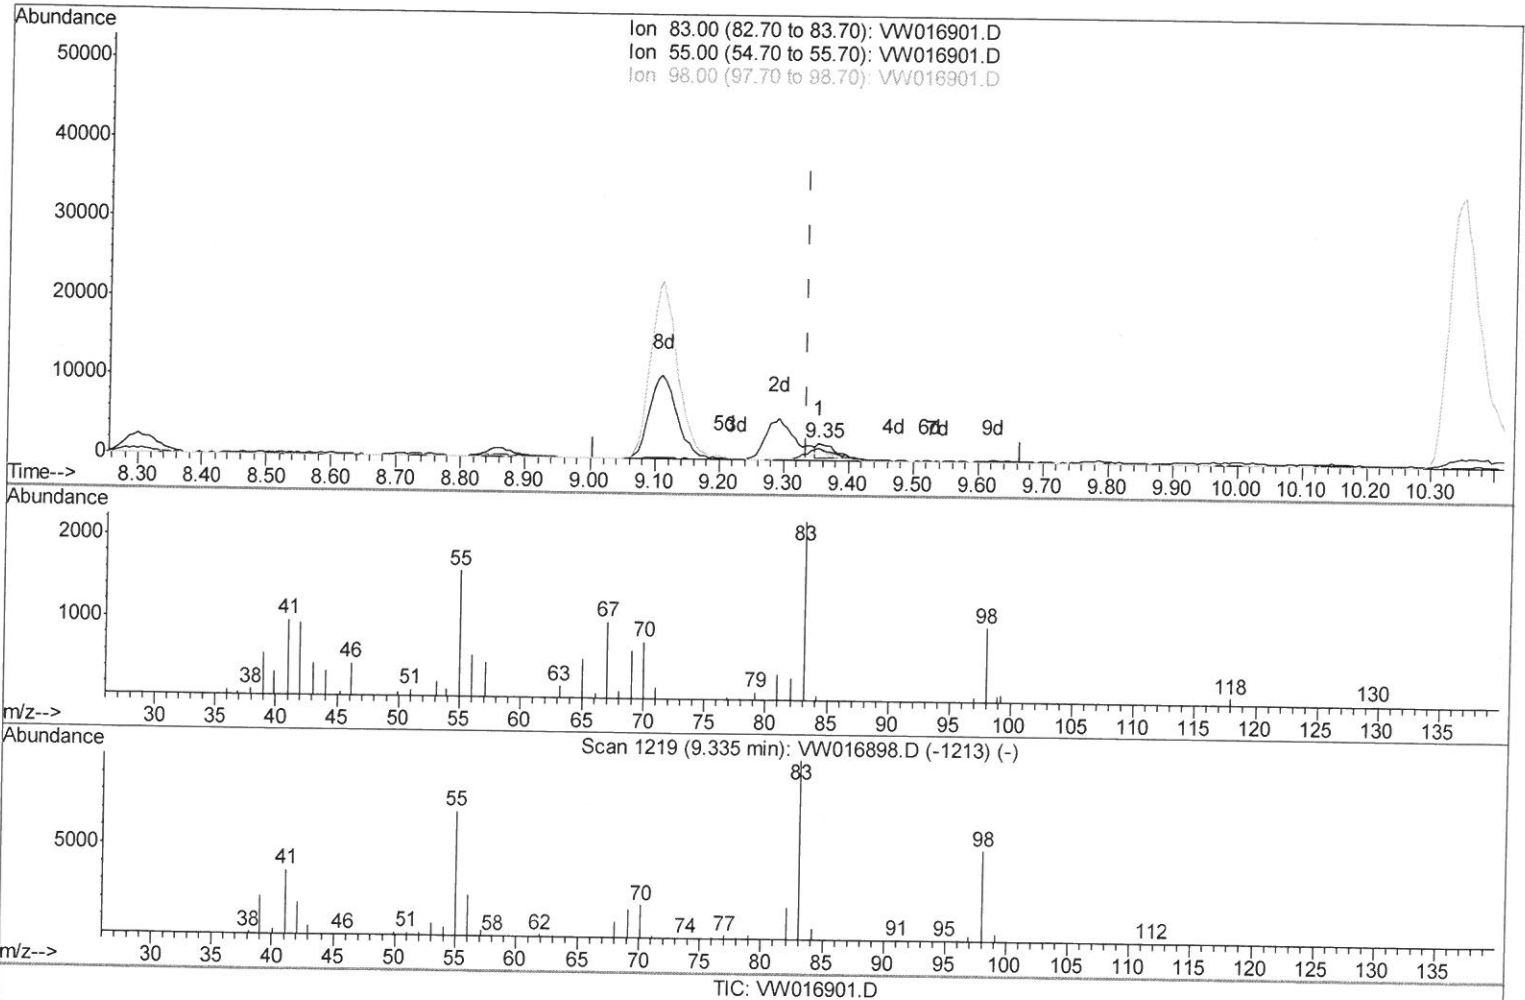

(36) Methylcyclohexane (T)

9.354min (+0.018) 1.46ug/L

response 3273

Ion	Exp%	Act%
83.00	100	100
55.00	67.80	120.35#
98.00	51.80	98.47#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
Data File : VW016901.D
Acq On : 14 Oct 2020 13:36
Operator : SY/VA
Sample : L4382-11
Misc : 5.53G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG3X9

Manual Integrations
APPROVED

MMDadoda
10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:36:58 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 15 08:29:28 2020
Response via : Initial Calibration

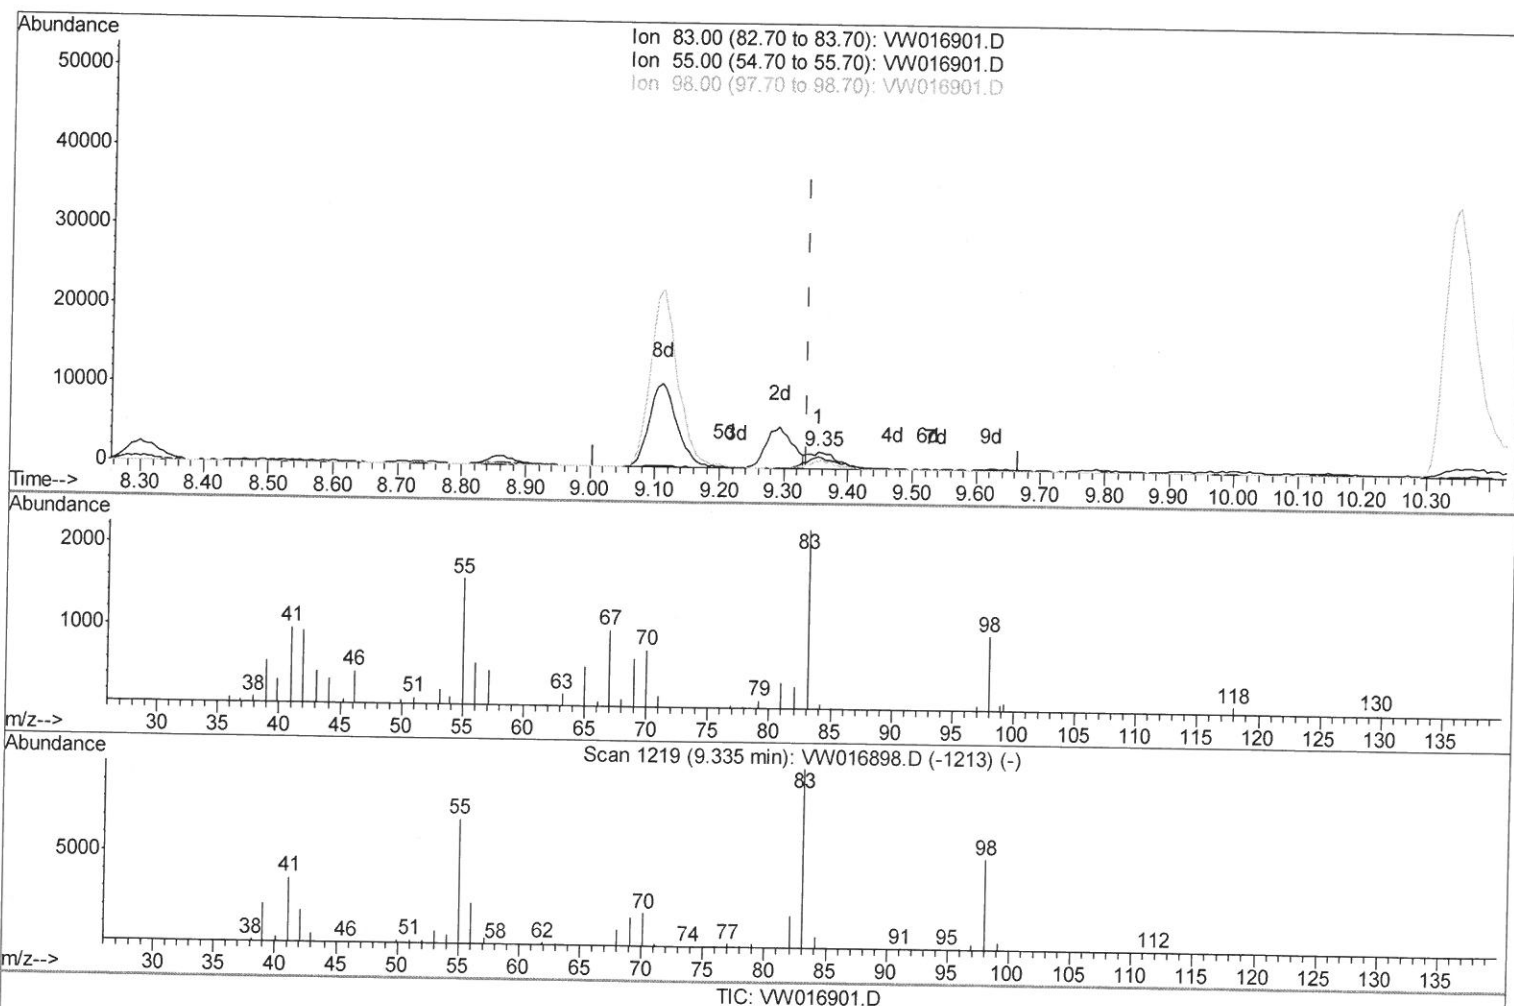

(36) Methylcyclohexane (T)

9.354min (+0.018) 3.08ug/L m

response 6897

Ion	Exp%	Act%
83.00	100	100
55.00	67.80	57.11
98.00	51.80	46.73
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
 Data File : VW016901.D
 Acq On : 14 Oct 2020 13:36
 Operator : SY/VA
 Sample : L4382-11
 Misc : 5.53G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3X9

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:51:18 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 08:29:28 2020
 Response via : Initial Calibration

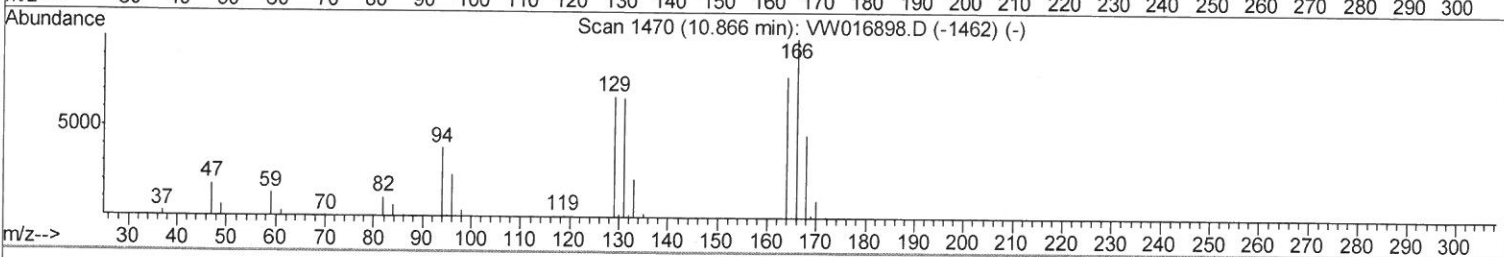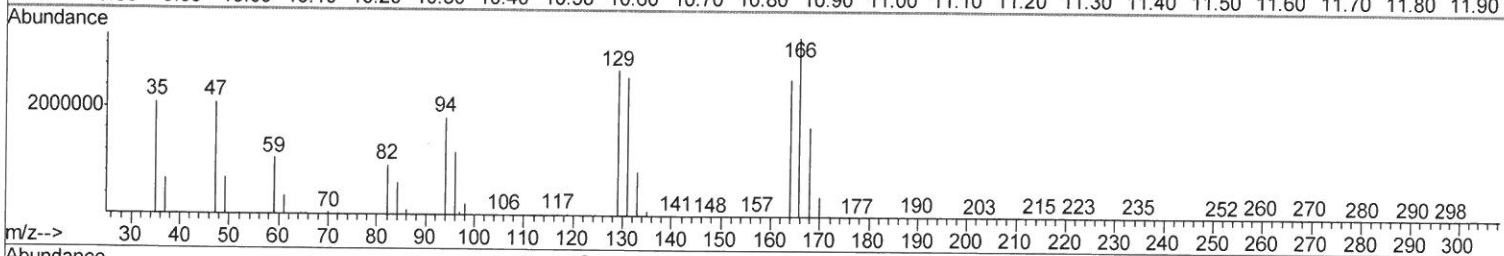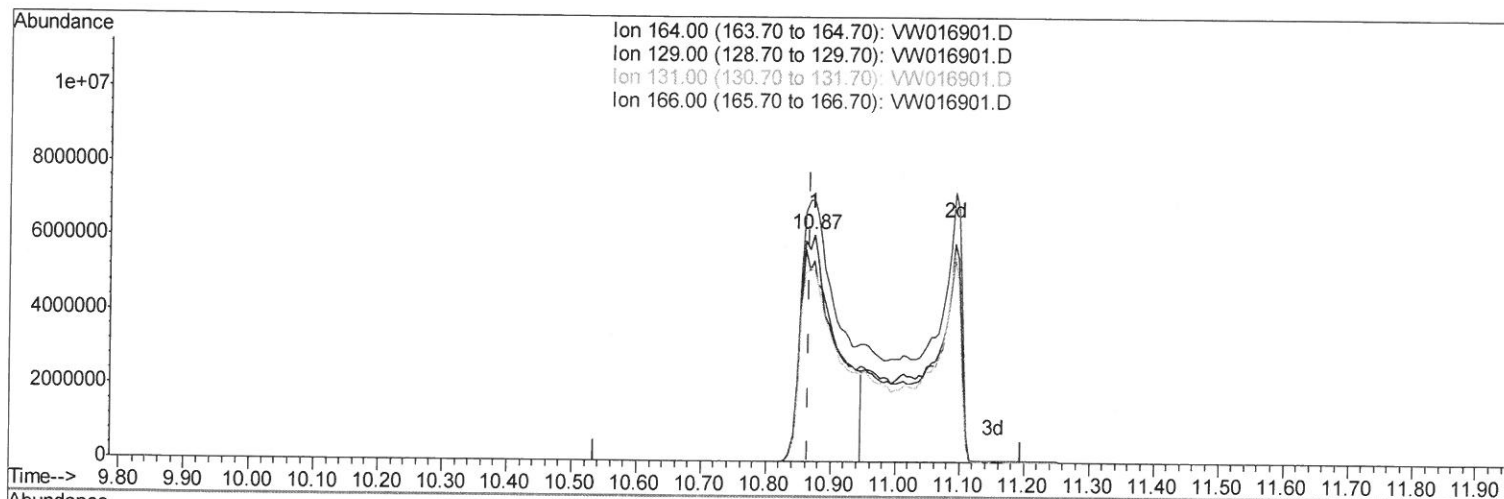

TIC: VW016901.D

(47) Tetrachloroethene (T)

10.872min (+0.006) 19373.60ug/L

response 23901387

Ion	Exp%	Act%
164.00	100	100
129.00	88.20	88.46
131.00	85.30	84.29
166.00	126.20	115.07

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
 Data File : VW016901.D
 Acq On : 14 Oct 2020 13:36
 Operator : SY/VA
 Sample : L4382-11
 Misc : 5.53G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3X9

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:53:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 08:29:28 2020
 Response via : Initial Calibration

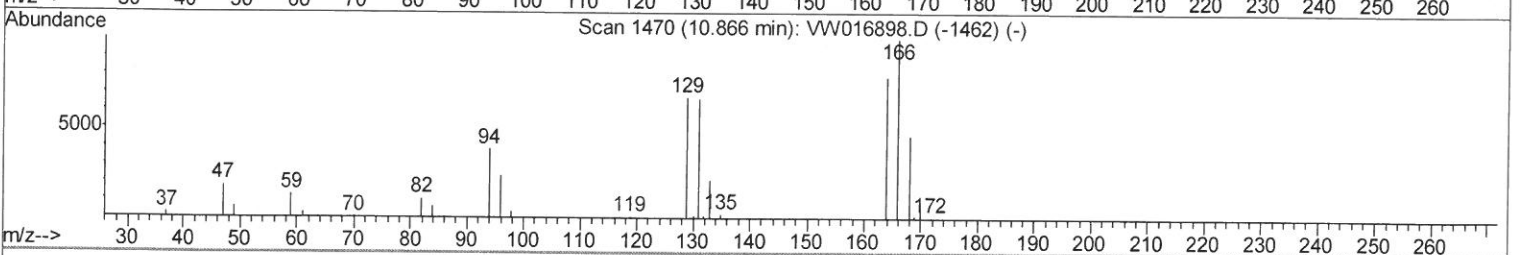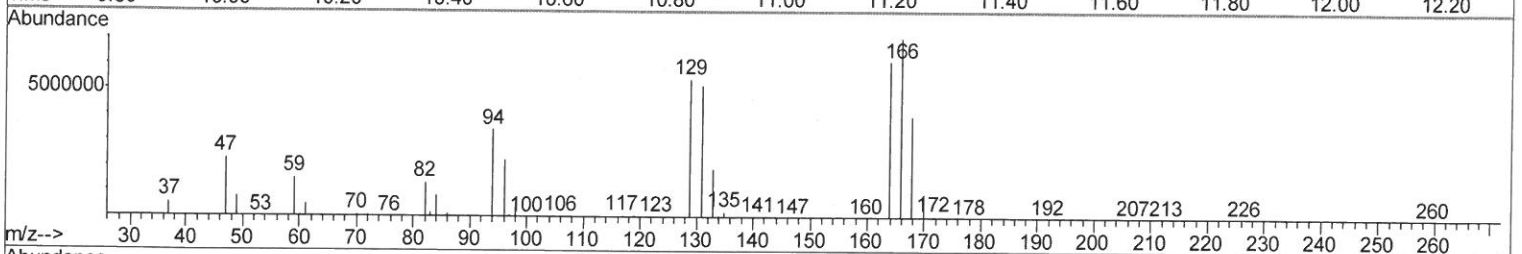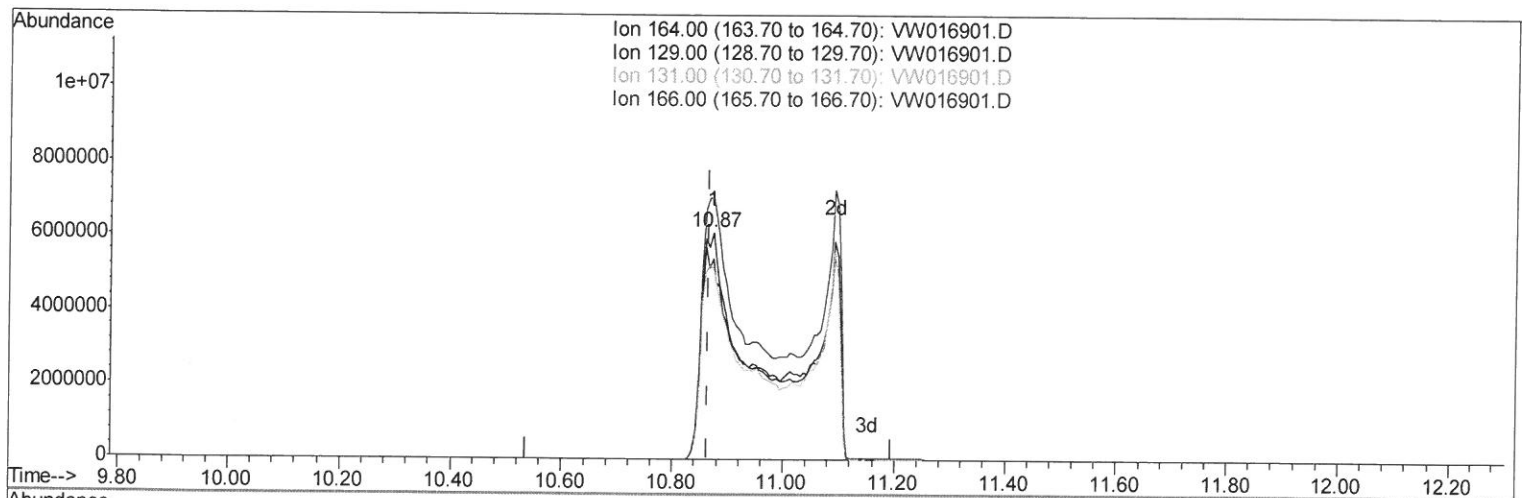

TIC: VW016901.D

(47) Tetrachloroethene (T)

10.872min (+0.006) 41513.47ug/L m > 10/19/20 Sy

response 51215537

Ion	Exp%	Act%
164.00	100	100
129.00	88.20	88.46
131.00	85.30	84.29
166.00	126.20	115.07

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
 Data File : VW016901.D
 Acq On : 14 Oct 2020 13:36
 Operator : SY/VA
 Sample : L4382-11
 Misc : 5.53G/10ML/MSVOA W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3X9

Manual Integrations
 APPROVED

MMDadoda
 10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:56:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 15 08:29:28 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.86	114	190092	25.00	ug/L	0.02
28) Chlorobenzene-d5	11.66	117	87604	25.00	ug/L	0.03
60) 1,4-Dichlorobenzene-d4	13.57	152	27633	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	64394	34.34	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	137.36%		
7) Chloroethane-d5	2.89	69	54568	34.69	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	138.76%		
10) 1,1-Dichloroethene-d2	4.04	63	96543	24.24	ug/L	0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	96.96%		
20) 2-Butanone-d5	7.09	46	27553	64.87	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	129.74%		
24) Chloroform-d	7.66	84	117988	29.41	ug/L	0.01
Spiked Amount 25.000	Range 40 - 150		Recovery =	117.64%		
26) 1,2-Dichloroethane-d4	8.32	65	69838	36.05	ug/L	0.01
Spiked Amount 25.000	Range 70 - 130		Recovery =	144.20%#		
29) Benzene-d6	8.29	84	209544	52.67	ug/L	0.02
Spiked Amount 25.000	Range 20 - 135		Recovery =	210.68%#		
33) 1,2-Dichloropropane-d6	9.29	67	58725	54.92	ug/L	0.01
Spiked Amount 25.000	Range 70 - 120		Recovery =	219.68%#		
37) Toluene-d8	10.35	98	126590	33.72	ug/L	0.02
Spiked Amount 25.000	Range 30 - 130		Recovery =	134.88%#		
38) trans-1,3-Dichloropropene-	10.59	79	24913	52.83	ug/L	0.01
Spiked Amount 25.000	Range 30 - 135		Recovery =	211.32%#		
39) 2-Hexanone-d5	0.00	63	0d	0.00	ug/L	
Spiked Amount 50.000	Range 20 - 135		Recovery =	0.00%#		
48) 1,1,2,2-Tetrachloroethane-	12.70	84	37559	43.48	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	173.92%#		
61) 1,2-Dichlorobenzene-d4	13.86	152	21694	24.75	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.00%		

Target Compounds

					Ovalue	
5) Vinyl chloride	2.36	62	2273	0.874	ug/L	1
12) 1,1-Dichloroethene	4.06	96	44249	18.004	ug/L	89
13) Acetone	4.13	43	5382	16.744	ug/L	93
14) Carbon disulfide	4.40	76	13548	1.922	ug/L	93
16) Methylene chloride	4.94	84	9687	3.693	ug/L	96
18) trans-1,2-Dichloroethene	5.46	96	2982m	1.161	ug/L	
22) cis-1,2-Dichloroethene	7.20	96	5982m	2.283	ug/L	
30) Cyclohexane	7.98	56	3827	2.107	ug/L	# 50
34) Benzene	8.35	78	111835	23.772	ug/L	100
35) Trichloroethene	9.11	95	2649067	1990.715	ug/L	99
36) Methylcyclohexane	9.35	83	6897m	3.083	ug/L	
44) Toluene	10.40	91	62517	11.979	ug/L	97
47) Tetrachloroethene	10.87	164	51215537m	41513.466	ug/L	
52) Chlorobenzene	11.69	112	6167	1.761	ug/L	98
53) Ethylbenzene	11.76	91	38292	6.541	ug/L	98
54) m,p-Xylene	11.86	106	68867	30.245	ug/L	96
55) o-xylene	12.18	106	48371	22.234	ug/L	100

10/19/20 54

10/19/20 54

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
Data File : VW016901.D
Acq On : 14 Oct 2020 13:36
Operator : SY/VA
Sample : L4382-11
Misc : 5.53G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG3X9

Manual Integrations
APPROVED

MMDadoda
10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:56:13 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 15 08:29:28 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
57) Isopropylbenzene	12.48	105	28861	4.845	ug/L	97
63) 1,3-Dichlorobenzene	13.51	146	3524	2.004	ug/L #	12
64) 1,4-Dichlorobenzene	13.58	146	82378	46.838	ug/L #	84
65) 1,2-Dichlorobenzene	13.88	146	129121	82.002	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101520\
Data File : VW016901.D
Acq On : 14 Oct 2020 13:36
Operator : SY/VA
Sample : L4382-11
Misc : 5.53G/10ML/MSVOA W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG3X9

Manual Integrations
APPROVED

MMDadoda
10/19/2020 10:59:08 AM

Quant Time: Oct 15 08:56:13 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100720S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 15 08:29:28 2020
Response via : Initial Calibration

