

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101521\
 Data File : VW020542.D
 Acq On : 15 Oct 2021 18:35
 Operator : SY/VA
 Sample : M4213-01
 Misc : 3.28g/10mL/MSVOA_W/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JDGE3

Quant Time: Oct 16 06:58:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Oct 16 06:56:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	206448	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	151893	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	35540	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	63065	20.994	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.960%
7) Chloroethane-d5	2.879	69	39098	24.639	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.560%
11) 1,1-Dichloroethene-d2	4.013	63	91573	14.877	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.520%
21) 2-Butanone-d5	7.086	46	27842	30.454	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.900%
24) Chloroform-d	7.647	84	141228	21.461	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.840%
26) 1,2-Dichloroethane-d4	8.305	65	82326	21.904	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.600%
32) Benzene-d6	8.275	84	260907	26.114	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	104.440%
36) 1,2-Dichloropropane-d6	9.274	67	88565	27.198	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.800%
41) Toluene-d8	10.323	98	204965	22.864	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.440%
43) trans-1,3-Dichloroprop...	10.579	79	26875	20.310	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.240%
47) 2-Hexanone-d5	10.927	63	18913	37.756	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.520%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	50328	20.447	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.800%
66) 1,2-Dichlorobenzene-d4	13.853	152	29726	21.382	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	85.520%
Target Compounds						Qvalue
16) Methylene chloride	4.909	84	18906	4.711	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101521\
Data File : VW020542.D
Acq On : 15 Oct 2021 18:35
Operator : SY/VA
Sample : M4213-01
Misc : 3.28g/10mL/MSVOA_W/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JDGE3

Quant Time: Oct 16 06:58:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Oct 16 06:56:08 2021
Response via : Initial Calibration

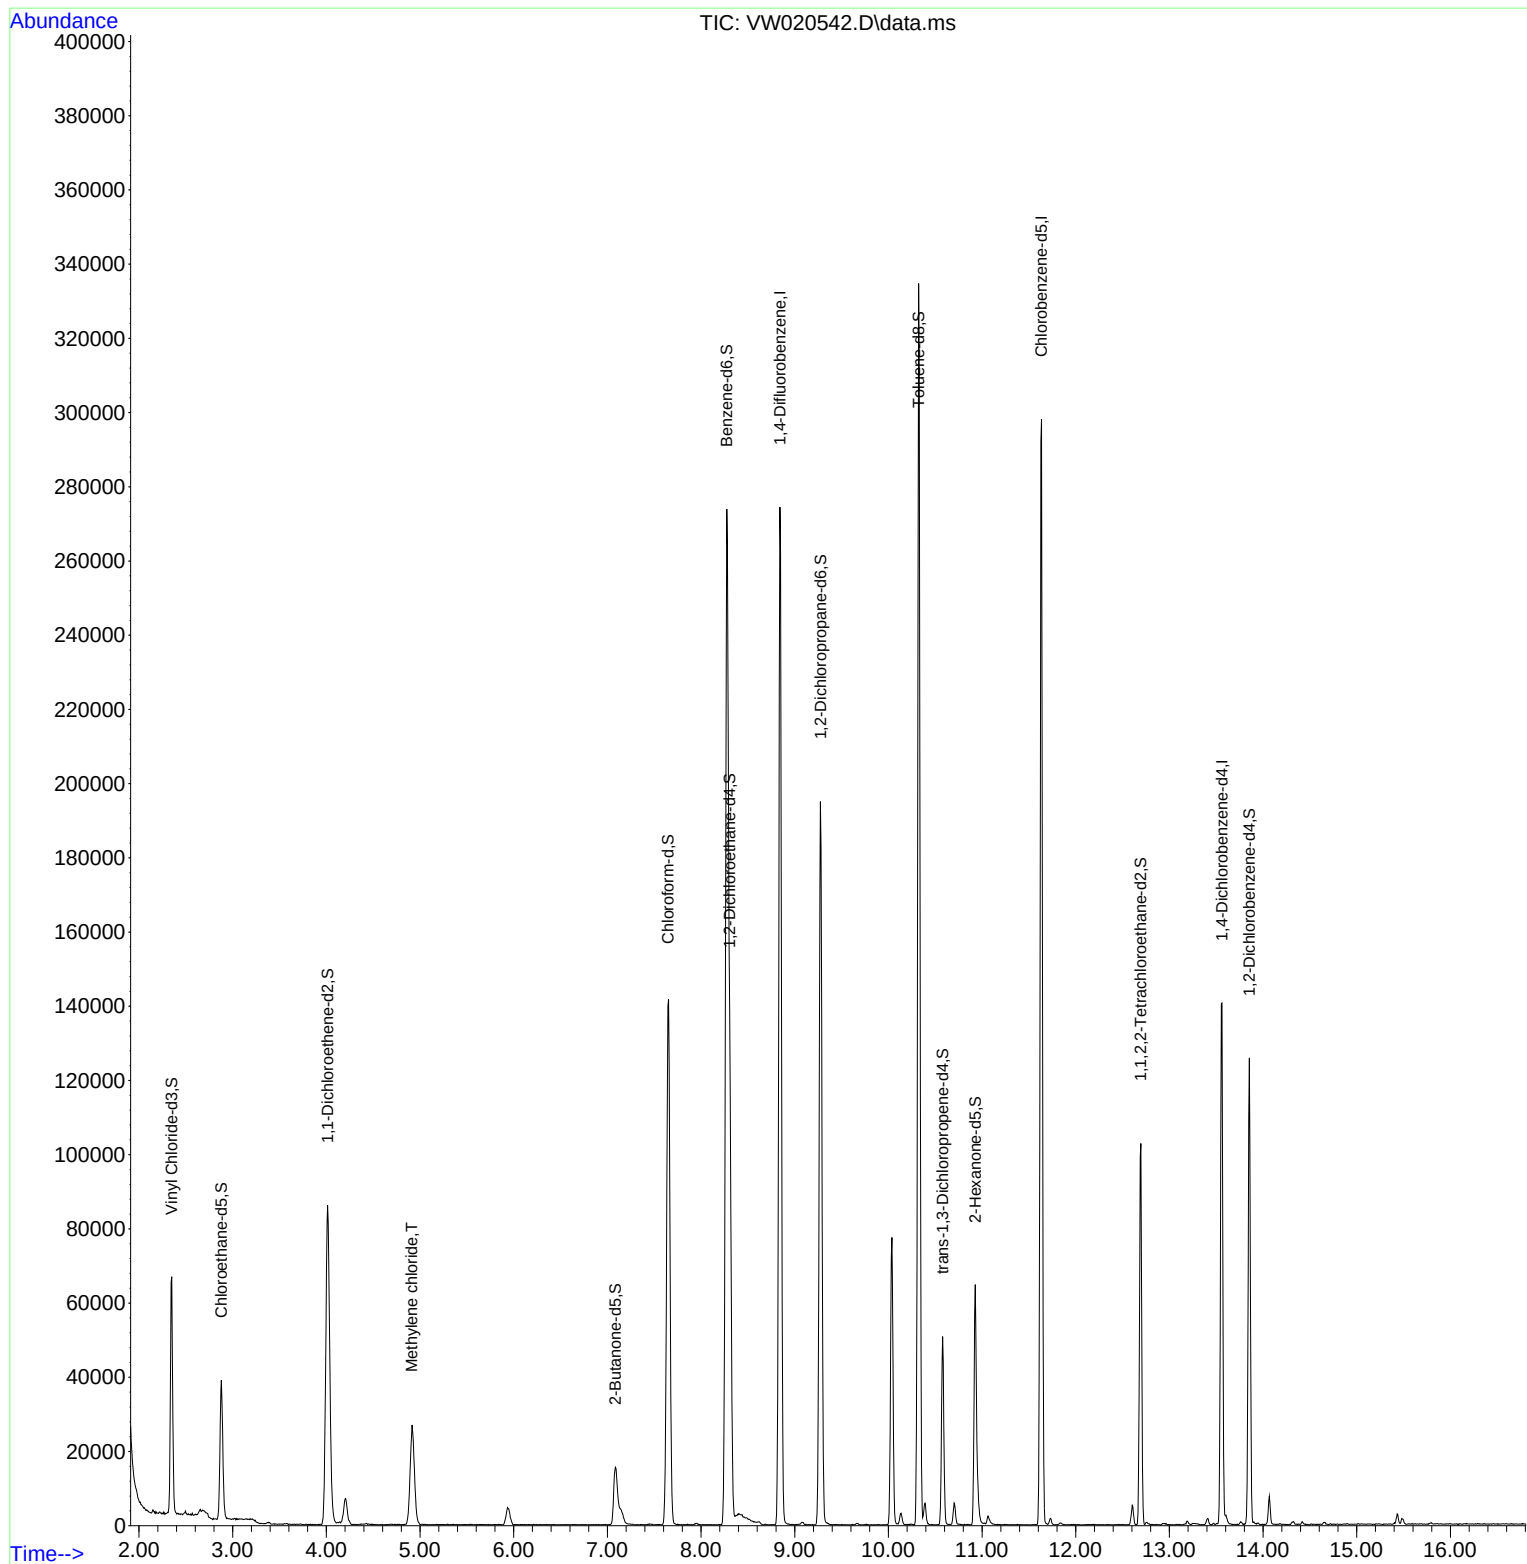

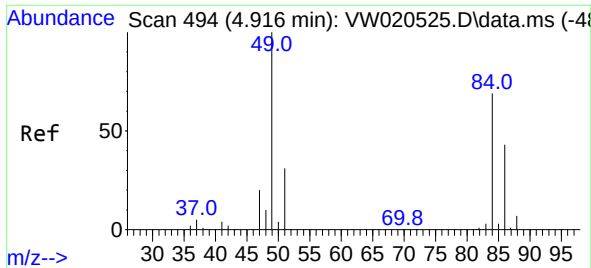

#16
Methylene chloride
Concen: 4.711 ug/L
RT: 4.909 min Scan# 493
Delta R.T. -0.006 min
Lab File: VW020542.D
Acq: 15 Oct 2021 18:35

Instrument :
MSVOA_W
ClientSampleId :
JDGE3

Tgt Ion:	84	Resp:	18906
Ion	Ratio	Lower	Upper
84	100		
86	59.1	44.7	83.1
49	140.4	101.7	188.9

