
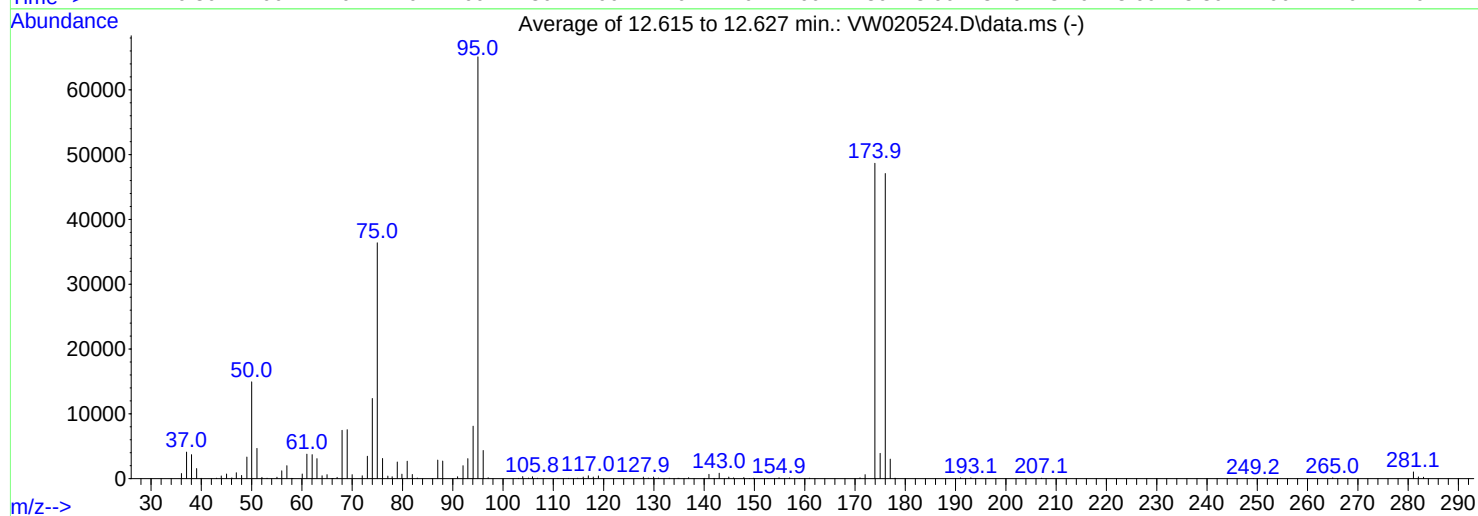


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101521\
 Data File : VW020524.D
 Acq On : 15 Oct 2021 08:45
 Operator : SY/VA
 Sample : BFB453
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB453

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0
 Last Update : Sat Oct 16 06:56:08 2021

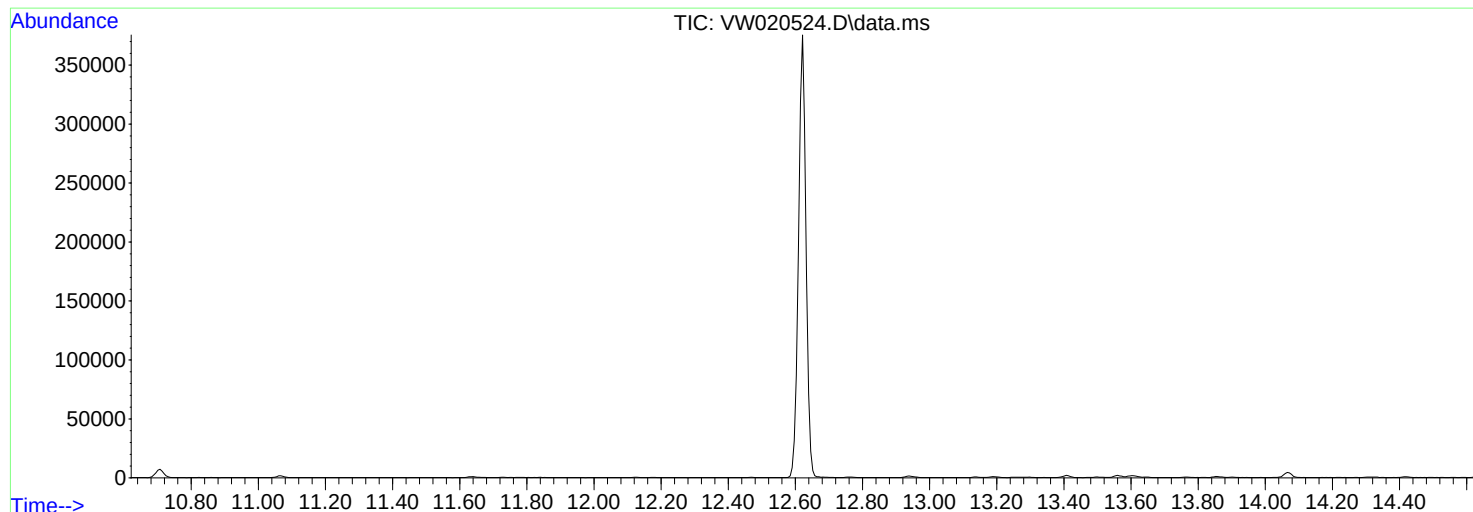

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	14932	PASS
75	95	30	80	55.9	36400	PASS
95	95	100	100	100.0	65101	PASS
96	95	5	9	6.7	4355	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.8	48667	PASS
175	174	5	9	8.0	3900	PASS
176	174	95	105	96.8	47093	PASS
177	176	5	10	6.4	3024	PASS

m/z	Abundance
36.00	648.0
37.10	3381.0
38.00	3205.0
39.00	1289.0
39.90	135.0
43.10	55.0
44.00	488.0
45.00	468.0
45.90	76.0
46.90	707.0
48.00	380.0
49.00	2871.0
50.00	12570.0
51.10	3759.0
52.10	143.0
53.10	60.0
55.10	187.0
56.00	1064.0
57.00	1715.0
58.20	64.0
60.10	596.0
61.00	3426.0
62.10	3265.0
63.00	2576.0
64.00	315.0
65.00	436.0
67.00	189.0
68.00	6318.0
69.00	6943.0
70.00	533.0
72.00	414.0
73.00	3114.0
74.00	10980.0
75.00	32120.0
76.00	2808.0
77.00	414.0
77.90	207.0
78.90	2198.0
79.90	679.0
80.90	2247.0
81.90	549.0
83.00	95.0
85.90	64.0
87.00	2728.0
88.00	2526.0
91.00	336.0
92.10	1868.0
93.00	2659.0
94.00	7263.0
95.00	57984.0
96.10	4024.0
97.10	111.0
103.90	278.0
105.00	93.0
105.90	278.0
106.90	75.0
110.90	61.0
113.00	71.0
114.80	63.0
116.00	219.0
117.00	433.0
117.90	209.0
118.90	405.0
127.90	237.0
128.90	88.0
130.00	204.0
130.90	92.0
134.80	76.0
136.90	158.0
140.00	60.0
140.90	662.0
141.90	80.0
143.00	815.0
144.90	144.0
145.80	104.0
147.90	191.0
149.90	80.0
152.70	62.0
155.00	133.0
156.90	124.0
158.90	56.0
160.90	88.0
170.90	111.0
172.00	512.0
174.00	46552.0
175.00	3864.0
176.00	47272.0
177.00	2944.0
177.90	73.0
190.90	60.0
193.00	60.0
207.00	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

281.10	585.0
282.10	148.0
283.10	128.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

m/z	Abundance
40.00	107.0
43.90	158.0
57.10	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

m/z	Abundance
36.10	777.0
37.00	4194.0
38.10	3851.0
39.10	1710.0
40.00	161.0
43.00	79.0
44.00	605.0
45.00	808.0
46.20	148.0
47.00	881.0
48.00	612.0
49.10	3319.0
50.00	15123.0
51.00	5071.0
52.10	204.0
53.10	95.0
55.00	242.0
56.00	1362.0
57.00	2051.0
58.00	78.0
60.00	801.0
61.00	3661.0
62.10	3682.0
63.00	3194.0
64.00	449.0
65.00	831.0
66.00	77.0
67.00	199.0
68.00	7520.0
69.00	7499.0
70.00	603.0
72.10	404.0
73.00	3271.0
74.00	11775.0
75.00	36168.0
76.10	3002.0
77.20	321.0
77.90	350.0
79.00	2674.0
79.90	698.0
80.90	2793.0
82.00	648.0
83.00	57.0
87.00	2776.0
88.00	2771.0
90.90	283.0
92.00	1953.0
93.00	3004.0
94.10	7725.0
95.00	62544.0
96.10	4092.0
97.00	163.0
103.00	81.0
103.90	356.0
105.00	98.0
105.90	300.0
106.80	64.0
110.90	83.0
113.00	55.0
114.90	58.0
115.90	222.0
117.00	404.0
117.90	261.0
119.00	416.0
127.90	249.0
128.90	100.0
129.90	202.0
130.90	92.0
133.00	139.0
134.80	122.0
136.90	118.0
140.90	677.0
142.00	97.0
143.00	750.0
145.00	323.0
145.90	122.0
147.90	165.0
149.00	70.0
149.90	80.0
154.80	114.0
157.00	108.0
160.90	66.0
171.00	119.0
172.00	683.0
174.00	44368.0
175.00	3293.0
176.00	40720.0
177.00	2777.0
177.90	78.0
191.00	173.0
193.10	210.0
207.10	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

249.20	73.0
265.00	222.0
281.00	1585.0
282.00	462.0
283.10	350.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

m/z	Abundance
36.00	929.0
37.00	4736.0
38.00	4039.0
39.00	1700.0
40.00	147.0
43.10	65.0
44.00	621.0
45.00	884.0
46.00	141.0
47.00	1160.0
48.00	524.0
49.00	3797.0
50.00	17104.0
51.00	5215.0
52.00	228.0
53.00	107.0
55.00	262.0
56.00	1227.0
57.00	2384.0
58.00	95.0
60.00	794.0
61.00	4226.0
62.00	4186.0
63.00	3506.0
64.00	603.0
65.00	581.0
66.20	79.0
67.00	209.0
68.00	8563.0
69.00	8202.0
70.00	712.0
71.90	525.0
73.00	4008.0
74.00	14342.0
75.00	40912.0
76.10	3501.0
77.10	456.0
78.00	363.0
78.90	2848.0
79.90	743.0
81.00	3066.0
82.00	737.0
82.90	112.0
87.00	3075.0
88.00	2894.0
91.00	307.0
92.10	2186.0
93.00	3613.0
94.00	9334.0
95.00	74776.0
96.00	4950.0
97.10	152.0
103.10	62.0
103.90	327.0
105.10	127.0
105.80	295.0
106.90	87.0
113.00	60.0
114.90	127.0
116.00	281.0
116.90	541.0
118.00	298.0
119.00	463.0
127.90	266.0
128.90	121.0
129.90	335.0
130.90	117.0
133.10	122.0
135.00	126.0
136.90	151.0
140.00	76.0
141.00	653.0
143.00	952.0
144.80	254.0
145.90	131.0
147.90	150.0
149.80	80.0
154.90	175.0
157.10	104.0
158.90	84.0
161.00	89.0
171.10	168.0
172.00	684.0
173.90	55080.0
175.00	4542.0
176.00	53288.0
177.00	3352.0
178.00	97.0
191.00	111.0
192.90	104.0
207.10	88.0
265.00	114.0

Instrument :
MSVOA_W
ClientSampleId :
BFB453

281.10

282.10

283.00

913.0

243.0

177.0

Instrument :

MSVOA_W

ClientSampleId :

BFB453