

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101619\
 Data File : VW013602.D
 Acq On : 16 Oct 2019 16:26
 Operator : SY/VA
 Sample : K5378-22
 Misc : 3.32G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0027

Quant Time: Oct 16 17:50:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 16 16:38:03 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	396327	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	312699	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	114646	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	102329	22.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.24%
7) Chloroethane-d5	2.89	69	81838	23.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.00%
10) 1,1-Dichloroethene-d2	4.01	63	168716	17.92	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.68%
20) 2-Butanone-d5	7.08	46	43572	31.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.78%
24) Chloroform-d	7.65	84	211502	24.57	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.28%
26) 1,2-Dichloroethane-d4	8.31	65	105922	23.75	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.00%
29) Benzene-d6	8.27	84	454242	27.12	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.48%
33) 1,2-Dichloropropane-d6	9.27	67	135844	27.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.36%
37) Toluene-d8	10.32	98	396475	24.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.76%
38) trans-1,3-Dichloropropene-	10.57	79	44082	19.91	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.64%
39) 2-Hexanone-d5	10.93	63	33324	33.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.04%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	85668	21.50	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.00%
61) 1,2-Dichlorobenzene-d4	13.85	152	101213	24.57	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.28%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.55	75	11576	3.798 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101619\
Data File : VW013602.D
Acq On : 16 Oct 2019 16:26
Operator : SY/VA
Sample : K5378-22
Misc : 3.32G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0027

Quant Time: Oct 16 17:50:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 16 16:38:03 2019
Response via : Initial Calibration

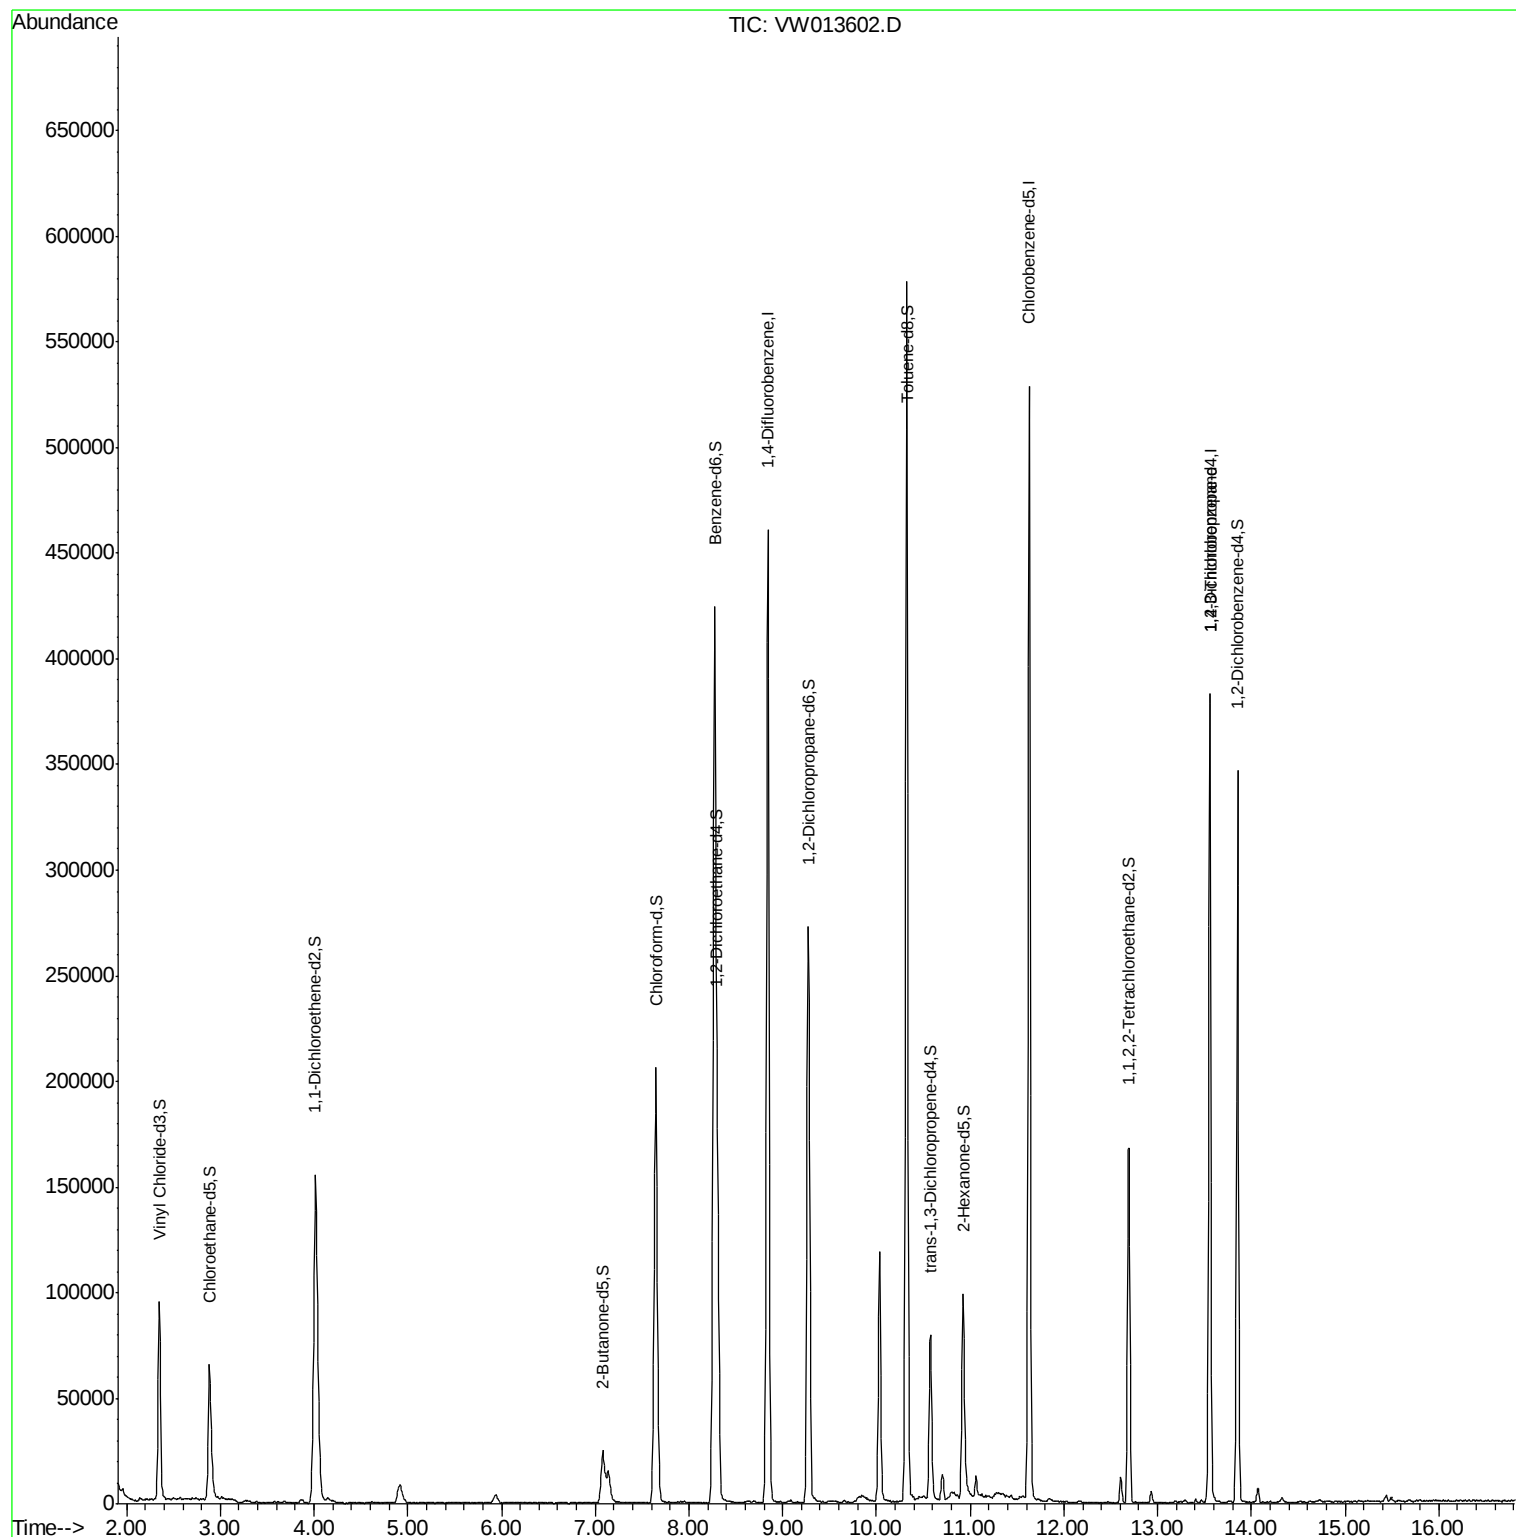

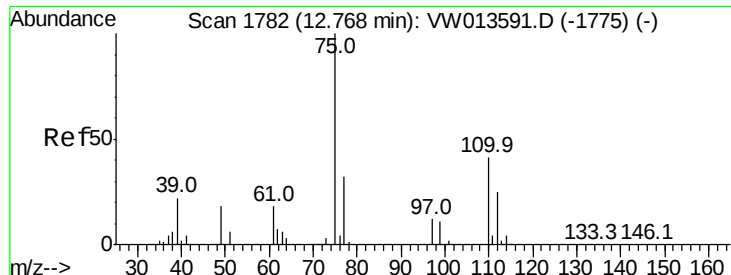

#59

1,2,3-Trichloropropane

Concen: 3.798 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW013602.D

Acq: 16 Oct 2019 16:26

Instrument :

MSVOA_W

ClientSampleId :

C0027

Tot Ion: 75 Resp: 11576

Ion Ratio Lower Upper

75 100

77 36.0 25.5 38.3

