


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW101718\
 Data File : VW006143.D
 Acq On : 17 Oct 2018 23:46
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
 Title : SW846 8260
 Last Update : Thu Oct 18 17:01:24 2018

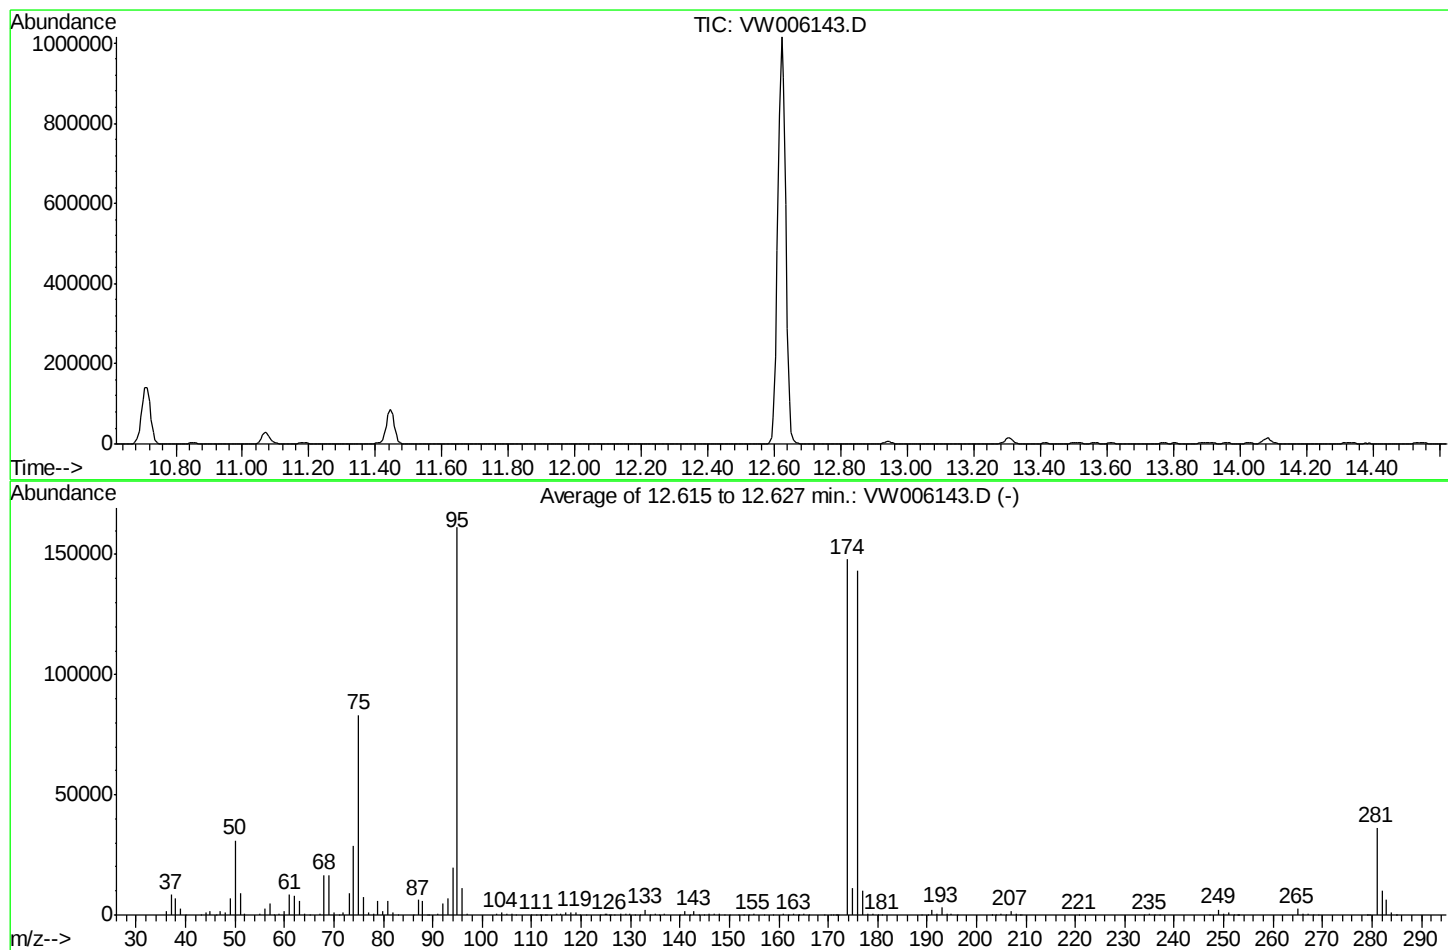

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	30901	PASS
75	95	30	60	51.6	83205	PASS
95	95	100	100	100.0	161322	PASS
96	95	5	9	6.9	11102	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.8	148029	PASS
175	174	5	9	7.4	10997	PASS
176	174	95	101	96.9	143418	PASS
177	176	5	9	6.9	9959	PASS