

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101719\
 Data File : VW013611.D
 Acq On : 17 Oct 2019 12:29
 Operator : SY/VA
 Sample : K5378-10
 Misc : 5.08G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 17 16:59:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 17 16:56:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	438395	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	398457	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	192069	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	104760	20.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.52%
7) Chloroethane-d5	2.89	69	81536	21.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.68%
10) 1,1-Dichloroethene-d2	4.02	63	170494	16.37	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.48%
20) 2-Butanone-d5	7.08	46	85936	56.86	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.72%
24) Chloroform-d	7.65	84	226902	23.83	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.32%
26) 1,2-Dichloroethane-d4	8.30	65	128003	25.94	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.76%
29) Benzene-d6	8.27	84	498204	23.34	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.36%
33) 1,2-Dichloropropane-d6	9.27	67	150338	23.74	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.96%
37) Toluene-d8	10.32	98	459651	22.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.76%
38) trans-1,3-Dichloropropene-	10.58	79	63351	22.46	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.84%
39) 2-Hexanone-d5	10.93	63	68036	53.71	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.42%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	133787	26.35	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.40%
61) 1,2-Dichlorobenzene-d4	13.85	152	169373	24.54	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.16%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.56	75	18979	4.887 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101719\
Data File : VW013611.D
Acq On : 17 Oct 2019 12:29
Operator : SY/VA
Sample : K5378-10
Misc : 5.08G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 17 16:59:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 17 16:56:38 2019
Response via : Initial Calibration

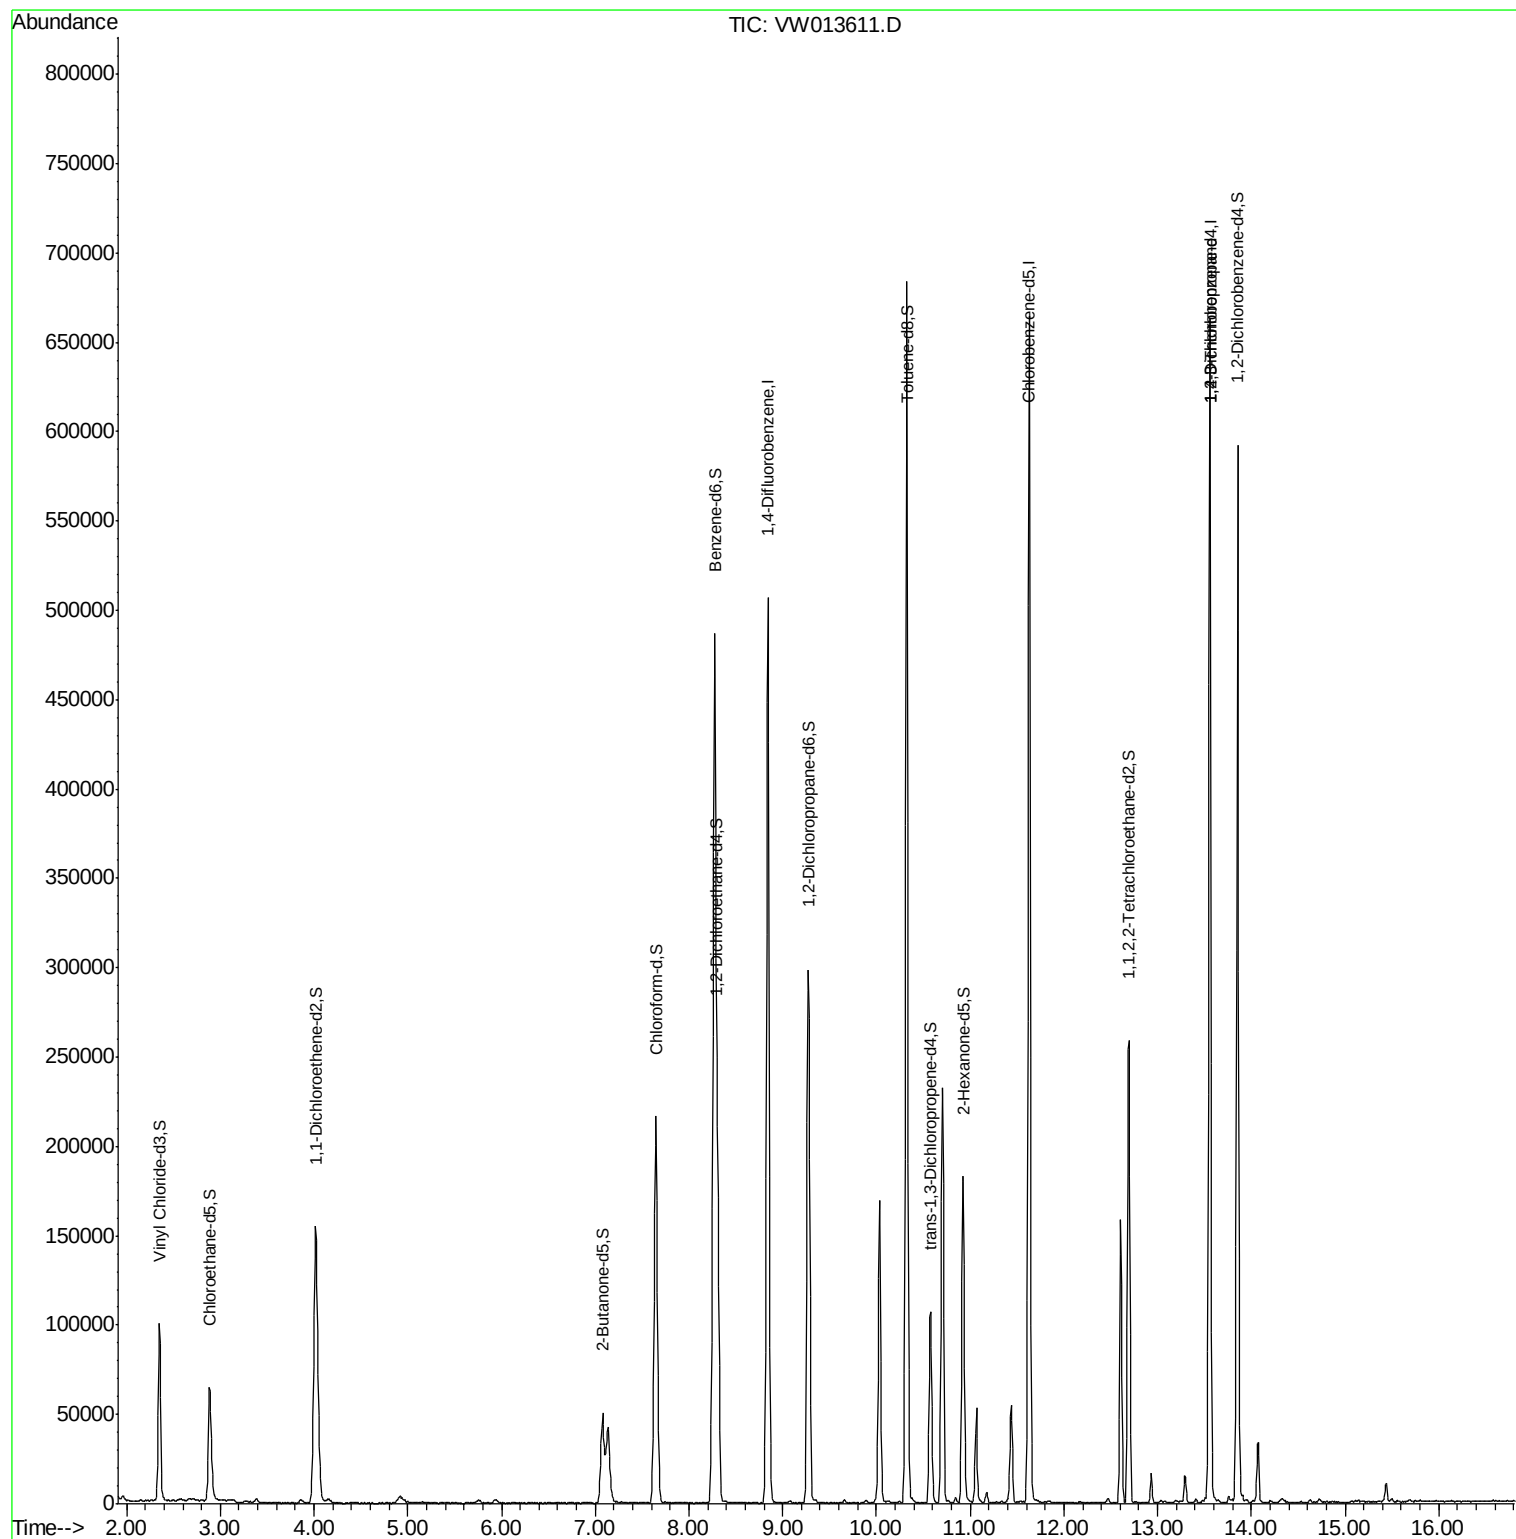

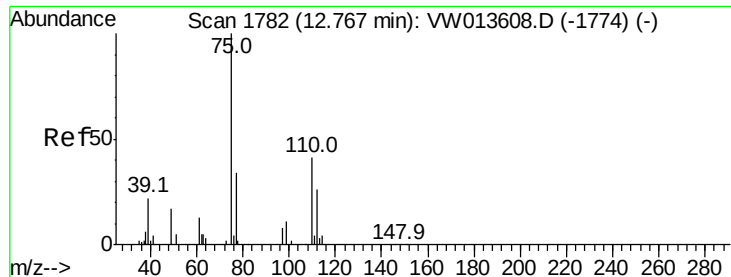

#59

1,2,3-Trichloropropane

Concen: 4.887 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW013611.D

Acq: 17 Oct 2019 12:29

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 18979

Ion Ratio Lower Upper

75 100

77 37.5 25.5 38.3

