

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101719\
 Data File : VW013610.D
 Acq On : 17 Oct 2019 11:35
 Operator : SY/VA
 Sample : K5395-02
 Misc : 4.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0029

Quant Time: Oct 17 17:07:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 17 16:56:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	433042	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	365041	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	159009	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	100538	20.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.16%
7) Chloroethane-d5	2.89	69	86354	22.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.76%
10) 1,1-Dichloroethene-d2	4.02	63	179813	17.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.92%
20) 2-Butanone-d5	7.07	46	72535	48.59	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.18%
24) Chloroform-d	7.65	84	244956	26.04	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.16%
26) 1,2-Dichloroethane-d4	8.30	65	129240	26.52	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.08%
29) Benzene-d6	8.27	84	537847	27.51	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	110.04%
33) 1,2-Dichloropropane-d6	9.27	67	159019	27.41	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.64%
37) Toluene-d8	10.32	98	492911	26.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	106.24%
38) trans-1,3-Dichloropropene-	10.58	79	65349	25.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.16%
39) 2-Hexanone-d5	10.93	63	55083	47.47	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.94%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	116547	25.06	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.24%
61) 1,2-Dichlorobenzene-d4	13.85	152	153903	26.93	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.72%


Target Compounds					Ovalue
13) Acetone	4.13	43	15947	9.294 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101719\
Data File : VW013610.D
Acq On : 17 Oct 2019 11:35
Operator : SY/VA
Sample : K5395-02
Misc : 4.02G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0029

Quant Time: Oct 17 17:07:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101019S.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 17 16:56:38 2019
Response via : Initial Calibration

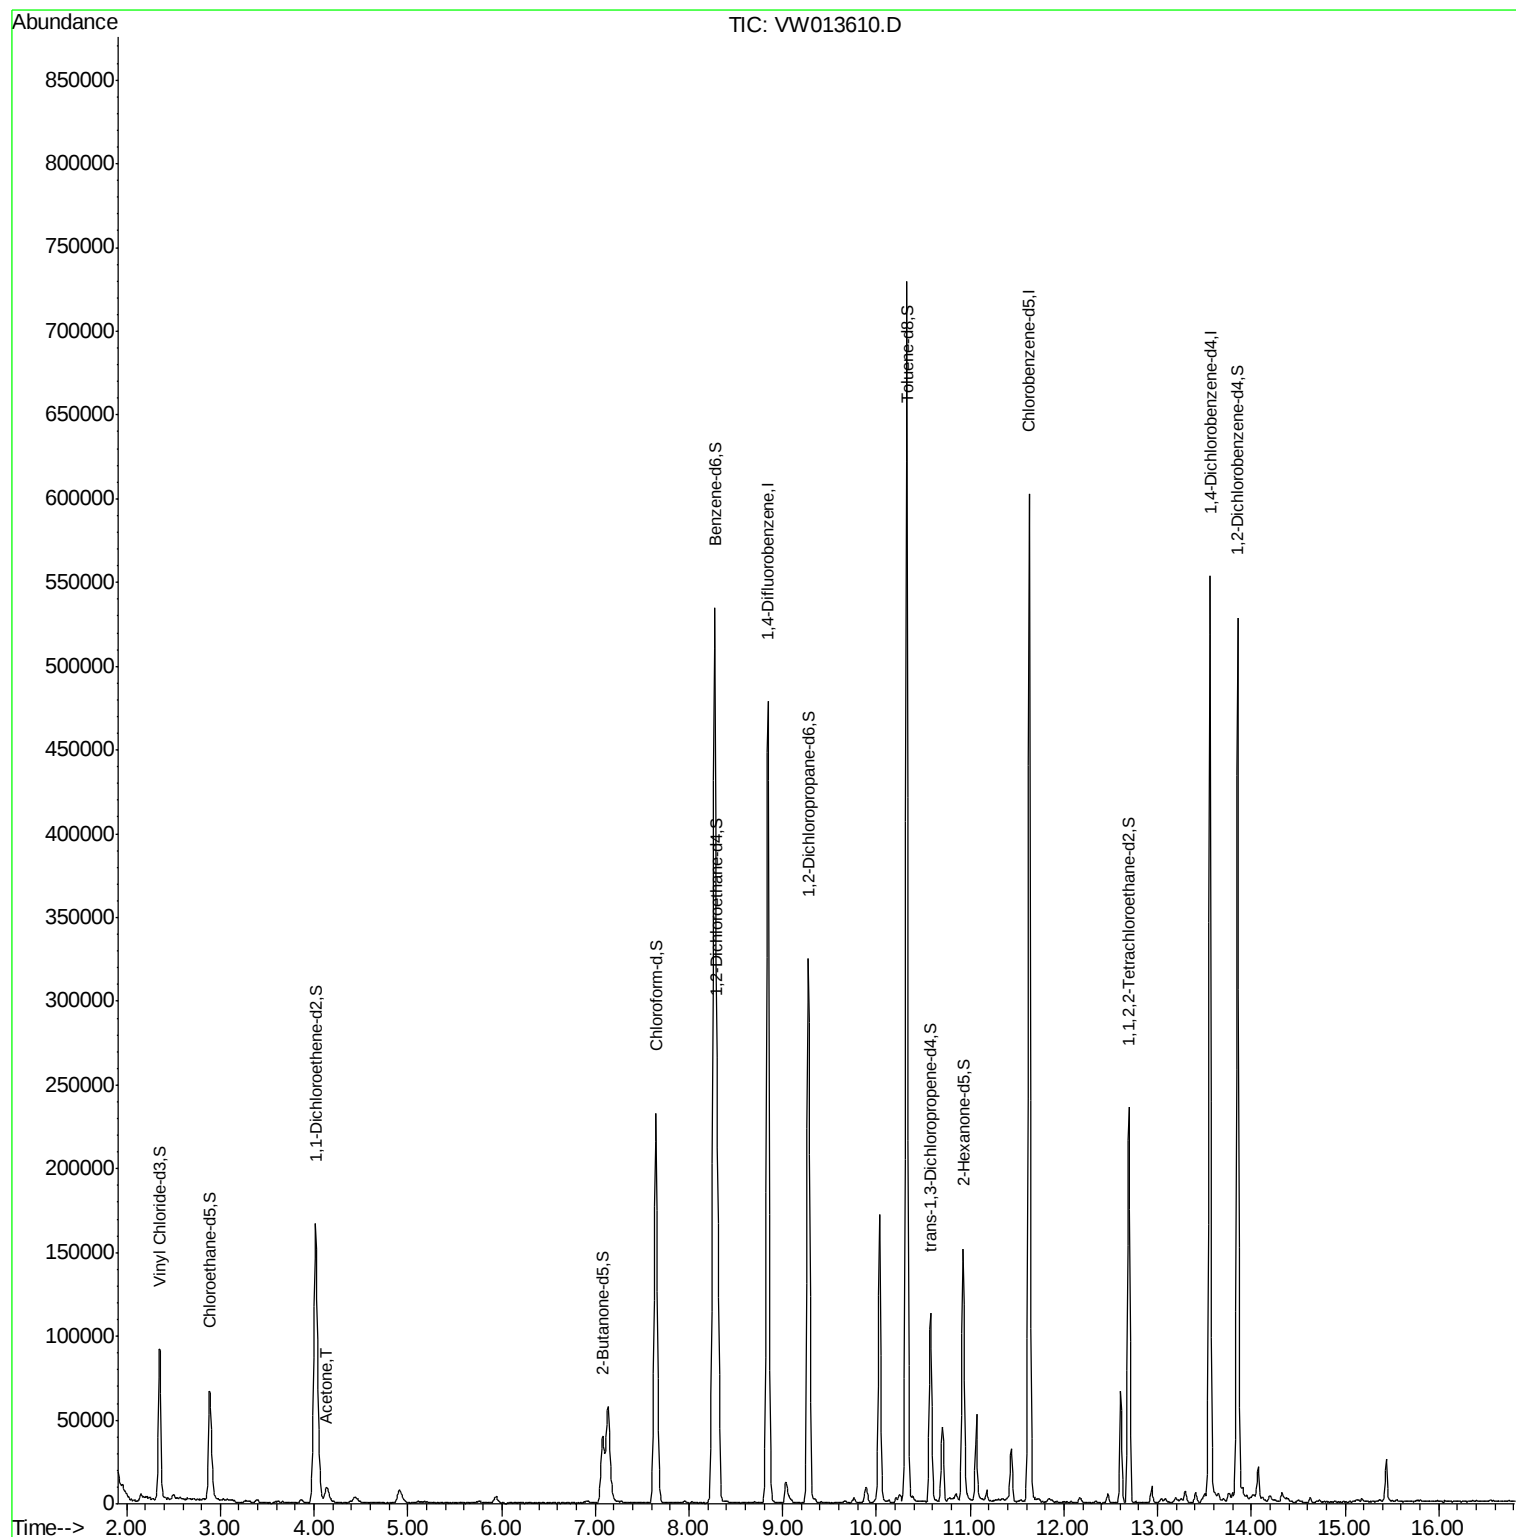

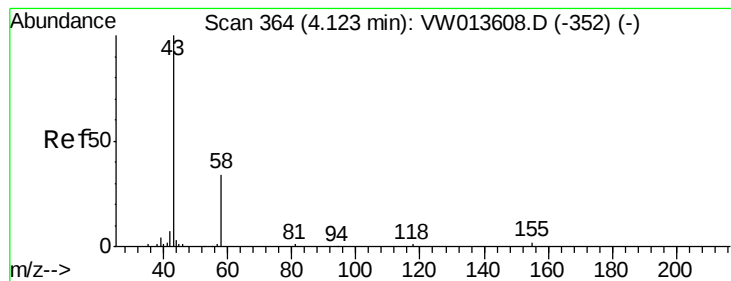

#13

Acetone

Concen: 9.294 ug/L

RT: 4.13 min Scan# 366

Delta R.T. 0.01 min

Lab File: VW013610.D

Acq: 17 Oct 2019 11:35

Instrument :

MSVOA_W

ClientSampleId :

C0029

Tot Ion: 43 Resp: 15947

Ion Ratio Lower Upper

43 100

58 33.2 0.0 67.8

