




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
 Data File : VW030648.D
 Acq On : 17 Oct 2024 18:59
 Operator : SY/MD
 Sample : P4414-19
 Misc : 5.16g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F79

Manual IntegrationsAPPROVED

Quant Time: Oct 18 01:44:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 18 01:38:16 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/18/2024
 Supervised By :Semsettin Yesilyurt 10/18/2024

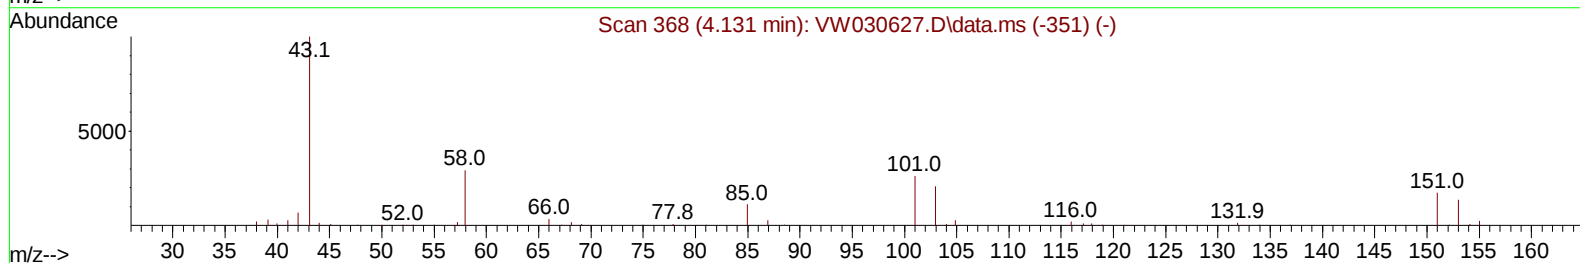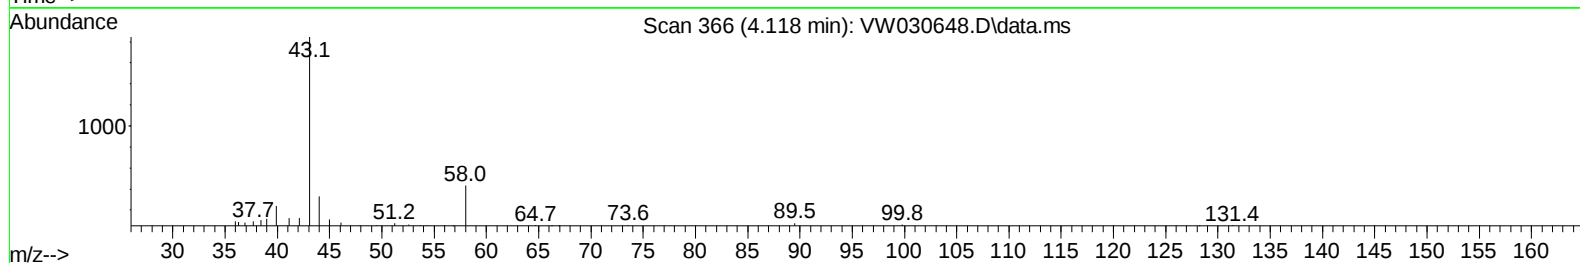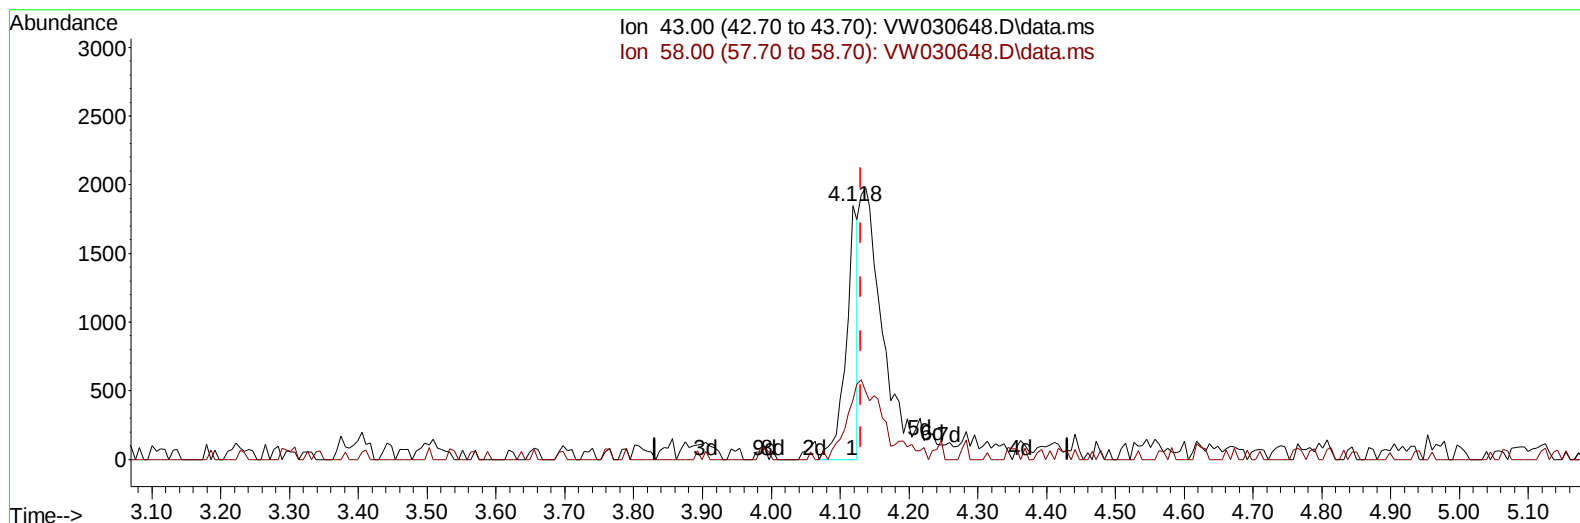

TIC: VW030648.D\data.ms

(13) Acetone (T)

4.118min (-0.012) 16.94 ug/L

response 2266

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.80	54.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
Data File : VW030648.D
Acq On : 17 Oct 2024 18:59
Operator : SY/MD
Sample : P4414-19
Misc : 5.16g/10mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F79

Manual IntegrationsAPPROVED

Quant Time: Oct 18 01:44:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 18 01:38:16 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/18/2024
Supervised By :Semsettin Yesilyurt 10/18/2024

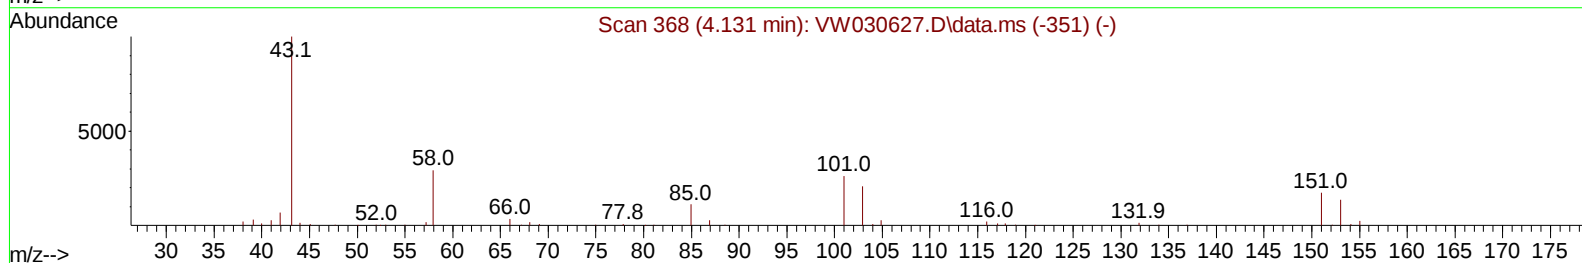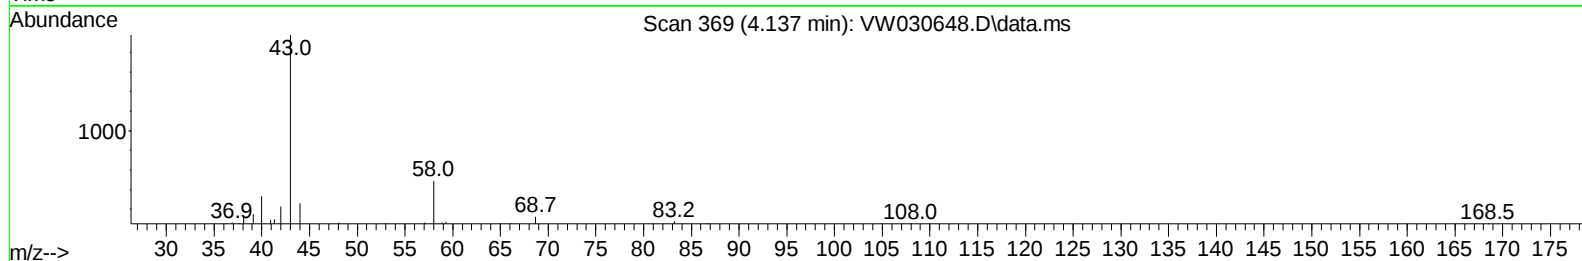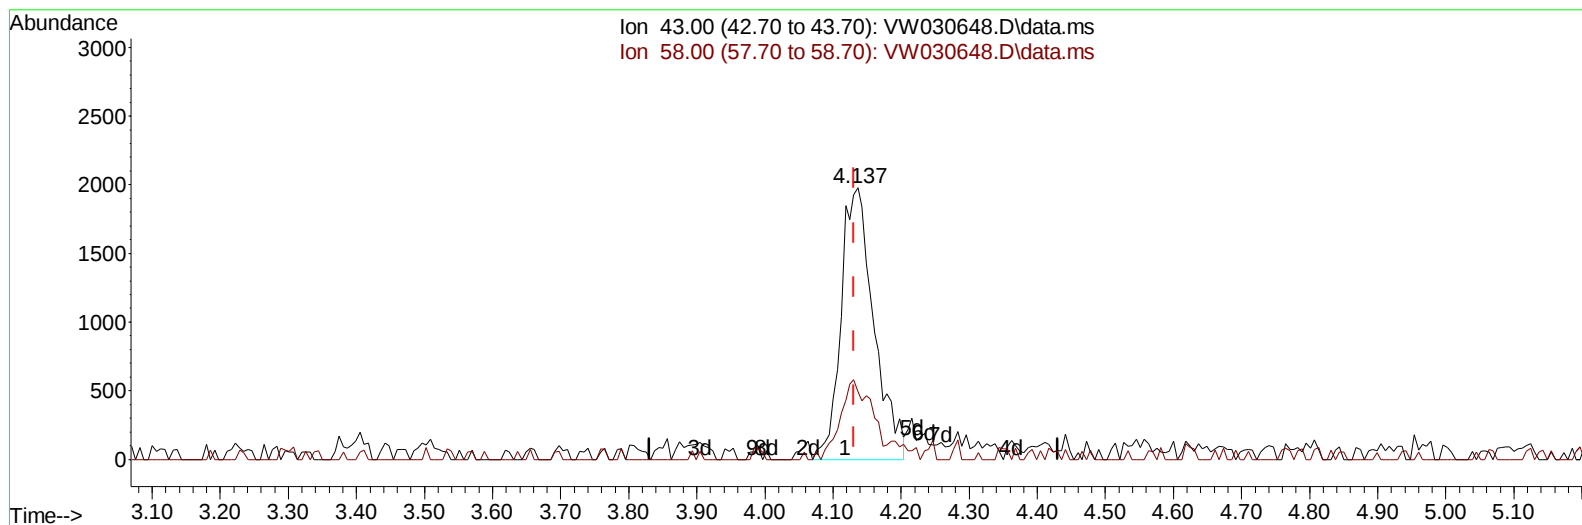

TIC: VW030648.D\data.ms

(13) Acetone (T)

4.137min (+ 0.006) 49.89 ug/L m

response 6673

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	28.80	18.42
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
Data File : VW030648.D
Acq On : 17 Oct 2024 18:59
Operator : SY/MD
Sample : P4414-19
Misc : 5.16g/10mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F79

Manual IntegrationsAPPROVED

Quant Time: Oct 18 01:44:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 18 01:38:16 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/18/2024
Supervised By :Semsettin Yesilyurt 10/18/2024

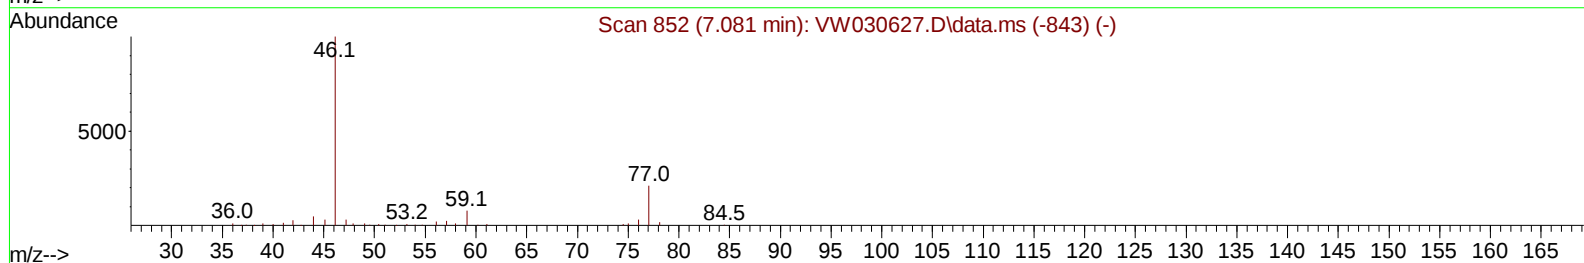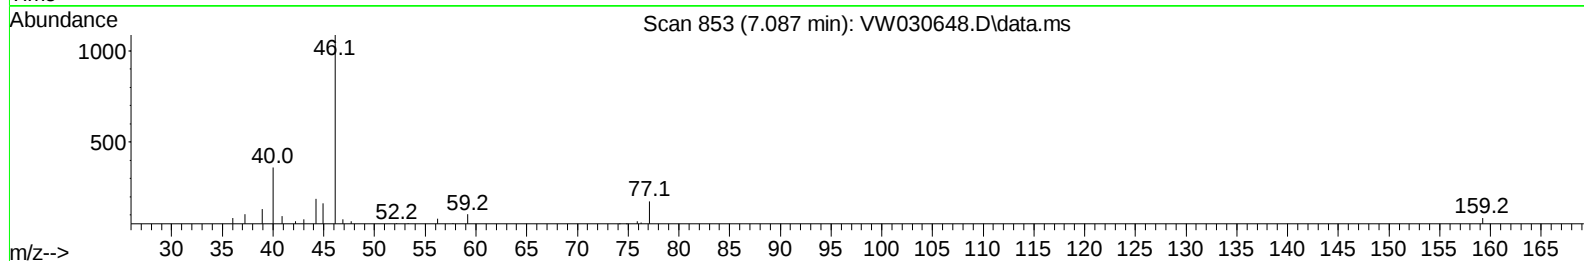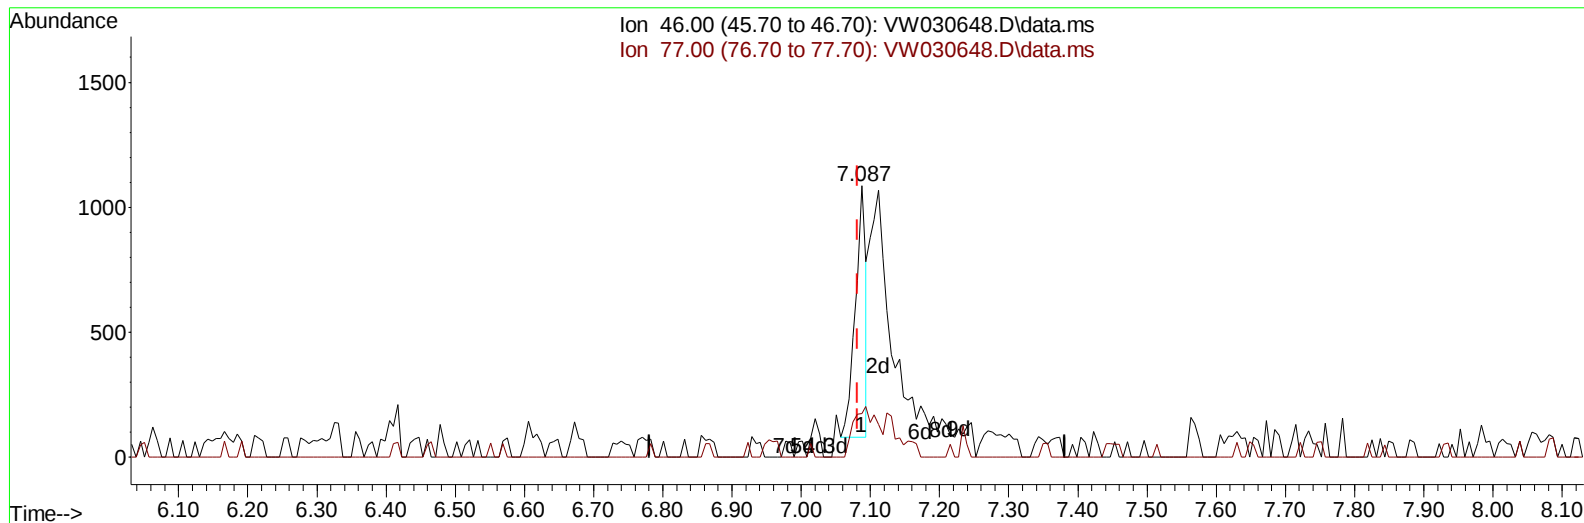

TIC: VW030648.D\data.ms

(21) 2-Butanone-d5 (S)

7.087min (+ 0.006) 11.74 ug/L

response 1073

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.20	30.85
0.00	0.00	0.00
0.00	0.00	0.00


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
 Data File : VW030648.D
 Acq On : 17 Oct 2024 18:59
 Operator : SY/MD
 Sample : P4414-19
 Misc : 5.16g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F79

Manual IntegrationsAPPROVED

Quant Time: Oct 18 01:44:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 18 01:38:16 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/18/2024
 Supervised By :Semsettin Yesilyurt 10/18/2024

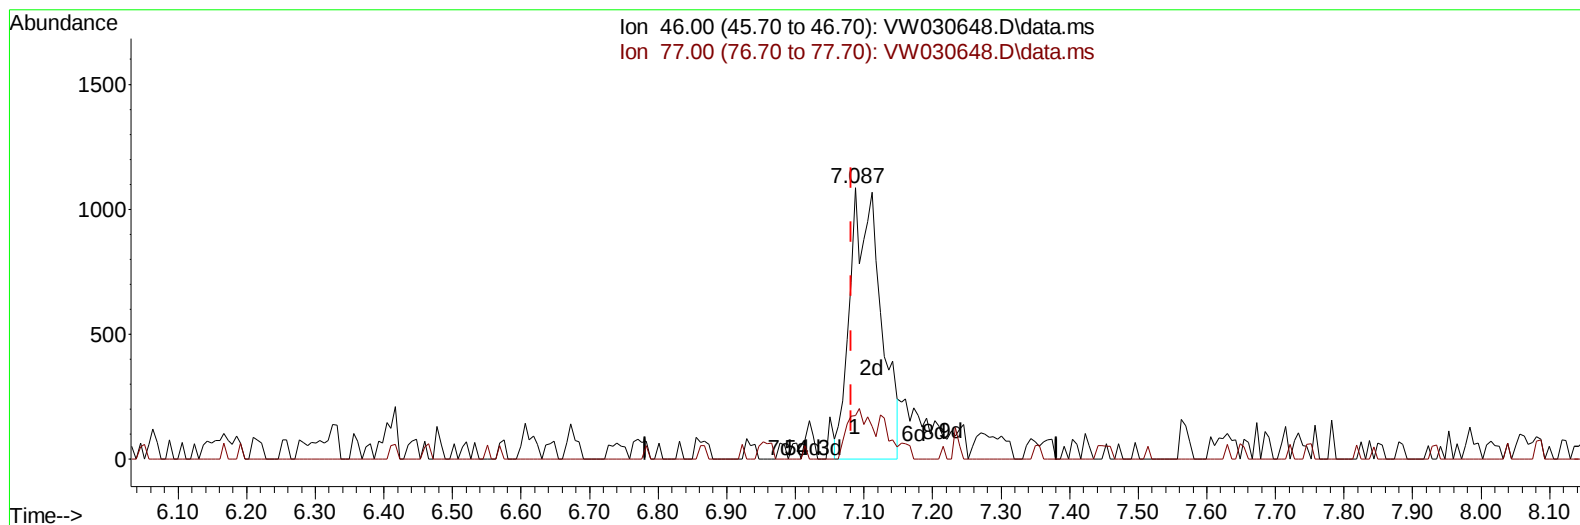

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw101724\
 Data File : VW030648.D
 Acq On : 17 Oct 2024 18:59
 Operator : SY/MD
 Sample : P4414-19
 Misc : 5.16g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F79

Manual IntegrationsAPPROVED

Quant Time: Oct 18 01:44:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 18 01:38:16 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/18/2024
 Supervised By :Semsettin Yesilyurt 10/18/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		32297	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		29969	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.562	152		10885	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.356	65		7617	15.004	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150		Recovery =	60.000%		
7) Chloroethane-d5	2.893	69		6543	17.027	ug/L	-0.01
Spiked Amount 25.000	Range 30	- 150		Recovery =	68.120%		
11) 1,1-Dichloroethene-d2	4.021	65		2832	13.412	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	53.640%		
21) 2-Butanone-d5	7.087	46		3331m	36.460	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	72.920%		
24) Chloroform-d	7.654	84		18992	20.562	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	82.240%		
26) 1,2-Dichloroethane-d4	8.307	65		11440	23.819	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	95.280%		
32) Benzene-d6	8.276	84		27320	15.707	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	62.840%		
36) 1,2-Dichloropropane-d6	9.276	67		10489	20.545	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	82.200%		
41) Toluene-d8	10.325	98		16818	10.592	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	42.360%		
43) trans-1,3-Dichloroprop...	10.587	79		2979	13.935	ug/L	0.01
Spiked Amount 25.000	Range 30	- 135		Recovery =	55.760%		
47) 2-Hexanone-d5	10.928	63		2009	30.552	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	61.100%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		9994	26.656	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	106.640%		
66) 1,2-Dichlorobenzene-d4	13.854	152		6628	17.996	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	72.000%#		
Target Compounds							
13) Acetone	4.137	43		6673m	49.891	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
Data File : VW030648.D
Acq On : 17 Oct 2024 18:59
Operator : SY/MD
Sample : P4414-19
Misc : 5.16g/10mL/MSVOA_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F79

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/18/2024
Supervised By :Semsettin Yesilyurt 10/18/2024

Quant Time: Oct 18 01:44:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 18 01:38:16 2024
Response via : Initial Calibration

