

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
 Data File : VW030636.D
 Acq On : 17 Oct 2024 14:08
 Operator : SY/MD
 Sample : P4414-06
 Misc : 4.95g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F91

Quant Time: Oct 18 01:41:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 18 01:38:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	448075	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	425407	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	195937	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	82309	11.687	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	46.760%
7) Chloroethane-d5	2.893	69	84930	15.930	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.720%
11) 1,1-Dichloroethene-d2	4.021	65	30964	10.570	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	42.280%#
21) 2-Butanone-d5	7.075	46	63966	50.467	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.940%
24) Chloroform-d	7.648	84	254049	19.826	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.320%
26) 1,2-Dichloroethane-d4	8.301	65	137732	20.670	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.680%
32) Benzene-d6	8.276	84	382610	15.496	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	62.000%
36) 1,2-Dichloropropane-d6	9.270	67	145078	20.019	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	80.080%
41) Toluene-d8	10.325	98	304536	13.511	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	54.040%
43) trans-1,3-Dichloroprop...	10.575	79	52737	17.379	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.520%
47) 2-Hexanone-d5	10.922	63	48646	52.117	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.240%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	128104	24.070	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.280%
66) 1,2-Dichlorobenzene-d4	13.848	152	131406	19.821	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.280%
Target Compounds						
					Qvalue	
13) Acetone	4.118	43	11841	6.381	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
Data File : VW030636.D
Acq On : 17 Oct 2024 14:08
Operator : SY/MD
Sample : P4414-06
Misc : 4.95g/10mL/MSVOA_W/SOIL/B
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F91

Quant Time: Oct 18 01:41:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 18 01:38:16 2024
Response via : Initial Calibration

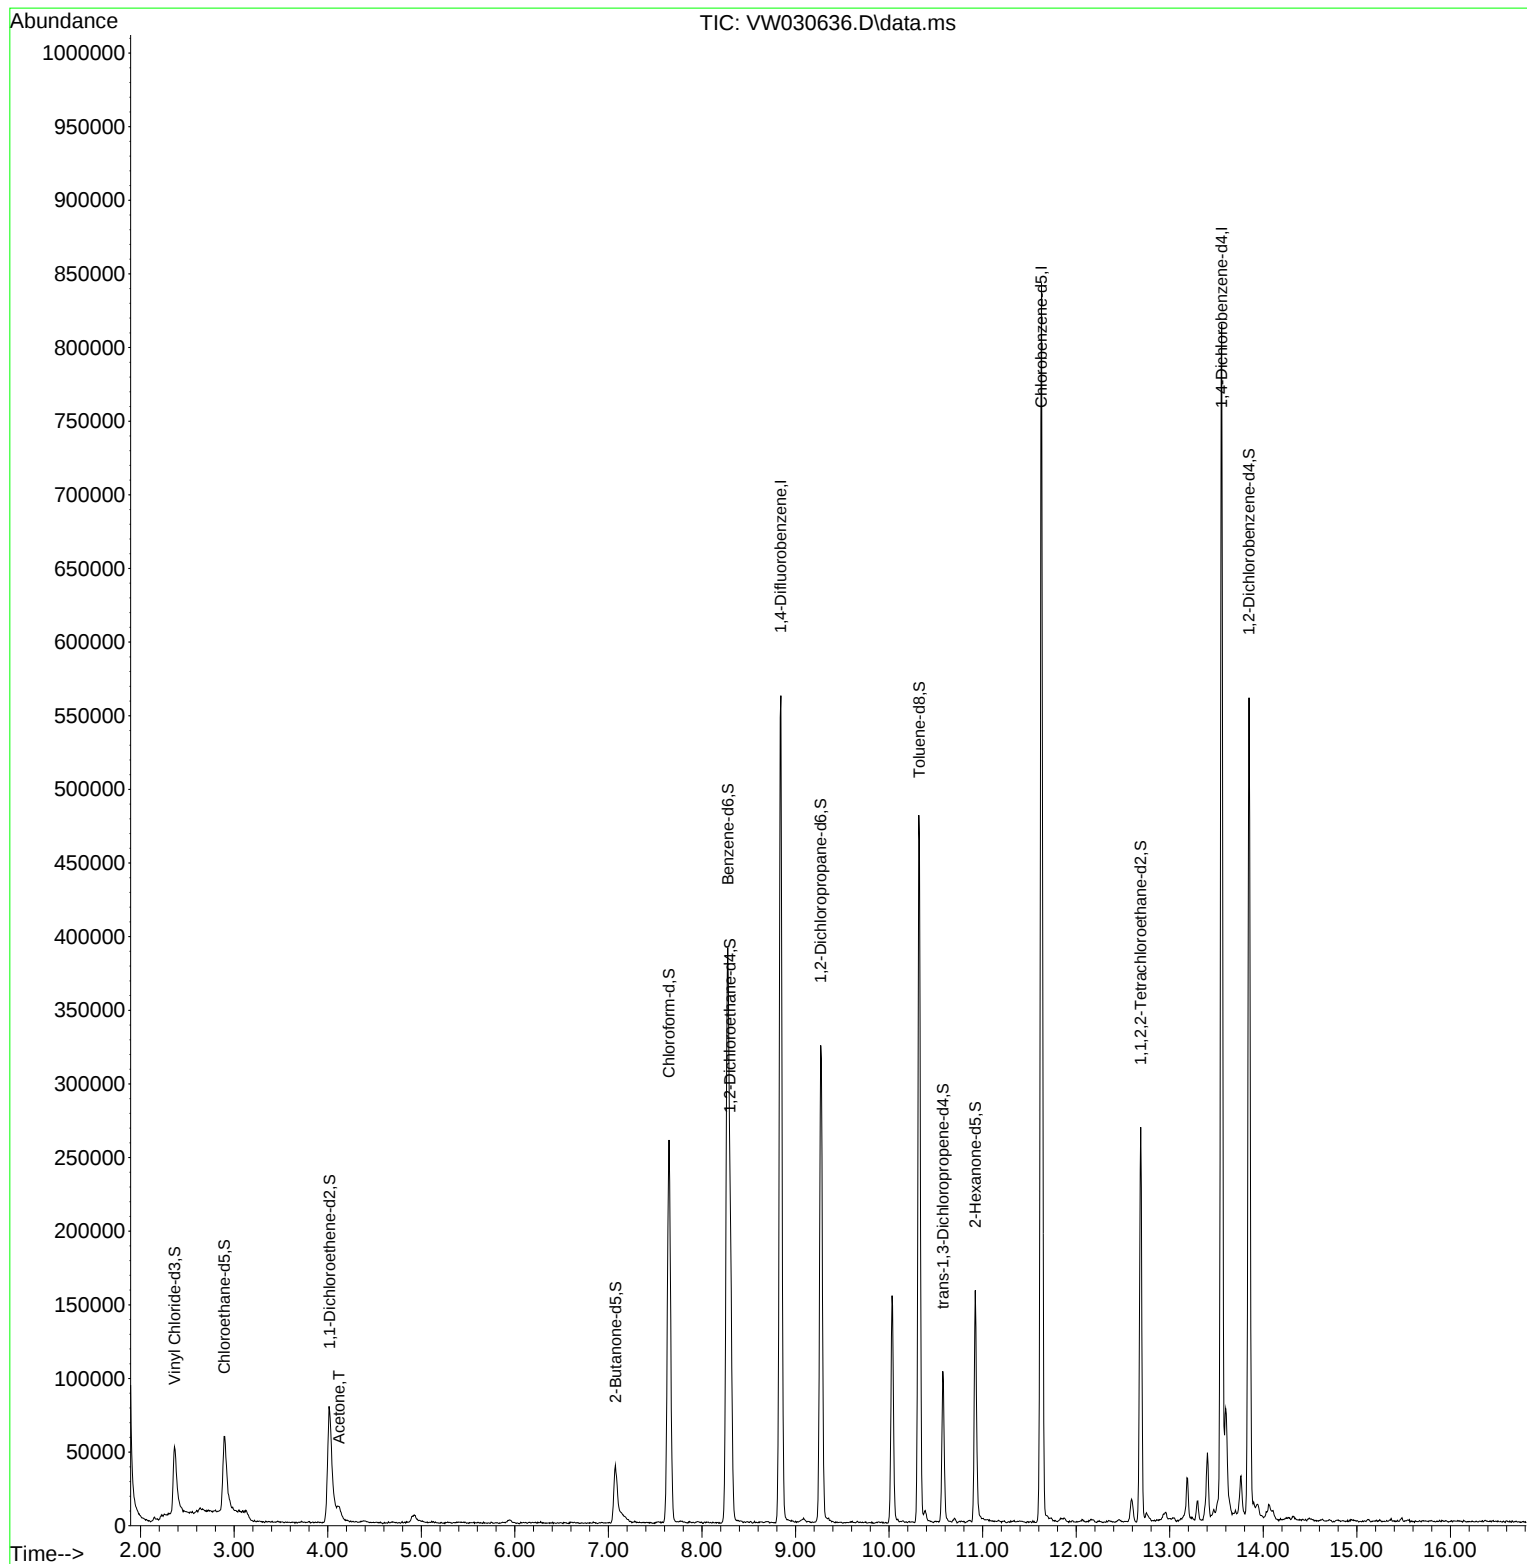

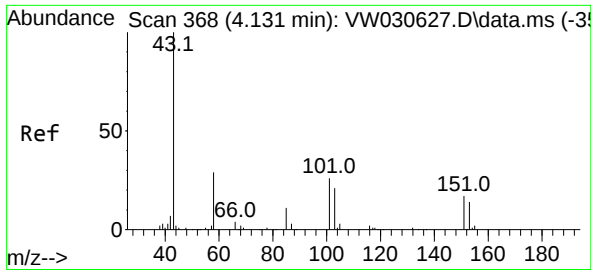

#13
 Acetone
 Concen: 6.381 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW030636.D
 Acq: 17 Oct 2024 14:08

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F91

Tgt Ion: 43 Resp: 11841
 Ion Ratio Lower Upper
 43 100
 58 33.8 0.0 57.6

