

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
 Data File : VW030637.D
 Acq On : 17 Oct 2024 14:32
 Operator : SY/MD
 Sample : P4414-05
 Misc : 4.71g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F77

Quant Time: Oct 18 01:41:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 18 01:38:16 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	391674	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	343548	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	120302	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	73383	11.920	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	47.680%
7) Chloroethane-d5	2.899	69	80365	17.245	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.960%
11) 1,1-Dichloroethene-d2	4.015	65	27835	10.870	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.480%#
21) 2-Butanone-d5	7.075	46	46242	41.737	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.480%
24) Chloroform-d	7.648	84	227263	20.289	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.160%
26) 1,2-Dichloroethane-d4	8.307	65	119497	20.516	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	82.080%
32) Benzene-d6	8.276	84	345039	17.304	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	69.200%
36) 1,2-Dichloropropane-d6	9.270	67	127339	21.758	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.040%
41) Toluene-d8	10.318	98	261552	14.369	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	57.480%
43) trans-1,3-Dichloroprop...	10.575	79	41339	16.869	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.480%
47) 2-Hexanone-d5	10.922	63	33851	44.908	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.820%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	96484	22.449	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.800%
66) 1,2-Dichlorobenzene-d4	13.848	152	80531	19.784	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.120%
Target Compounds						
13) Acetone	4.118	43	14652	9.033	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
Data File : VW030637.D
Acq On : 17 Oct 2024 14:32
Operator : SY/MD
Sample : P4414-05
Misc : 4.71g/10mL/MSVOA_W/SOIL/B
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4F77

Quant Time: Oct 18 01:41:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 18 01:38:16 2024
Response via : Initial Calibration

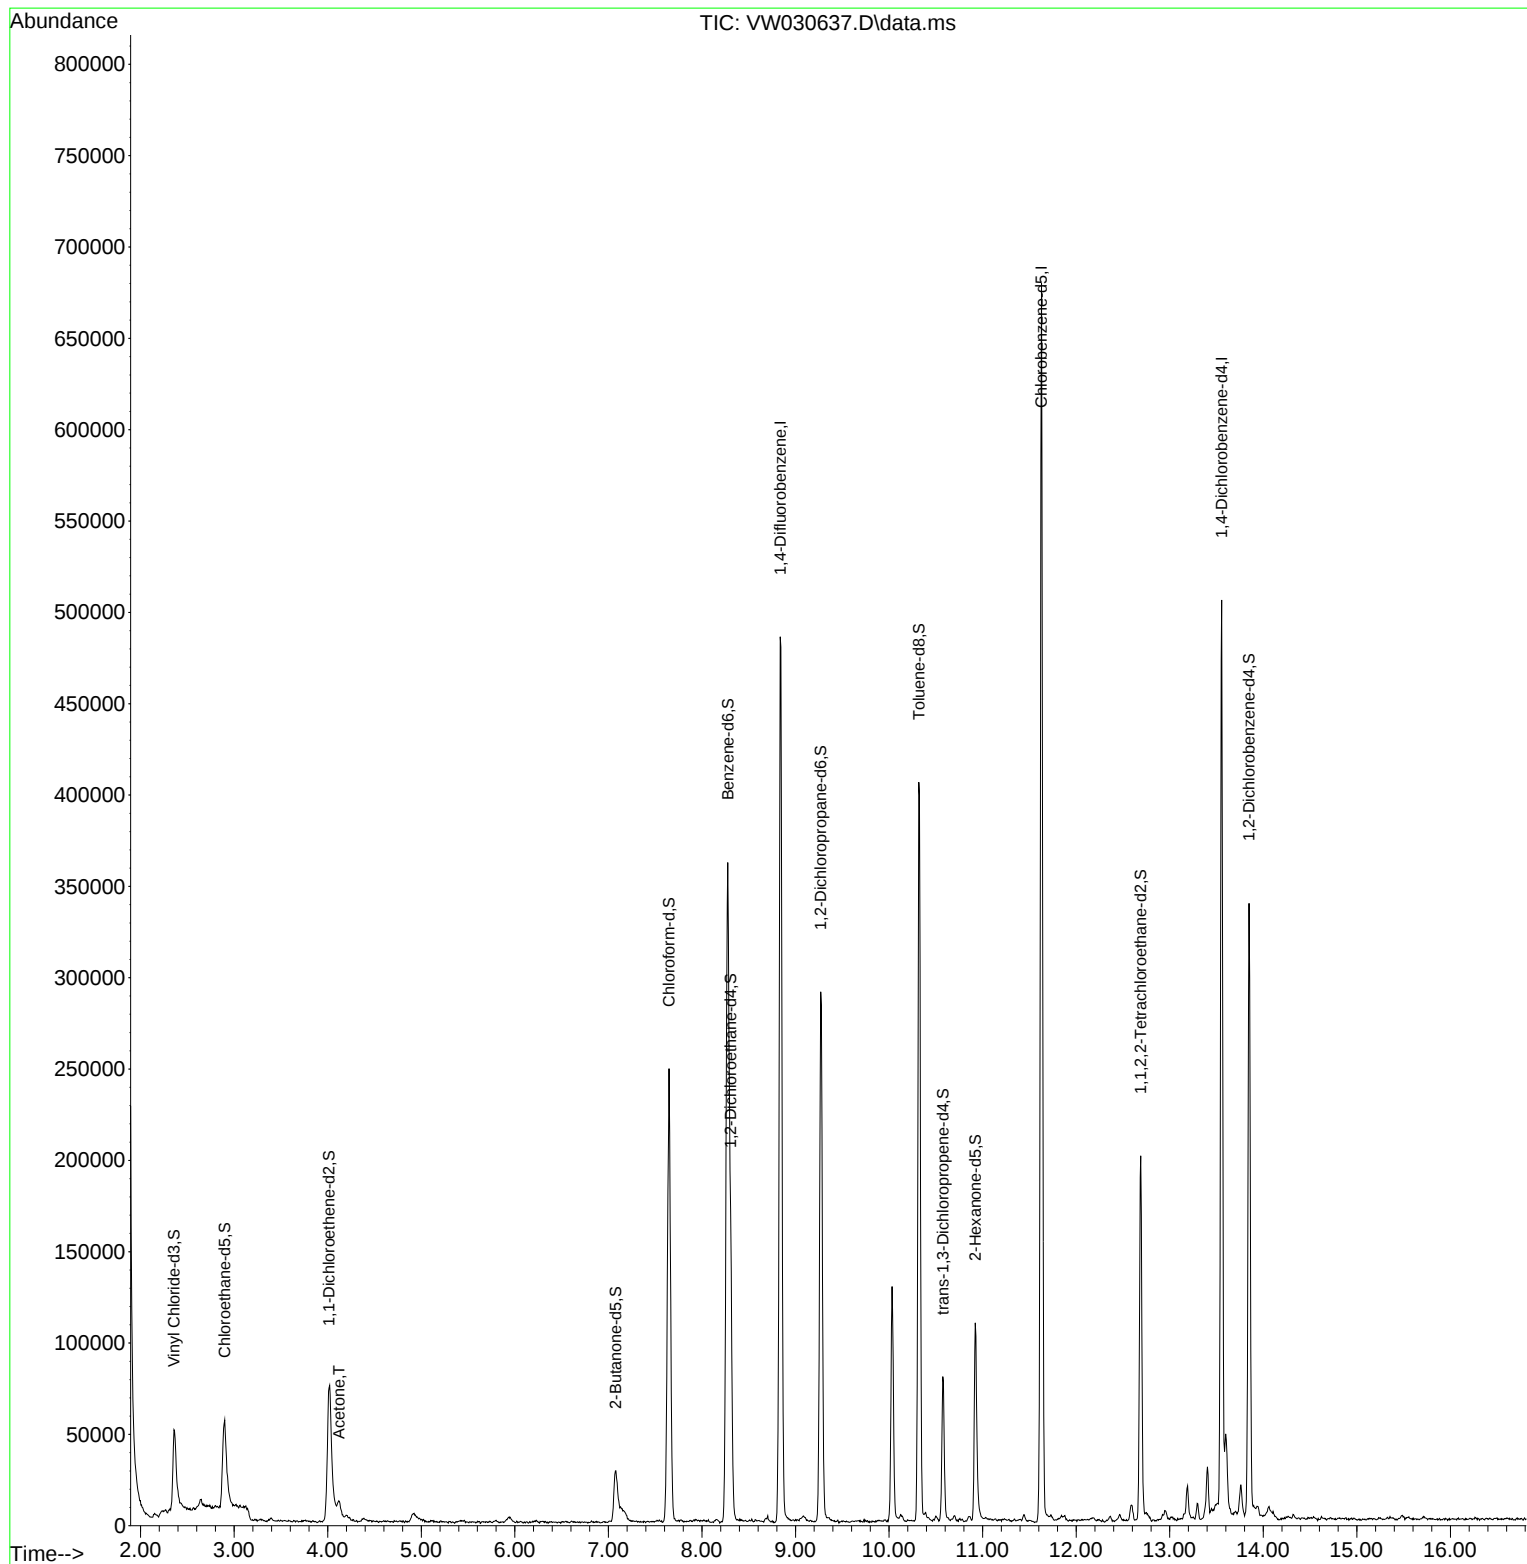

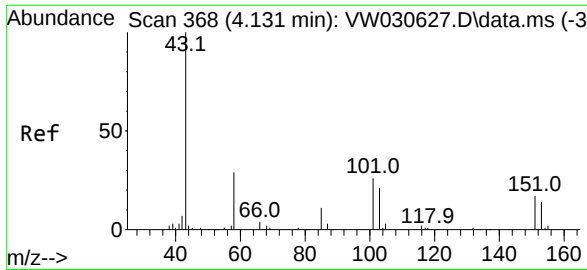

#13
 Acetone
 Concen: 9.033 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. -0.012 min
 Lab File: VW030637.D
 Acq: 17 Oct 2024 14:32

Instrument :
 MSVOA_W
 ClientSampleId :
 A4F77

Tgt Ion: 43 Resp: 14652
 Ion Ratio Lower Upper
 43 100
 58 30.9 0.0 57.6

