
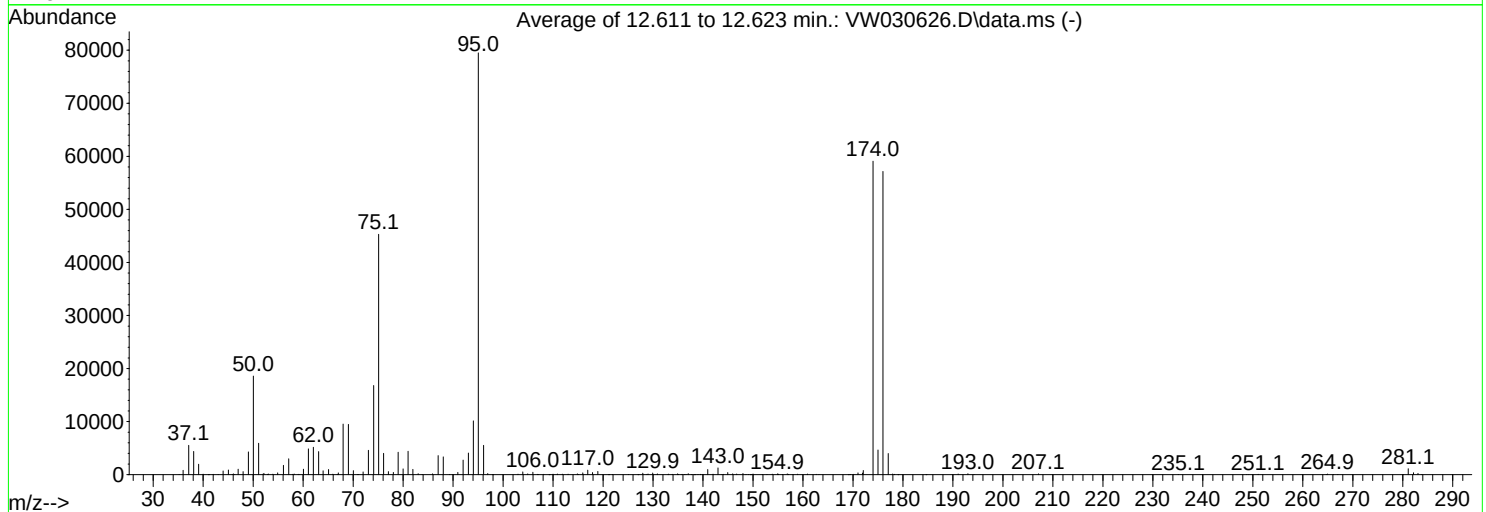


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101724\
Data File : VW030626.D
Acq On : 17 Oct 2024 08:56
Operator : SY/MD
Sample : BFB578
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB578

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Title : SFAM01.0
Last Update : Fri Oct 18 01:38:16 2024

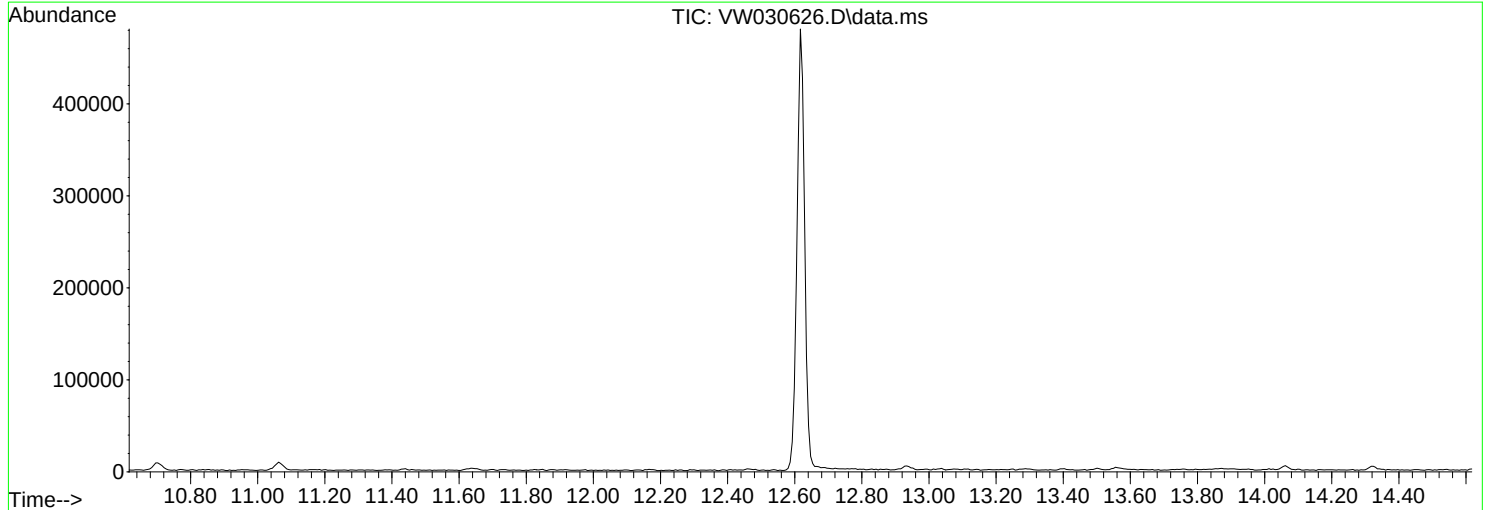

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	18592	PASS
75	95	30	80	57.0	45309	PASS
95	95	100	100	100.0	79507	PASS
96	95	5	9	7.0	5529	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.3	59091	PASS
175	174	5	9	7.9	4658	PASS
176	174	95	101	96.7	57160	PASS
177	176	5	9	6.9	3972	PASS

m/z	Abundance
35.90	56.0
36.20	65.0
36.80	65.0
38.30	100.0
40.00	225.0
41.10	76.0
41.60	52.0
42.60	103.0
43.00	89.0
44.00	225.0
45.30	75.0
47.90	76.0
50.20	53.0
54.90	73.0
58.70	50.0
65.90	71.0
68.00	50.0

Instrument :
MSVOA_W
ClientSampleId :
BFB578

m/z	Abundance
36.00	770.0
37.10	5331.0
38.10	4504.0
39.20	2135.0
40.00	345.0
41.10	96.0
42.00	53.0
42.60	77.0
43.20	95.0
44.00	943.0
45.00	692.0
46.10	209.0
47.00	995.0
48.00	607.0
49.10	3959.0
50.00	18120.0
51.10	5413.0
52.00	376.0
52.90	193.0
54.00	83.0
54.90	373.0
56.00	1535.0
57.10	2796.0
58.30	179.0
59.10	112.0
60.00	855.0
61.10	4682.0
62.00	4824.0
63.10	4211.0
64.00	814.0
65.10	1022.0
66.00	187.0
66.80	236.0
67.10	254.0
68.10	8621.0
69.00	8347.0
70.10	669.0
70.90	102.0
71.90	414.0
73.00	3979.0
74.10	14858.0
75.10	40640.0
76.10	3811.0
77.10	563.0
78.00	354.0
79.00	4147.0
80.00	969.0
81.00	3900.0
82.00	989.0
83.00	124.0
85.90	114.0
87.00	2618.0
88.10	2714.0
89.30	57.0
90.00	55.0
91.00	459.0
92.00	2542.0
93.10	3296.0
94.10	8444.0
95.00	69968.0
96.10	5031.0
96.90	116.0
97.90	58.0
103.00	124.0
104.00	425.0
105.00	148.0
106.00	474.0
106.90	60.0
108.20	102.0
110.00	180.0
110.90	128.0
111.90	82.0
113.00	101.0
114.90	128.0
116.00	349.0
116.90	721.0
117.80	269.0
119.00	671.0
125.10	93.0
127.00	58.0
128.00	226.0
128.80	199.0
129.90	217.0
130.80	120.0
133.00	182.0
133.80	93.0
134.90	208.0
136.60	111.0
137.10	148.0
138.30	55.0
140.90	872.0
143.00	1231.0

Instrument :
MSVOA_W
ClientSampleId :
BFB578

144.20	130.0
144.90	408.0
146.00	139.0
146.80	108.0
147.90	232.0
149.50	54.0
151.80	77.0
153.80	101.0
154.90	246.0
156.80	259.0
159.00	120.0
161.00	132.0
162.70	93.0
163.20	62.0
170.10	74.0
171.00	381.0
171.90	910.0
174.00	38944.0
175.00	3755.0
176.00	41272.0
177.10	3078.0
177.90	98.0
179.00	51.0
191.10	256.0
193.10	235.0
194.20	109.0
207.10	231.0
235.10	87.0
248.80	76.0
249.20	109.0
251.10	94.0
265.00	239.0
266.10	118.0
267.00	60.0
280.10	94.0
281.10	1836.0
282.10	624.0
283.00	381.0
283.80	65.0

Instrument :
MSVOA_W
ClientSampleId :
BFB578

m/z	Abundance
36.00	911.0
37.10	5932.0
38.10	4782.0
39.10	2043.0
40.10	307.0
41.10	90.0
42.00	74.0
43.00	204.0
44.10	935.0
45.10	976.0
46.00	231.0
46.90	1050.0
48.10	761.0
49.10	4867.0
50.10	20576.0
51.10	6451.0
52.20	384.0
53.10	200.0
54.00	124.0
55.00	497.0
56.00	2047.0
57.10	3326.0
58.10	163.0
58.90	88.0
60.10	1346.0
61.00	5184.0
62.10	5674.0
63.10	4892.0
64.00	692.0
65.10	1048.0
66.00	204.0
67.00	404.0
68.00	11145.0
69.10	10580.0
70.10	962.0
72.00	676.0
73.10	5495.0
74.10	18928.0
75.10	51328.0
76.10	4377.0
77.10	515.0
78.10	521.0
79.00	4703.0
80.00	1428.0
81.00	5404.0
81.90	1059.0
83.00	182.0
83.80	82.0
85.90	121.0
87.00	4179.0
88.00	3715.0
89.30	79.0
90.00	62.0
91.00	447.0
92.00	2752.0
93.00	4714.0
94.00	11857.0
95.10	90112.0
96.10	6579.0
96.90	208.0
102.90	66.0
104.00	593.0
104.80	131.0
105.90	434.0
106.90	122.0
108.10	91.0
110.00	67.0
110.90	138.0
111.90	98.0
113.00	96.0
114.90	221.0
116.00	394.0
117.00	1007.0
117.90	495.0
119.00	568.0
121.90	62.0
127.90	335.0
129.00	220.0
130.00	424.0
130.90	170.0
133.20	173.0
133.90	50.0
134.90	265.0
135.90	75.0
137.00	193.0
137.70	55.0
139.00	69.0
139.50	62.0
140.00	78.0
140.90	1118.0
142.00	85.0
143.00	1316.0

Instrument :
MSVOA_W
ClientSampleId :
BFB578

144.00	98.0
145.00	388.0
145.90	168.0
146.70	169.0
148.00	147.0
148.60	112.0
150.00	178.0
151.90	58.0
153.90	78.0
154.90	212.0
155.90	71.0
156.90	195.0
158.00	75.0
159.00	83.0
160.90	104.0
162.60	79.0
169.10	55.0
170.20	123.0
171.00	365.0
172.10	1257.0
174.00	72272.0
175.00	5264.0
176.00	64880.0
177.00	4489.0
177.90	104.0
178.30	145.0
184.60	55.0
190.90	95.0
192.90	181.0
207.10	151.0
251.00	79.0
264.80	119.0
281.10	1115.0
282.20	354.0
283.10	176.0

Instrument :
MSVOA_W
ClientSampleId :
BFB578

m/z	Abundance
35.20	60.0
36.00	1129.0
37.10	5301.0
38.10	4168.0
39.00	1748.0
40.10	284.0
40.90	80.0
42.00	104.0
43.00	91.0
44.10	918.0
45.00	967.0
45.80	106.0
46.30	139.0
47.10	1036.0
48.10	597.0
49.00	4068.0
50.10	17240.0
51.10	5874.0
52.10	331.0
53.00	128.0
53.90	115.0
54.90	366.0
56.10	1697.0
57.10	2854.0
57.90	189.0
59.20	91.0
60.00	928.0
61.00	4670.0
62.10	4948.0
63.10	3946.0
64.00	635.0
65.10	832.0
66.00	107.0
67.00	314.0
68.10	8975.0
69.10	9472.0
70.00	632.0
71.10	98.0
72.10	494.0
73.10	4336.0
74.10	16592.0
75.10	43960.0
76.10	3845.0
77.00	650.0
78.00	438.0
79.00	3788.0
80.00	901.0
81.00	3902.0
82.00	948.0
83.00	223.0
85.90	210.0
87.00	4009.0
88.00	3638.0
90.90	374.0
92.00	2974.0
93.10	4201.0
94.10	10079.0
95.10	78440.0
96.10	4976.0
97.00	326.0
103.10	92.0
103.90	490.0
105.00	220.0
106.00	439.0
107.10	105.0
109.20	56.0
110.00	63.0
110.80	145.0
111.80	130.0
113.00	85.0
114.80	120.0
115.10	120.0
115.90	267.0
117.00	779.0
118.00	389.0
118.90	565.0
121.10	55.0
127.90	283.0
129.00	188.0
129.90	233.0
130.90	139.0
133.10	116.0
135.10	211.0
135.70	78.0
136.30	88.0
137.10	190.0
137.80	55.0
139.50	119.0
140.00	95.0
141.00	932.0
142.00	164.0
143.00	1292.0

Instrument :
MSVOA_W
ClientSampleId :
BFB578

143.80	112.0
145.00	408.0
146.00	163.0
146.70	115.0
148.10	263.0
149.10	76.0
150.00	209.0
152.80	60.0
153.90	68.0
155.10	251.0
157.10	152.0
158.90	114.0
160.80	125.0
169.50	74.0
171.10	213.0
172.00	1108.0
174.00	66056.0
175.00	4954.0
176.00	65328.0
177.00	4348.0
178.00	137.0
190.90	65.0
193.10	98.0
207.10	84.0
264.70	95.0
281.20	418.0
282.30	137.0
283.10	218.0

Instrument :
MSVOA_W
ClientSampleId :
BFB578