

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101818\
 Data File : VW006175.D
 Acq On : 18 Oct 2018 15:01
 Operator : VA/AP
 Sample : J5575-03
 Misc : 5.53G/5ML/MSVOA W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SSSI-1015-S-DH-27

Quant Time: Oct 19 06:01:50 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 18 17:01:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.95
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.85
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.63
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.57

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101818\
Data File : VW006175.D
Acq On : 18 Oct 2018 15:01
Operator : VA/AP
Sample : J5575-03
Misc : 5.53G/5ML/MSVOA W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SSSI-1015-S-DH-27

Quant Time: Oct 19 06:01:50 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 18 17:01:24 2018
Response via : Initial Calibration

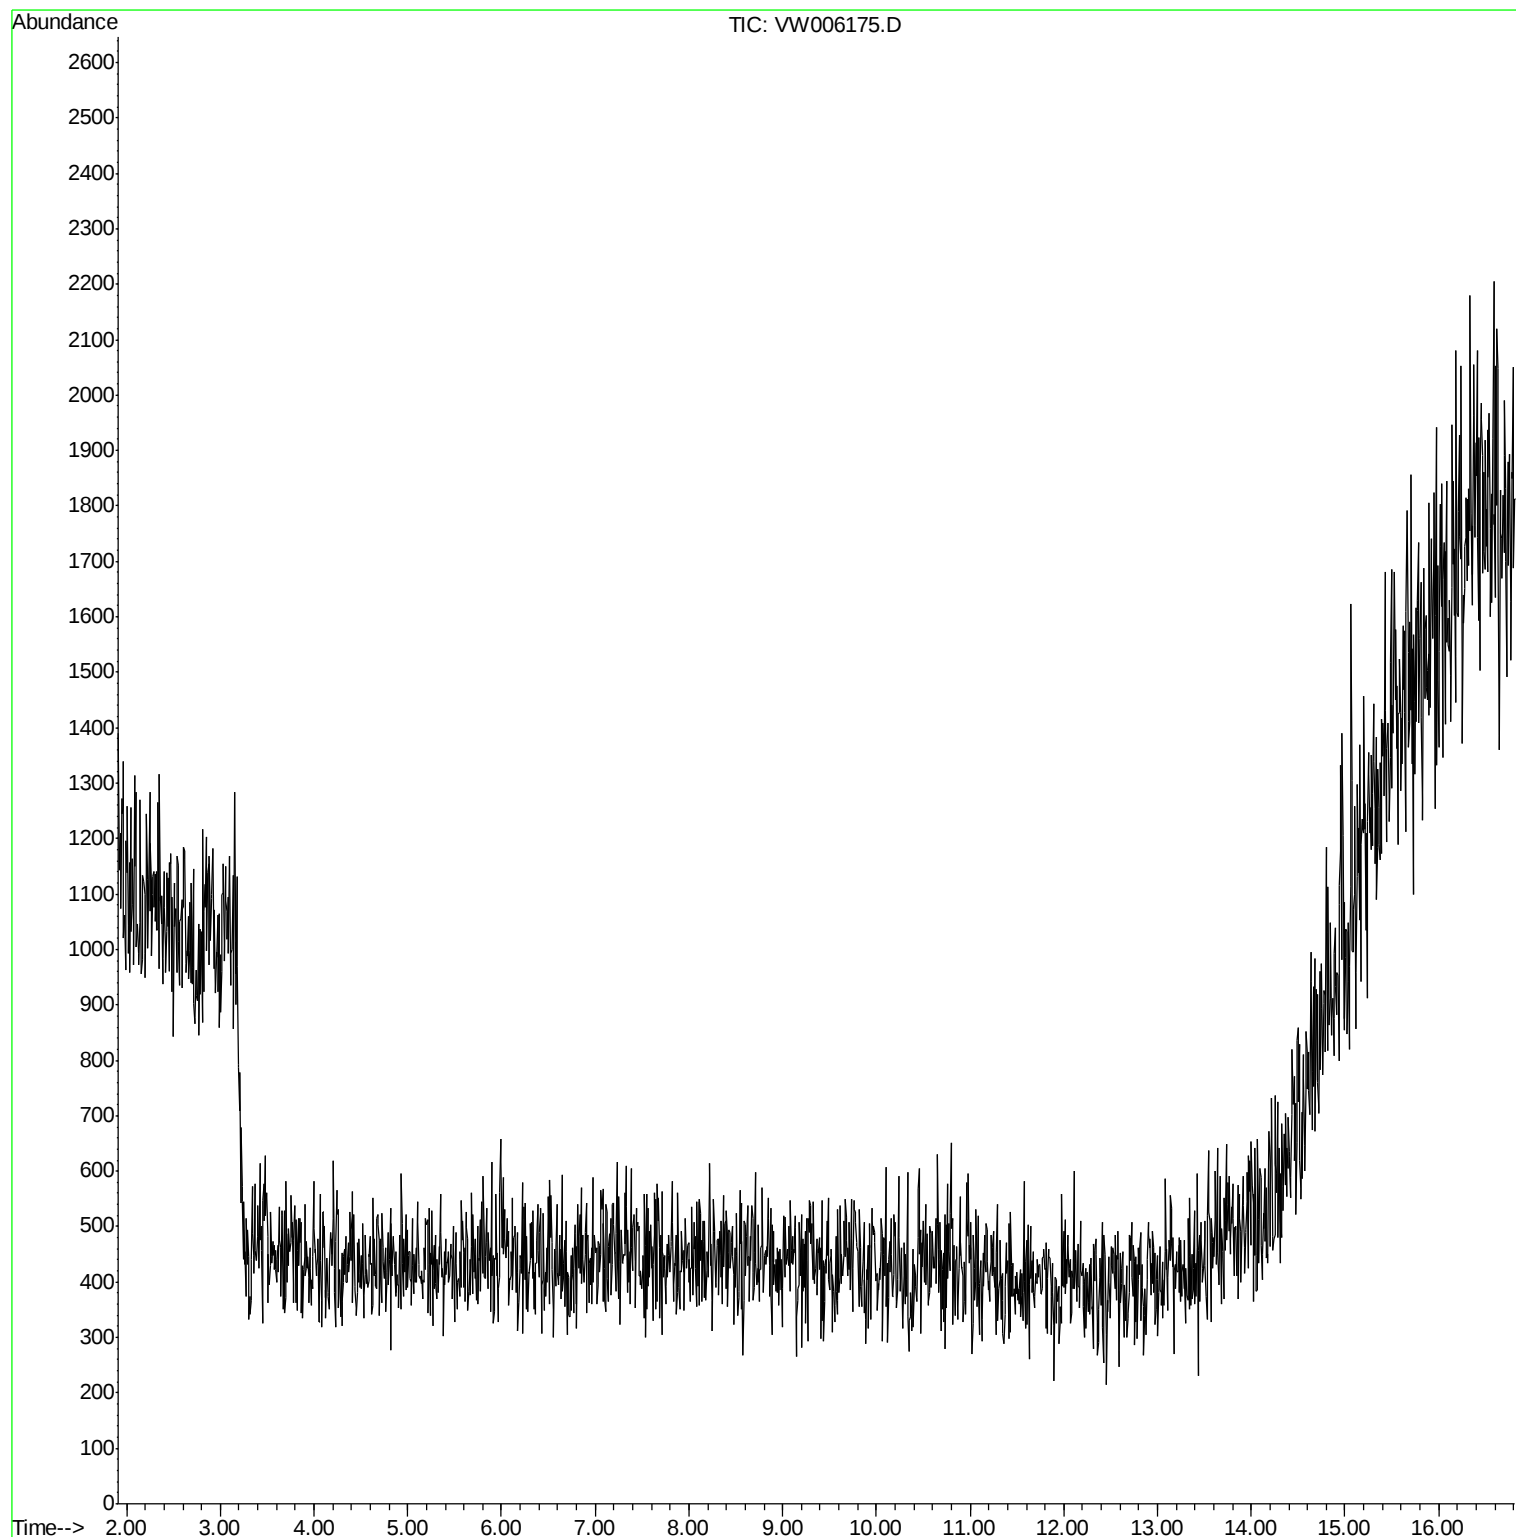

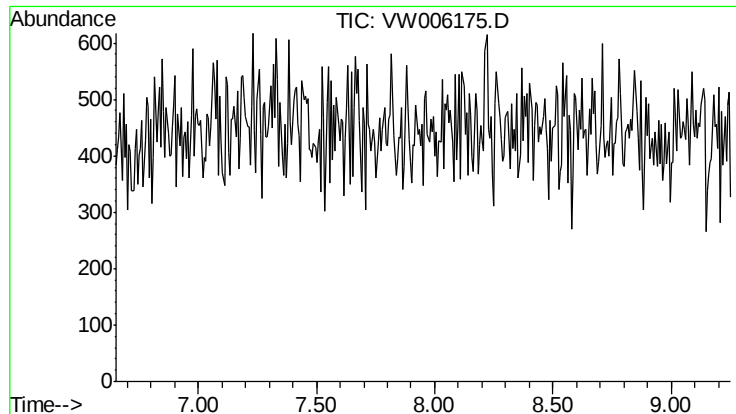

#1

Pentafluorobenzene

Concen: 0.000 ug/l

Expected RT: 7.95 min

Lab File: VW006175.D

Acq: 18 Oct 2018 15:01

Tot Ion: 168


Sig	Exp Ratio
168	100
99	49.9

Instrument :

MSVOA_W

ClientSampleId :

SSSI-1015-S-DH-27

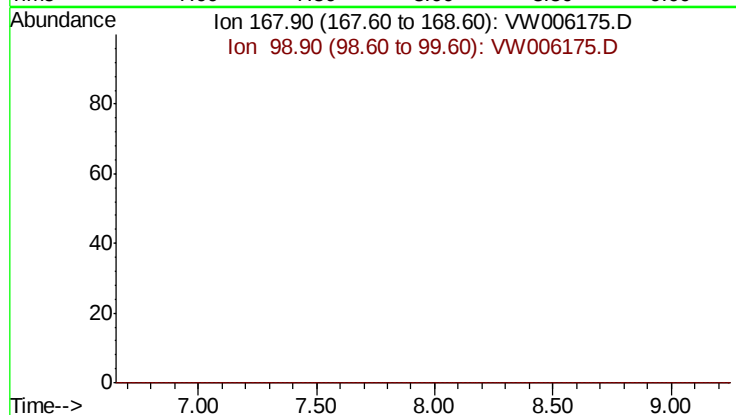

#33

1,2-Dichloroethane-d4

Concen: 0.000 ug/l



Expected RT: 8.31 min


Lab File: VW006175.D

Acq: 18 Oct 2018 15:01

Tgt Ion: 65

Sig	Exp Ratio
65	100
67	50.5

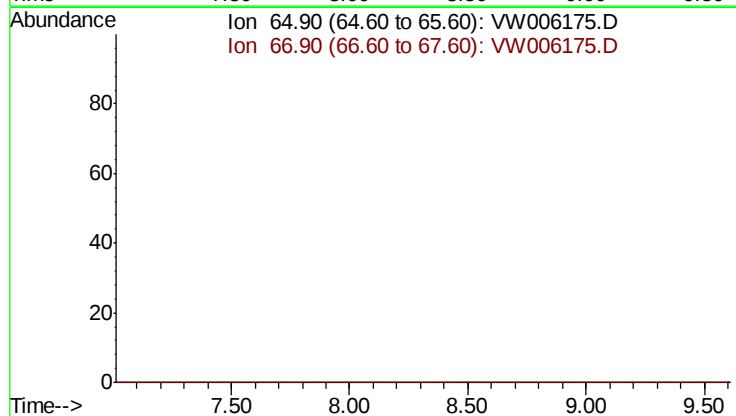
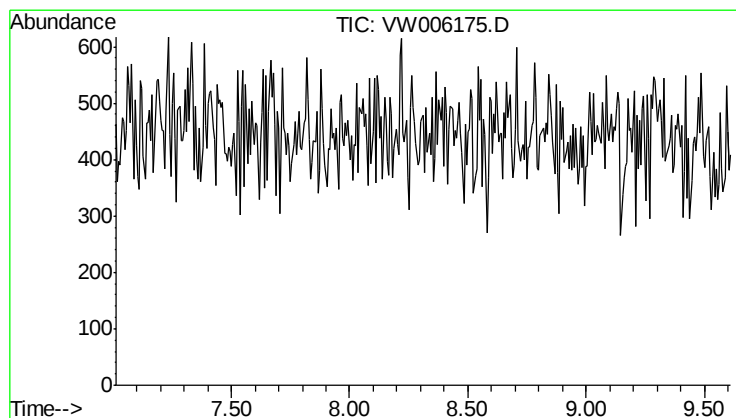


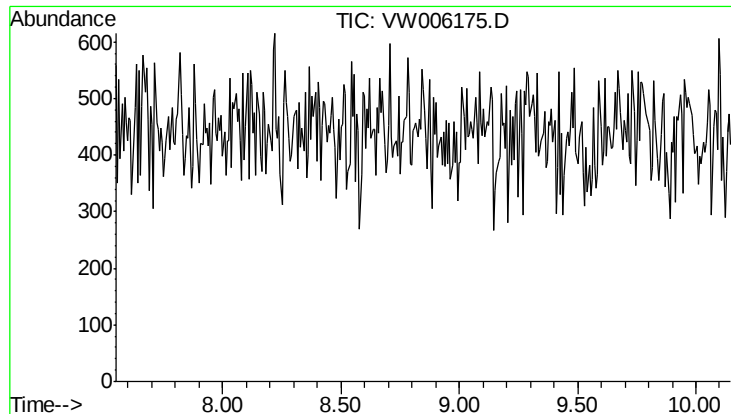

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.85 min
 Lab File: VW006175.D
 Acq: 18 Oct 2018 15:01


Instrument :
 MSVOA_W
 ClientSampleId :
 SSSI-1015-S-DH-27


Tot Ion	114
Sig	Exp Ratio
114	100
63	18.4
88	14.5

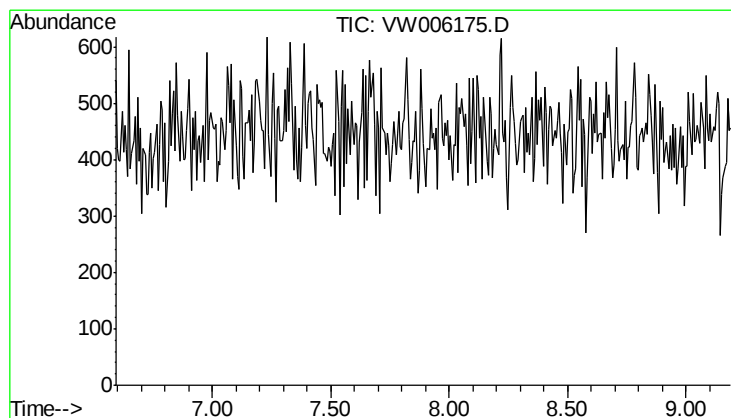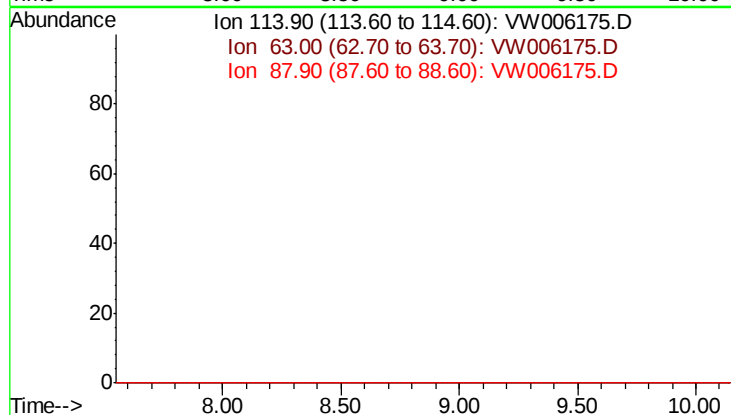

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.89 min
 Lab File: VW006175.D
 Acq: 18 Oct 2018 15:01

Tgt Ion	113
Sig	Exp Ratio
113	100
111	101.7
192	23.4

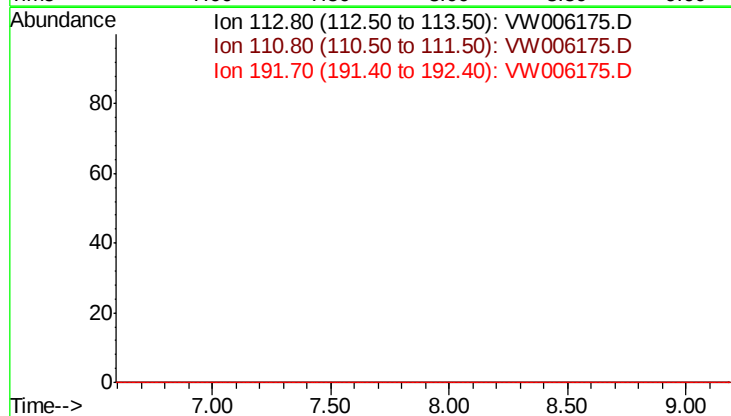


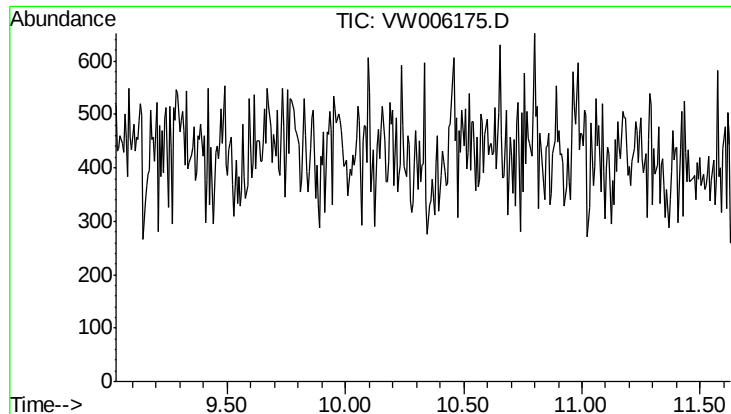


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.33 min

Lab File: VW006175.D
Acq: 18 Oct 2018 15:01

Instrument :
MSVOA_W
ClientSampleId :
SSSI-1015-S-DH-27


Tot Ion	98
Sig	Exp Ratio
98	100
100	64.5

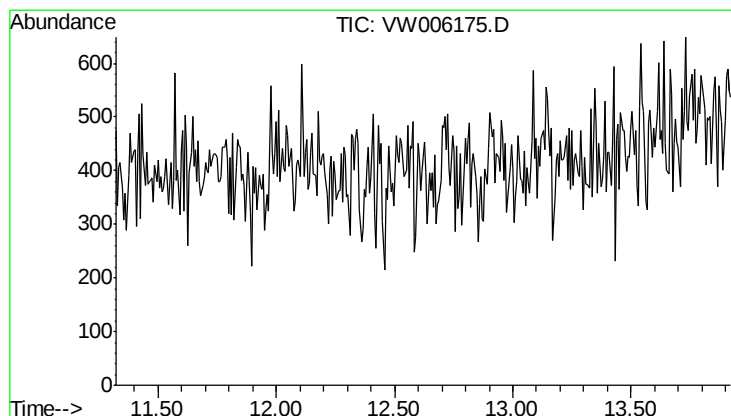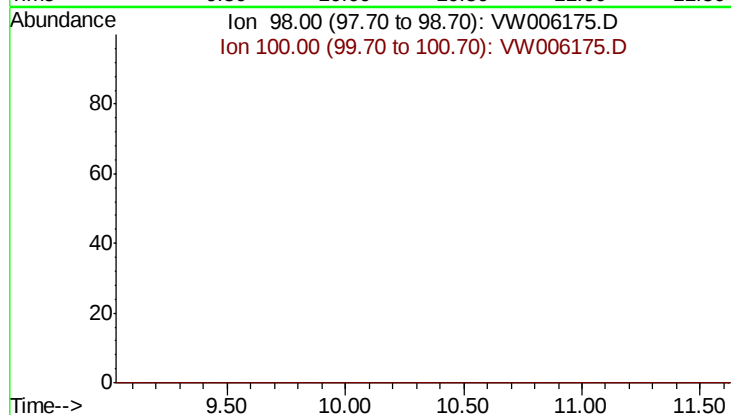


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.62 min

Lab File: VW006175.D
Acq: 18 Oct 2018 15:01

Tgt Ion	95
Sig	Exp Ratio
95	100
174	93.0
176	90.8

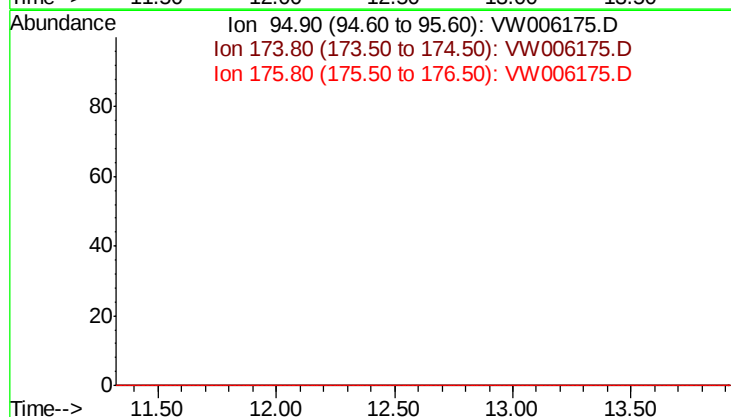


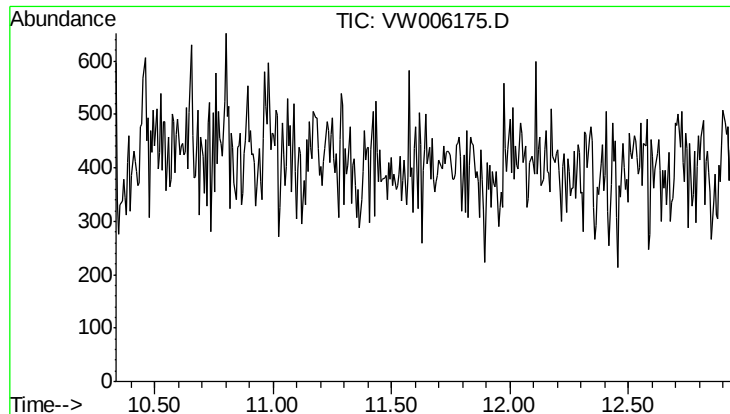


#63
Chlorobenzene-d5
Concen: 0.000 ug/l
Expected RT: 11.63 min

Lab File: VW006175.D
Acq: 18 Oct 2018 15:01

Instrument :
MSVOA_W
ClientSampleId :
SSSI-1015-S-DH-27

Tot Ion	117
Sig	Exp Ratio
117	100
82	52.6
119	32.2

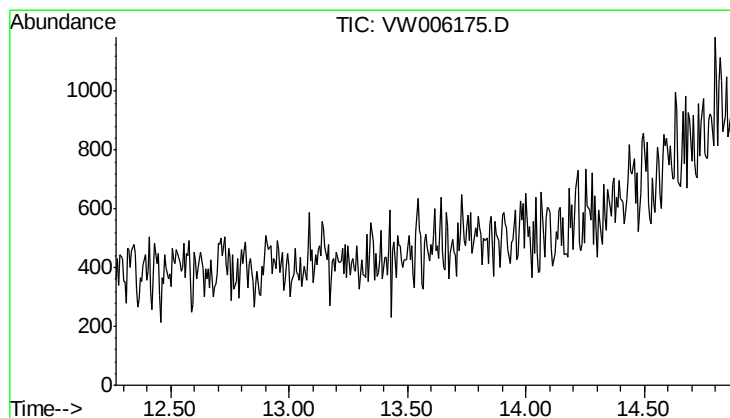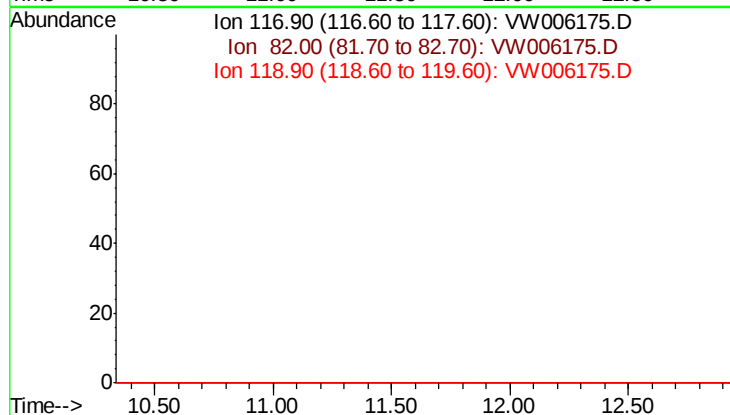

#72
1,4-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 13.57 min

Lab File: VW006175.D
Acq: 18 Oct 2018 15:01

Tgt Ion	152
Sig	Exp Ratio
152	100
115	55.5
150	174.6

