

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101818\
 Data File : VW006210.D
 Acq On : 19 Oct 2018 08:13
 Operator : VA/AP
 Sample : J5195-03
 Misc : 4.87G/5ML/MSVOA W/SOIL
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 JC-02-101818-A

Quant Time: Oct 19 08:35:39 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 18 17:01:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	115418	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	163982	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	96941	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	22885	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	54930	57.41	ug/l	0.00
Spiked Amount			Recovery	=	114.82%	
35) Dibromofluoromethane	7.89	113	53516	55.23	ug/l	0.00
Spiked Amount			Recovery	=	110.46%	
50) Toluene-d8	10.33	98	123457	33.49	ug/l	0.00
Spiked Amount			Recovery	=	66.98%	
62) 4-Bromofluorobenzene	12.62	95	31985	23.10	ug/l	0.00
Spiked Amount			Recovery	=	46.20%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	5.24	59	142	2.207	ug/l #	71
16) Acetone	4.15	43	19792	101.455	ug/l	91
18) Methyl Acetate	4.68	43	1593	3.308	ug/l	93
20) Methylene Chloride	4.92	84	6899	5.361	ug/l	88
25) 2-Butanone	7.16	43	647	2.503	ug/l #	46
29) Tetrahydrofuran	7.56	42	214	1.347	ug/l #	47
31) Cyclohexane	7.95	56	2324	1.327	ug/l #	18
36) 1,1-Dichloropropene	7.95	75	7553	4.997	ug/l #	48
37) Ethyl Acetate	7.16	43	647	1.152	ug/l #	1
38) Carbon Tetrachloride	7.95	117	10371	6.259	ug/l #	18
39) Methylcyclohexane	9.34	83	4644	2.311	ug/l	91
55) 1,1,2-Trichloroethane	10.77	97	3608	4.560	ug/l #	19
56) Ethyl methacrylate	10.66	69	1385	1.428	ug/l #	1
73) Isopropylbenzene	12.47	105	7561	4.677	ug/l	99
74) N-amyl acetate	12.26	43	973	3.099	ug/l #	65
75) 1,1,2,2-Tetrachloroethane	12.69	83	533	2.168	ug/l #	26
76) 1,2,3-Trichloropropane	12.62	75	15834	90.585	ug/l #	100
78) n-propylbenzene	12.81	91	6559	3.487	ug/l	93
80) 1,3,5-Trimethylbenzene	12.95	105	1777	1.304	ug/l	96
81) trans-1,4-Dichloro-2-buten	12.62	75	15834	216.535	ug/l #	11
83) tert-Butylbenzene	13.21	119	1613	1.323	ug/l	73
84) 1,2,4-Trimethylbenzene	13.26	105	2580	1.871	ug/l	90
85) sec-Butylbenzene	13.39	105	5165	2.998	ug/l #	70
89) n-Butylbenzene	13.83	91	1977	1.387	ug/l #	64
90) Hexachloroethane	14.10	117	1444	5.471	ug/l #	4
95) Naphthalene	15.38	128	1540	1.711	ug/l #	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101818\
Data File : VW006210.D
Acq On : 19 Oct 2018 08:13
Operator : VA/AP
Sample : J5195-03
Misc : 4.87G/5ML/MSVOA W/SOIL
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
JC-02-101818-A

Quant Time: Oct 19 08:35:39 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 18 17:01:24 2018
Response via : Initial Calibration

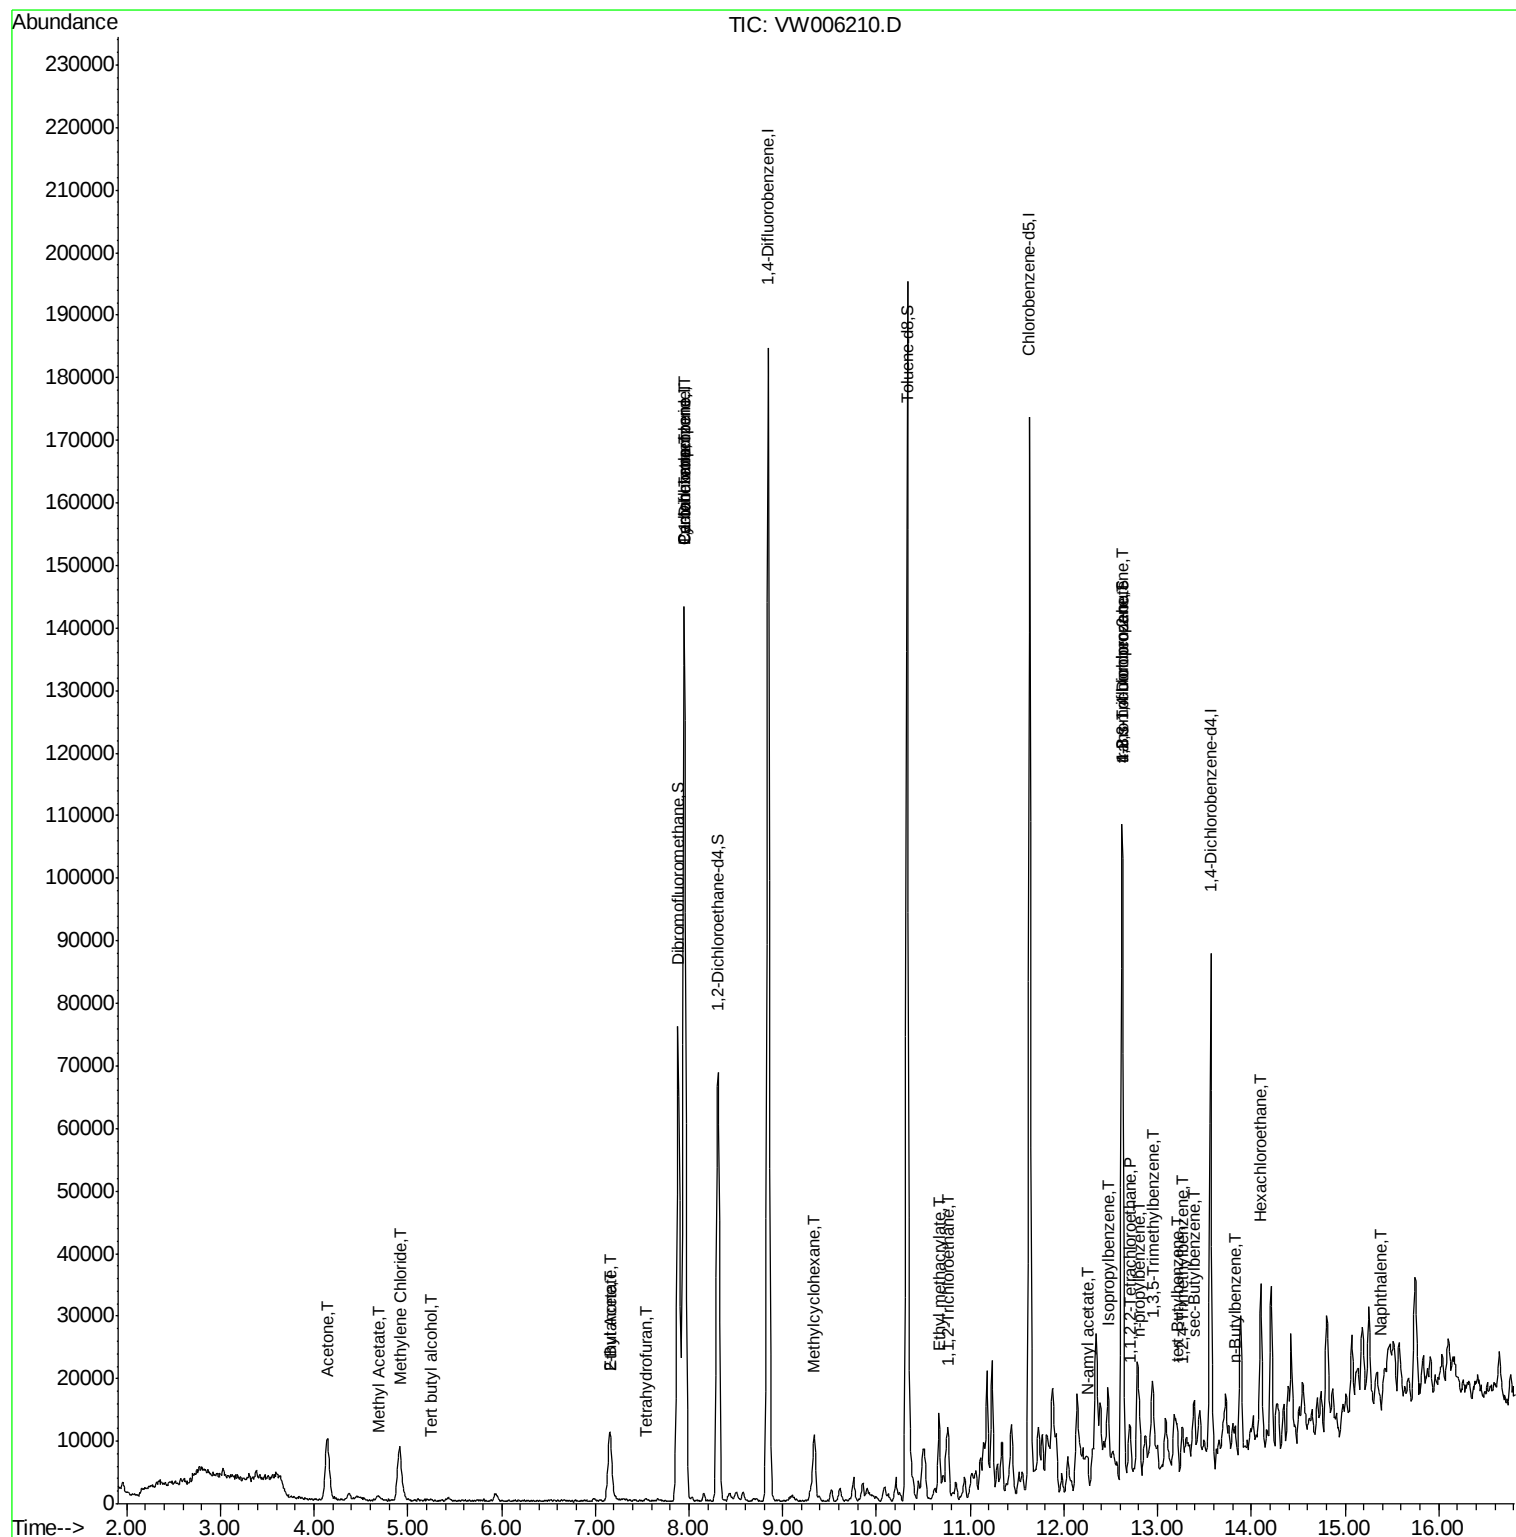

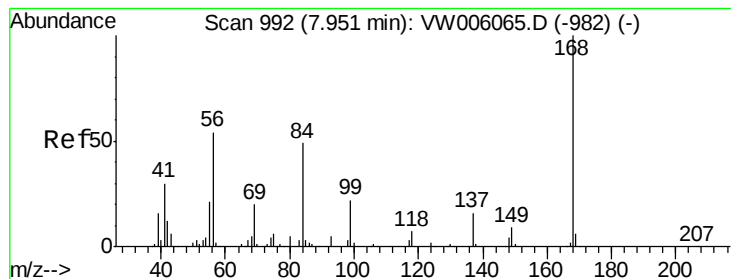

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.00 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :


JC-02-101818-A

Tot Ion:168 Resp: 115418

Ion Ratio Lower Upper




168 100

99 49.8 39.9 59.9



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

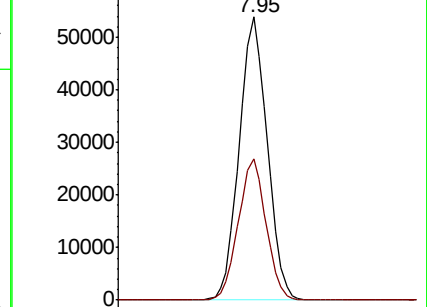

#11

Tert butyl alcohol

Concen: 2.207 ug/l

RT: 5.24 min Scan# 547

Delta R.T. 0.01 min

Lab File: VW006210.D


Acq: 19 Oct 2018 08:13

Tgt Ion: 59 Resp: 142

Ion Ratio Lower Upper



59 100


57 0.0 8.7 13.1#



Abundance Ion 59.00 (58.70 to 59.70): VW

Ion 57.00 (56.70 to 57.70): VW

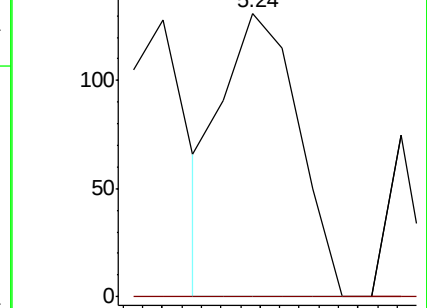



#16

Acetone

Concen: 101.455 ug/l

RT: 4.15 min Scan# 368

Delta R.T. 0.00 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :





JC-02-101818-A

Tot Ion: 43 Resp: 19792

Ion Ratio Lower Upper

43 100

58 25.0 24.0 36.0

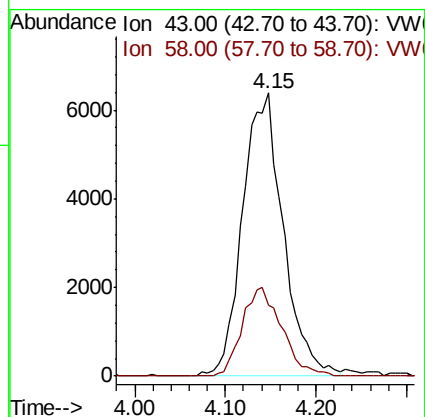

#18

Methyl Acetate

Concen: 3.308 ug/l

RT: 4.68 min Scan# 456

Delta R.T. -0.00 min

Lab File: VW006210.D




Acq: 19 Oct 2018 08:13


Tgt Ion: 43 Resp: 1593

Ion Ratio Lower Upper

43 100

74 22.0 20.5 30.7

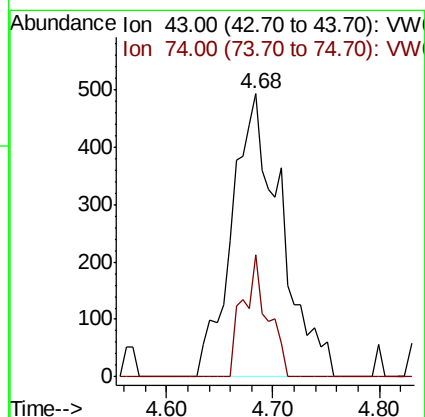



#20

Methylene Chloride

Concen: 5.361 ug/l

RT: 4.92 min Scan# 494

Delta R.T. 0.00 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :

JC-02-101818-A

Tot Ion: 84 Resp: 6899


Ion Ratio Lower Upper

84 100

49 97.2 93.6 140.4

51 40.8 29.0 43.4

86 67.8 52.6 79.0






Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

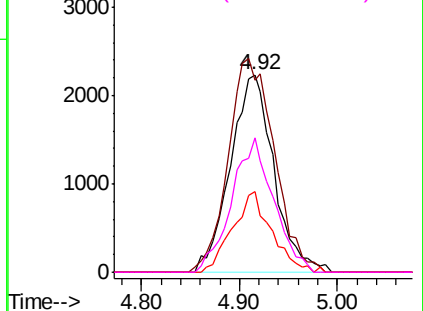

#25

2-Butanone

Concen: 2.503 ug/l

RT: 7.16 min Scan# 863

Delta R.T. -0.02 min

Lab File: VW006210.D


Acq: 19 Oct 2018 08:13

Tgt Ion: 43 Resp: 647

Ion Ratio Lower Upper



43 100


72 0.0 22.8 34.2#



Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 72.00 (71.70 to 72.70): VW

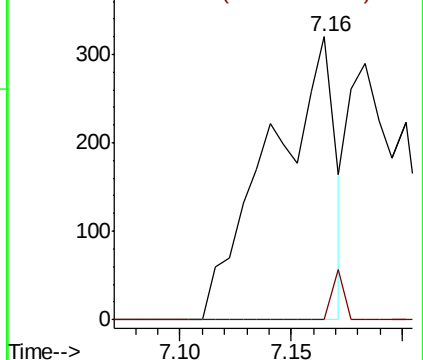



#29

Tetrahydrofuran

Concen: 1.347 ug/l

RT: 7.56 min Scan# 927

Delta R.T. 0.01 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :

JC-02-101818-A


Tot Ion: 42 Resp: 214

Ion Ratio Lower Upper

42 100

72 11.7 38.0 57.0#




71 9.8 35.3 52.9#



Abundance Ion 42.00 (41.70 to 42.70): VW

Ion 72.00 (71.70 to 72.70): VW

Ion 71.00 (70.70 to 71.70): VW

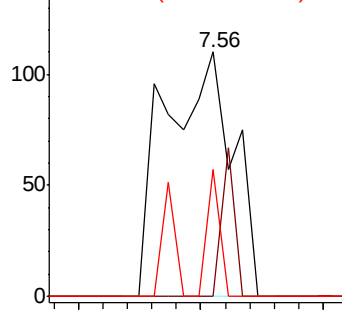

#31

Cyclohexane

Concen: 1.327 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.01 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13


Tgt Ion: 56 Resp: 2324

Ion Ratio Lower Upper

56 100

69 132.5 29.4 44.0#



84 140.6 74.0 111.0#




Abundance Ion 56.00 (55.70 to 56.70): VW

Ion 69.00 (68.70 to 69.70): VW

Ion 84.00 (83.70 to 84.70): VW

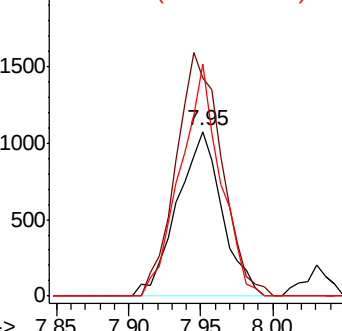



#33

1,2-Dichloroethane-d4

Concen: 57.405 ug/l

RT: 8.31 min Scan# 1051

Delta R.T. -0.00 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :





JC-02-101818-A

Tot Ion: 65 Resp: 54930

Ion Ratio Lower Upper

65 100

67 52.9 0.0 101.0

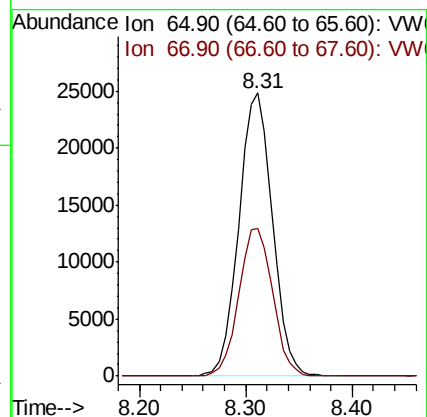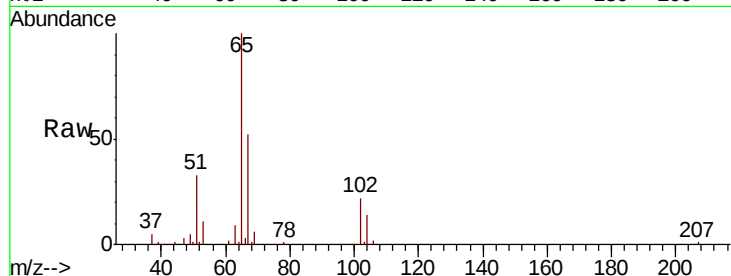

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.85 min Scan# 1139

Delta R.T. -0.00 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13




Tgt Ion: 114 Resp: 163982


Ion Ratio Lower Upper

114 100

63 18.2 0.0 36.8

88 15.2 0.0 29.0

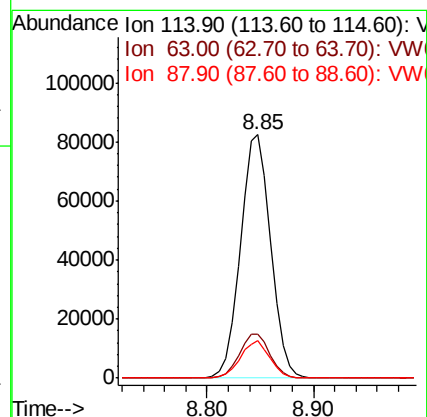



#35

Dibromofluoromethane

Concen: 55.230 ug/l

RT: 7.89 min Scan# 982

Delta R.T. -0.00 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :

JC-02-101818-A


Tot Ion:113 Resp: 53516

Ion Ratio Lower Upper

113 100

111 102.4 81.4 122.0




192 23.4 18.7 28.1

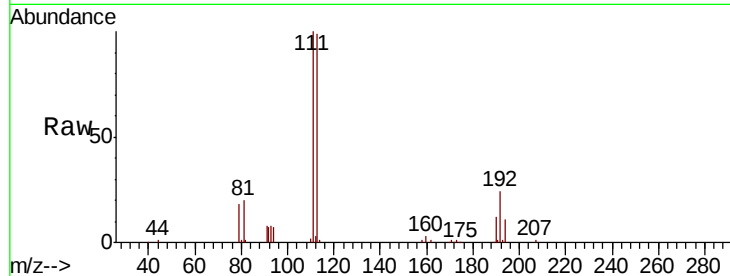

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

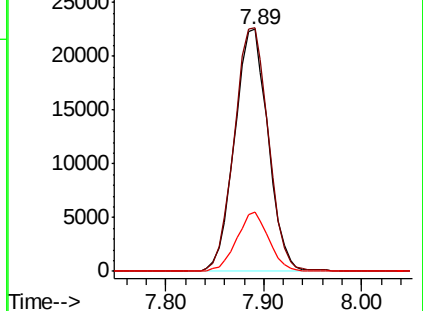

#36

1,1-Dichloropropene

Concen: 4.997 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.13 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13


Tgt Ion: 75 Resp: 7553

Ion Ratio Lower Upper

75 100

110 8.6 19.1 57.1#



77 0.0 25.0 37.4#




Abundance Ion 74.90 (74.60 to 75.60): VW

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VW

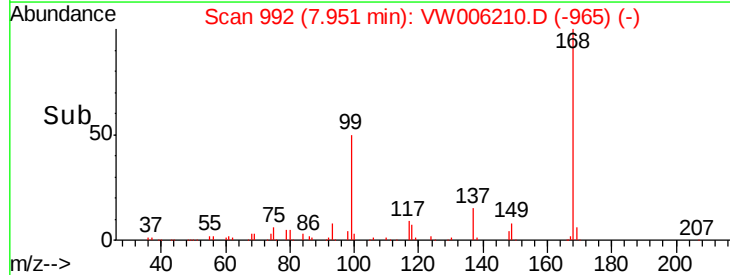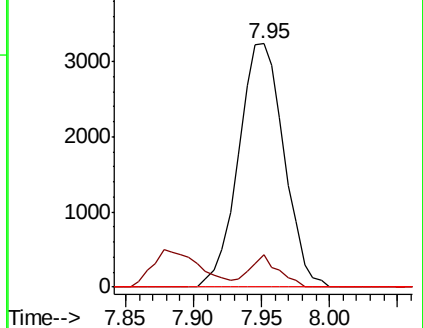

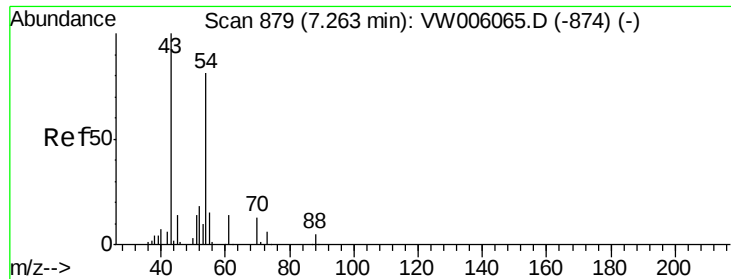

#37

Ethyl Acetate

Concen: 1.152 ug/l

RT: 7.16 min Scan# 863

Delta R.T. -0.10 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :

JC-02-101818-A


Tot Ion: 43 Resp: 647

Ion Ratio Lower Upper

43 100

61 85.8 11.5 17.3#

70 0.0 9.2 13.8#

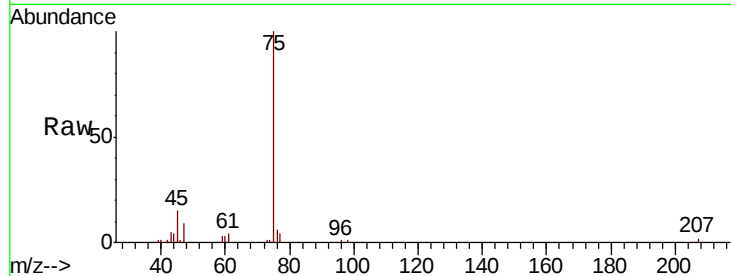

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 60.90 (60.60 to 61.60): VW

Ion 70.00 (69.70 to 70.70): VW

7.16



300

200

100

0

Time-->



#38

Carbon Tetrachloride

Concen: 6.259 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.12 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13


Tgt Ion: 117 Resp: 10371

Ion Ratio Lower Upper

117 100

119 6.6 75.2 112.8#

121 0.0 25.3 37.9#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

7.95

6000

5000

4000


3000


2000

1000

0

Time-->







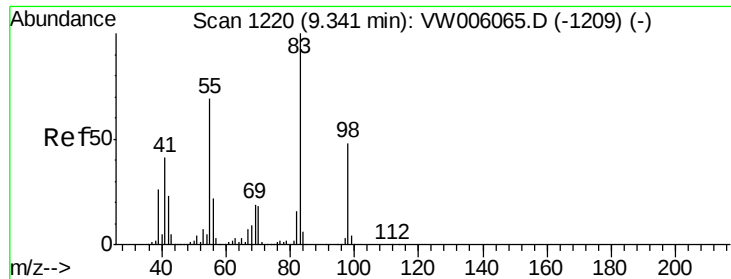

#39
Methvlcvclohexane
Concen: 2.311 ug/l
RT: 9.34 min Scan# 1219
Delta R.T. -0.01 min
Lab File: VW006210.D
Acq: 19 Oct 2018 08:13




Instrument :
MSVOA_W
ClientSampleId :
JC-02-101818-A


Tot Ion: 83 Resp: 4644
Ion Ratio Lower Upper
83 100
55 61.0 55.0 82.6
98 42.5 38.6 57.8

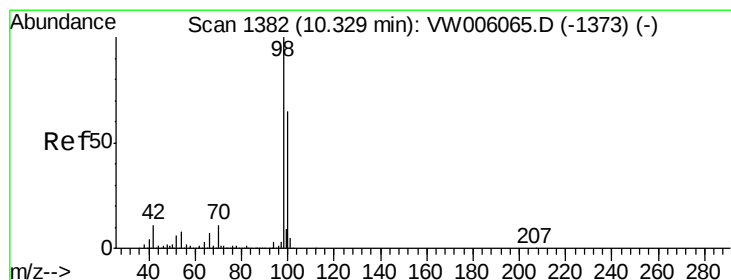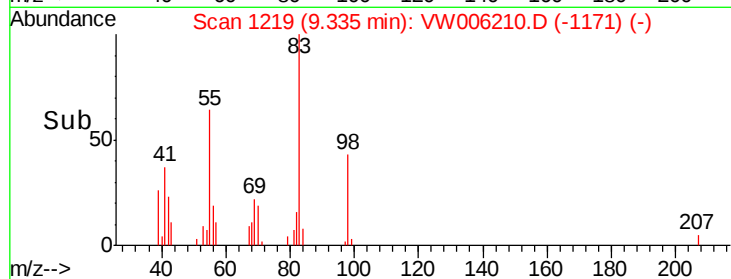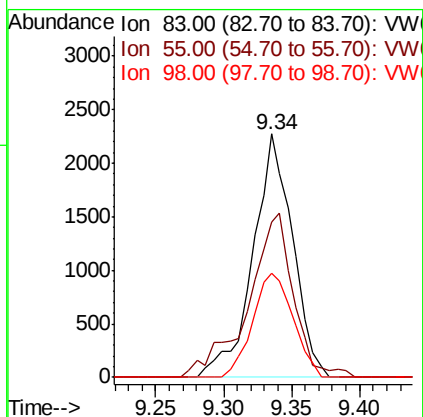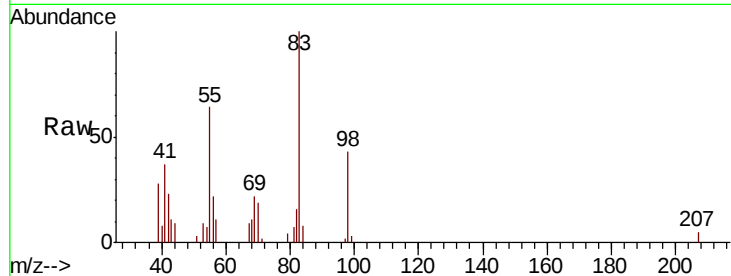

#50
Toluene-d8
Concen: 33.490 ug/l
RT: 10.33 min Scan# 1382
Delta R.T. -0.00 min
Lab File: VW006210.D
Acq: 19 Oct 2018 08:13

Tgt Ion: 98 Resp: 123457
Ion Ratio Lower Upper
98 100
100 64.5 51.6 77.4


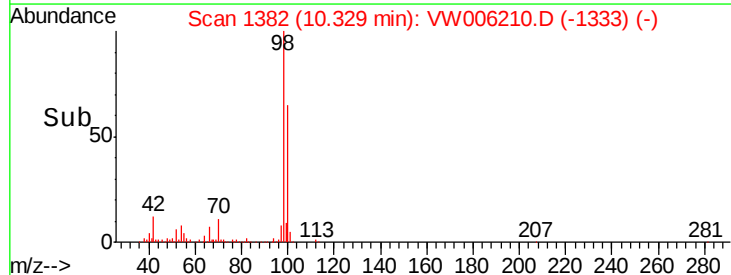
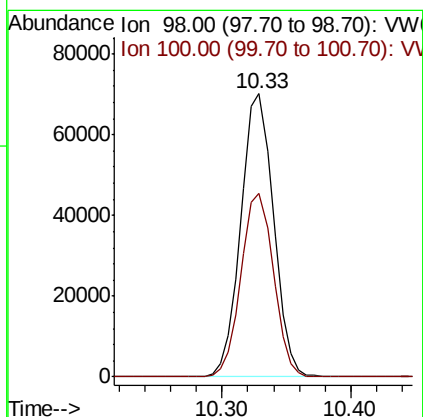



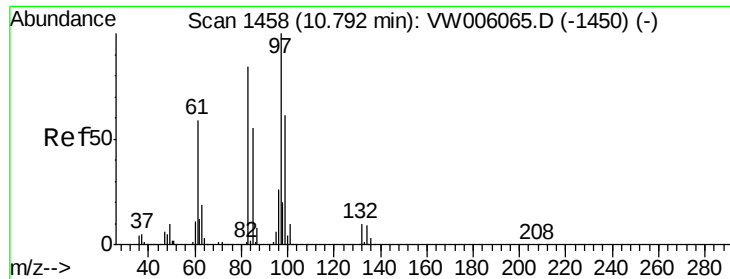

#55
 1,1,2-Trichloroethane
 Concen: 4.560 ug/l
 RT: 10.77 min Scan# 1454
 Delta R.T. -0.02 min
 Lab File: VW006210.D
 Acq: 19 Oct 2018 08:13




Instrument :
 MSVOA_W
 ClientSampleId :
 JC-02-101818-A


Tot Ion	Ratio	Lower	Upper
97	100		
83	7.6	67.2	100.8#
85	0.0	43.7	65.5#
99	0.0	48.5	72.7#

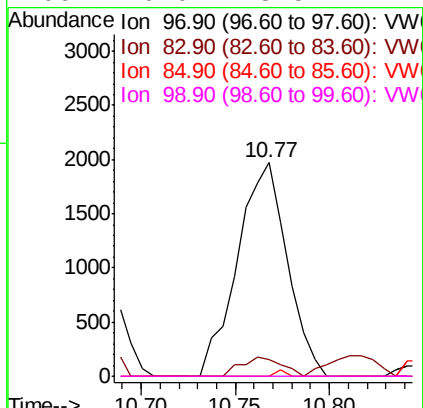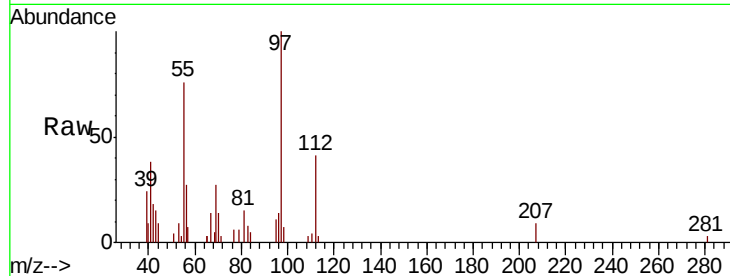

#56
 Ethyl methacrylate
 Concen: 1.428 ug/l
 RT: 10.66 min Scan# 1437
 Delta R.T. 0.01 min
 Lab File: VW006210.D
 Acq: 19 Oct 2018 08:13

Tgt Ion	Ratio	Lower	Upper
69	100		
41	165.6	52.8	79.2#
39	95.4	30.6	45.8#



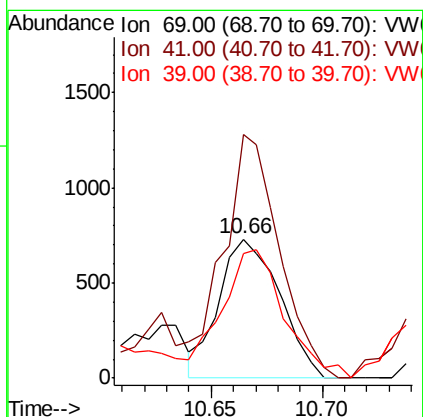





#62
4-Bromofluorobenzene
Concen: 23.101 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. -0.00 min
Lab File: VW006210.D
Acq: 19 Oct 2018 08:13




Instrument :
MSVOA_W
ClientSampleId :
JC-02-101818-A


Tot Ion: 95 Resp: 31985
Ion Ratio Lower Upper
95 100
174 90.7 0.0 186.0
176 89.0 0.0 181.6

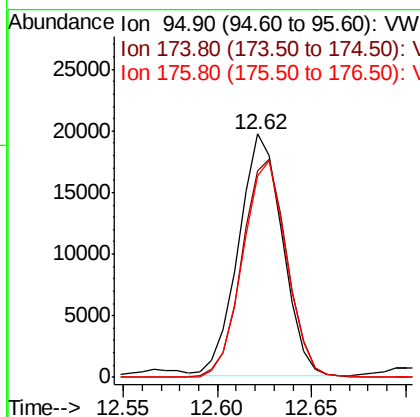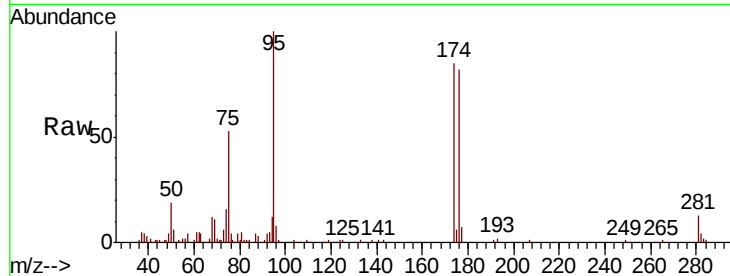

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW006210.D
Acq: 19 Oct 2018 08:13

Tgt Ion: 117 Resp: 96941
Ion Ratio Lower Upper
117 100
82 52.8 42.1 63.1
119 30.5 25.8 38.6

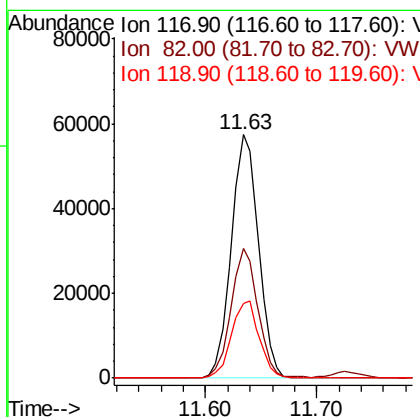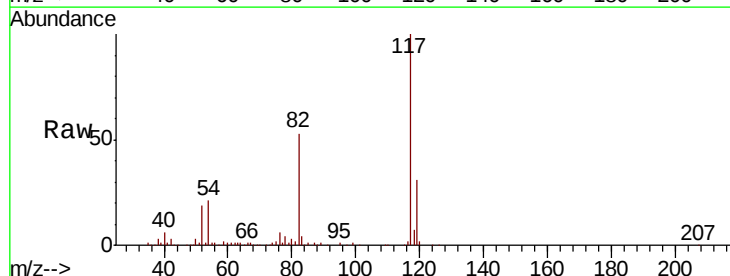

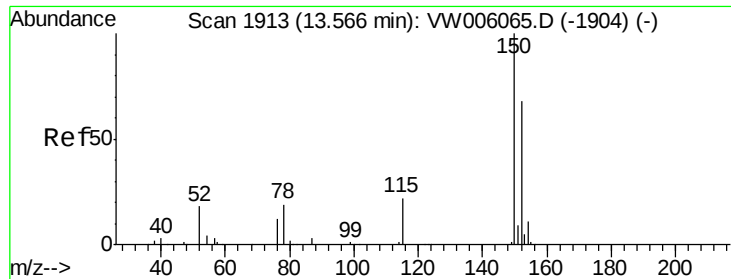


#72




1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.57 min Scan# 1913
Delta R.T. -0.00 min
Lab File: VW006210.D
Acq: 19 Oct 2018 08:13

Instrument :
MSVOA_W
ClientSampleId :
JC-02-101818-A

Tot Ion	Ratio	Lower	Upper
152	100		
115	54.6	27.8	83.3
150	153.9	0.0	349.2

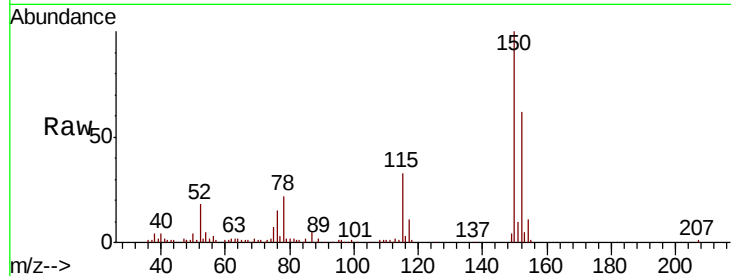


Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

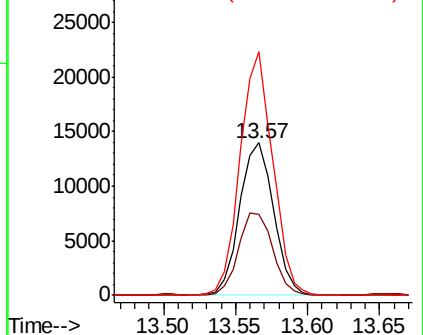



#73


Isopropylbenzene
Concen: 4.677 ug/l
RT: 12.47 min Scan# 1733
Delta R.T. -0.00 min
Lab File: VW006210.D
Acq: 19 Oct 2018 08:13

Tgt Ion	Ratio	Lower	Upper
105	100		
120	27.8	13.6	40.7



Abundance Ion 105.00 (104.70 to 105.70): V
Ion 120.00 (119.70 to 120.70): V

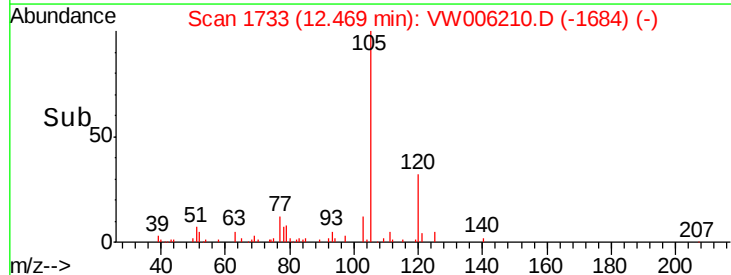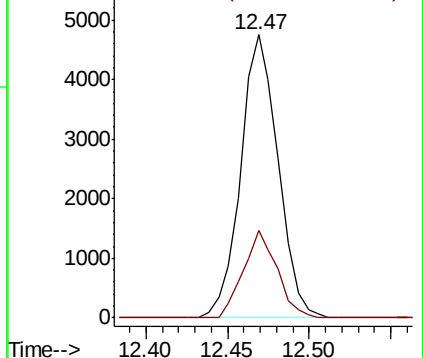



#74

N-amvl acetate

Concen: 3.099 ug/l

RT: 12.26 min Scan# 1699

Delta R.T. -0.02 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :

JC-02-101818-A

Tot Ion: 43 Resp: 973


Ion Ratio Lower Upper

43 100

70 30.0 34.2 51.4#

55 0.0 19.2 28.8#

61 0.0 19.0 28.6#



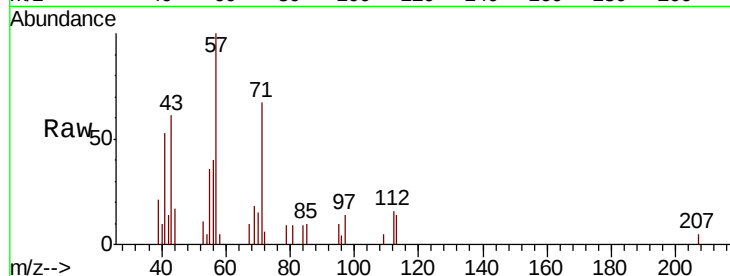


Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 70.00 (69.70 to 70.70): VW

Ion 55.00 (54.70 to 55.70): VW

Ion 61.00 (60.70 to 61.70): VW

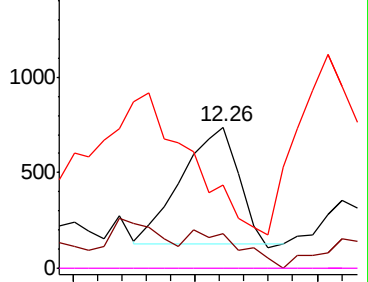

#75

1,1,2,2-Tetrachloroethane

Concen: 2.168 ug/l

RT: 12.69 min Scan# 1770

Delta R.T. -0.02 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13


Tgt Ion: 83 Resp: 533

Ion Ratio Lower Upper

83 100

131 0.0 5.9 17.7#



85 0.0 31.9 95.9#




Abundance Ion 82.90 (82.60 to 83.60): VW

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): VW

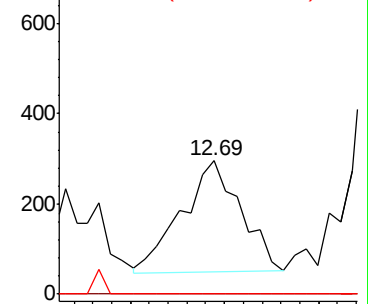

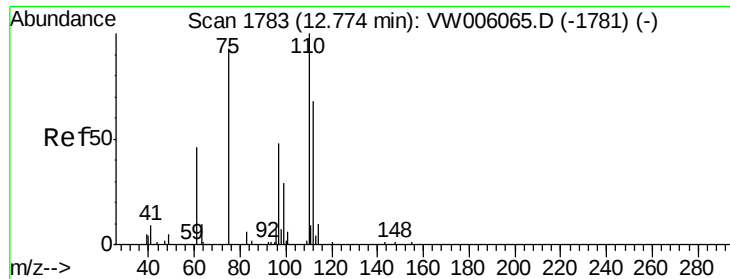

#76

1,2,3-Trichloropropane

Concen: 90.585 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.15 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :


JC-02-101818-A

Tot Ion: 75 Resp: 15834

Ion Ratio Lower Upper

75 100

77 1.4 0.0 0.0#

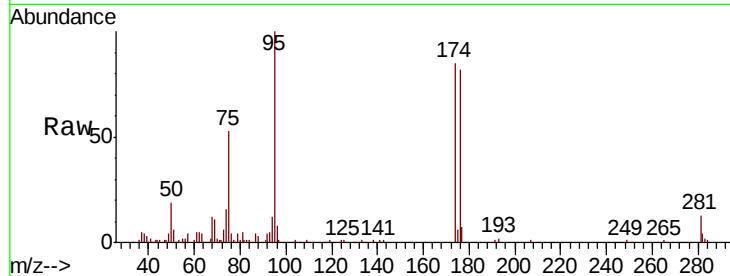

Abundance Ion 74.90 (74.60 to 75.60): VW

Ion 77.00 (76.70 to 77.70): VW

12000

10000

8000

6000



4000

2000

0

Time-->

12.55 12.60 12.65 12.70

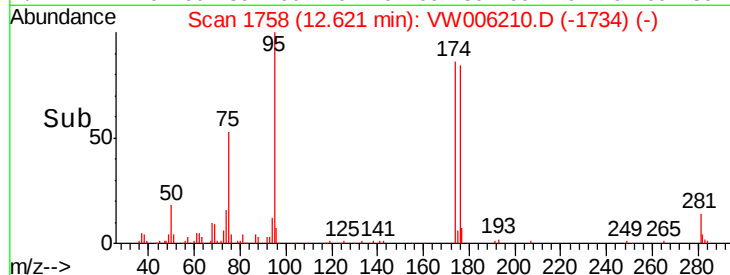

#78

n-propylbenzene

Concen: 3.487 ug/l

RT: 12.81 min Scan# 1789

Delta R.T. -0.00 min

Lab File: VW006210.D


Acq: 19 Oct 2018 08:13

Tgt Ion: 91 Resp: 6559

Ion Ratio Lower Upper

91 100

120 20.9 12.2 36.6



Abundance Ion 91.00 (90.70 to 91.70): VW

Ion 120.00 (119.70 to 120.70): V

4000

3000


2000


1000

0

Time-->

12.75 12.80 12.85







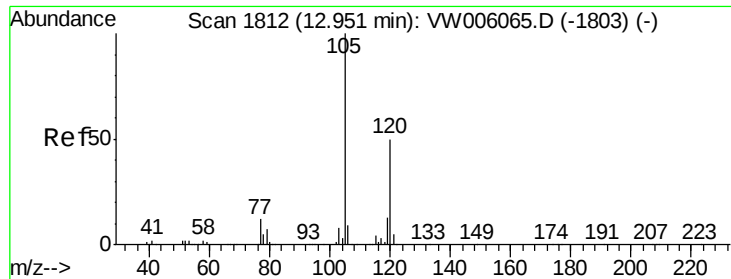

#80
 1,3,5-Trimethylbenzene
 Concen: 1.304 ug/l
 RT: 12.95 min Scan# 1812
 Delta R.T. -0.00 min
 Lab File: VW006210.D
 Acq: 19 Oct 2018 08:13




Instrument :
 MSVOA_W
 ClientSampleId :
 JC-02-101818-A


Tot Ion:105 Resp: 1777
 Ion Ratio Lower Upper
 105 100
 120 47.3 24.9 74.6

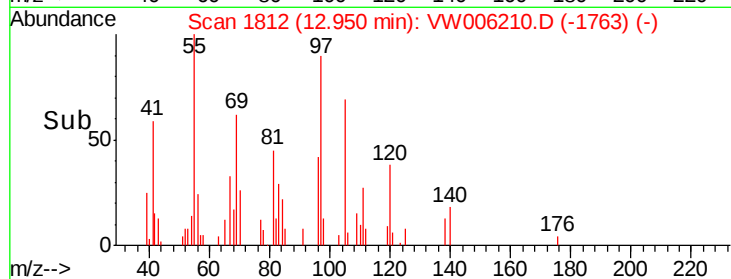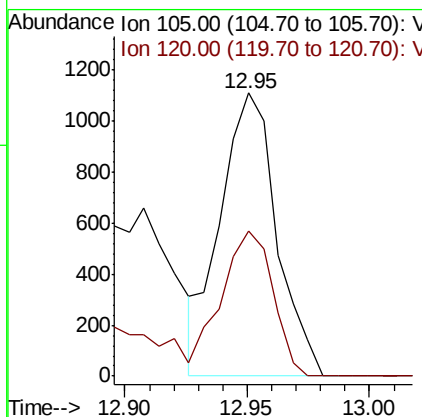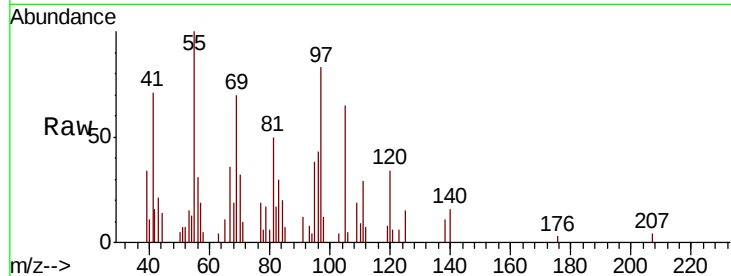

#81
 trans-1,4-Dichloro-2-butene
 Concen: 216.535 ug/l
 RT: 12.62 min Scan# 1758
 Delta R.T. 0.10 min
 Lab File: VW006210.D
 Acq: 19 Oct 2018 08:13

Tgt Ion: 75 Resp: 15834
 Ion Ratio Lower Upper
 75 100
 53 1.9 79.8 119.6#
 89 0.0 37.5 56.3#



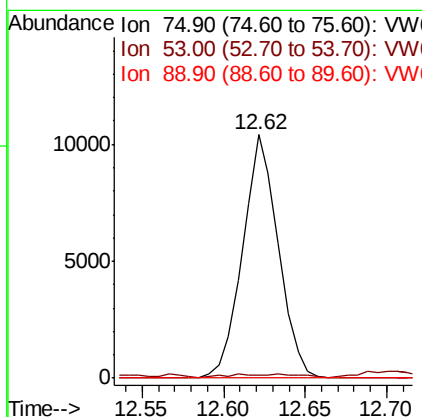





#83
tert-Butylbenzene
Concen: 1.323 ug/l
RT: 13.21 min Scan# 1855
Delta R.T. -0.00 min
Lab File: VW006210.D
Acq: 19 Oct 2018 08:13




Instrument :
MSVOA_W
ClientSampleId :
JC-02-101818-A


Tot Ion:119 Resp: 1613
Ion Ratio Lower Upper
119 100
91 93.2 32.3 96.9
134 25.4 13.6 40.8

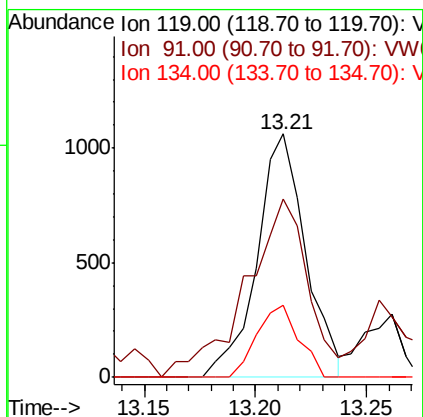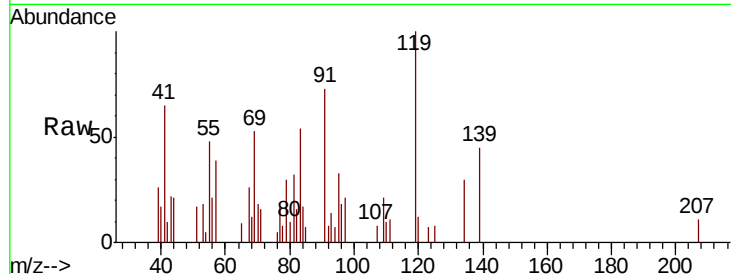

#84
1,2,4-Trimethylbenzene
Concen: 1.871 ug/l
RT: 13.26 min Scan# 1863
Delta R.T. 0.01 min
Lab File: VW006210.D
Acq: 19 Oct 2018 08:13

Tgt Ion:105 Resp: 2580
Ion Ratio Lower Upper
105 100
120 39.7 23.1 69.3

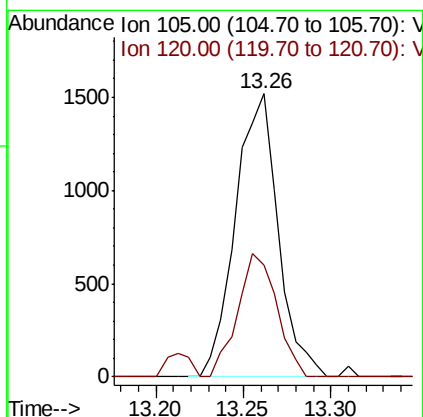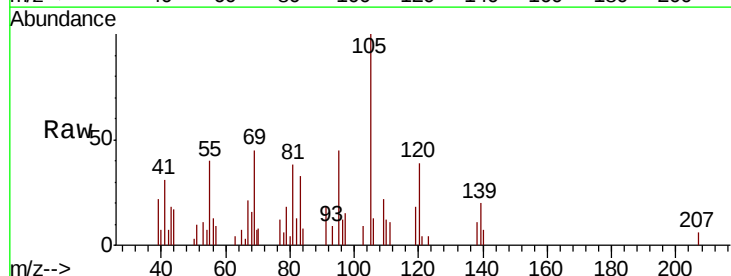

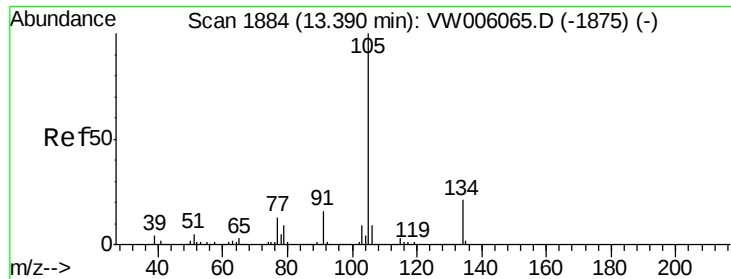

#85

sec-Butylbenzene

Concen: 2.998 ug/l

RT: 13.39 min Scan# 1884

Delta R.T. -0.00 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :





JC-02-101818-A

Tot Ion:105 Resp: 5165

Ion Ratio Lower Upper

105 100

134 35.2 10.5 31.6#

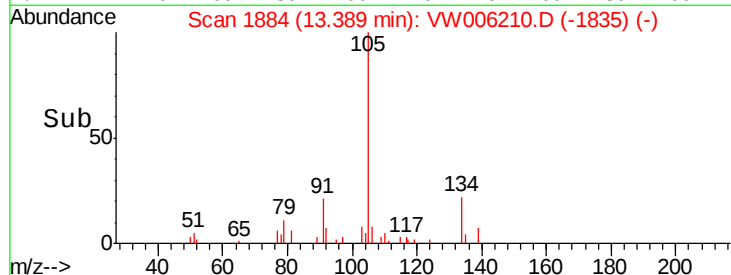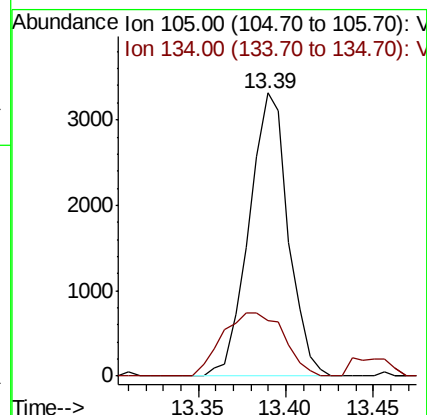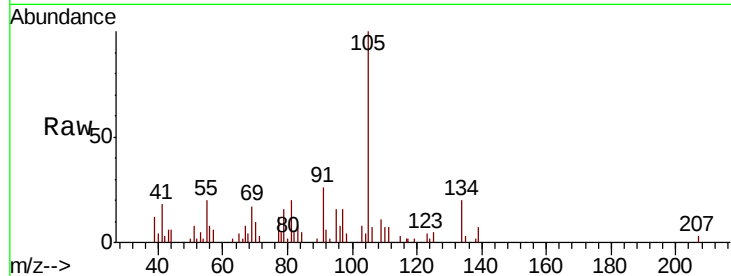

#89

n-Butylbenzene

Concen: 1.387 ug/l

RT: 13.83 min Scan# 1956

Delta R.T. -0.00 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13




Tgt Ion: 91 Resp: 1977


Ion Ratio Lower Upper

91 100

92 33.6 26.6 79.7

134 0.0 14.0 41.9#

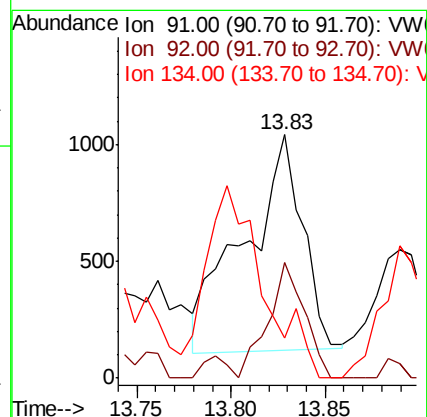



#90

Hexachloroethane

Concen: 5.471 ug/l

RT: 14.10 min Scan# 2001

Delta R.T. -0.00 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Instrument :

MSVOA_W

ClientSampleId :





JC-02-101818-A

Tot Ion:117 Resp: 1444

Ion Ratio Lower Upper

117 100

201 0.0 45.3 135.9#

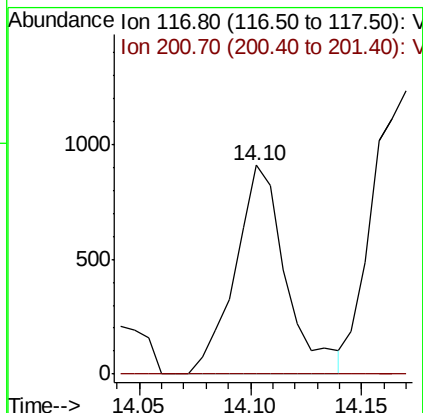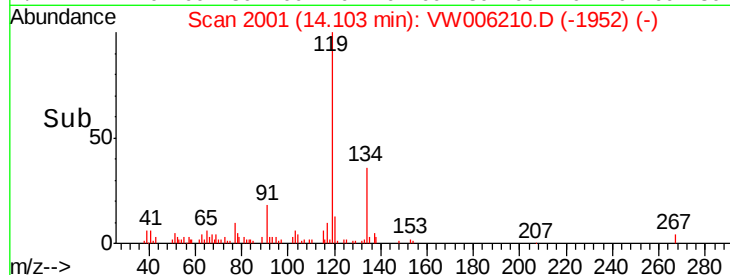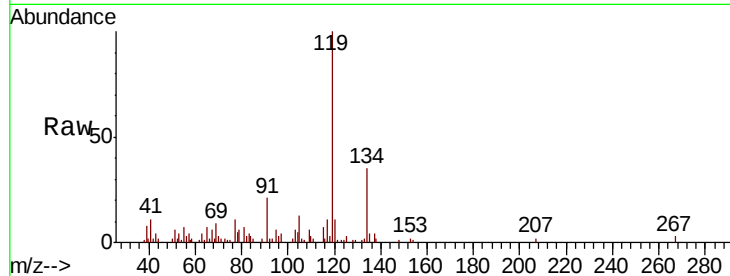

#95

Naphthalene

Concen: 1.711 ug/l

RT: 15.38 min Scan# 2211

Delta R.T. 0.01 min

Lab File: VW006210.D

Acq: 19 Oct 2018 08:13

Tgt Ion:128 Resp: 1540

Ion Ratio Lower Upper

128 100

127 0.0 10.3 15.5#

129 14.2 8.7 13.1#

