

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW101818\
 Data File : VW006213.D
 Acq On : 19 Oct 2018 09:31
 Operator : VA/AP
 Sample : J5202-03RE
 Misc : 6.24G/5ML/MSVOA_W/SOIL
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 PL-03-101718-BRE

Quant Time: Oct 19 11:18:48 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 18 17:01:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	202373	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	306419	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	227929	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	83884	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	100494	59.90	ug/l	0.00
Spiked Amount 50.000			Recovery	=	119.80%	
35) Dibromofluoromethane	7.89	113	97699	53.96	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.92%	
50) Toluene-d8	10.33	98	299532	43.48	ug/l	0.00
Spiked Amount 50.000			Recovery	=	86.96%	
62) 4-Bromofluorobenzene	12.62	95	90756	35.08	ug/l	0.00
Spiked Amount 50.000			Recovery	=	70.16%	
Target Compounds						
8) Diethyl Ether	3.69	74	1788	1.96	ug/l	71
20) Methylene Chloride	4.91	84	8666	3.36	ug/l	92
40) Benzene	8.33	78	19852	2.56	ug/l	97
52) Toluene	10.39	92	82899	15.96	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW101818\
Data File : VW006213.D
Acq On : 19 Oct 2018 09:31
Operator : VA/AP
Sample : J5202-03RE
Misc : 6.24G/5ML/MSVOA_W/SOIL
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
PL-03-101718-BRE

Quant Time: Oct 19 11:18:48 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 18 17:01:24 2018
Response via : Initial Calibration

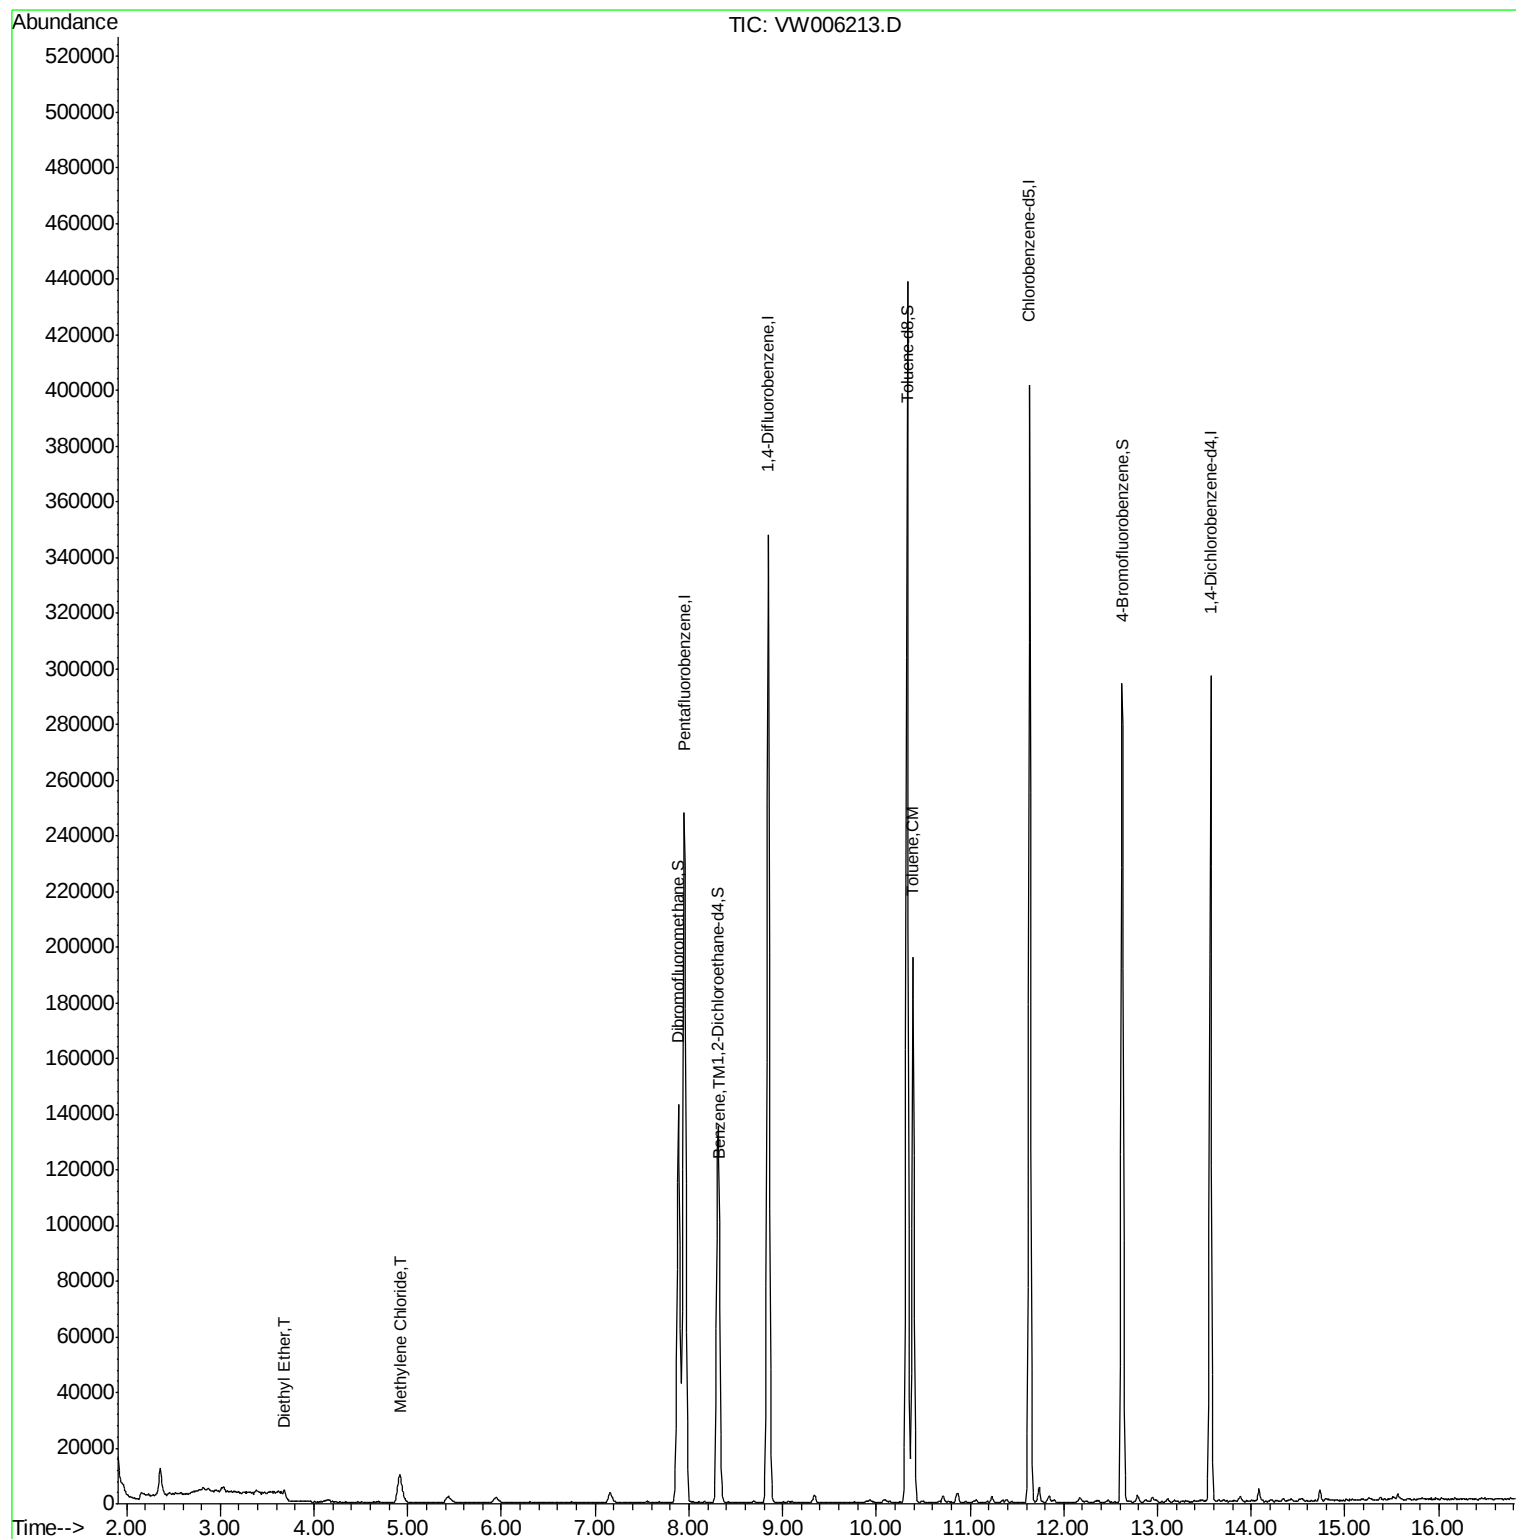

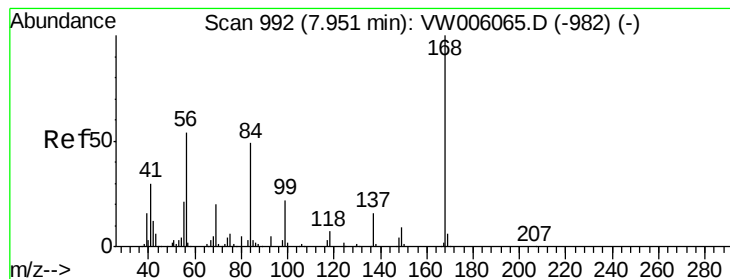

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW006213.D

Acq: 19 Oct 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :


PL-03-101718-BRE

Tgt Ion:168 Resp: 202373

Ion Ratio Lower Upper

168 100

99 49.6 39.9 59.9

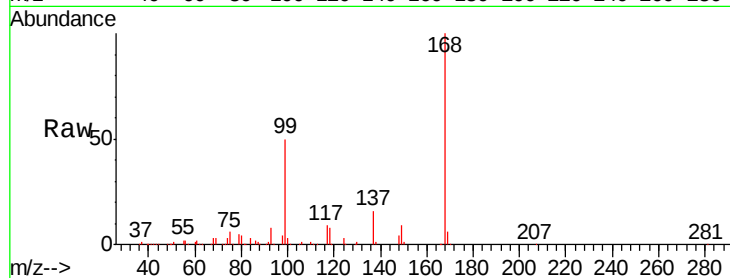

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00 8.10

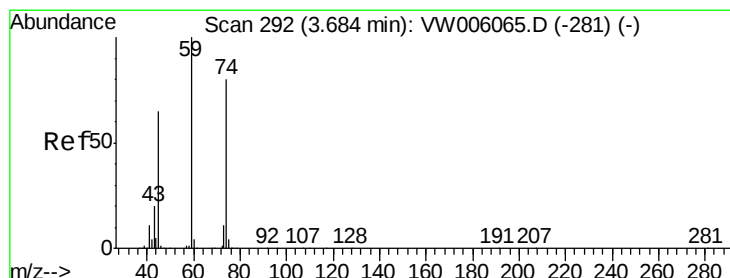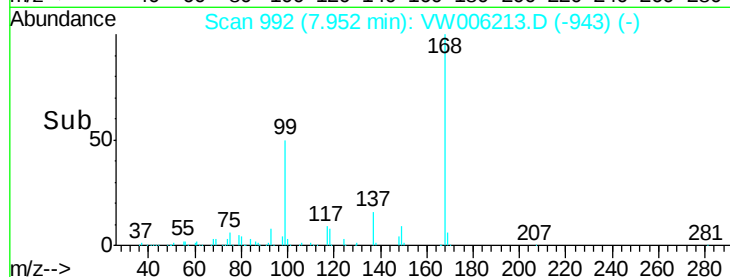

#8

Diethyl Ether

Concen: 1.96 ug/l

RT: 3.69 min Scan# 293

Delta R.T. 0.01 min

Lab File: VW006213.D


Acq: 19 Oct 2018 09:31

Tgt Ion: 74 Resp: 1788

Ion Ratio Lower Upper

74 100

45 112.4 42.8 128.3

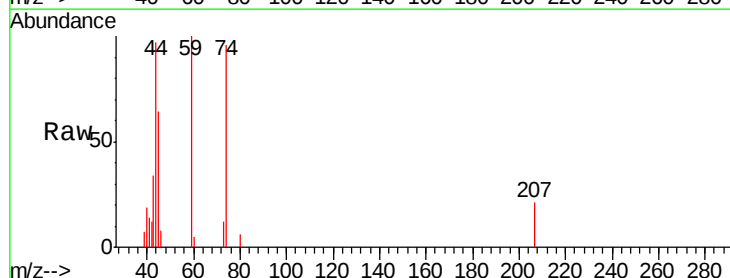

Abundance Ion 74.00 (73.70 to 74.70): VW

Ion 45.00 (44.70 to 45.70): VW

3.69

1000

800


600

400

200

0

Time--> 3.60 3.65 3.70 3.75




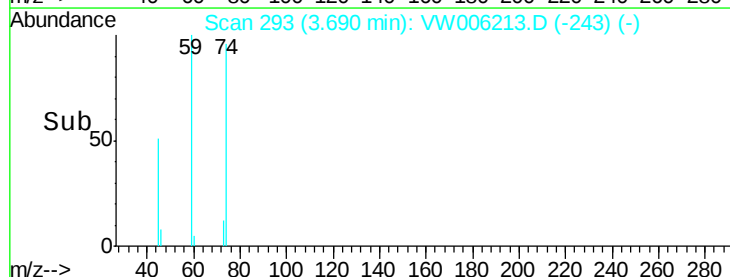




#20
Methylene Chloride
Concen: 3.36 ug/l
RT: 4.91 min Scan# 493
Delta R.T. -0.01 min
Lab File: VW006213.D
Acq: 19 Oct 2018 09:31




Instrument :
MSVOA_W
ClientSampleId :
PL-03-101718-BRE


Tgt Ion: 84 Resp: 8666
Ion Ratio Lower Upper
84 100
49 106.4 93.6 140.4
51 36.9 29.0 43.4
86 57.7 52.6 79.0

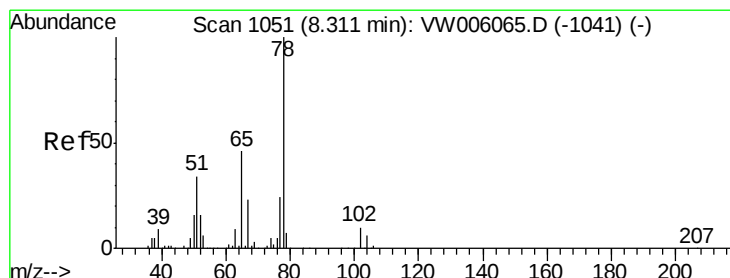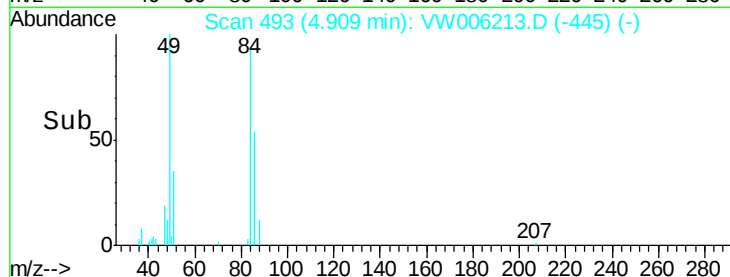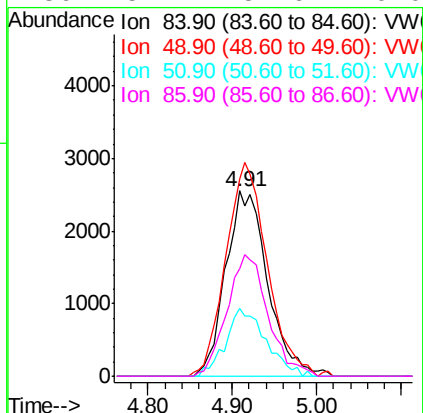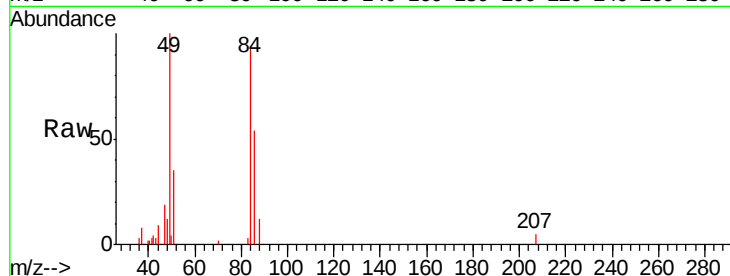

#33
1,2-Dichloroethane-d4
Concen: 59.90 ug/l
RT: 8.31 min Scan# 1051
Delta R.T. 0.00 min
Lab File: VW006213.D
Acq: 19 Oct 2018 09:31

Tgt Ion: 65 Resp: 100494
Ion Ratio Lower Upper
65 100
67 51.8 0.0 101.0

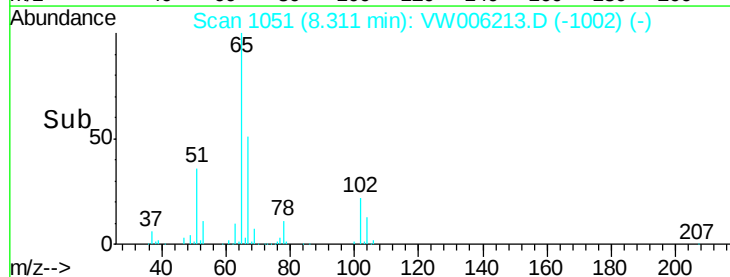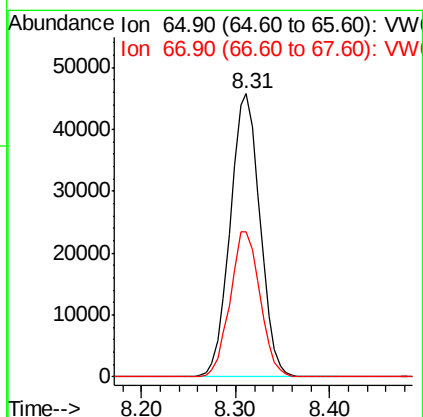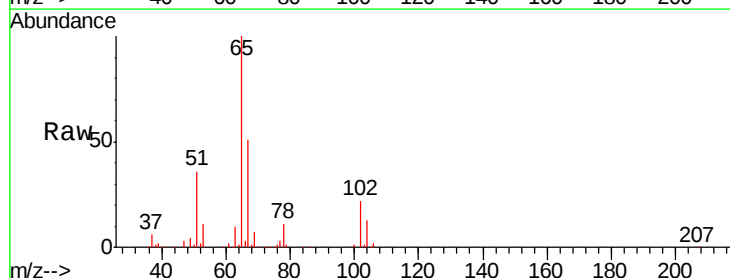


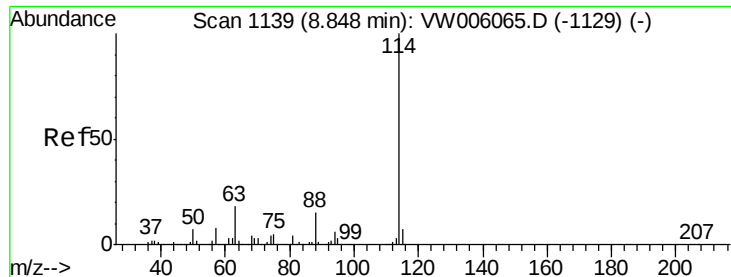

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. 0.00 min
 Lab File: VW006213.D
 Acq: 19 Oct 2018 09:31

Instrument :
 MSVOA_W
 ClientSampleId :
 PL-03-101718-BRE




Tgt Ion	Ratio	Lower	Upper
114	100		
63	18.2	0.0	36.8
88	14.5	0.0	29.0

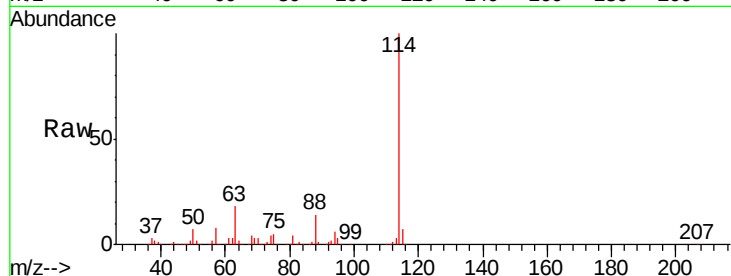

Abundance Ion 113.90 (113.60 to 114.60): V


Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

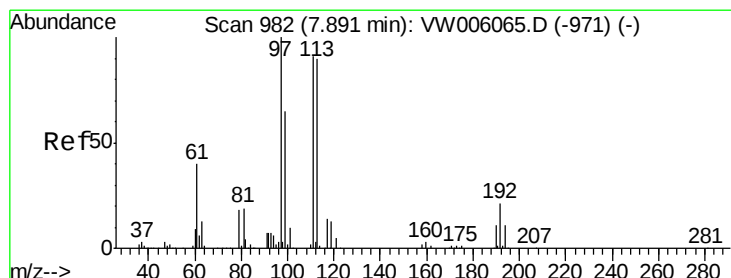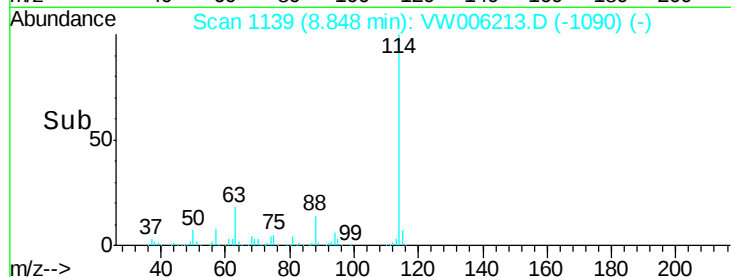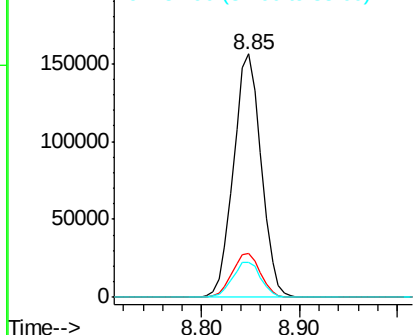

#35
 Dibromofluoromethane
 Concen: 53.96 ug/l
 RT: 7.89 min Scan# 982
 Delta R.T. 0.00 min
 Lab File: VW006213.D
 Acq: 19 Oct 2018 09:31



Tgt Ion	Ratio	Lower	Upper
113	100		
111	103.8	81.4	122.0
192	23.0	18.7	28.1

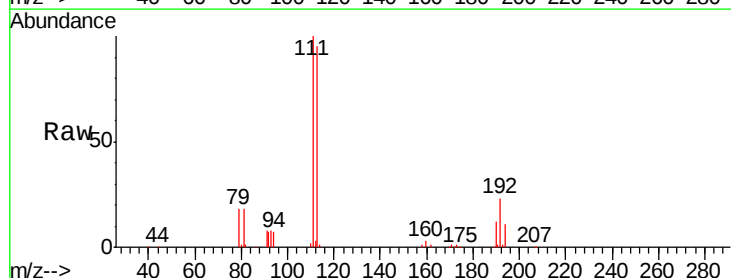


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

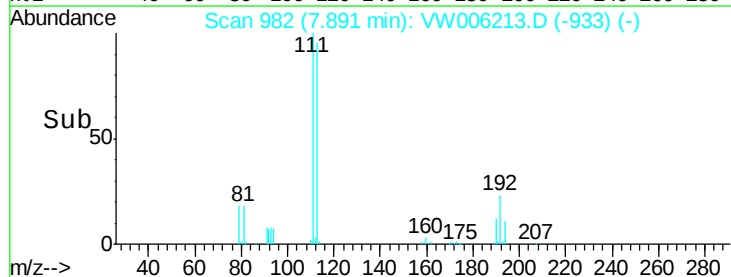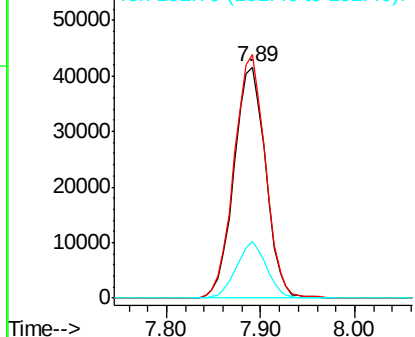

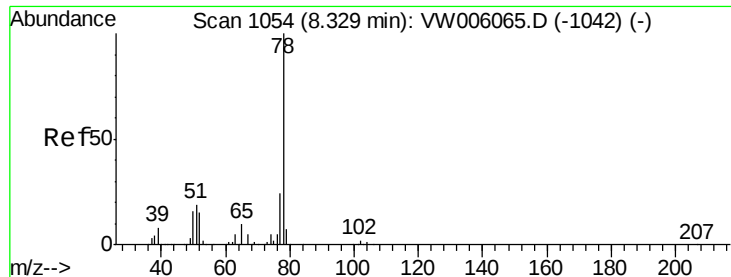

#40

Benzene

Concen: 2.56 ug/l

RT: 8.33 min Scan# 1054

Delta R.T. 0.00 min

Lab File: VW006213.D

Acq: 19 Oct 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :





PL-03-101718-BRE

Tgt Ion: 78 Resp: 19852

Ion Ratio Lower Upper

78 100

77 22.7 19.4 29.0

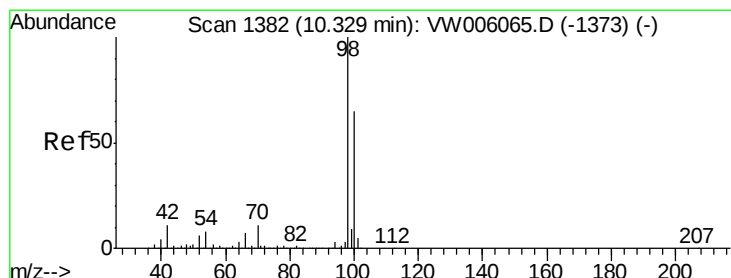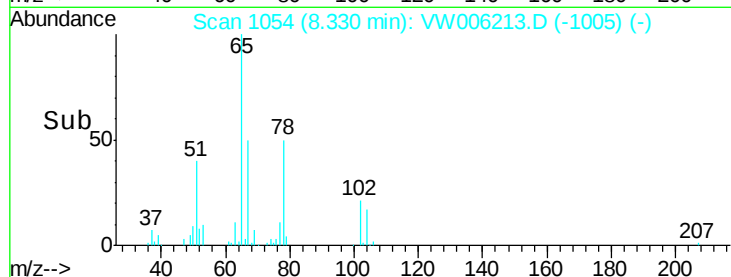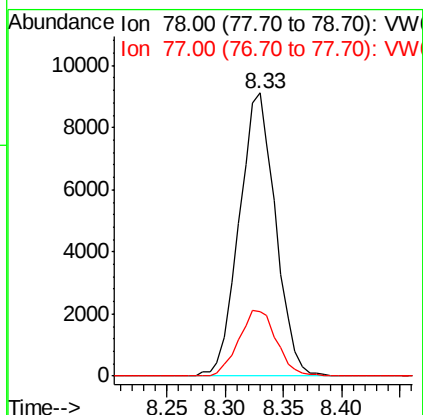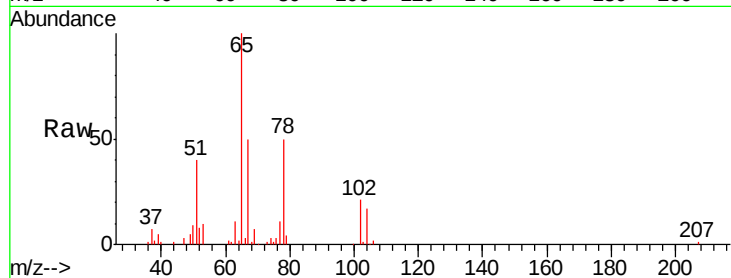

#50

Toluene-d8

Concen: 43.48 ug/l

RT: 10.33 min Scan# 1382

Delta R.T. 0.00 min

Lab File: VW006213.D




Acq: 19 Oct 2018 09:31


Tgt Ion: 98 Resp: 299532

Ion Ratio Lower Upper

98 100

100 63.7 51.6 77.4

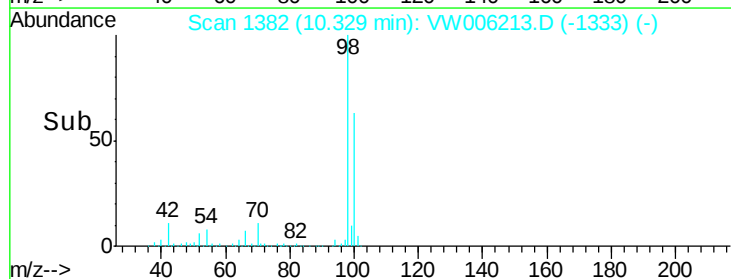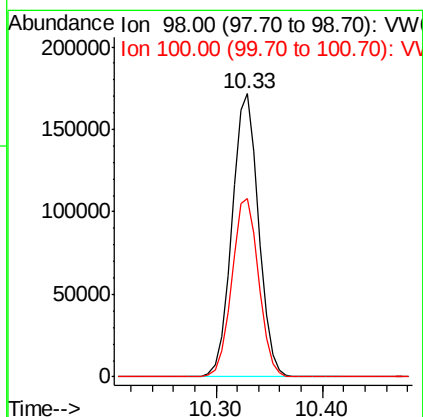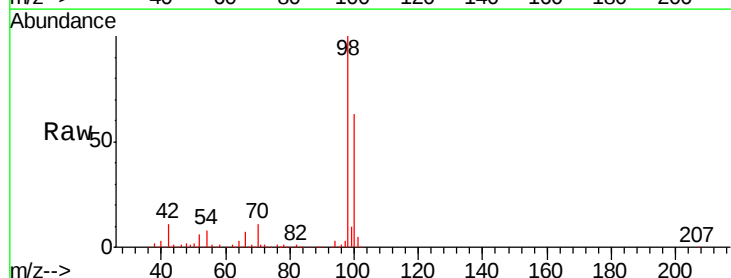

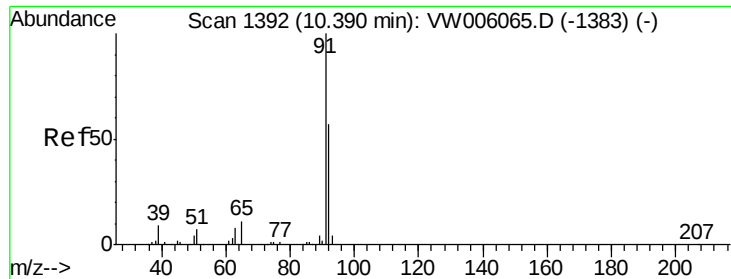

#52

Toluene

Concen: 15.96 ug/l

RT: 10.39 min Scan# 1392

Delta R.T. 0.00 min

Lab File: VW006213.D

Acq: 19 Oct 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :





PL-03-101718-BRE

Tgt Ion: 92 Resp: 82899

Ion Ratio Lower Upper

92 100

91 173.5 140.0 210.0

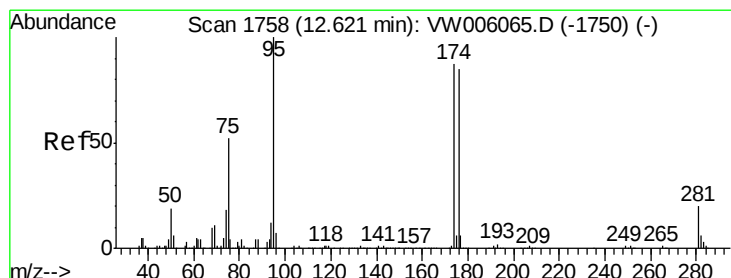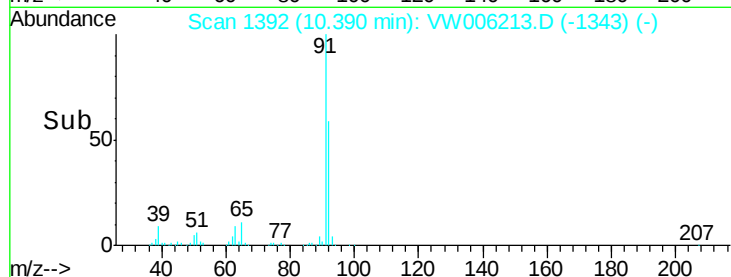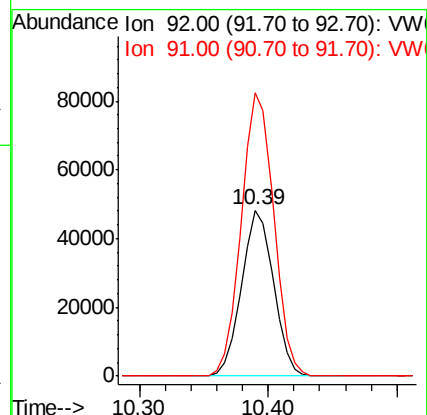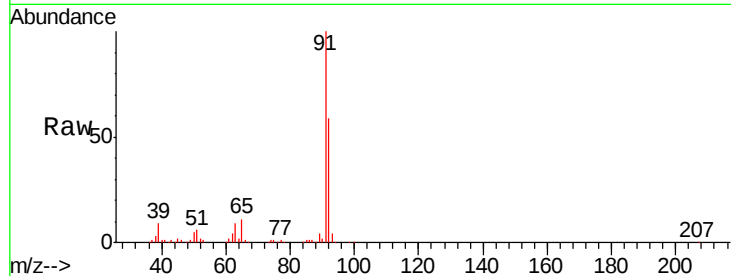

#62

4-Bromofluorobenzene

Concen: 35.08 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW006213.D

Acq: 19 Oct 2018 09:31




Tgt Ion: 95 Resp: 90756


Ion Ratio Lower Upper

95 100

174 94.3 0.0 186.0

176 91.6 0.0 181.6

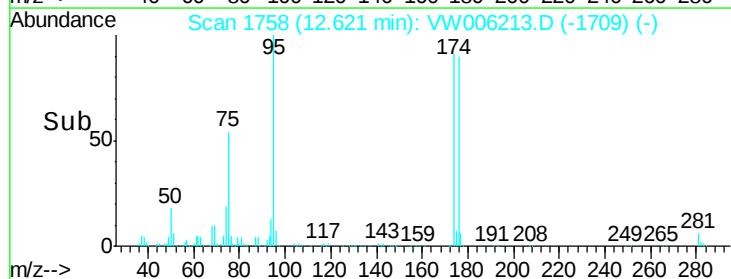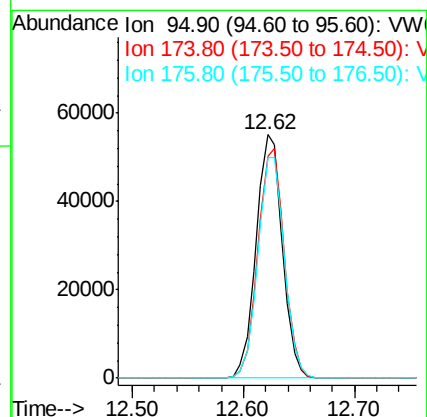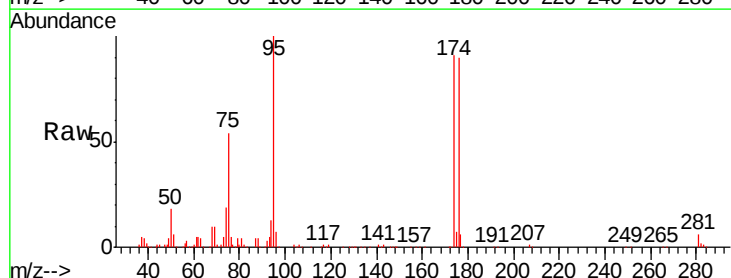

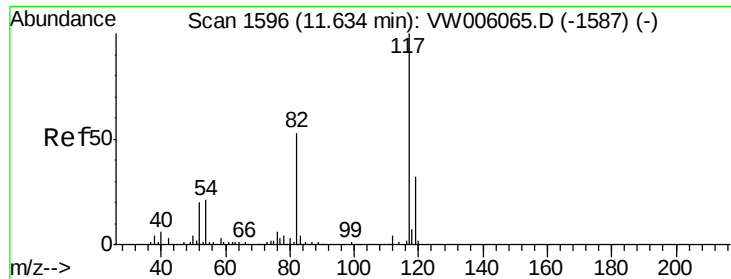

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. 0.00 min

Lab File: VW006213.D

Acq: 19 Oct 2018 09:31

Instrument :

MSVOA_W

ClientSampleId :

PL-03-101718-BRE


Tgt Ion:117 Resp: 227929

Ion Ratio Lower Upper

117 100

82 53.3 42.1 63.1




119 32.7 25.8 38.6

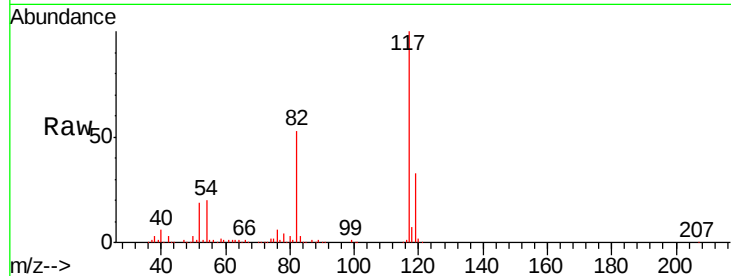

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): V

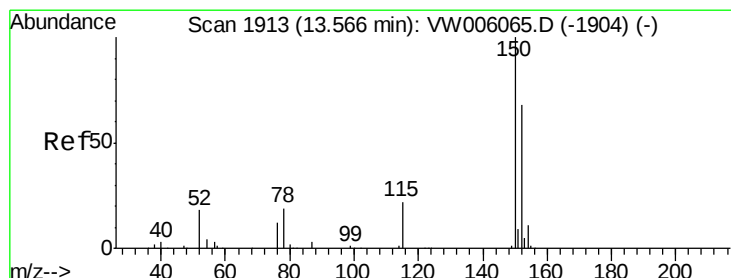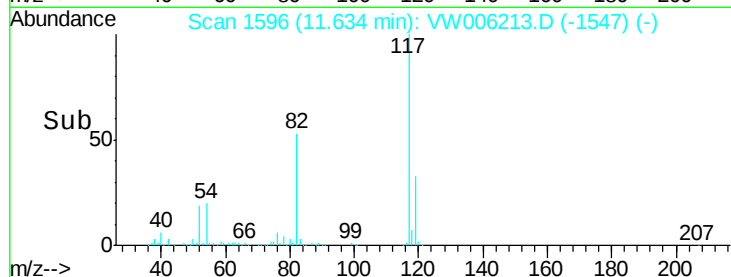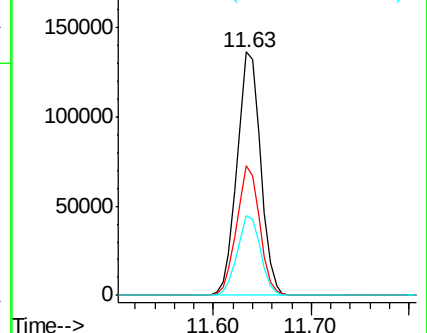

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.57 min Scan# 1913

Delta R.T. 0.00 min

Lab File: VW006213.D

Acq: 19 Oct 2018 09:31


Tgt Ion:152 Resp: 83884

Ion Ratio Lower Upper

152 100

115 55.1 27.8 83.3

150 153.4 0.0 349.2

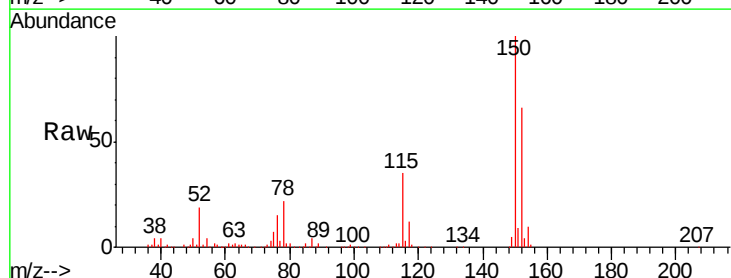

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

