

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101821\
 Data File : VW020572.D
 Acq On : 18 Oct 2021 19:46
 Operator : SY/VA
 Sample : VW1018SBL02
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK465

Quant Time: Oct 19 07:52:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Oct 19 07:51:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	161031	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	155290	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	72689	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	52510	22.410	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.640%
7) Chloroethane-d5	2.879	69	26327	21.270	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.080%
11) 1,1-Dichloroethene-d2	4.007	63	77630	16.168	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.680%
21) 2-Butanone-d5	7.086	46	42035	58.946	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.900%
24) Chloroform-d	7.647	84	125521	24.453	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.800%
26) 1,2-Dichloroethane-d4	8.305	65	77192	26.330	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.320%
32) Benzene-d6	8.275	84	233029	22.813	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.240%
36) 1,2-Dichloropropane-d6	9.274	67	80753	24.257	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.040%
41) Toluene-d8	10.323	98	209282	22.834	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.320%
43) trans-1,3-Dichloroprop...	10.579	79	32435	23.975	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.920%
47) 2-Hexanone-d5	10.927	63	28040	54.752	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.500%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	64852	25.771	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.080%
66) 1,2-Dichlorobenzene-d4	13.853	152	73863	25.976	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.920%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	12636	4.037	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101821\
Data File : VW020572.D
Acq On : 18 Oct 2021 19:46
Operator : SY/VA
Sample : VW1018SBL02
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK465

Quant Time: Oct 19 07:52:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Oct 19 07:51:45 2021
Response via : Initial Calibration

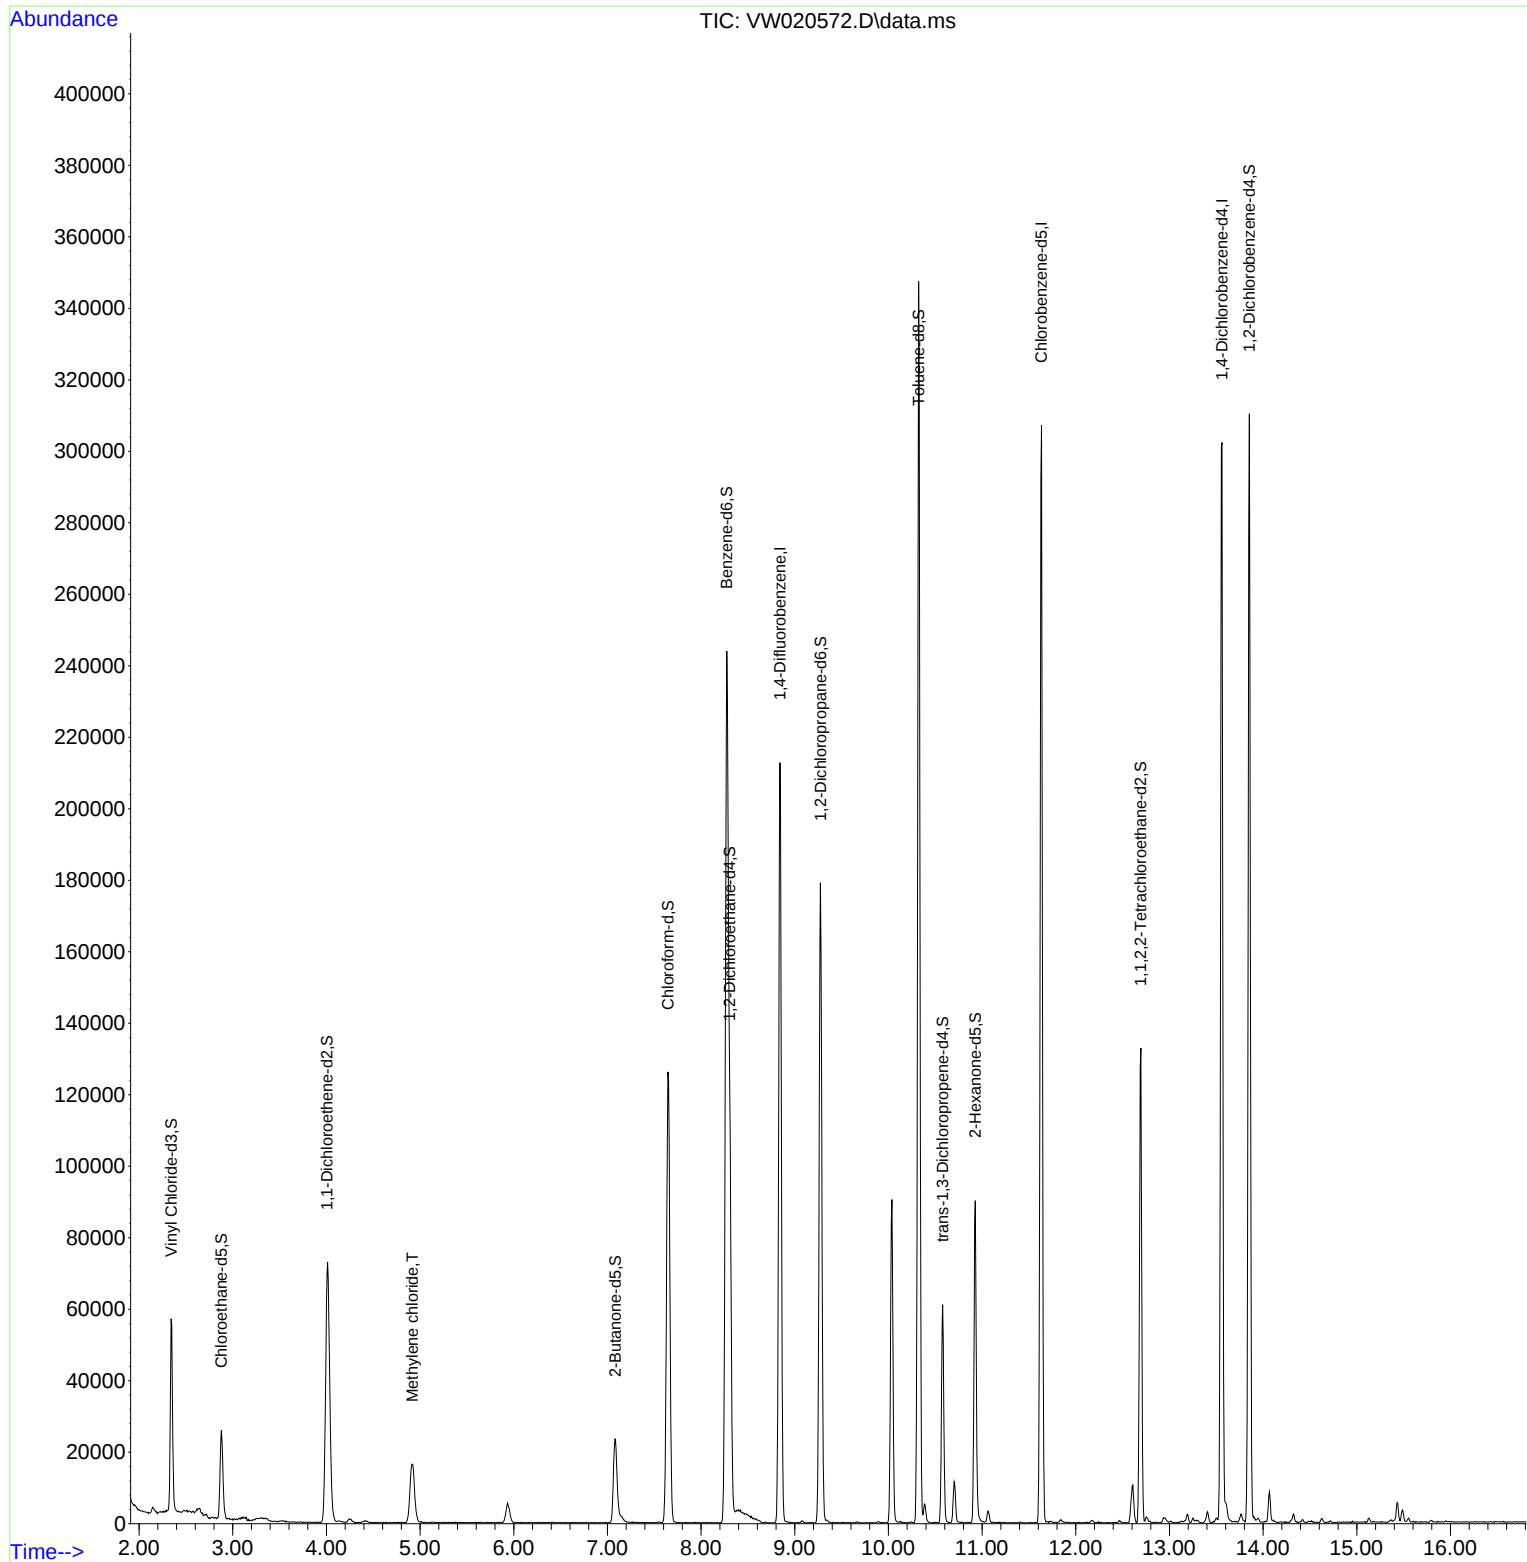

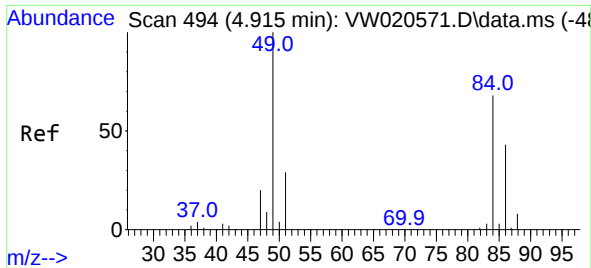

#16
Methylene chloride
Concen: 4.037 ug/L
RT: 4.915 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW020572.D
Acq: 18 Oct 2021 19:46

Instrument :
MSVOA_W
ClientSampleId :
VBLK465

Tgt Ion: 84 Resp: 12636
Ion Ratio Lower Upper
84 100
86 65.7 44.7 83.1
49 145.3 101.7 188.9

