
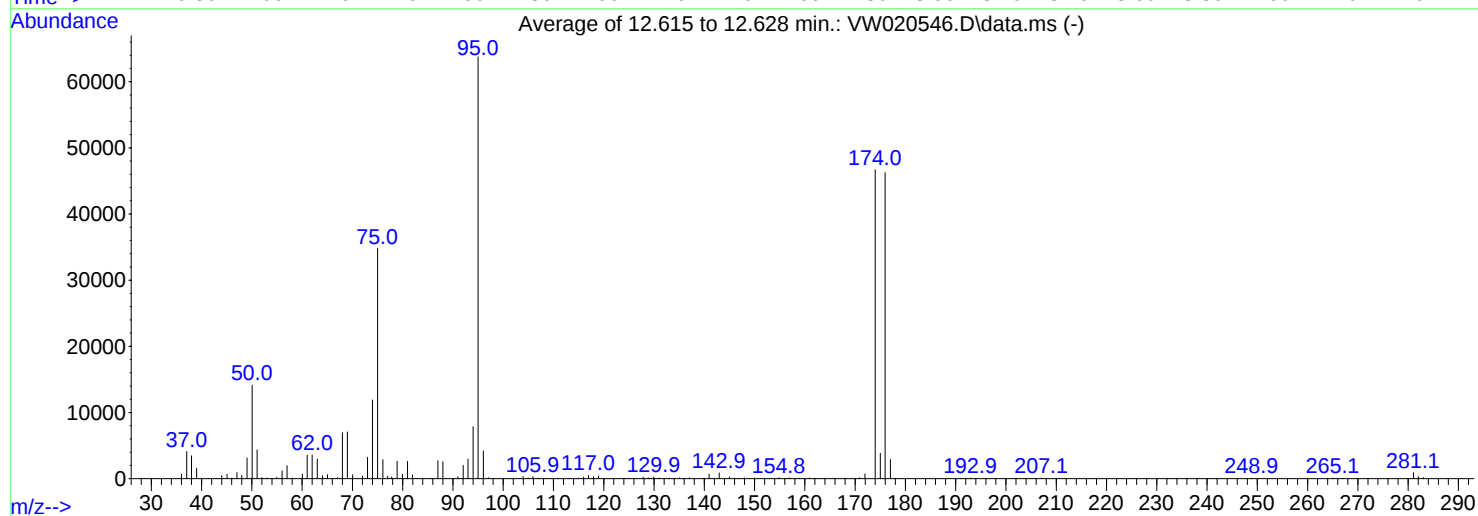


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101821\
 Data File : VW020546.D
 Acq On : 18 Oct 2021 07:45
 Operator : SY/VA
 Sample : BFB454
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB454

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0
 Last Update : Thu Oct 21 01:08:32 2021

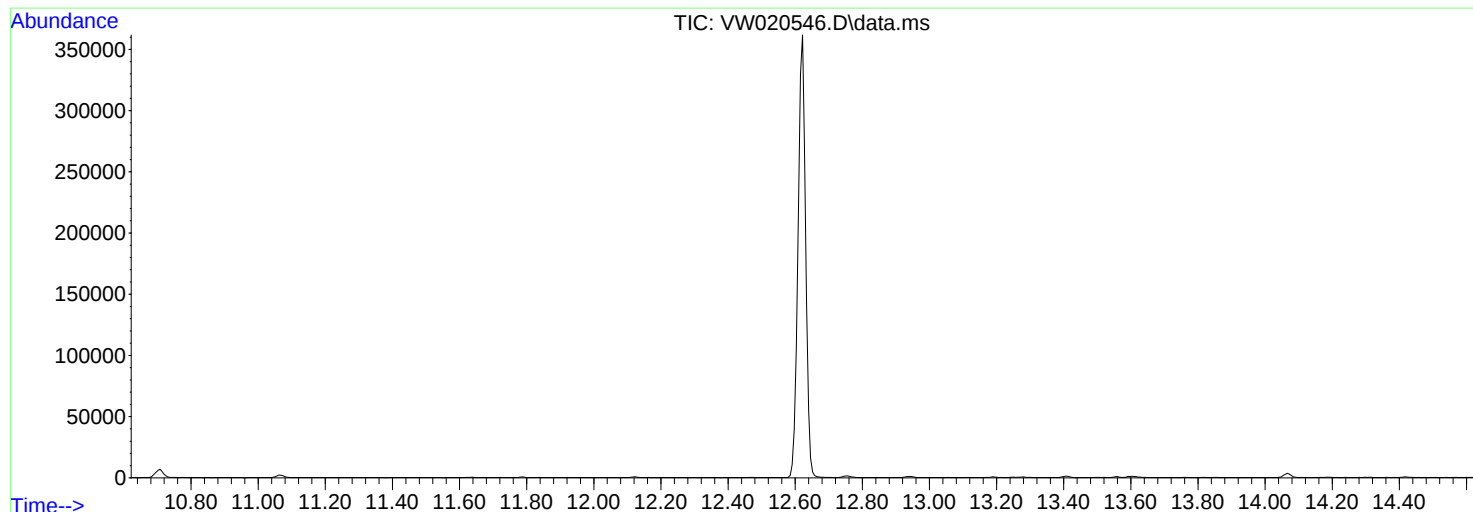

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	14125	PASS
75	95	30	80	54.6	34781	PASS
95	95	100	100	100.0	63752	PASS
96	95	5	9	6.6	4219	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.3	46699	PASS
175	174	5	9	8.2	3850	PASS
176	174	95	105	99.0	46251	PASS
177	176	5	10	6.2	2872	PASS

m/z	Abundance
36.00	781.0
37.10	4592.0
38.00	3944.0
39.00	1668.0
40.00	186.0
42.90	54.0
44.10	681.0
45.00	731.0
46.00	122.0
47.10	991.0
48.00	565.0
49.10	3481.0
50.10	15881.0
51.10	4793.0
52.00	219.0
53.00	109.0
55.00	198.0
56.00	1333.0
57.00	2277.0
58.10	139.0
60.10	775.0
61.00	3839.0
62.00	4108.0
63.00	3272.0
64.10	499.0
65.00	599.0
67.00	265.0
68.00	7984.0
69.00	7864.0
70.10	640.0
72.00	471.0
73.00	3529.0
74.00	13553.0
75.00	38928.0
76.00	3270.0
77.00	394.0
77.90	365.0
78.90	2812.0
79.90	766.0
81.00	2855.0
81.90	654.0
82.90	73.0
86.00	98.0
87.00	3152.0
88.00	2947.0
91.00	297.0
92.00	2272.0
93.00	3351.0
94.00	8694.0
95.00	73848.0
96.10	4711.0
97.10	172.0
104.00	336.0
104.90	110.0
105.90	420.0
107.00	59.0
109.70	52.0
110.90	91.0
112.90	88.0
114.90	63.0
115.90	294.0
116.90	517.0
117.90	290.0
118.90	475.0
127.90	285.0
128.90	100.0
130.00	257.0
130.90	123.0
132.90	84.0
133.90	62.0
135.00	120.0
137.00	123.0
140.00	72.0
140.90	771.0
142.10	133.0
143.00	961.0
145.00	278.0
146.00	114.0
146.90	53.0
147.90	175.0
150.00	106.0
153.00	62.0
154.90	207.0
157.00	131.0
158.90	92.0
161.00	106.0
170.90	177.0
172.00	821.0
174.00	52440.0
175.00	4093.0
175.90	52288.0
177.00	3198.0

Instrument :
MSVOA_W
ClientSampleId :
BFB454

177.90	76.0
192.90	93.0
207.10	81.0
248.90	66.0
265.10	94.0
281.00	877.0
282.00	296.0
283.10	166.0

Instrument :
MSVOA_W
ClientSampleId :
BFB454

m/z	Abundance
36.00	548.0
37.00	3089.0
38.00	2567.0
39.00	1271.0
40.00	156.0
44.00	509.0
45.10	550.0
46.20	90.0
47.00	702.0
48.00	406.0
49.00	2494.0
50.10	11233.0
51.00	3315.0
52.10	132.0
53.10	55.0
54.90	183.0
56.00	951.0
57.00	1526.0
58.20	59.0
60.00	541.0
61.00	2969.0
62.00	2734.0
63.00	2390.0
64.00	386.0
65.10	508.0
68.00	5434.0
69.00	5766.0
70.00	464.0
72.00	370.0
73.00	2708.0
74.00	9444.0
75.00	28440.0
76.10	2328.0
77.00	309.0
77.70	158.0
78.90	2042.0
80.00	547.0
81.00	2008.0
81.90	423.0
87.00	2232.0
88.00	2071.0
91.00	248.0
92.00	1609.0
93.00	2364.0
94.00	6867.0
95.00	51856.0
96.00	3598.0
97.10	125.0
103.90	281.0
105.00	89.0
105.90	223.0
115.00	70.0
115.90	196.0
117.00	399.0
118.00	249.0
118.90	317.0
127.80	198.0
128.90	132.0
129.90	241.0
130.90	117.0
135.00	111.0
137.10	101.0
141.00	647.0
142.00	124.0
143.00	751.0
143.90	71.0
145.00	178.0
146.00	67.0
148.00	104.0
150.10	71.0
154.80	126.0
156.90	111.0
158.80	57.0
160.90	75.0
170.90	109.0
172.00	608.0
174.00	41840.0
175.00	3644.0
176.00	44144.0
177.00	2670.0
177.90	82.0
207.10	57.0
281.00	390.0
282.00	134.0
283.10	95.0

Instrument :
MSVOA_W
ClientSampleId :
BFB454

m/z	Abundance
40.00	101.0
44.00	148.0
57.00	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB454

m/z	Abundance
36.00	797.0
37.00	4552.0
38.00	3875.0
39.00	1687.0
40.00	190.0
42.90	67.0
44.10	641.0
45.00	691.0
45.90	137.0
47.10	1043.0
48.00	499.0
49.00	3428.0
50.00	15262.0
51.00	4931.0
52.00	196.0
52.90	142.0
54.90	237.0
56.00	1219.0
57.00	2230.0
58.00	110.0
60.00	792.0
61.00	3843.0
62.00	3937.0
63.00	3274.0
64.00	495.0
65.00	726.0
65.90	90.0
67.20	203.0
68.00	7380.0
69.00	7582.0
70.00	663.0
72.00	419.0
73.00	3419.0
74.00	12709.0
75.00	36976.0
76.00	3028.0
77.00	368.0
77.80	213.0
78.90	2997.0
80.00	727.0
80.90	3002.0
82.00	612.0
82.90	68.0
85.80	122.0
87.00	2772.0
88.00	2658.0
91.00	317.0
92.10	2127.0
93.00	3174.0
94.00	8009.0
95.00	65552.0
96.10	4348.0
97.10	155.0
103.90	326.0
105.00	100.0
105.90	322.0
106.90	82.0
110.80	68.0
113.00	61.0
114.80	93.0
116.00	217.0
116.90	539.0
118.00	241.0
119.00	412.0
124.90	70.0
127.90	165.0
128.80	152.0
129.90	233.0
131.00	82.0
133.10	151.0
133.80	63.0
135.10	133.0
137.00	115.0
140.00	60.0
141.00	599.0
142.90	922.0
145.00	373.0
145.90	82.0
146.90	83.0
147.90	119.0
149.90	86.0
153.00	63.0
154.90	110.0
157.00	116.0
158.90	80.0
160.90	95.0
170.90	177.0
171.90	784.0
174.00	45816.0
175.00	3812.0
176.00	42320.0
177.00	2747.0

Instrument :
MSVOA_W
ClientSampleId :
BFB454

178.10	85.0
191.00	200.0
193.00	167.0
207.10	125.0
248.90	94.0
265.00	169.0
267.00	64.0
281.10	1458.0
282.10	416.0
283.00	279.0

Instrument :
MSVOA_W
ClientSampleId :
BFB454