

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\WV101918\
 Data File : VW006239.D
 Acq On : 19 Oct 2018 21:21
 Operator : VA/AP
 Sample : J5604-03
 Misc : 4.98G/5ML/MSVOA W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 MS-VB-25868-BOX-1

Quant Time: Oct 20 01:22:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 18 17:01:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	141936	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	227200	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	136464	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	43580	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	90601	76.99	ug/l	0.00
Spiked Amount			Recovery	=	153.98%	
35) Dibromofluoromethane	7.89	113	79727	59.39	ug/l	0.00
Spiked Amount			Recovery	=	118.78%	
50) Toluene-d8	10.33	98	192703	37.73	ug/l	0.00
Spiked Amount			Recovery	=	75.46%	
62) 4-Bromofluorobenzene	12.62	95	50770	26.47	ug/l	0.00
Spiked Amount			Recovery	=	52.94%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	5.24	59	568	7.177	ug/l #	71
16) Acetone	4.16	43	40635	179.917	ug/l	100
18) Methyl Acetate	4.68	43	694	1.172	ug/l #	73
20) Methylene Chloride	4.92	84	6646	3.835	ug/l	91
25) 2-Butanone	7.20	43	8528	26.827	ug/l	95
29) Tetrahydrofuran	7.55	42	976	4.995	ug/l #	87
31) Cyclohexane	7.96	56	4747	2.205	ug/l #	46
36) 1,1-Dichloropropene	7.95	75	9120	4.355	ug/l #	49
37) Ethyl Acetate	7.20	43	8528	10.961	ug/l #	67
38) Carbon Tetrachloride	7.95	117	12959	5.645	ug/l #	17
39) Methylcyclohexane	9.34	83	6236	2.240	ug/l	92
40) Benzene	8.32	78	112212	19.534	ug/l	98
51) 4-Methyl-2-Pentanone	10.23	43	2399	3.010	ug/l	95
52) Toluene	10.39	92	104391	27.106	ug/l	99
55) 1,1,2-Trichloroethane	10.77	97	1137	1.037	ug/l #	32
58) 2-Chloroethyl Vinyl ether	9.93	63	785	1.529	ug/l #	84
59) 2-Hexanone	10.98	43	844	1.483	ug/l	87
67) Ethyl Benzene	11.74	91	30161	5.957	ug/l	97
68) m/p-Xylenes	11.84	106	58404	29.187	ug/l	100
69) o-Xylene	12.17	106	39581	20.755	ug/l	100
70) Styrene	12.18	104	8953	2.887	ug/l #	33
73) Isopropylbenzene	12.47	105	16716	5.429	ug/l	90
74) N-amyl acetate	12.26	43	4422	7.395	ug/l #	58
75) 1,1,2,2-Tetrachloroethane	12.69	83	4255	9.087	ug/l #	29
76) 1,2,3-Trichloropropane	12.62	75	25292	75.983	ug/l #	100
77) Bromobenzene	12.95	156	29826	39.552	ug/l #	1
78) n-propylbenzene	12.81	91	14465	4.038	ug/l	93
79) 2-Chlorotoluene	13.11	91	4103	2.039	ug/l	76
80) 1,3,5-Trimethylbenzene	12.95	105	29692	11.440	ug/l	98
81) trans-1,4-Dichloro-2-buten	12.62	75	25292	181.629	ug/l #	12
82) 4-Chlorotoluene	13.11	91	3898	1.849	ug/l	77
83) tert-Butylbenzene	13.21	119	95387	41.076	ug/l	96
84) 1,2,4-Trimethylbenzene	13.26	105	71861	27.361	ug/l	100
85) sec-Butylbenzene	13.39	105	10064	3.068	ug/l	78

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW101918\
Data File : VW006239.D
Acq On : 19 Oct 2018 21:21
Operator : VA/AP
Sample : J5604-03
Misc : 4.98G/5ML/MSVOA W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1

Quant Time: Oct 20 01:22:29 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 18 17:01:24 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
86) p-Isopropyltoluene	13.51	119	23160	7.805	ug/l	95
88) 1,4-Dichlorobenzene	13.58	146	3871	2.591	ug/l #	51
89) n-Butylbenzene	13.83	91	9364	3.451	ug/l #	69
90) Hexachloroethane	14.10	117	3385	6.735	ug/l #	4
92) 1,2-Dibromo-3-Chloropropan	14.51	75	192	2.290	ug/l #	14
95) Naphthalene	15.38	128	142104	82.933	ug/l	95
96) 1,2,3-Trichlorobenzene	15.59	180	2172	2.438	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW101918\
Data File : VW006239.D
Acq On : 19 Oct 2018 21:21
Operator : VA/AP
Sample : J5604-03
Misc : 4.98G/5ML/MSVOA W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1

Quant Time: Oct 20 01:22:29 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 18 17:01:24 2018
Response via : Initial Calibration

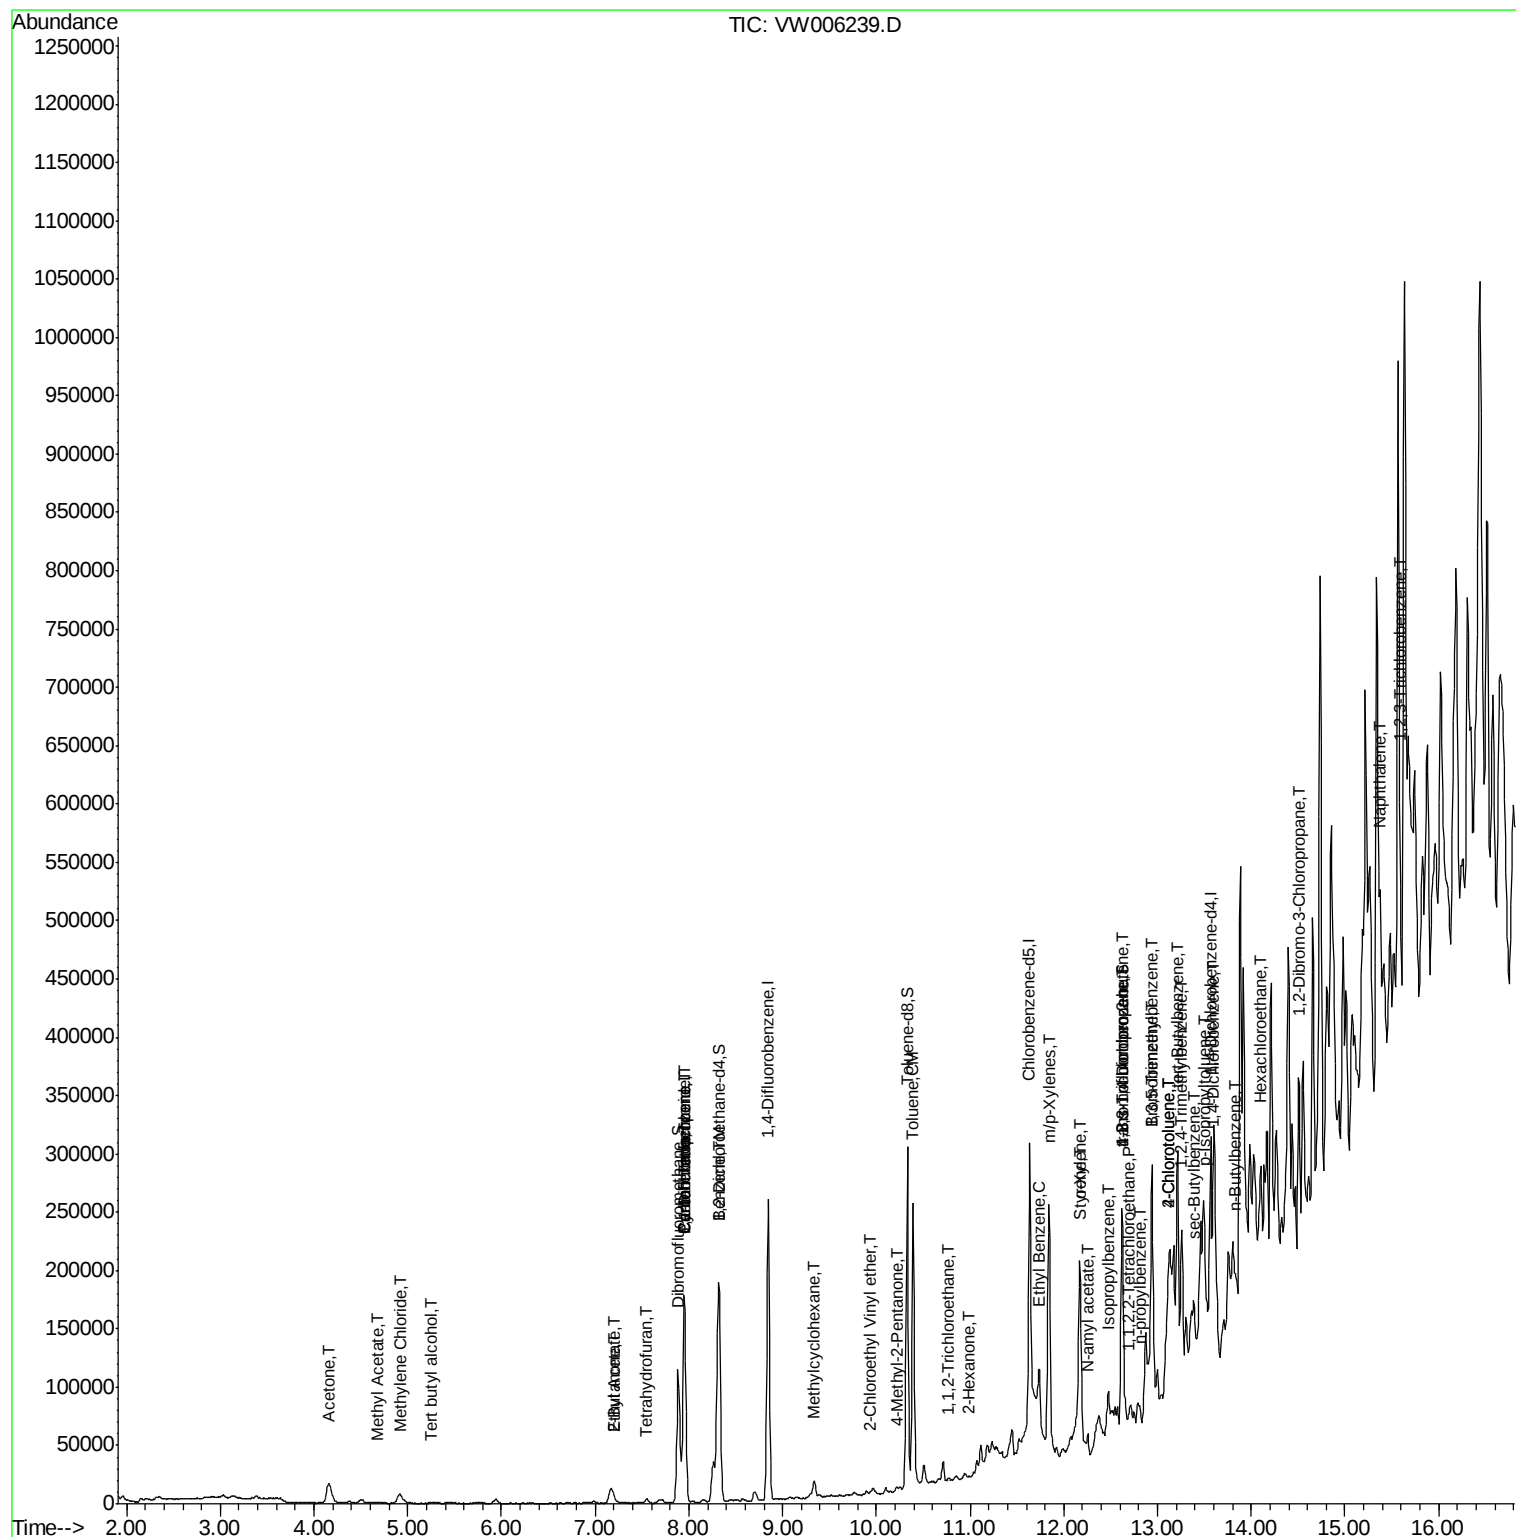

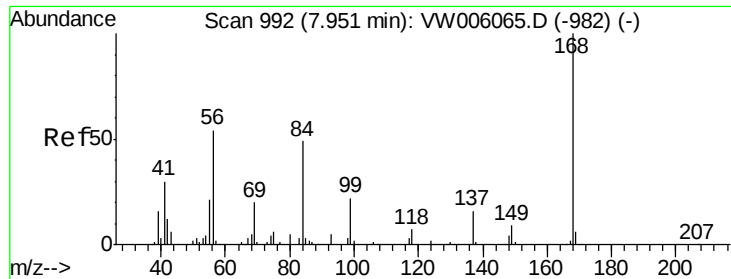

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :


MS-VB-25868-BOX-1

Tot Ion:168 Resp: 141936

Ion Ratio Lower Upper




168 100

99 49.4 39.9 59.9



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

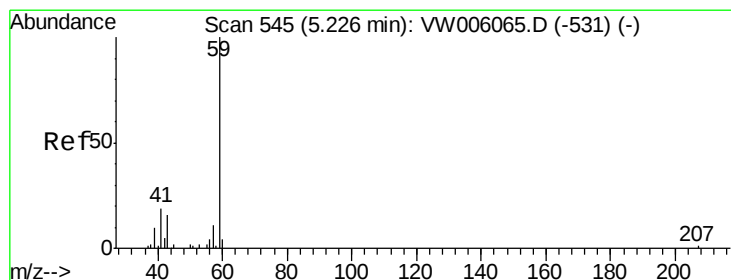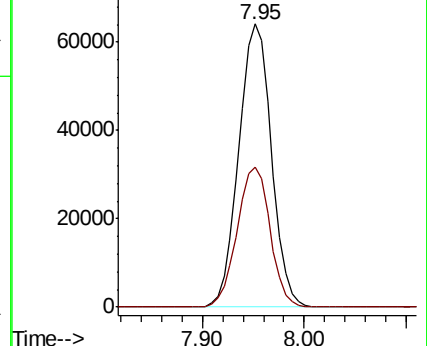

#11

Tert butyl alcohol

Concen: 7.177 ug/l

RT: 5.24 min Scan# 548

Delta R.T. 0.02 min

Lab File: VW006239.D


Acq: 19 Oct 2018 21:21

Tgt Ion: 59 Resp: 568

Ion Ratio Lower Upper



59 100


57 0.0 8.7 13.1#

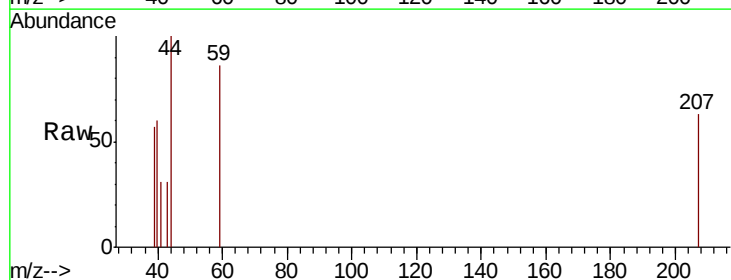

Abundance Ion 59.00 (58.70 to 59.70): VW

Ion 57.00 (56.70 to 57.70): VW




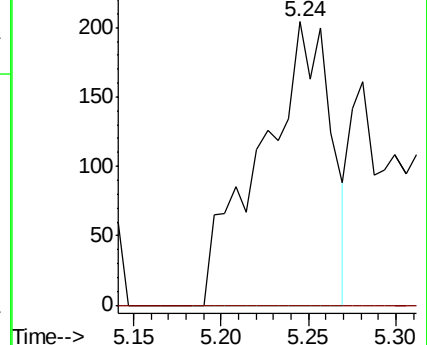




#16
Acetone
Concen: 179.917 ug/l
RT: 4.16 min Scan# 370
Delta R.T. 0.01 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21




Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1




Tot Ion: 43 Resp: 40635
Ion Ratio Lower Upper
43 100
58 29.8 24.0 36.0

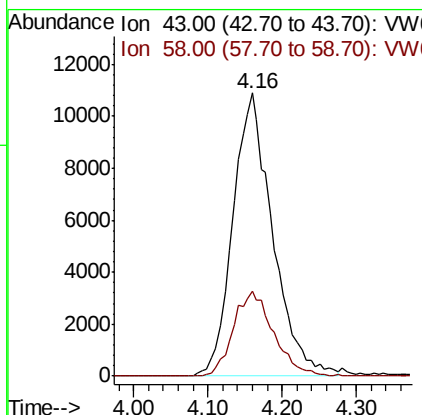

#18
Methyl Acetate
Concen: 1.172 ug/l
RT: 4.68 min Scan# 455
Delta R.T. -0.01 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion: 43 Resp: 694
Ion Ratio Lower Upper
43 100
74 11.8 20.5 30.7#



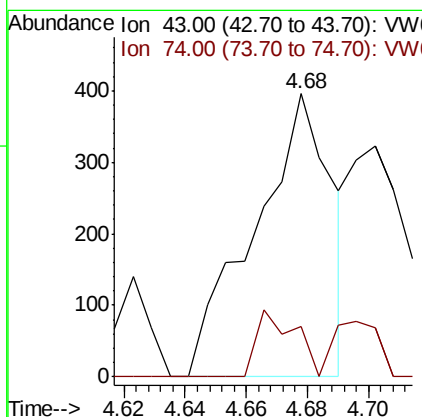





#20
Methvlene Chloride
Concen: 3.835 ug/l
RT: 4.92 min Scan# 494
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21


Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1


Tot Ion: 84 Resp: 6646
Ion Ratio Lower Upper
84 100
49 109.4 93.6 140.4
51 40.4 29.0 43.4
86 54.5 52.6 79.0

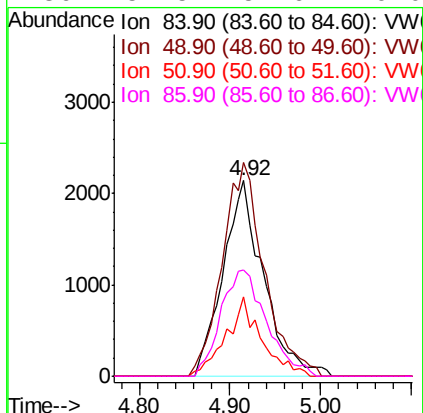

#25
2-Butanone
Concen: 26.827 ug/l
RT: 7.20 min Scan# 869
Delta R.T. 0.02 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion: 43 Resp: 8528
Ion Ratio Lower Upper
43 100
72 31.0 22.8 34.2

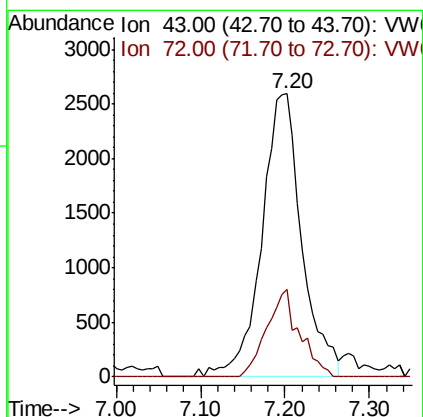



#29

Tetrahydrofuran

Concen: 4.995 ug/l

RT: 7.55 min Scan# 926

Delta R.T. 0.01 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampled :

MS-VB-25868-BOX-1


Tot Ion: 42 Resp: 976

Ion Ratio Lower Upper




42 100

72 35.1 38.0 57.0#

71 40.1 35.3 52.9



Abundance Ion 42.00 (41.70 to 42.70): VW
Ion 72.00 (71.70 to 72.70): VW
Ion 71.00 (70.70 to 71.70): VW

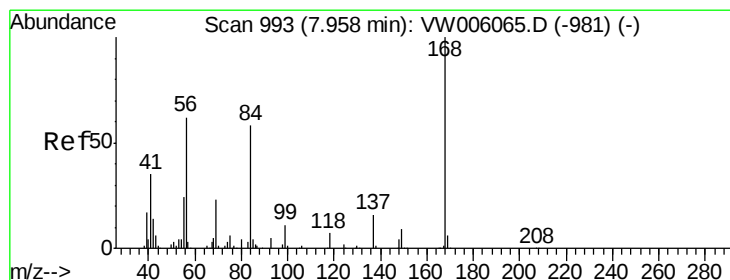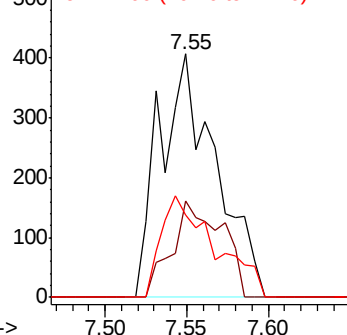

#31

Cyclohexane

Concen: 2.205 ug/l

RT: 7.96 min Scan# 993

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21


Tgt Ion: 56 Resp: 4747

Ion Ratio Lower Upper



56 100


69 112.5 29.4 44.0#

84 116.7 74.0 111.0#



Abundance Ion 56.00 (55.70 to 56.70): VW
Ion 69.00 (68.70 to 69.70): VW
Ion 84.00 (83.70 to 84.70): VW




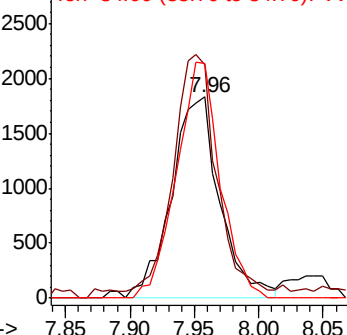




#33
 1,2-Dichloroethane-d4
 Concen: 76.994 ug/l
 RT: 8.31 min Scan# 1051
 Delta R.T. 0.00 min
 Lab File: VW006239.D
 Acq: 19 Oct 2018 21:21




Instrument :
 MSVOA_W
 ClientSampleId :
 MS-VB-25868-BOX-1


Tot Ion: 65 Resp: 90601
 Ion Ratio Lower Upper
 65 100
 67 51.9 0.0 101.0

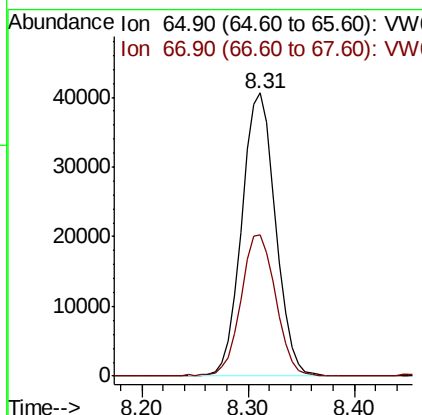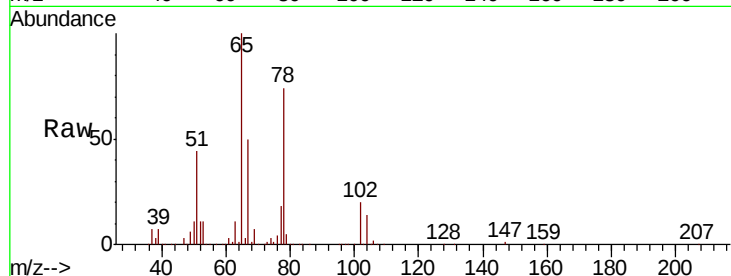

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. 0.00 min
 Lab File: VW006239.D
 Acq: 19 Oct 2018 21:21

Tgt Ion: 114 Resp: 227200
 Ion Ratio Lower Upper
 114 100
 63 18.5 0.0 36.8
 88 14.6 0.0 29.0

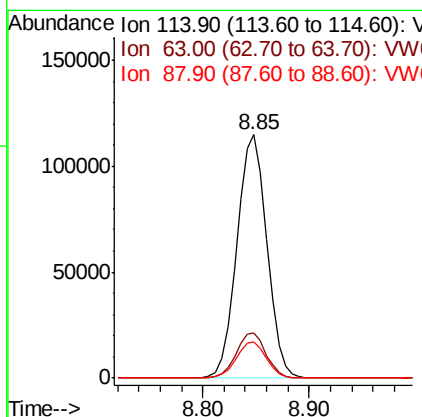

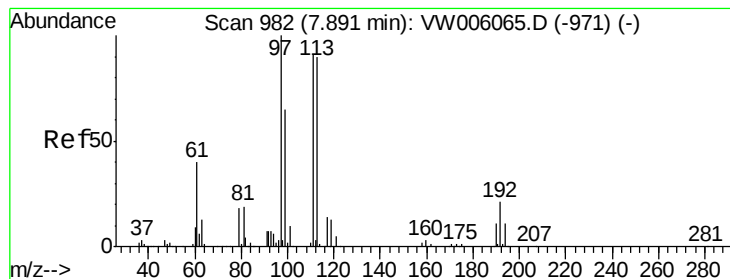

#35

Dibromofluoromethane

Concen: 59.386 ug/l

RT: 7.89 min Scan# 982

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :

MS-VB-25868-BOX-1


Tot Ion:113 Resp: 79727

Ion Ratio Lower Upper

113 100

111 101.5 81.4 122.0




192 22.9 18.7 28.1



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

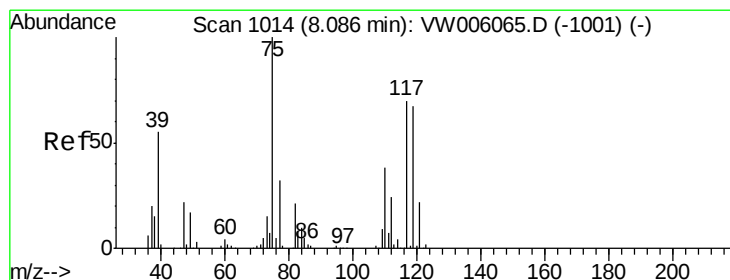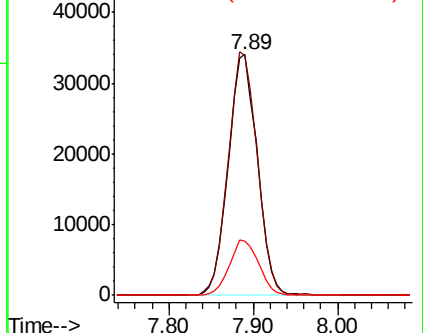

#36

1,1-Dichloropropene

Concen: 4.355 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.14 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21


Tgt Ion: 75 Resp: 9120

Ion Ratio Lower Upper

75 100

110 10.1 19.1 57.1#



77 0.0 25.0 37.4#




Abundance Ion 74.90 (74.60 to 75.60): VW

Ion 109.90 (109.60 to 110.60): V

Ion 76.90 (76.60 to 77.60): VW



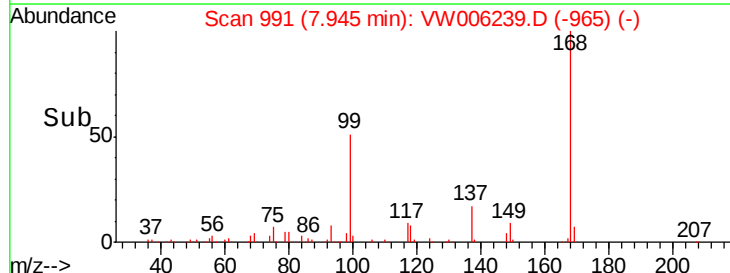
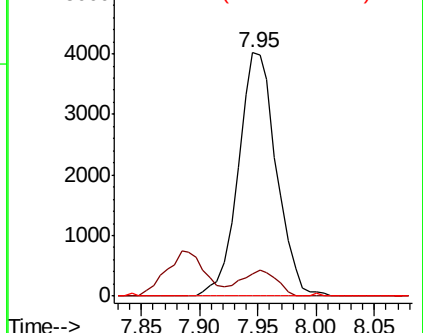




#37
Ethyl Acetate
Concen: 10.961 ug/l
RT: 7.20 min Scan# 869
Delta R.T. -0.06 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21




Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1


Tot Ion: 43 Resp: 8528
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 9.2 13.8#

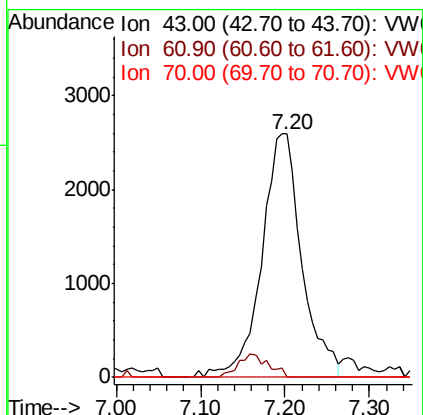

#38
Carbon Tetrachloride
Concen: 5.645 ug/l
RT: 7.95 min Scan# 992
Delta R.T. -0.12 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion: 117 Resp: 12959
Ion Ratio Lower Upper
117 100
119 5.8 75.2 112.8#
121 0.0 25.3 37.9#

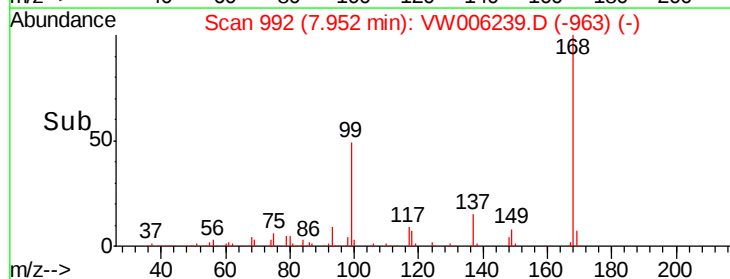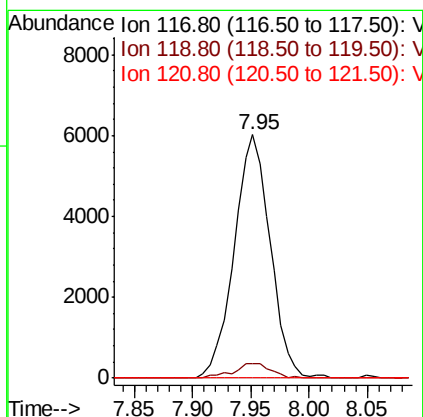







#39
Methvlcvclohexane
Concen: 2.240 ug/l
RT: 9.34 min Scan# 1219
Delta R.T. -0.01 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1

Tot Ion: 83 Resp: 6236
Ion Ratio Lower Upper
83 100
55 78.4 55.0 82.6
98 50.0 38.6 57.8




Abundance Ion 83.00 (82.70 to 83.70): VW
Ion 55.00 (54.70 to 55.70): VW
Ion 98.00 (97.70 to 98.70): VW


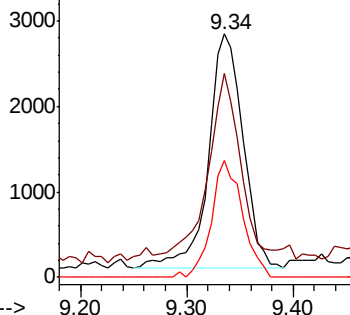



#40
Benzene
Concen: 19.534 ug/l
RT: 8.32 min Scan# 1053
Delta R.T. -0.01 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion: 78 Resp: 112212
Ion Ratio Lower Upper
78 100
77 23.2 19.4 29.0



Abundance Ion 78.00 (77.70 to 78.70): VW
Ion 77.00 (76.70 to 77.70): VW

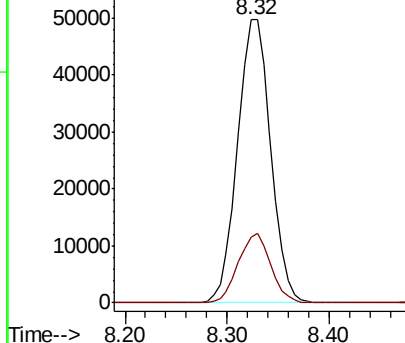



#50

Toluene-d8

Concen: 37.729 ug/l

RT: 10.33 min Scan# 1382

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :


MS-VB-25868-BOX-1

Tot Ion: 98 Resp: 192703

Ion Ratio Lower Upper




98 100

100 63.7 51.6 77.4



Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

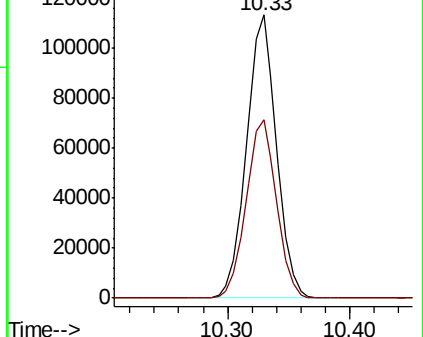

#51

4-Methyl-2-Pentanone

Concen: 3.010 ug/l

RT: 10.23 min Scan# 1365

Delta R.T. 0.01 min

Lab File: VW006239.D


Acq: 19 Oct 2018 21:21

Tgt Ion: 43 Resp: 2399

Ion Ratio Lower Upper



43 100


58 42.7 31.5 47.3



Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

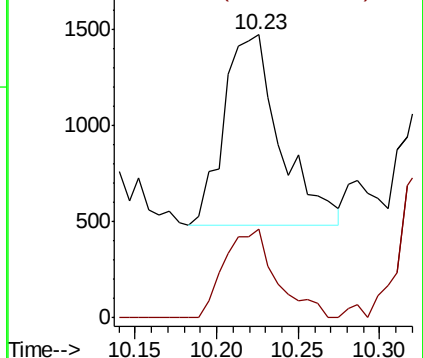

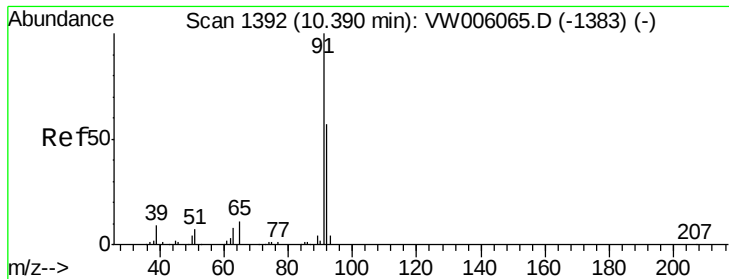

#52

Toluene

Concen: 27.106 ug/l

RT: 10.39 min Scan# 1392

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :


MS-VB-25868-BOX-1

Tot Ion: 92 Resp: 104391

Ion Ratio Lower Upper




92 100

91 173.8 140.0 210.0

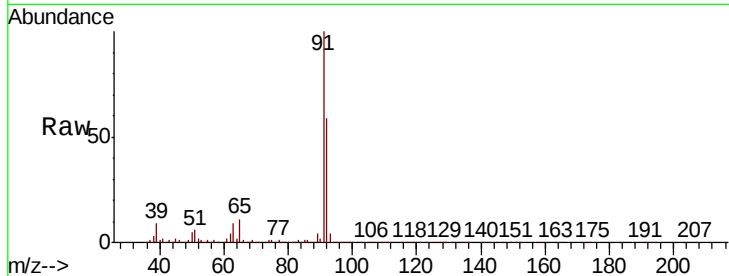

Abundance Ion 92.00 (91.70 to 92.70): VW

Ion 91.00 (90.70 to 91.70): VW

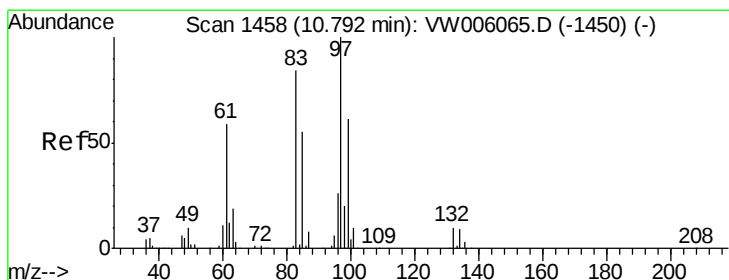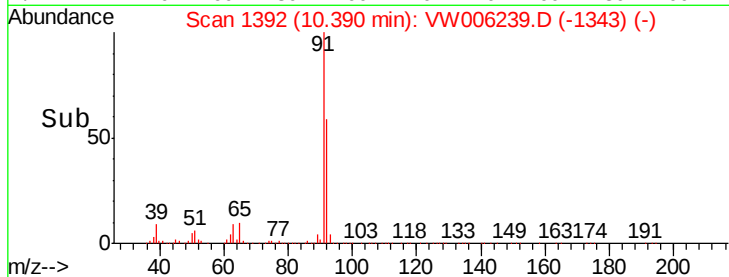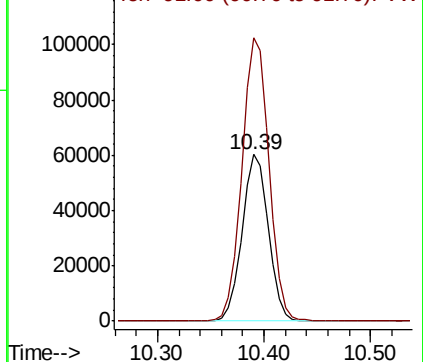

#55

1,1,2-Trichloroethane

Concen: 1.037 ug/l

RT: 10.77 min Scan# 1454

Delta R.T. -0.02 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Tgt Ion: 97 Resp: 1137


Ion Ratio Lower Upper

97 100

83 8.5 67.2 100.8#

85 22.3 43.7 65.5#

99 10.3 48.5 72.7#


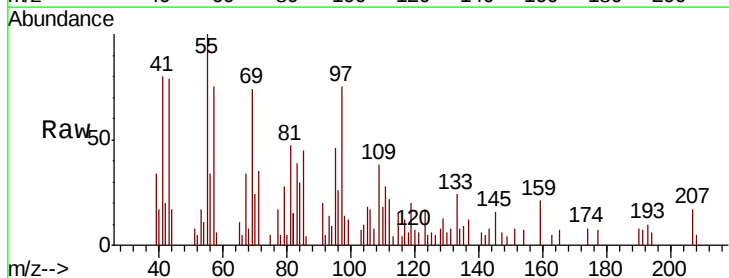



Abundance Ion 96.90 (96.60 to 97.60): VW

Ion 82.90 (82.60 to 83.60): VW

Ion 84.90 (84.60 to 85.60): VW

Ion 98.90 (98.60 to 99.60): VW



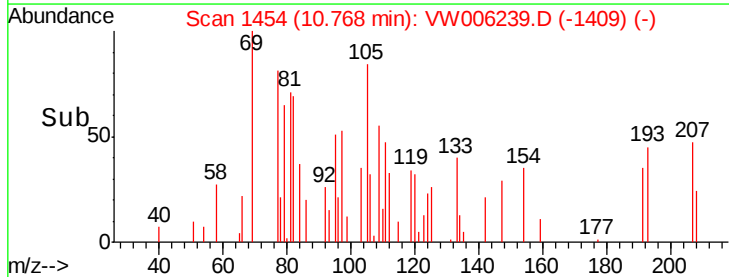
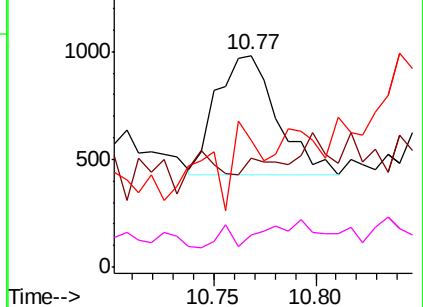




#58
 2-Chloroethyl Vinyl ether
 Concen: 1.529 ug/l
 RT: 9.93 min Scan# 1316
 Delta R.T. 0.00 min
 Lab File: VW006239.D
 Acq: 19 Oct 2018 21:21




Instrument :
 MSVOA_W
 ClientSampleId :
 MS-VB-25868-BOX-1


Tot Ion: 63 Resp: 785
 Ion Ratio Lower Upper
 63 100
 106 21.9 24.5 36.7#

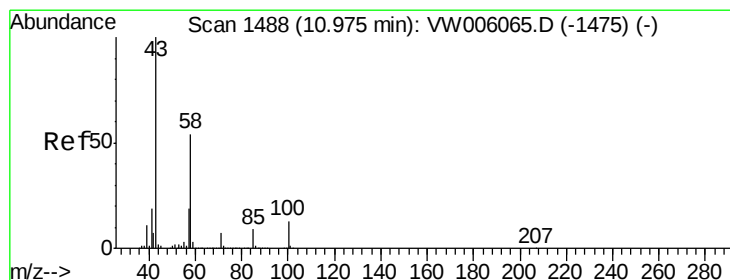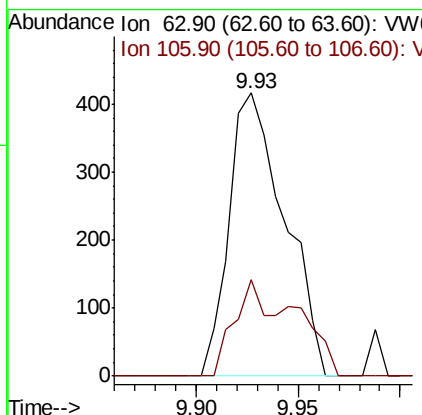

#59
 2-Hexanone
 Concen: 1.483 ug/l
 RT: 10.98 min Scan# 1489
 Delta R.T. 0.01 min
 Lab File: VW006239.D
 Acq: 19 Oct 2018 21:21

Tgt Ion: 43 Resp: 844
 Ion Ratio Lower Upper
 43 100
 58 62.7 26.9 80.6

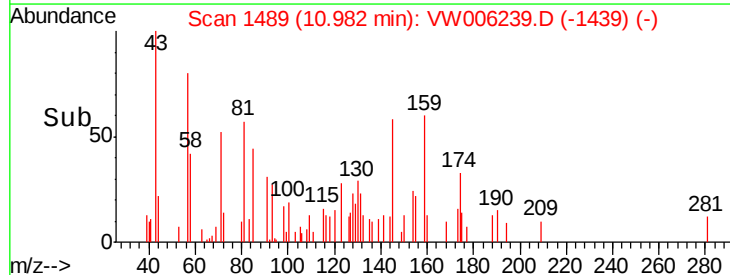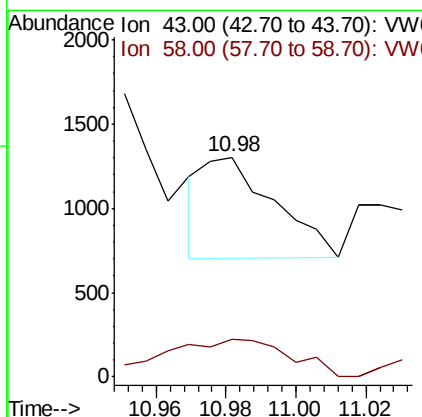



#62

4-Bromofluorobenzene

Concen: 26.465 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :

MS-VB-25868-BOX-1


Tot Ion: 95 Resp: 50770

Ion Ratio Lower Upper

95 100

174 90.4 0.0 186.0




176 89.4 0.0 181.6



Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

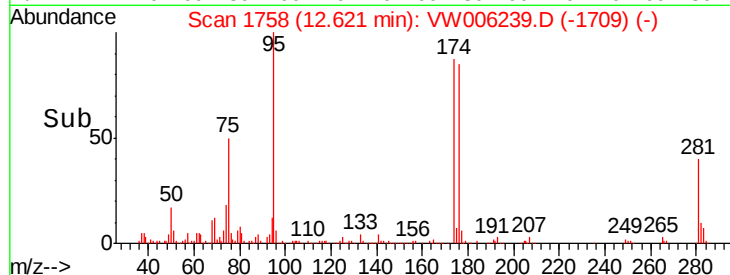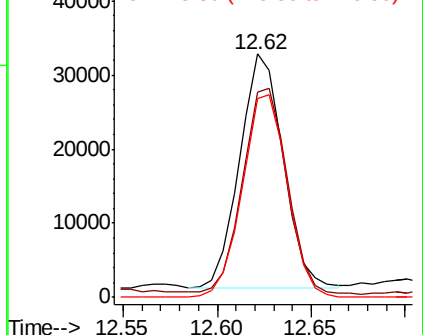

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21


Tgt Ion: 117 Resp: 136464

Ion Ratio Lower Upper

117 100

82 52.7 42.1 63.1



119 32.2 25.8 38.6




Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW




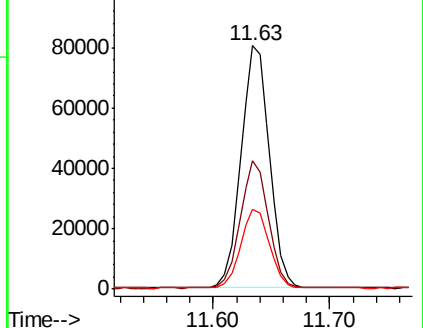




#67
Ethyl Benzene
Concen: 5.957 ug/l
RT: 11.74 min Scan# 1613
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21




Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1


Tot Ion: 91 Resp: 30161
Ion Ratio Lower Upper
91 100
106 31.0 26.1 39.1

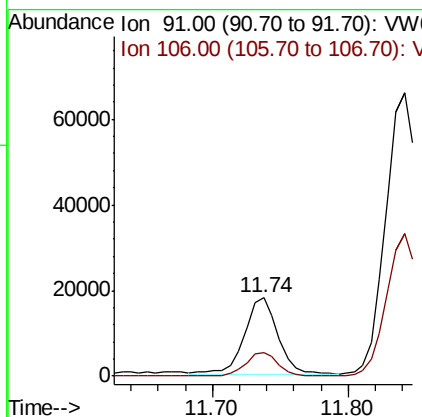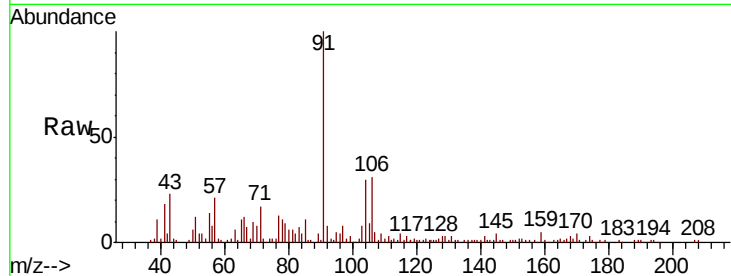

#68
m/p-Xylenes
Concen: 29.187 ug/l
RT: 11.84 min Scan# 1630
Delta R.T. -0.01 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion: 106 Resp: 58404
Ion Ratio Lower Upper
106 100
91 199.4 159.1 238.7

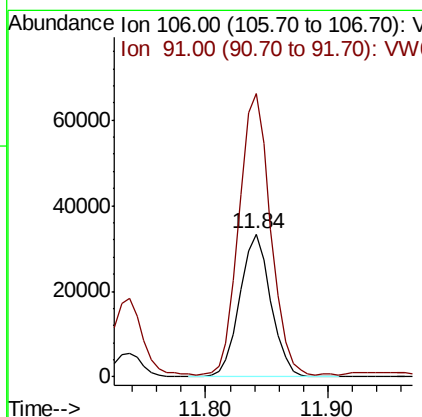







#69
o-Xylene
Concen: 20.755 ug/l
RT: 12.17 min Scan# 1684
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1

Tot Ion:106 Resp: 39581
Ion Ratio Lower Upper
106 100
91 210.5 105.4 316.1




Abundance Ion 106.00 (105.70 to 106.70): V
Ion 91.00 (90.70 to 91.70): VW


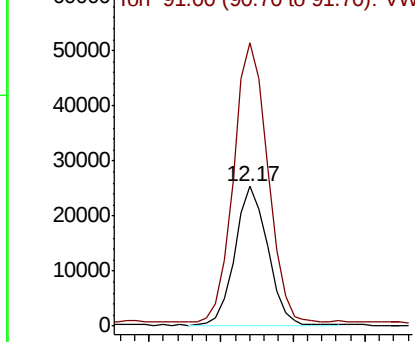



#70
Styrene
Concen: 2.887 ug/l
RT: 12.18 min Scan# 1686
Delta R.T. -0.01 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion:104 Resp: 8953
Ion Ratio Lower Upper
104 100
78 99.5 39.1 58.7#
103 99.3 44.3 66.5#



Abundance Ion 104.00 (103.70 to 104.70): V
Ion 78.00 (77.70 to 78.70): VW
Ion 103.00 (102.70 to 103.70): V

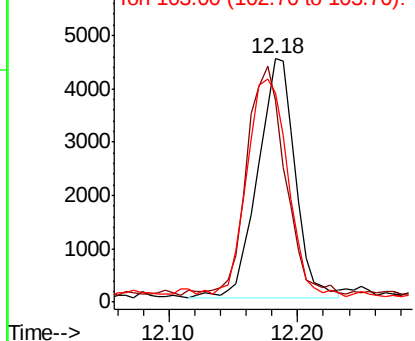







#72

1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.57 min Scan# 1913
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1




Tot Ion:152 Resp: 43580
Ion Ratio Lower Upper
152 100
115 67.5 27.8 83.3
150 148.9 0.0 349.2

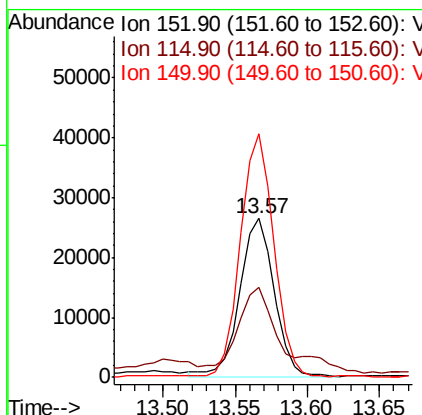


#73

Isopropylbenzene
Concen: 5.429 ug/l
RT: 12.47 min Scan# 1733
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion:105 Resp: 16716
Ion Ratio Lower Upper
105 100
120 22.0 13.6 40.7

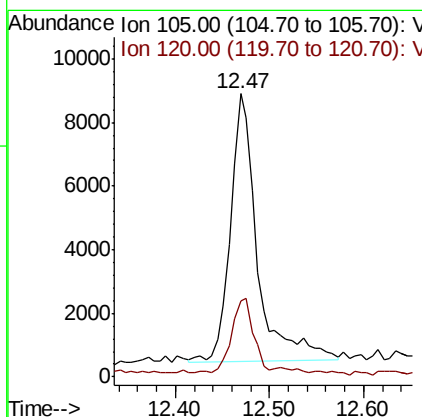



#74

N-amvl acetate

Concen: 7.395 ug/l

RT: 12.26 min Scan# 1698

Delta R.T. -0.02 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :

MS-VB-25868-BOX-1

Tot Ion: 43 Resp: 4422





Ion Ratio Lower Upper

43 100

70 10.6 34.2 51.4#

55 13.3 19.2 28.8#

61 0.0 19.0 28.6#

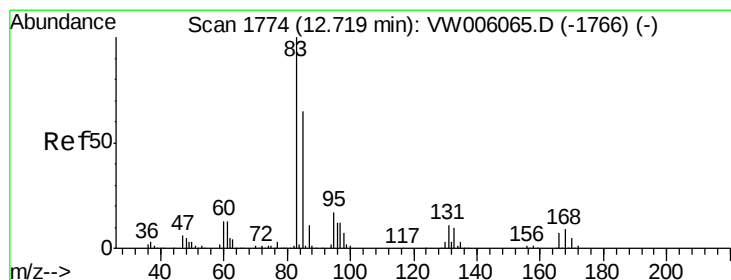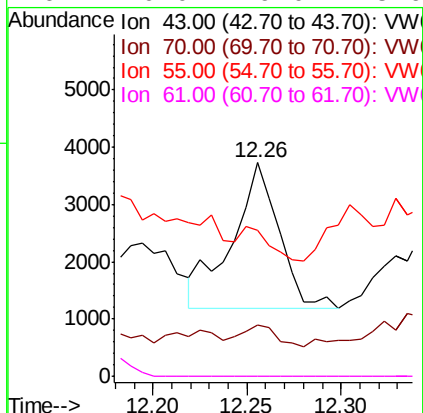

#75

1,1,2,2-Tetrachloroethane

Concen: 9.087 ug/l

RT: 12.69 min Scan# 1769

Delta R.T. -0.03 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21




Tgt Ion: 83 Resp: 4255


Ion Ratio Lower Upper

83 100

131 7.0 5.9 17.7

85 0.0 31.9 95.9#


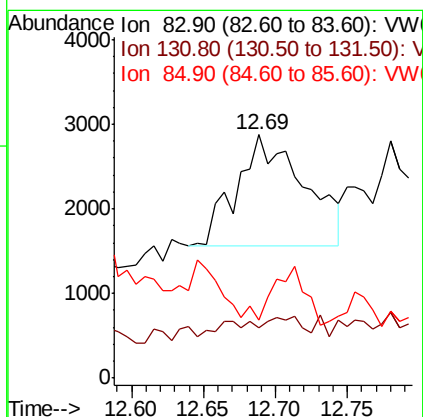




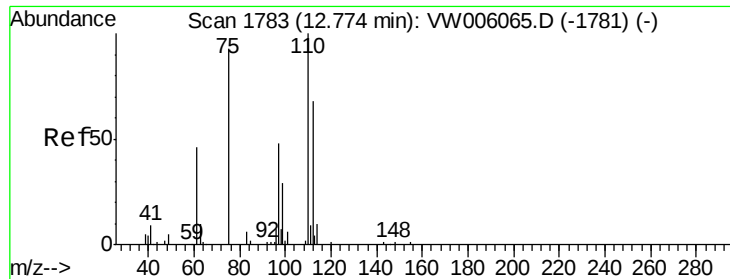

#76
 1,2,3-Trichloropropane
 Concen: 75.983 ug/l
 RT: 12.62 min Scan# 1758
 Delta R.T. -0.15 min
 Lab File: VW006239.D
 Acq: 19 Oct 2018 21:21




Instrument :
 MSVOA_W
 ClientSampleId :
 MS-VB-25868-BOX-1


Tot Ion: 75 Resp: 25292
 Ion Ratio Lower Upper
 75 100
 77 4.6 0.0 0.0#

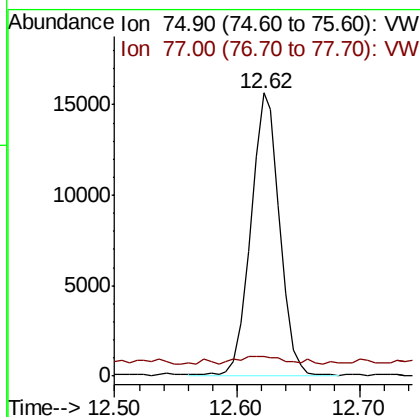

#77
 Bromobenzene
 Concen: 39.552 ug/l
 RT: 12.95 min Scan# 1812
 Delta R.T. 0.20 min
 Lab File: VW006239.D
 Acq: 19 Oct 2018 21:21

Tgt Ion: 156 Resp: 29826
 Ion Ratio Lower Upper
 156 100
 77 14.9 79.1 237.4#
 158 0.8 48.5 145.6#

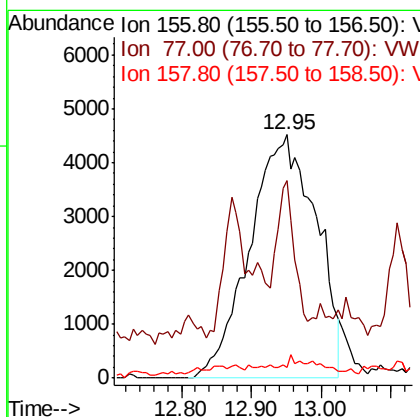

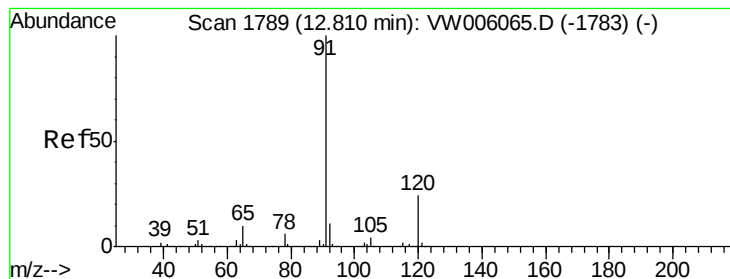

#78

n-propylbenzene

Concen: 4.038 ug/l

RT: 12.81 min Scan# 1789

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :


MS-VB-25868-BOX-1

Tot Ion: 91 Resp: 14465

Ion Ratio Lower Upper

91 100

120 21.0 12.2 36.6



Abundance Ion 91.00 (90.70 to 91.70): VW006065.D (-1783) (-)

Ion 120.00 (119.70 to 120.70): VW006065.D (-1783) (-)

12000

10000

8000

6000



4000

2000

0

12.75 12.80 12.85

Time-->



#79

2-Chlorotoluene

Concen: 2.039 ug/l

RT: 13.11 min Scan# 1838

Delta R.T. 0.21 min

Lab File: VW006239.D


Acq: 19 Oct 2018 21:21

Tgt Ion: 91 Resp: 4103

Ion Ratio Lower Upper

91 100

126 21.7 17.9 53.8



Abundance Ion 91.00 (90.70 to 91.70): VW006065.D (-1796) (-)

Ion 125.90 (125.60 to 126.60): VW006065.D (-1796) (-)

40000

30000


20000


10000

0

13.05 13.10 13.15

Time-->





#80

1,3,5-Trimethylbenzene

Concen: 11.440 ug/l

RT: 12.95 min Scan# 1812

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :





MS-VB-25868-BOX-1

Tot Ion:105 Resp: 29692

Ion Ratio Lower Upper

105 100

120 51.3 24.9 74.6

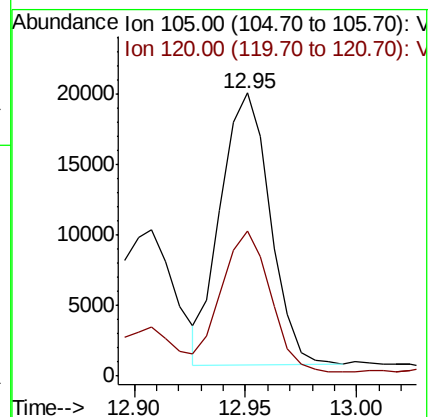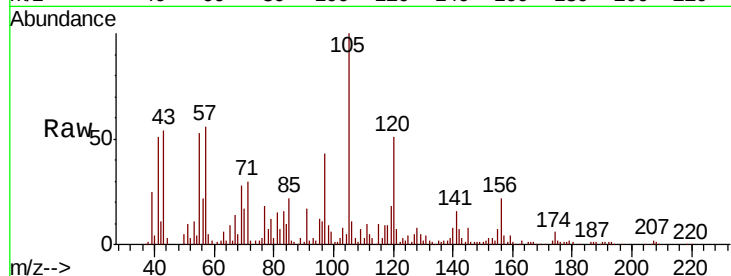

#81

trans-1,4-Dichloro-2-butene

Concen: 181.629 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.10 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21




Tgt Ion: 75 Resp: 25292


Ion Ratio Lower Upper

75 100

53 2.6 79.8 119.6#

89 1.3 37.5 56.3#



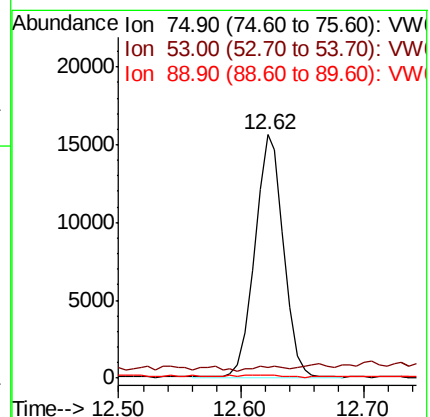





#82
4-Chlorotoluene
Concen: 1.849 ug/l
RT: 13.11 min Scan# 1838
Delta R.T. 0.12 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21




Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1


Tot Ion: 91 Resp: 3898
Ion Ratio Lower Upper
91 100
126 22.8 18.1 54.3

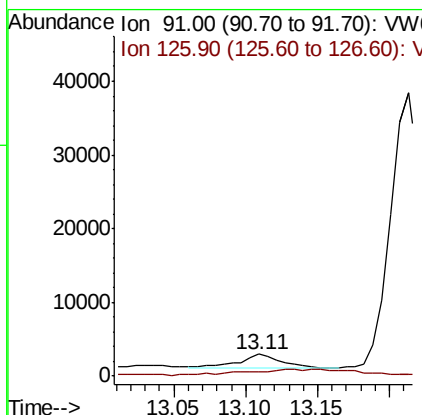

#83
tert-Butylbenzene
Concen: 41.076 ug/l
RT: 13.21 min Scan# 1855
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion: 119 Resp: 95387
Ion Ratio Lower Upper
119 100
91 62.7 32.3 96.9
134 23.8 13.6 40.8



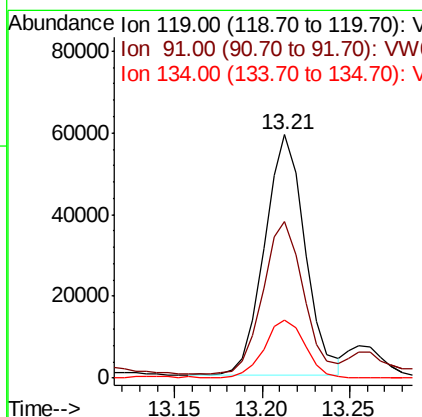





#84
 1,2,4-Trimethylbenzene
 Concen: 27.361 ug/l
 RT: 13.26 min Scan# 1862
 Delta R.T. 0.00 min
 Lab File: VW006239.D
 Acq: 19 Oct 2018 21:21




Instrument :
 MSVOA_W
 ClientSampleId :
 MS-VB-25868-BOX-1


Tot Ion:105 Resp: 71861
 Ion Ratio Lower Upper
 105 100
 120 46.4 23.1 69.3

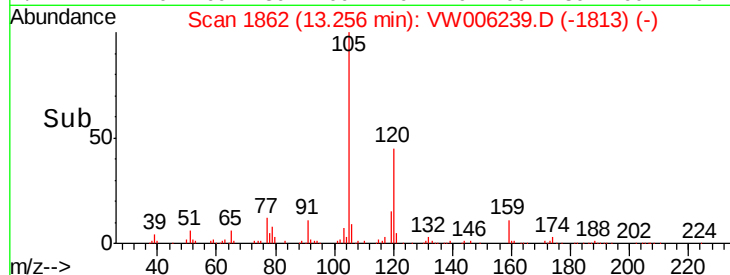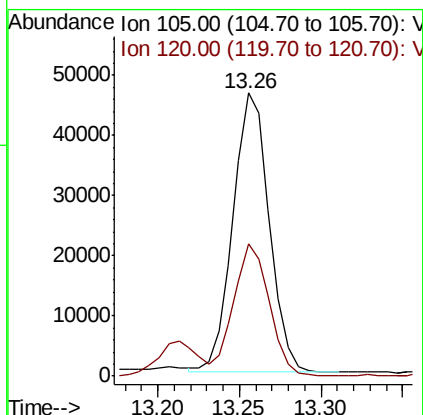

#85
 sec-Butylbenzene
 Concen: 3.068 ug/l
 RT: 13.39 min Scan# 1884
 Delta R.T. 0.00 min
 Lab File: VW006239.D
 Acq: 19 Oct 2018 21:21

Tgt Ion:105 Resp: 10064
 Ion Ratio Lower Upper
 105 100
 134 31.3 10.5 31.6



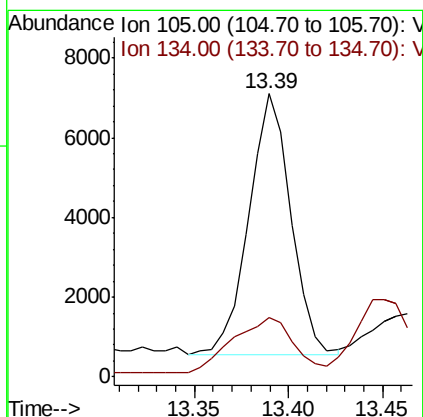





#86
p-Isopropyltoluene
Concen: 7.805 ug/l
RT: 13.51 min Scan# 1903
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21




Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1


Tot Ion:119 Resp: 23160
Ion Ratio Lower Upper
119 100
134 28.9 13.4 40.2
91 25.9 11.4 34.1

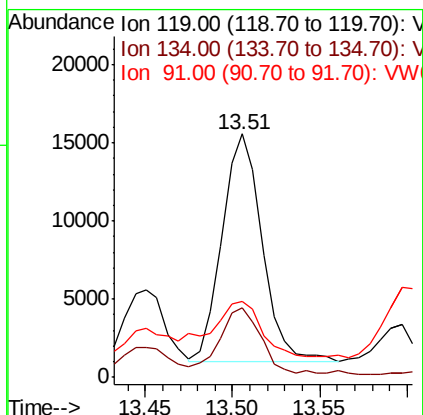

#88
1,4-Dichlorobenzene
Concen: 2.591 ug/l
RT: 13.58 min Scan# 1916
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion:146 Resp: 3871
Ion Ratio Lower Upper
146 100
111 106.9 18.6 56.0#
148 71.5 32.1 96.5


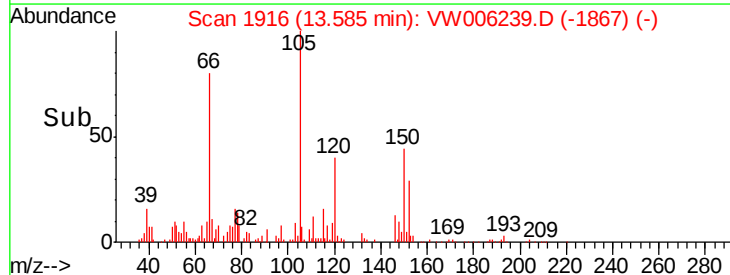
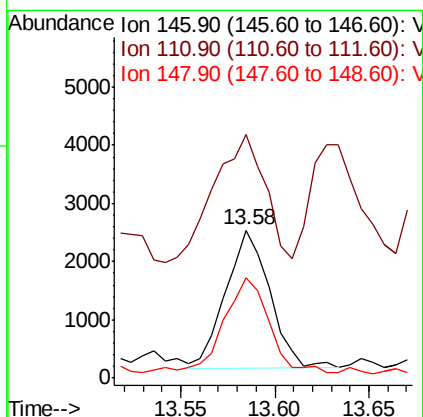





#89
n-Butylbenzene
Concen: 3.451 ug/l
RT: 13.83 min Scan# 1956
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21




Instrument :
MSVOA_W
ClientSampleId :
MS-VB-25868-BOX-1


Tot Ion: 91 Resp: 9364
Ion Ratio Lower Upper
91 100
92 67.0 26.6 79.7
134 0.0 14.0 41.9#

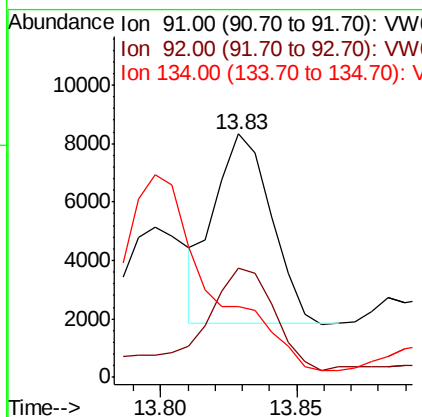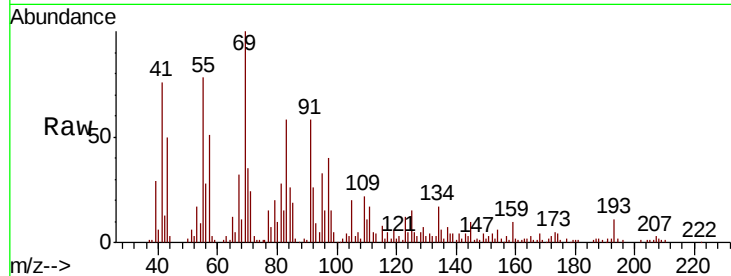

#90
Hexachloroethane
Concen: 6.735 ug/l
RT: 14.10 min Scan# 2001
Delta R.T. 0.00 min
Lab File: VW006239.D
Acq: 19 Oct 2018 21:21

Tgt Ion: 117 Resp: 3385
Ion Ratio Lower Upper
117 100
201 0.0 45.3 135.9#

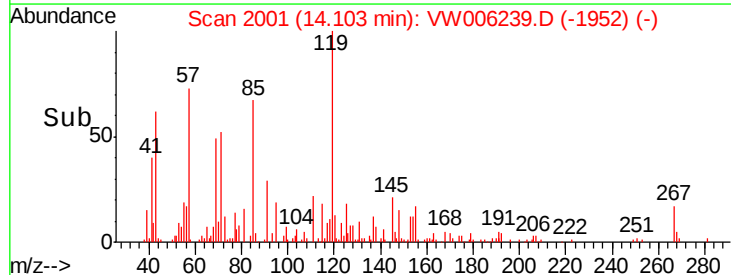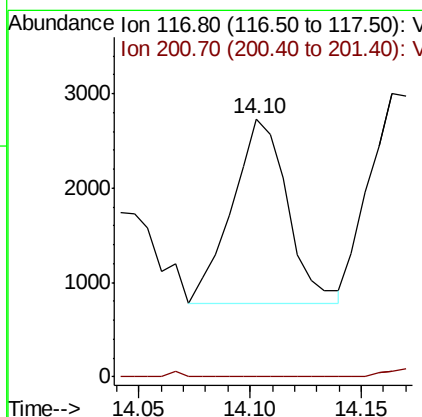



#92

1,2-Dibromo-3-Chloropropane

Concen: 2.290 ug/l

RT: 14.51 min Scan# 2068

Delta R.T. 0.02 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :

MS-VB-25868-BOX-1


Tot Ion: 75 Resp: 192

Ion Ratio Lower Upper

75 100

155 0.0 46.5 139.5#




157 32.8 59.8 179.4#



Abundance Ion 74.90 (74.60 to 75.60): VW

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V

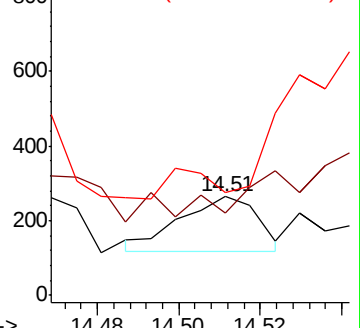

#95

Naphthalene

Concen: 82.933 ug/l

RT: 15.38 min Scan# 2210

Delta R.T. 0.00 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21


Tgt Ion: 128 Resp: 142104

Ion Ratio Lower Upper

128 100

127 15.0 10.3 15.5



129 12.8 8.7 13.1




Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

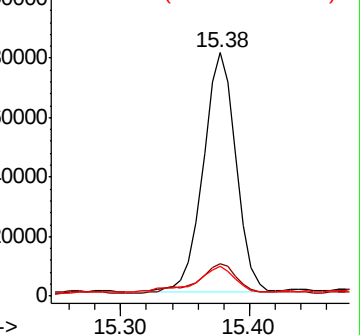



#96

1,2,3-Trichlorobenzene

Concen: 2.438 ug/l

RT: 15.59 min Scan# 2245

Delta R.T. 0.02 min

Lab File: VW006239.D

Acq: 19 Oct 2018 21:21

Instrument :

MSVOA_W

ClientSampleId :

MS-VB-25868-BOX-1


Tot Ion:180 Resp: 2172

Ion Ratio Lower Upper

180 100

182 0.0 47.8 143.3#

145 0.0 15.0 45.1#



Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.90 (144.60 to 145.60): V

