

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101921\
 Data File : VW020624.D
 Acq On : 19 Oct 2021 22:48
 Operator : SY/VA
 Sample : M4263-07
 Misc : 6.35g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7F2

Quant Time: Oct 20 05:29:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 20 02:32:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	238250	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	207648	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	74144	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	74954	21.621	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.480%
7) Chloroethane-d5	2.879	69	32673	17.842	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.360%
11) 1,1-Dichloroethene-d2	4.013	63	105819	14.896	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.600%
21) 2-Butanone-d5	7.080	46	43944	41.651	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.300%
24) Chloroform-d	7.647	84	170659	22.471	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.880%
26) 1,2-Dichloroethane-d4	8.305	65	98508	22.711	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.840%
32) Benzene-d6	8.275	84	332239	24.324	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.280%
36) 1,2-Dichloropropane-d6	9.274	67	110274	24.772	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.080%
41) Toluene-d8	10.323	98	300228	24.498	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.000%
43) trans-1,3-Dichloroprop...	10.579	79	41317	22.840	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.360%
47) 2-Hexanone-d5	10.927	63	31579	46.114	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.220%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	70553	20.968	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	83.880%
66) 1,2-Dichlorobenzene-d4	13.853	152	69669	24.021	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.080%
Target Compounds						
					Qvalue	
13) Acetone	4.123	43	31874	32.906	ug/L	98
15) Methyl Acetate	4.672	43	5267	2.928	ug/L	96
22) 2-Butanone	7.177	43	3104	2.560	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101921\
Data File : VW020624.D
Acq On : 19 Oct 2021 22:48
Operator : SY/VA
Sample : M4263-07
Misc : 6.35g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GB7F2

Quant Time: Oct 20 05:29:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 20 02:32:07 2021
Response via : Initial Calibration




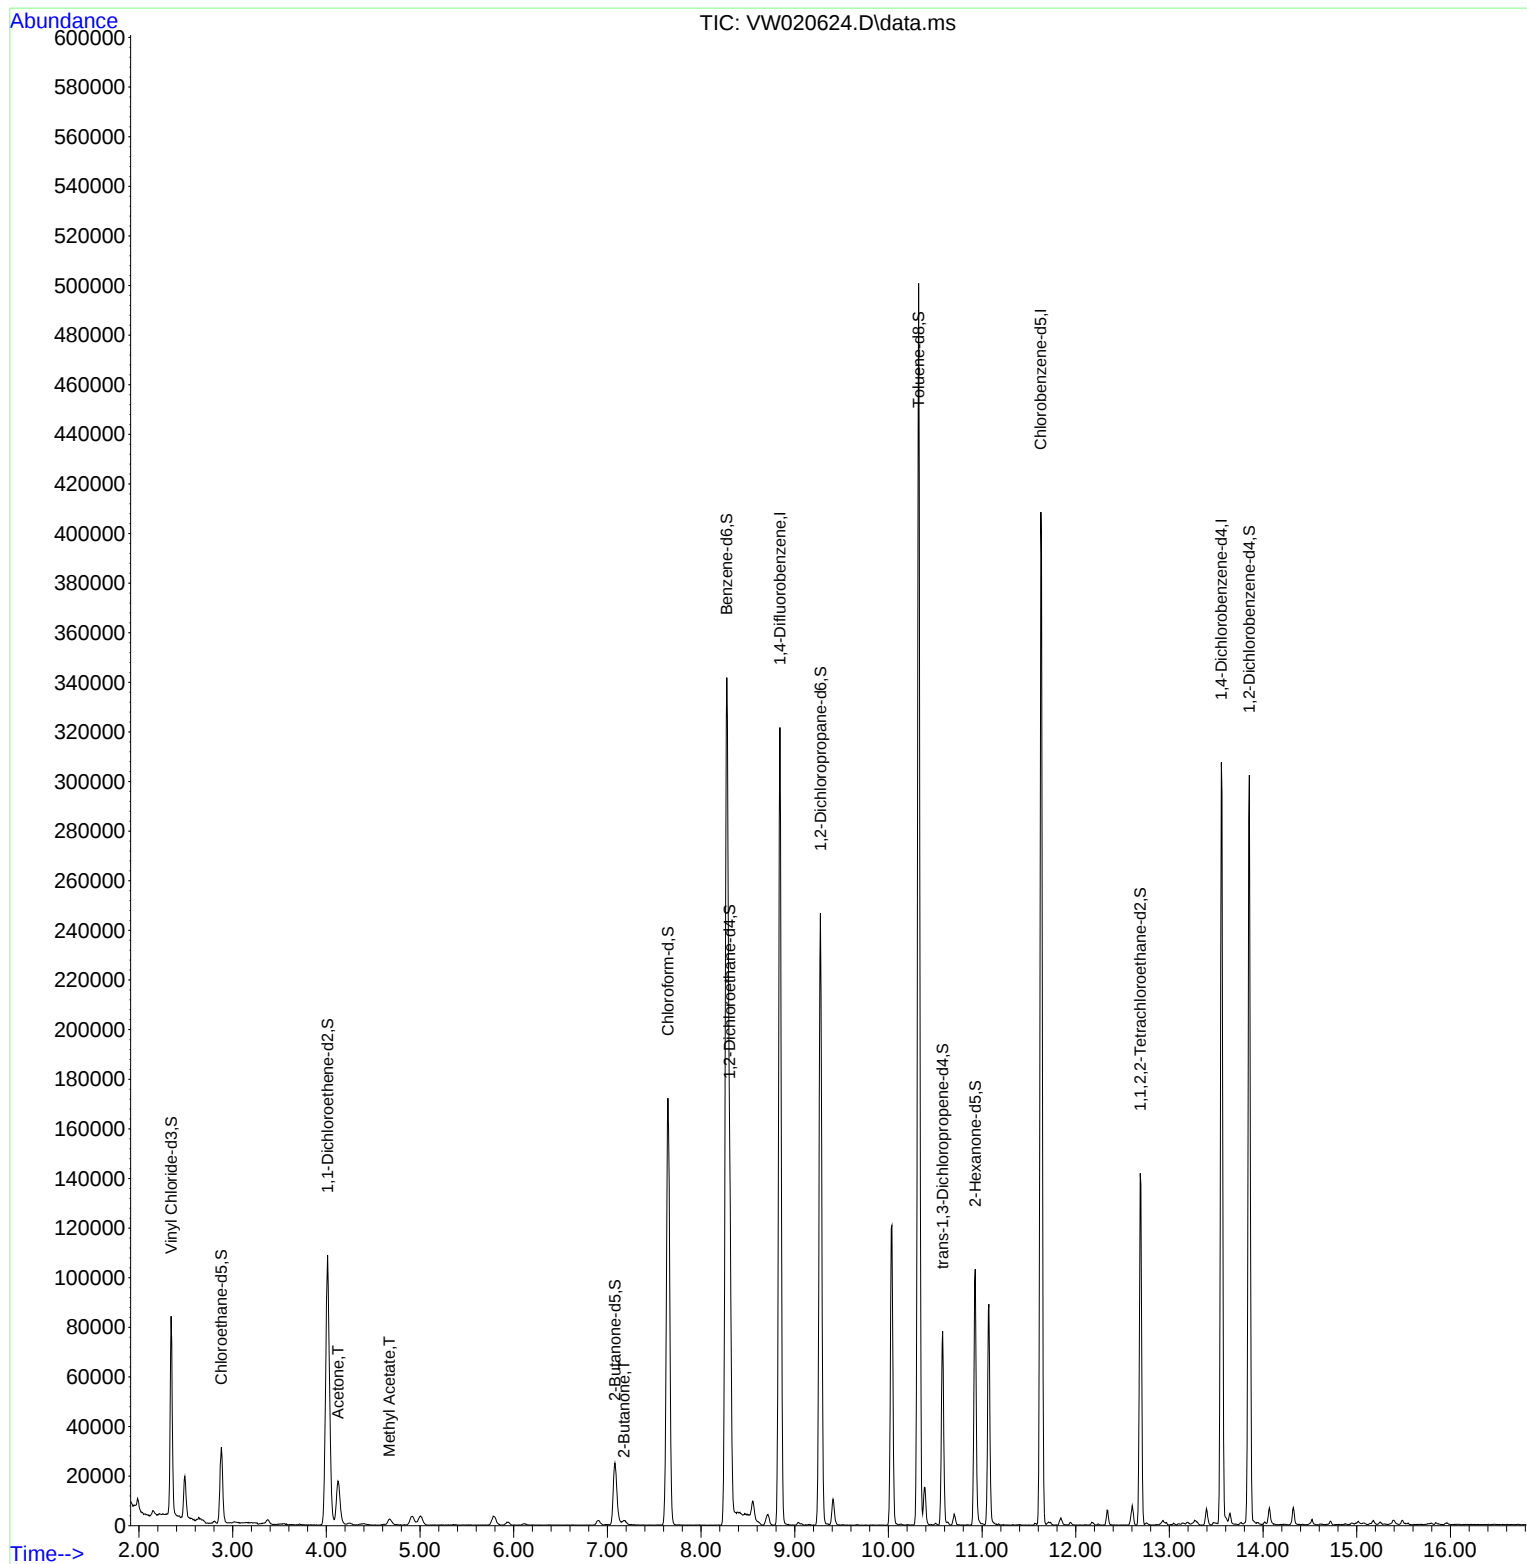


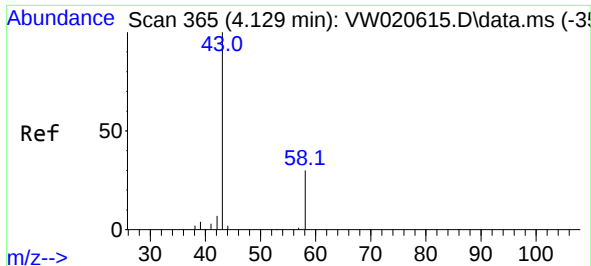

#13
Acetone
Concen: 32.906 ug/L
RT: 4.123 min Scan# 364
Delta R.T. -0.006 min
Lab File: VW020624.D
Acq: 19 Oct 2021 22:48




Instrument :
MSVOA_W
ClientSampled :
GB7F2


Tgt Ion: 43 Resp: 31874
Ion Ratio Lower Upper
43 100
58 28.0 0.0 58.4

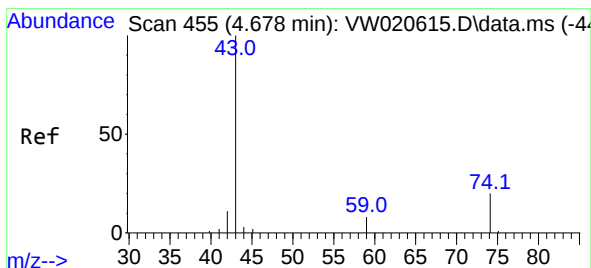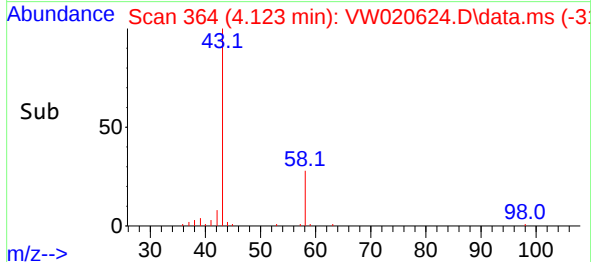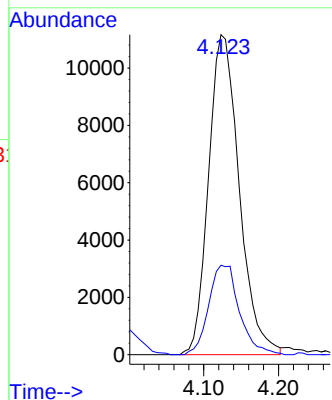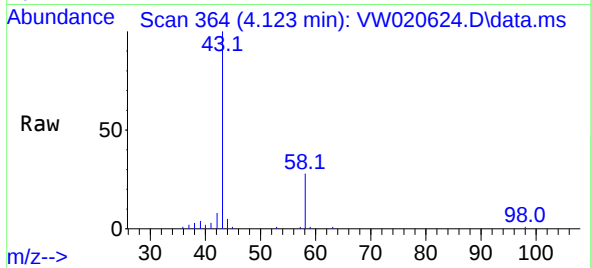

#15
Methyl Acetate
Concen: 2.928 ug/L
RT: 4.672 min Scan# 454
Delta R.T. -0.006 min
Lab File: VW020624.D
Acq: 19 Oct 2021 22:48

Tgt Ion: 43 Resp: 5267
Ion Ratio Lower Upper
43 100
74 18.3 16.1 24.1

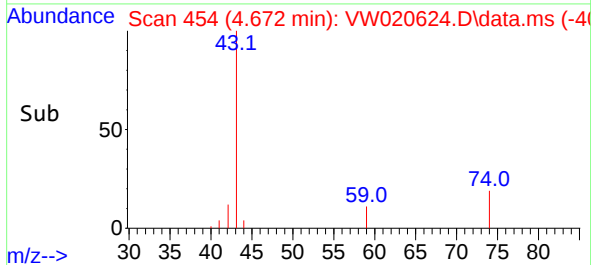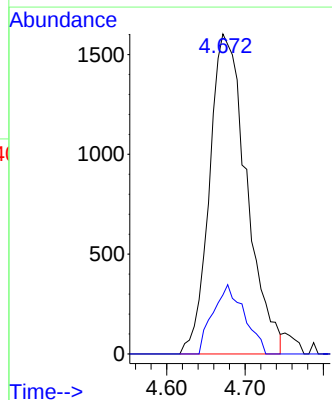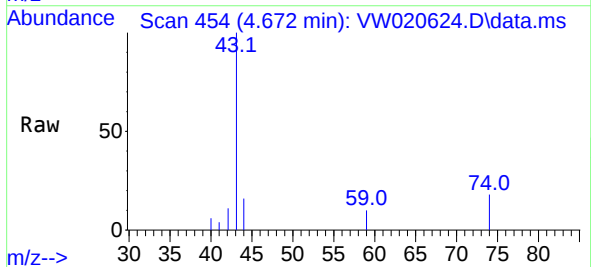

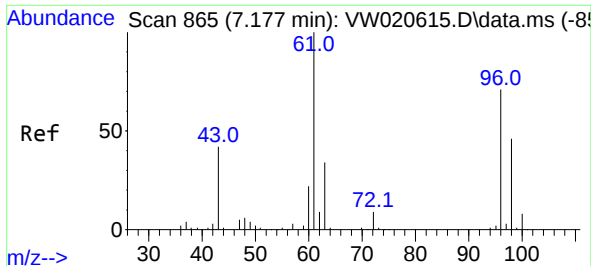

#22
 2-Butanone
 Concen: 2.560 ug/L
 RT: 7.177 min Scan# 865
 Delta R.T. -0.000 min
 Lab File: VW020624.D
 Acq: 19 Oct 2021 22:48

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7F2

Tgt Ion: 43 Resp: 3104
 Ion Ratio Lower Upper
 43 100
 72 20.5 12.2 36.6

