

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101921\
 Data File : VW020630.D
 Acq On : 20 Oct 2021 01:14
 Operator : SY/VA
 Sample : M4263-13
 Misc : 4.57g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7F8

Quant Time: Oct 20 05:30:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Oct 20 02:32:07 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	222537	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	211473	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	98409	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.343	65	67008	20.693	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.760%
7) Chloroethane-d5	2.873	69	25825	15.098	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.400%
11) 1,1-Dichloroethene-d2	4.007	63	95891	14.452	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.800%
21) 2-Butanone-d5	7.080	46	44412	45.066	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.140%
24) Chloroform-d	7.647	84	162698	22.936	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.760%
26) 1,2-Dichloroethane-d4	8.305	65	97691	24.113	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.440%
32) Benzene-d6	8.275	84	318366	22.887	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.560%
36) 1,2-Dichloropropane-d6	9.274	67	105220	23.209	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.840%
41) Toluene-d8	10.323	98	293218	23.493	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.960%
43) trans-1,3-Dichloroprop...	10.579	79	41254	22.393	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.560%
47) 2-Hexanone-d5	10.927	63	34130	48.938	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.880%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	76514	22.328	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	95332	24.764	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.040%
Target Compounds					Qvalue	
13) Acetone	4.129	43	4327	4.782	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101921\
Data File : VW020630.D
Acq On : 20 Oct 2021 01:14
Operator : SY/VA
Sample : M4263-13
Misc : 4.57g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GB7F8

Quant Time: Oct 20 05:30:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Oct 20 02:32:07 2021
Response via : Initial Calibration

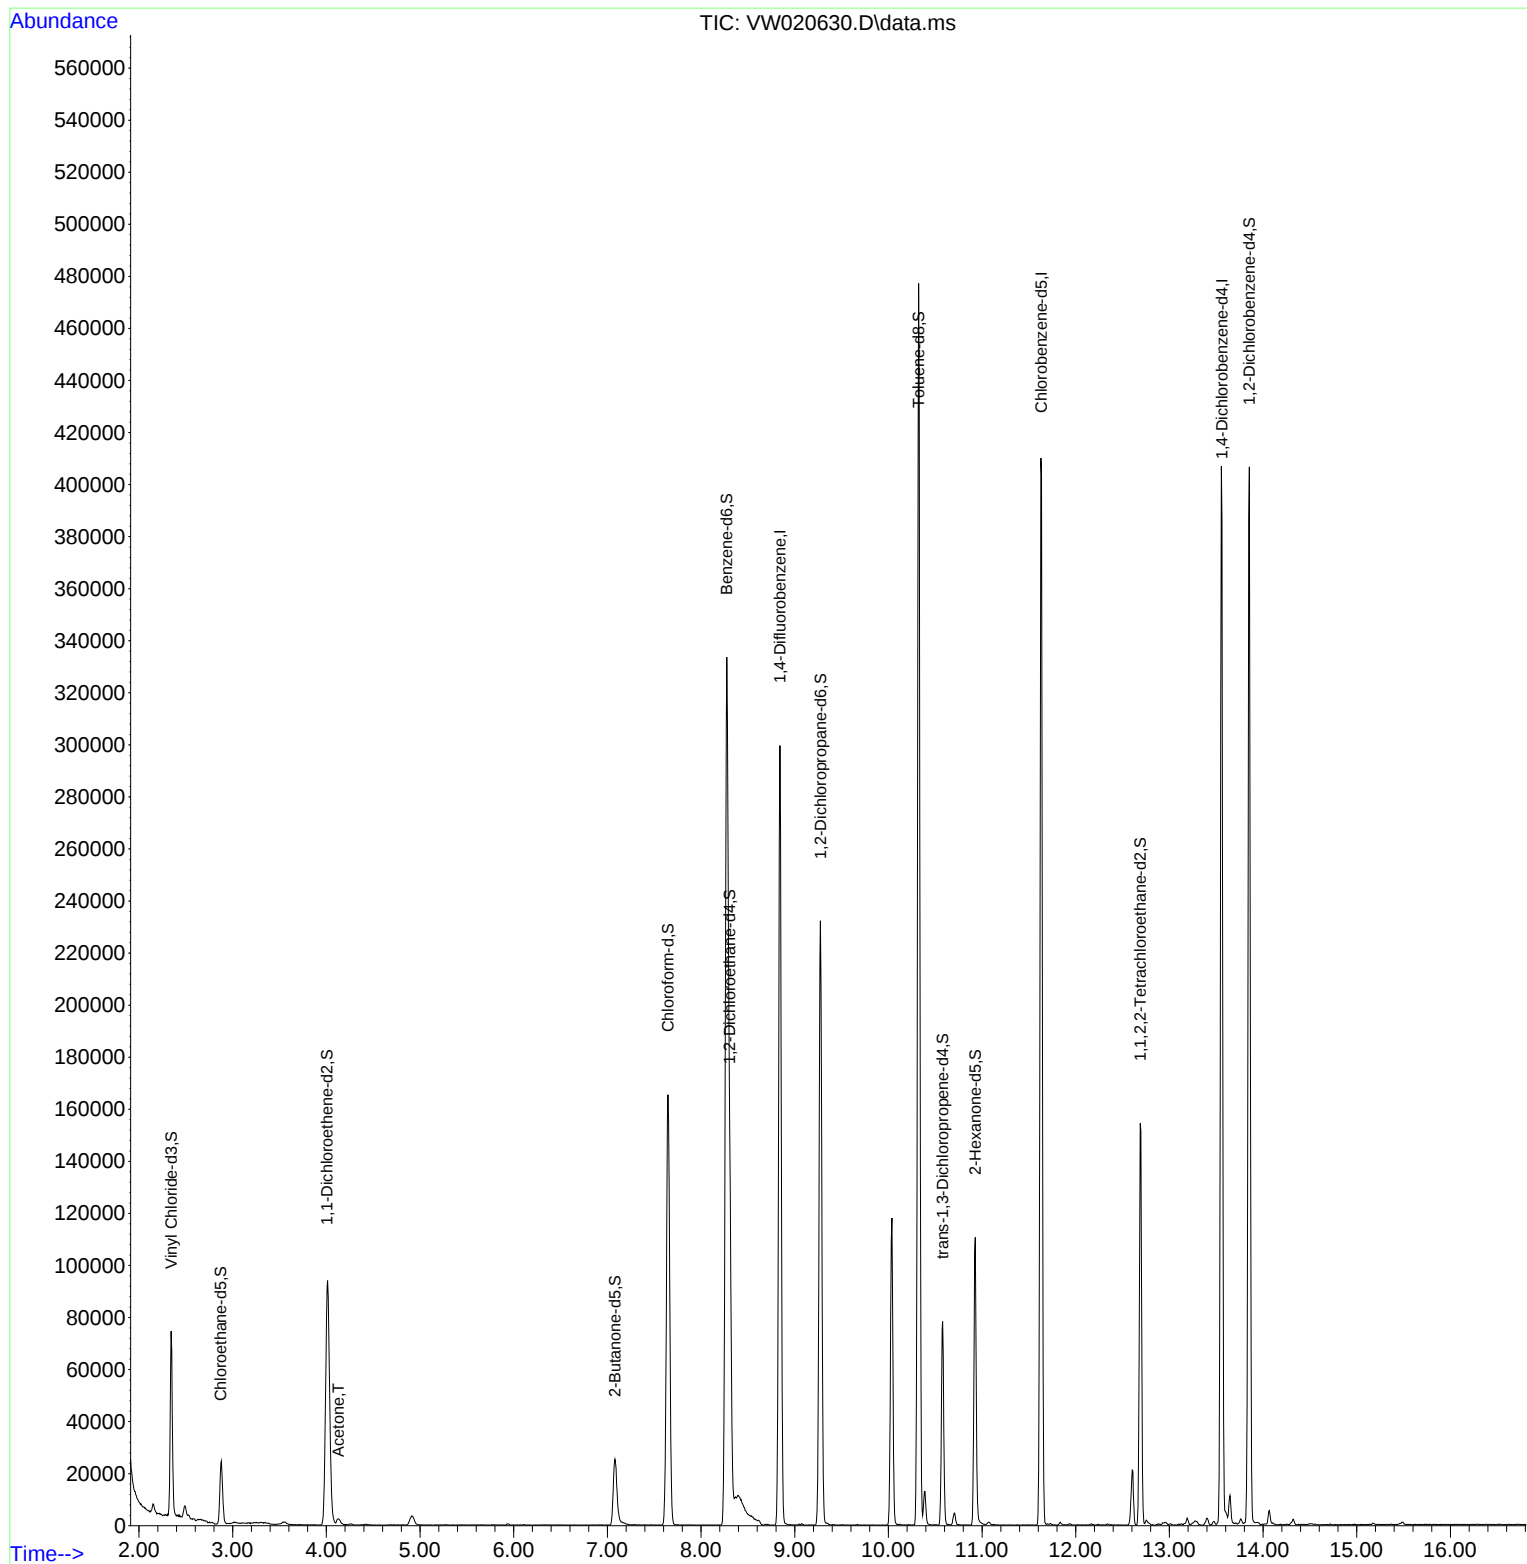

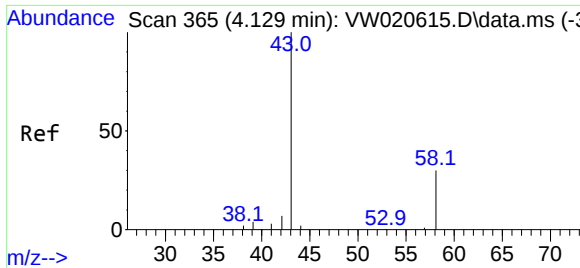

#13
 Acetone
 Concen: 4.782 ug/L
 RT: 4.129 min Scan# 365
 Delta R.T. -0.000 min
 Lab File: VW020630.D
 Acq: 20 Oct 2021 01:14

Instrument :
 MSVOA_W
 ClientSampleId :
 GB7F8

Tgt Ion: 43 Resp: 4327
 Ion Ratio Lower Upper
 43 100
 58 26.3 0.0 58.4

