
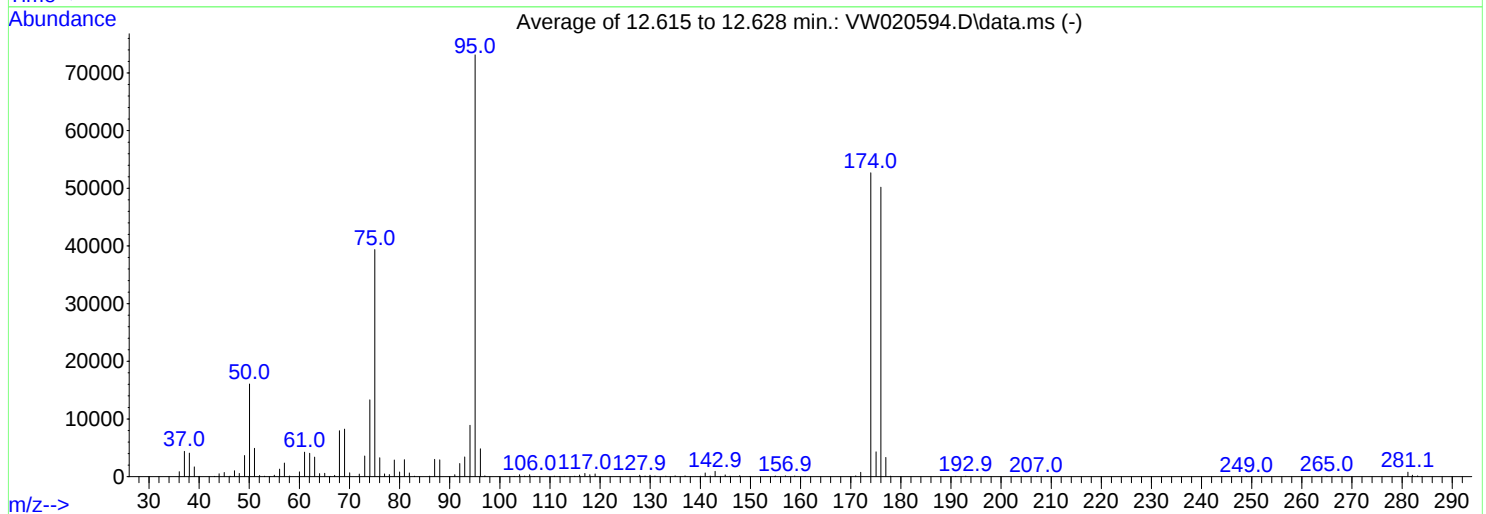


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW101921\
 Data File : VW020594.D
 Acq On : 19 Oct 2021 07:33
 Operator : SY/VA
 Sample : BFB455
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB455

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100821SMA.M
 Title : SFAM01.0
 Last Update : Thu Oct 21 01:08:32 2021

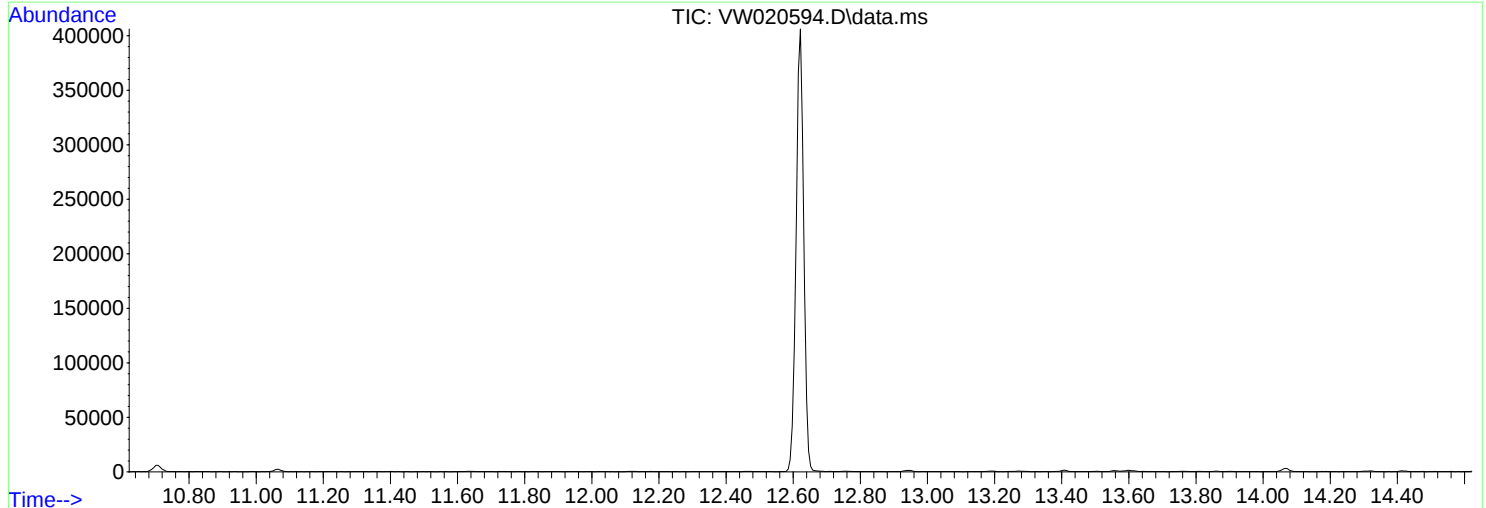

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	16069	PASS
75	95	30	80	53.8	39381	PASS
95	95	100	100	100.0	73141	PASS
96	95	5	9	6.6	4831	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.0	52691	PASS
175	174	5	9	8.2	4311	PASS
176	174	95	105	95.3	50195	PASS
177	176	5	10	6.6	3334	PASS

m/z	Abundance
36.10	661.0
37.10	3413.0
38.00	3071.0
39.10	1337.0
40.00	168.0
44.10	582.0
45.00	476.0
47.00	844.0
48.00	396.0
49.00	3067.0
50.00	12872.0
51.10	4109.0
52.10	157.0
53.10	79.0
55.00	198.0
56.00	1150.0
57.00	1975.0
58.00	95.0
60.00	666.0
61.10	3458.0
62.00	3220.0
63.00	2570.0
64.00	363.0
65.00	440.0
67.00	194.0
68.00	6842.0
69.00	6919.0
70.00	521.0
72.00	335.0
73.00	3222.0
74.10	11212.0
75.10	33296.0
76.10	2603.0
77.00	401.0
77.90	270.0
78.90	2691.0
80.00	741.0
80.90	2309.0
81.90	597.0
82.90	86.0
85.90	101.0
87.00	2445.0
88.00	2524.0
91.00	284.0
92.00	1910.0
93.00	2985.0
94.10	7527.0
95.10	63288.0
96.10	4320.0
96.90	124.0
104.00	266.0
104.90	119.0
106.00	323.0
110.90	68.0
111.90	63.0
112.80	64.0
114.90	63.0
115.90	242.0
116.90	437.0
117.90	299.0
119.00	377.0
128.00	246.0
128.90	121.0
129.90	200.0
130.90	86.0
134.90	155.0
137.00	130.0
140.10	72.0
141.00	635.0
141.90	86.0
143.00	774.0
145.00	242.0
145.90	113.0
147.90	132.0
149.90	66.0
155.00	149.0
156.90	122.0
158.90	105.0
160.90	77.0
170.90	98.0
172.00	641.0
174.00	48384.0
175.10	3983.0
176.00	45640.0
177.00	3128.0
177.90	62.0
281.10	325.0
282.10	161.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

Scan 1749 (12.567 min): VW020594.D\data.ms
BFB455

m/z	Abundance
40.00	119.0
43.90	136.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

m/z	Abundance
36.00	955.0
37.10	4825.0
38.00	4583.0
39.00	1804.0
40.00	184.0
43.10	78.0
44.00	700.0
45.00	852.0
46.10	162.0
47.00	1296.0
48.00	617.0
49.10	3822.0
50.10	17608.0
51.00	5150.0
52.00	256.0
53.00	110.0
54.10	52.0
55.00	297.0
56.00	1351.0
57.00	2526.0
58.10	105.0
60.00	883.0
61.00	4635.0
62.10	4386.0
63.00	3754.0
64.10	577.0
65.00	736.0
66.10	95.0
67.00	234.0
68.00	8099.0
69.00	8494.0
70.10	742.0
72.00	506.0
73.00	3801.0
74.10	13925.0
75.00	41032.0
76.00	3735.0
77.00	471.0
78.00	374.0
78.90	2953.0
80.00	767.0
81.00	3033.0
82.00	622.0
83.00	90.0
87.00	3251.0
88.00	2974.0
91.00	316.0
92.00	2282.0
93.00	3496.0
94.00	9349.0
95.00	74944.0
96.10	4993.0
97.00	155.0
102.90	65.0
103.90	346.0
105.00	88.0
105.90	337.0
106.80	74.0
110.80	72.0
112.80	57.0
115.00	90.0
115.90	286.0
116.90	629.0
118.00	307.0
119.00	530.0
127.80	262.0
129.00	116.0
129.90	230.0
131.00	120.0
133.10	126.0
135.00	117.0
137.00	106.0
140.00	64.0
140.90	567.0
142.00	121.0
143.00	1024.0
144.10	69.0
144.90	373.0
145.90	95.0
147.80	154.0
149.90	62.0
154.80	160.0
157.00	124.0
158.80	94.0
160.70	73.0
171.00	163.0
172.00	823.0
174.00	50320.0
175.00	4164.0
176.00	44456.0
177.00	3202.0
178.00	107.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

190.90	99.0
193.00	168.0
207.00	52.0
249.00	130.0
265.00	100.0
281.10	1265.0
282.10	402.0
283.10	234.0
283.90	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

m/z	Abundance
36.00	965.0
37.00	4942.0
38.10	4562.0
39.10	1906.0
40.00	169.0
43.10	54.0
44.10	622.0
45.00	818.0
46.20	131.0
47.10	968.0
48.00	660.0
49.00	4132.0
50.00	17728.0
51.10	5479.0
52.00	179.0
53.00	73.0
55.00	238.0
56.10	1397.0
57.00	2576.0
58.00	125.0
60.00	937.0
61.00	4673.0
62.10	4593.0
63.10	3836.0
64.00	655.0
65.10	612.0
66.10	76.0
67.10	279.0
68.00	8995.0
69.00	9333.0
70.00	756.0
71.90	512.0
73.10	3756.0
74.00	14848.0
75.00	43816.0
76.00	3512.0
77.00	548.0
77.90	419.0
79.00	3004.0
80.00	931.0
80.90	3484.0
82.00	705.0
83.00	90.0
86.00	166.0
87.00	3316.0
88.00	3259.0
91.00	380.0
92.00	2665.0
93.00	3722.0
94.10	9859.0
95.10	81192.0
96.10	5179.0
97.10	159.0
102.80	73.0
104.00	404.0
105.00	111.0
106.00	382.0
106.90	56.0
110.80	96.0
111.90	53.0
112.90	56.0
115.00	76.0
115.90	305.0
117.00	585.0
117.90	384.0
119.00	476.0
127.90	283.0
129.00	118.0
130.00	325.0
130.90	109.0
132.90	55.0
133.20	62.0
135.00	145.0
136.90	155.0
140.10	80.0
141.00	721.0
141.90	115.0
142.90	931.0
143.90	74.0
144.90	309.0
145.90	78.0
147.90	236.0
149.90	64.0
155.00	220.0
157.00	140.0
158.90	119.0
160.90	66.0
171.00	140.0
172.00	796.0
174.00	59368.0
175.10	4785.0
176.00	60488.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455

177.00	3671.0
177.90	91.0
191.00	87.0
192.90	77.0
265.00	68.0
281.20	760.0
282.00	217.0
283.10	157.0

Instrument :
MSVOA_W
ClientSampleId :
BFB455