

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102119\
 Data File : VW013627.D
 Acq On : 21 Oct 2019 11:11
 Operator : SY/VA
 Sample : VW1021SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK10

Quant Time: Oct 21 16:40:21 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 21 16:37:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	343143	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	332899	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	192729	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	100296	23.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.28%
7) Chloroethane-d5	2.90	69	89664	22.82	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.28%
10) 1,1-Dichloroethene-d2	4.03	63	153495	16.51	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.04%
20) 2-Butanone-d5	7.08	46	75215	49.95	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.90%
24) Chloroform-d	7.65	84	220788	23.00	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.00%
26) 1,2-Dichloroethane-d4	8.31	65	117616	23.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.68%
29) Benzene-d6	8.27	84	469005	23.45	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.80%
33) 1,2-Dichloropropane-d6	9.27	67	142391	23.84	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.36%
37) Toluene-d8	10.32	98	423660	22.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.88%
38) trans-1,3-Dichloropropene-	10.58	79	61383	22.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.12%
39) 2-Hexanone-d5	10.93	63	59027	51.69	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.38%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	119240	24.37	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.48%
61) 1,2-Dichlorobenzene-d4	13.85	152	160924	23.63	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.52%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.55	75	19746	5.016 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102119\
Data File : VW013627.D
Acq On : 21 Oct 2019 11:11
Operator : SY/VA
Sample : VW1021SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK10

Quant Time: Oct 21 16:40:21 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 21 16:37:58 2019
Response via : Initial Calibration

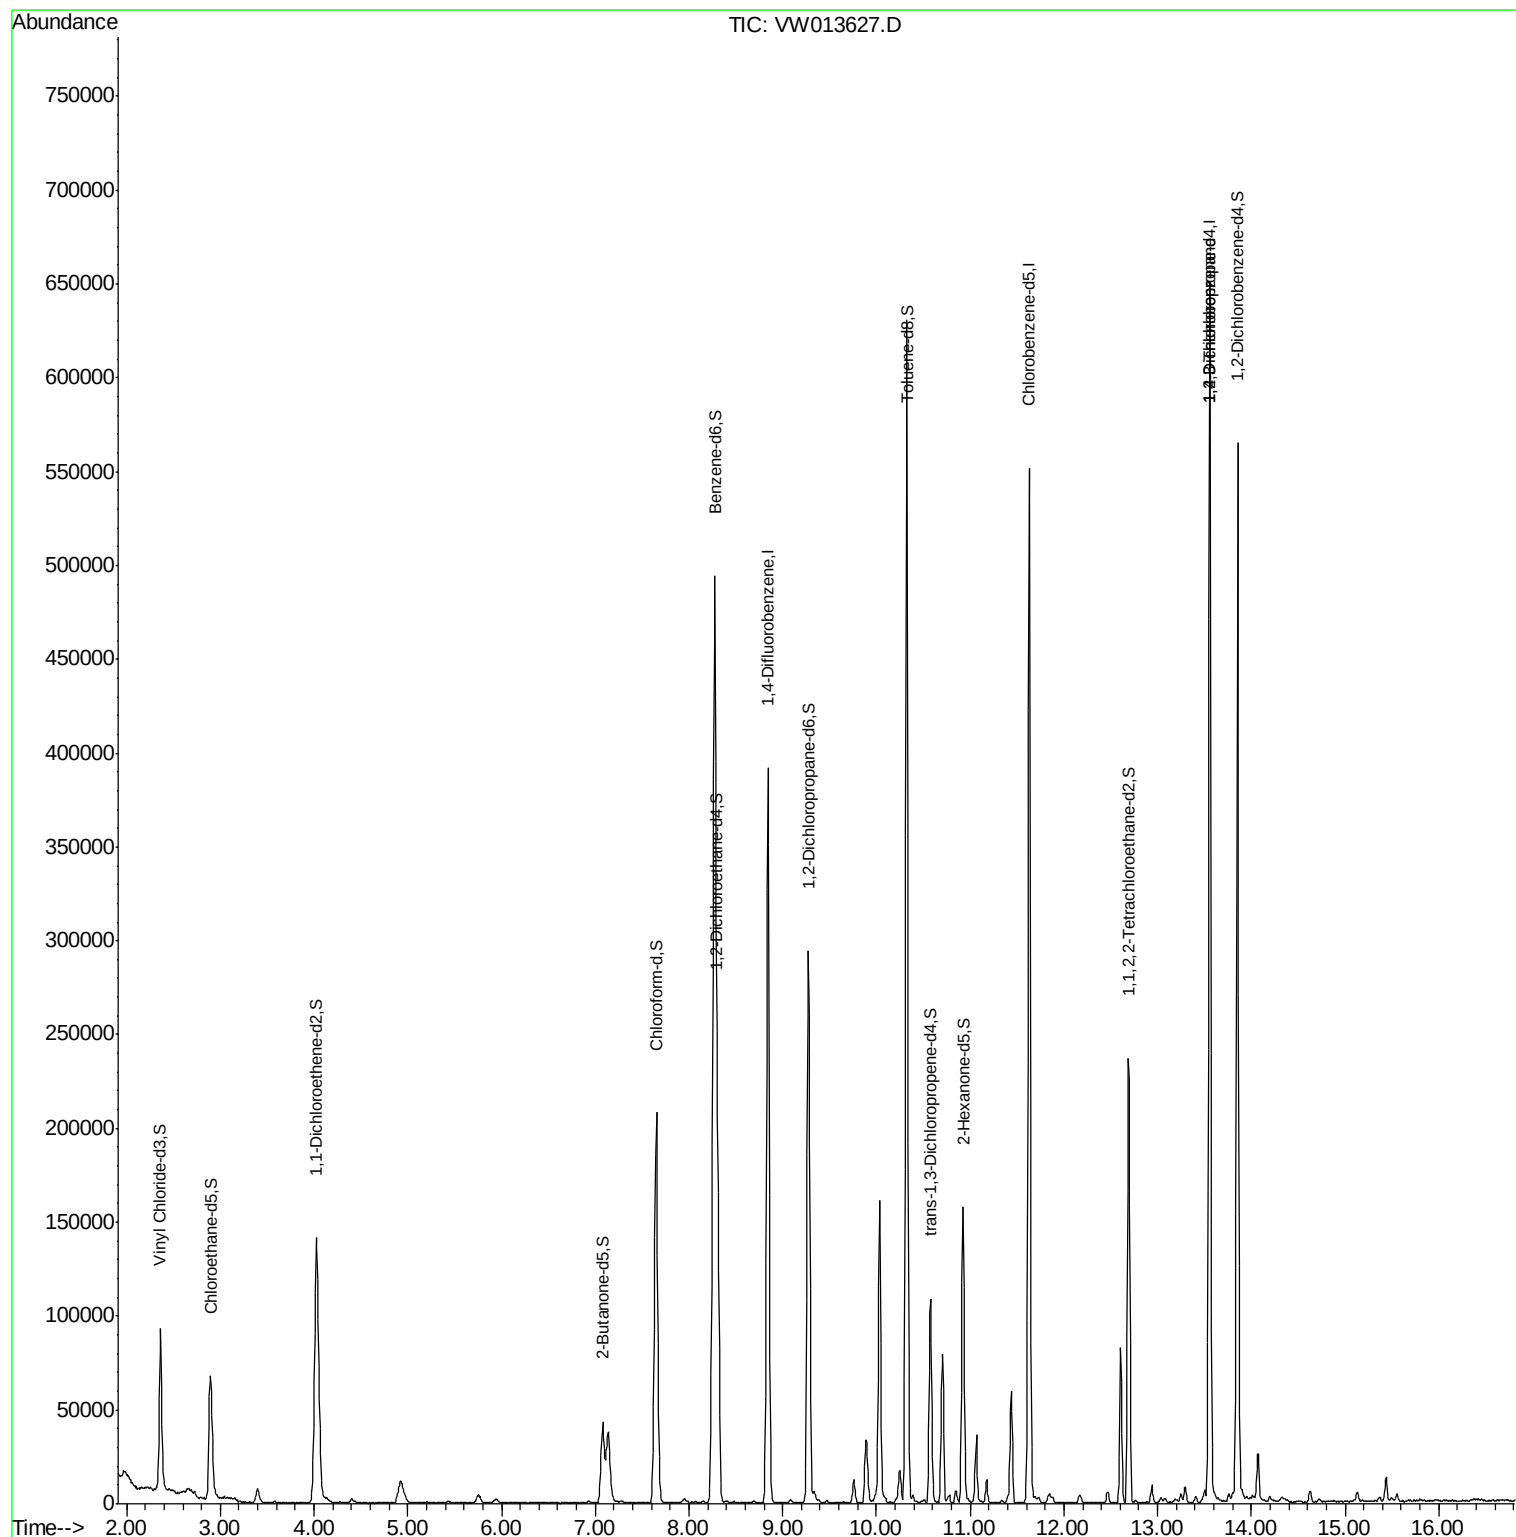

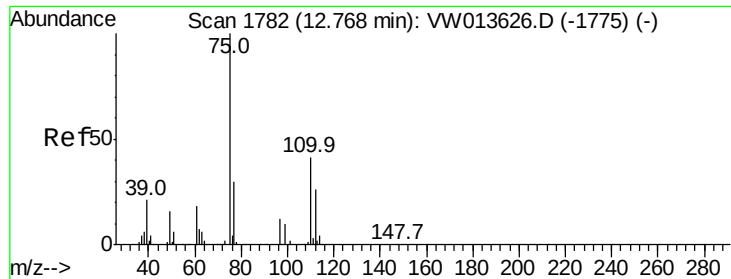

#59

1,2,3-Trichloropropane

Concen: 5.016 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW013627.D

Acq: 21 Oct 2019 11:11

Instrument :

MSVOA_W

ClientSampleId :

VBLK10

Tot Ion: 75 Resp: 19746

Ion Ratio Lower Upper

75 100

77 33.9 26.4 39.6

