

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102119\
 Data File : VW013634.D
 Acq On : 21 Oct 2019 14:33
 Operator : SY/VA
 Sample : K5422-02
 Misc : 5.58G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB3

Quant Time: Oct 21 17:28:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Oct 21 16:37:58 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	326534	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	278898	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	116773	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	117507	29.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	117.32%
7) Chloroethane-d5	2.89	69	97740	26.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.56%
10) 1,1-Dichloroethene-d2	4.02	63	176534	19.95	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.80%
20) 2-Butanone-d5	7.08	46	58733	40.99	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.98%
24) Chloroform-d	7.65	84	223653	24.48	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.92%
26) 1,2-Dichloroethane-d4	8.31	65	116964	24.48	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.92%
29) Benzene-d6	8.27	84	487502	29.09	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	116.36%
33) 1,2-Dichloropropane-d6	9.27	67	144671	28.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	115.64%
37) Toluene-d8	10.32	98	429670	27.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	111.20%
38) trans-1,3-Dichloropropene-	10.58	79	54573	24.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.68%
39) 2-Hexanone-d5	10.92	63	46465	48.57	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.14%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	97655	23.83	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	102011	24.72	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.88%


Target Compounds					Ovalue
16) Methylene chloride	4.92	84	41315	6.607 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102119\
Data File : VW013634.D
Acq On : 21 Oct 2019 14:33
Operator : SY/VA
Sample : K5422-02
Misc : 5.58G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AB3

Quant Time: Oct 21 17:28:02 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM101819S.M
Quant Title : VOC Analysis
QLast Update : Mon Oct 21 16:37:58 2019
Response via : Initial Calibration

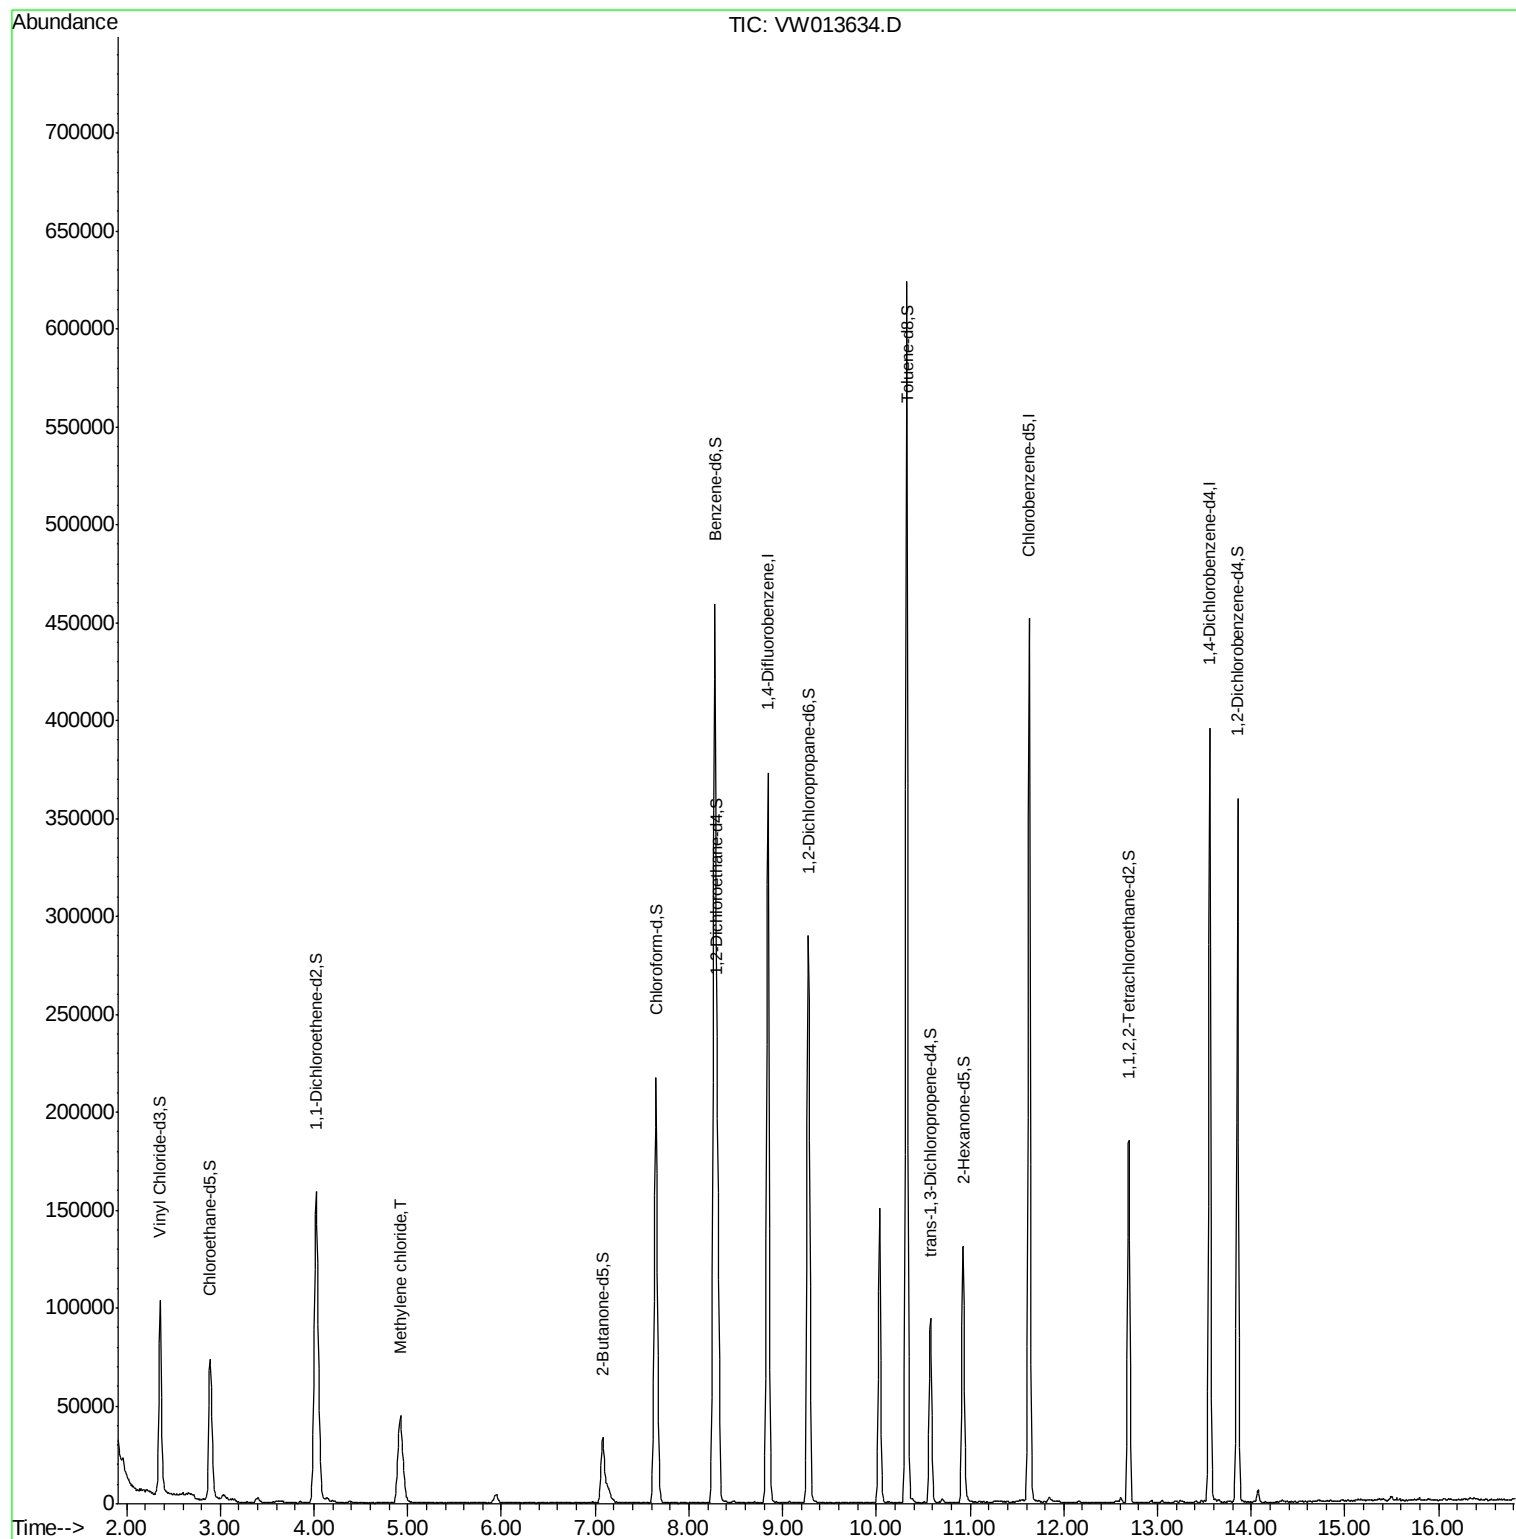


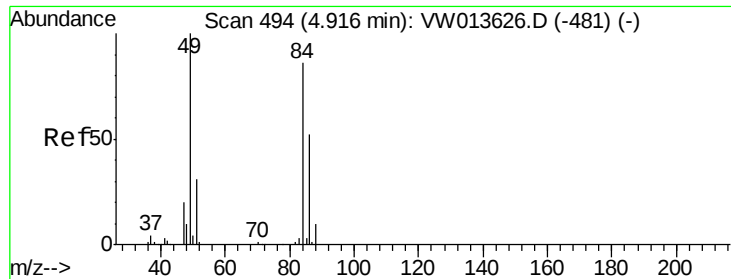

#16
 Methvlene chloride
 Concen: 6.607 ug/L
 RT: 4.92 min Scan# 495
 Delta R.T. 0.00 min
 Lab File: VW013634.D
 Acq: 21 Oct 2019 14:33

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AB3

Tot Ion: 84 Resp: 41315
 Ion Ratio Lower Upper
 84 100
 49 119.7 80.2 148.9
 86 59.1 42.7 79.3

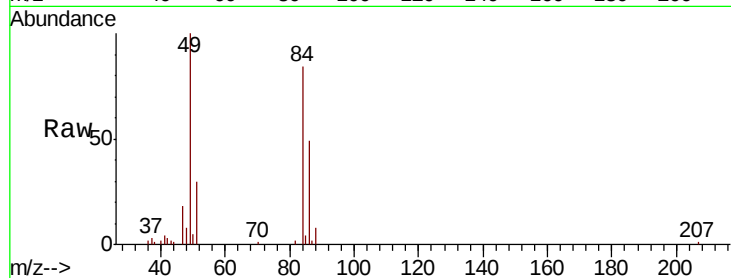

Abundance Ion 84.00 (83.70 to 84.70): VW
 Ion 49.00 (48.70 to 49.70): VW
 Ion 86.00 (85.70 to 86.70): VW

