

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102121\
 Data File : VW020674.D
 Acq On : 21 Oct 2021 18:17
 Operator : SY/VA
 Sample : M4207-05
 Misc : 5.08g/10mL/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 22 02:02:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102121SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Oct 22 01:58:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	202542	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	192615	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	90821	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	66148	23.344	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.360%
7) Chloroethane-d5	2.879	69	28407	26.202	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.800%
11) 1,1-Dichloroethene-d2	4.019	63	92275	17.617	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.480%
21) 2-Butanone-d5	7.080	46	45115	48.993	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.980%
24) Chloroform-d	7.653	84	135409	23.011	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.040%
26) 1,2-Dichloroethane-d4	8.305	65	85837	24.598	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.400%
32) Benzene-d6	8.275	84	262451	23.511	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.040%
36) 1,2-Dichloropropane-d6	9.275	67	86326	23.802	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.200%
41) Toluene-d8	10.323	98	234967	23.443	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.760%
43) trans-1,3-Dichloroprop...	10.579	79	36164	23.637	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.560%
47) 2-Hexanone-d5	10.927	63	32412	49.876	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.760%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	71782	23.831	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	80104	25.843	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.360%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	2884	0.621	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102121\
Data File : VW020674.D
Acq On : 21 Oct 2021 18:17
Operator : SY/VA
Sample : M4207-05
Misc : 5.08g/10mL/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Oct 22 02:02:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102121SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Oct 22 01:58:04 2021
Response via : Initial Calibration

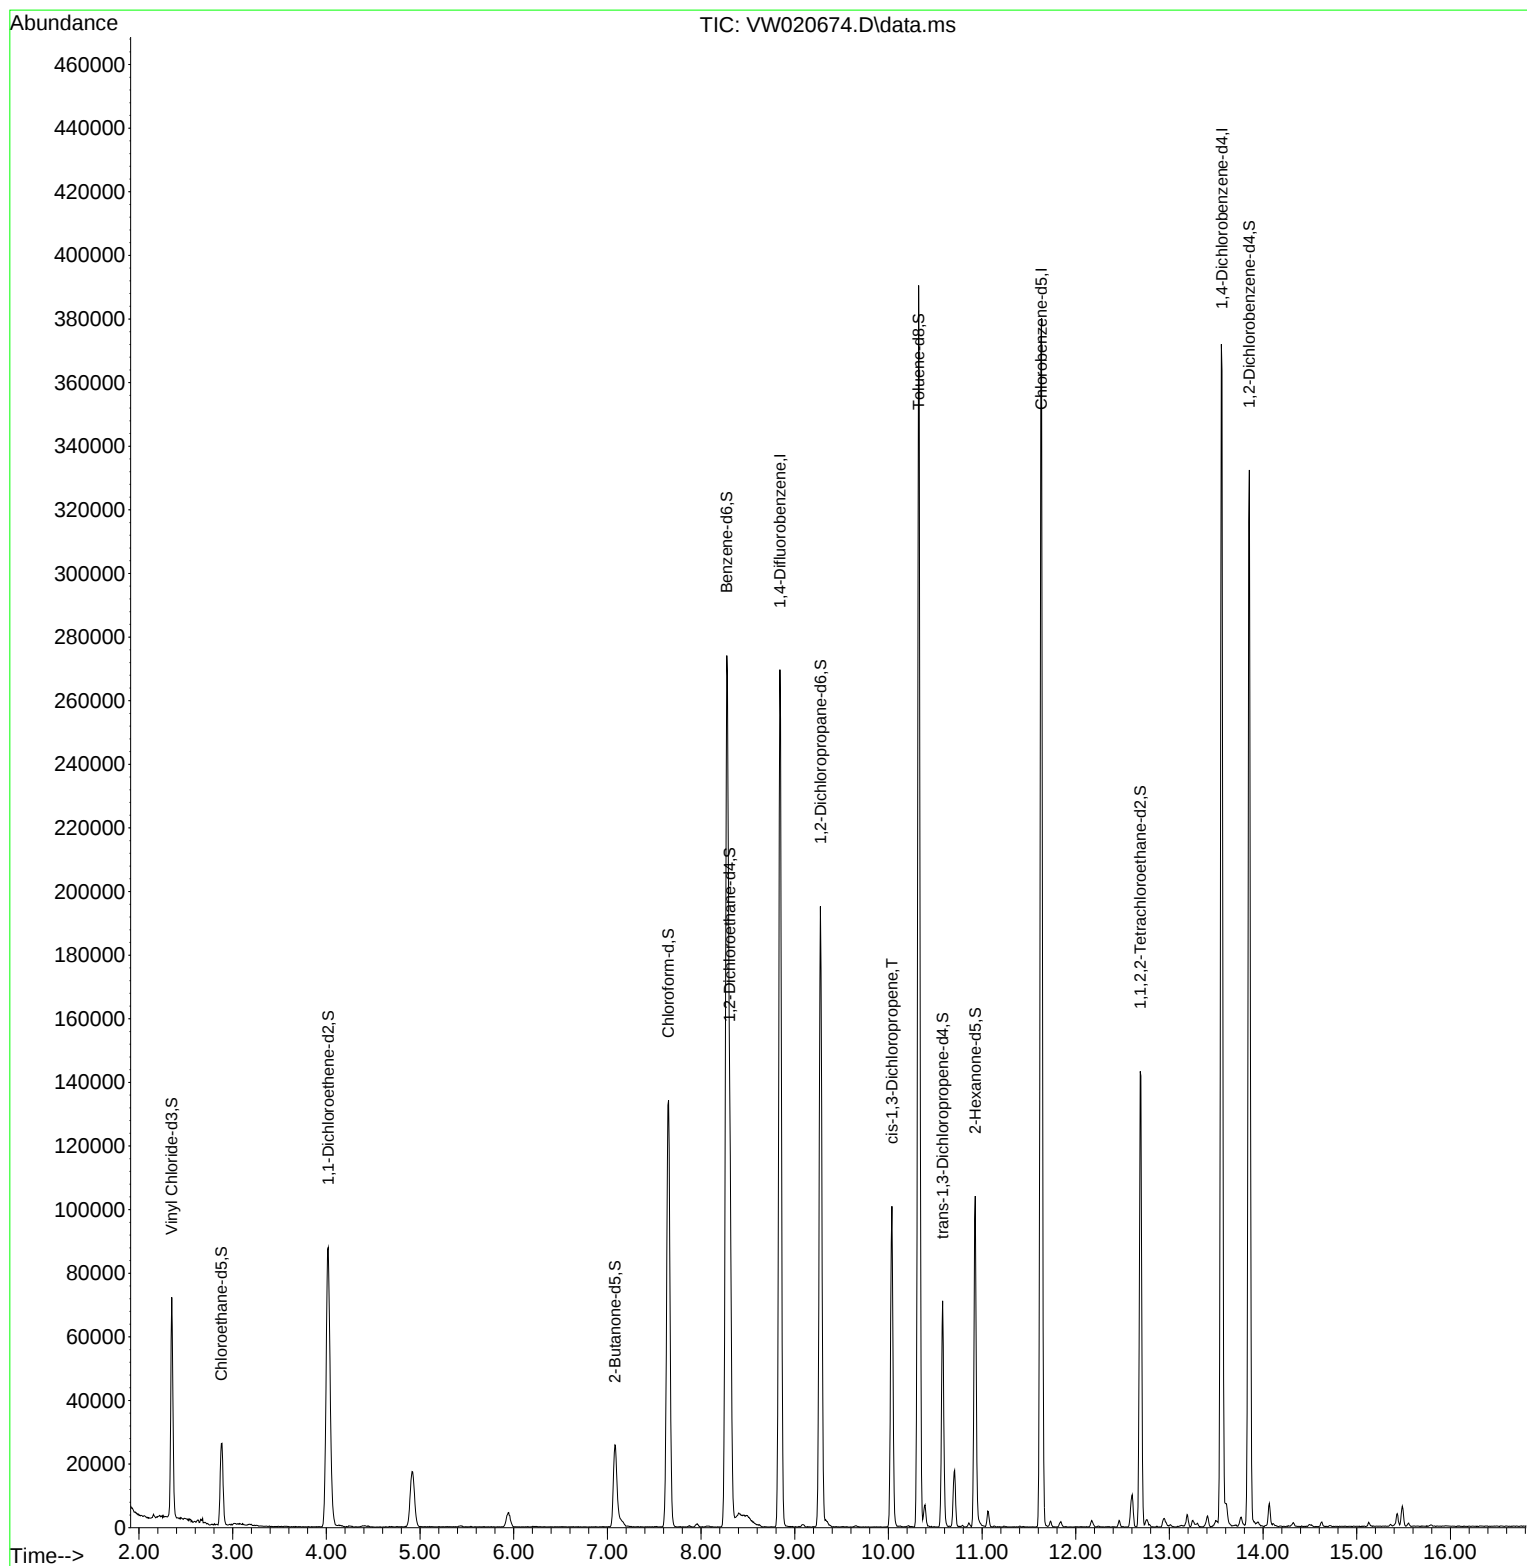

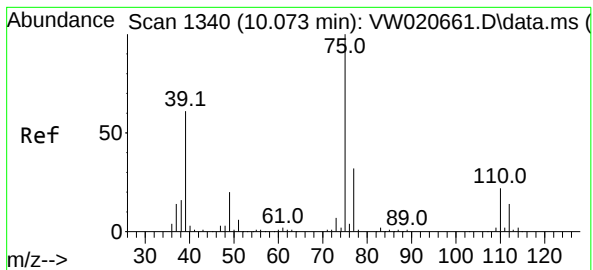

#39
 cis-1,3-Dichloropropene
 Concen: 0.621 ug/L
 RT: 10.037 min Scan# 1334
 Delta R.T. -0.036 min
 Lab File: VW020674.D
 Acq: 21 Oct 2021 18:17

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 2884
 Ion Ratio Lower Upper
 75 100
 77 49.3 21.8 40.6#

