
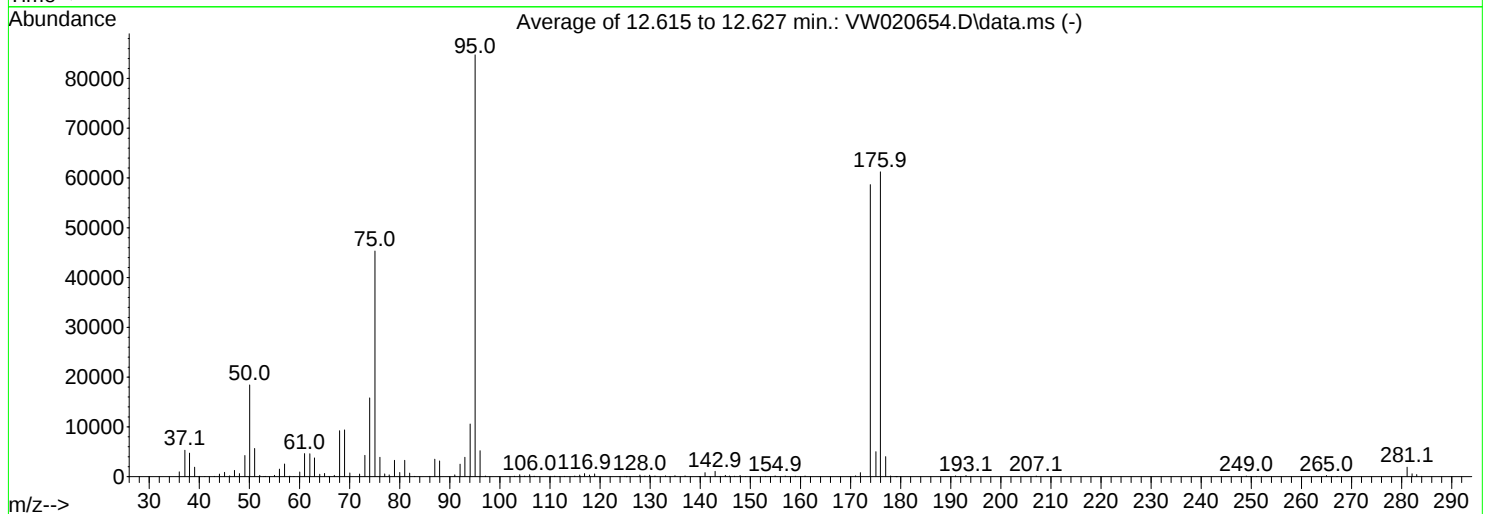


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102121\
 Data File : VW020654.D
 Acq On : 21 Oct 2021 06:25
 Operator : SY/VA
 Sample : BFB457
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB457

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM102121SMA.M
 Title : SFAM01.0
 Last Update : Fri Oct 22 01:58:04 2021

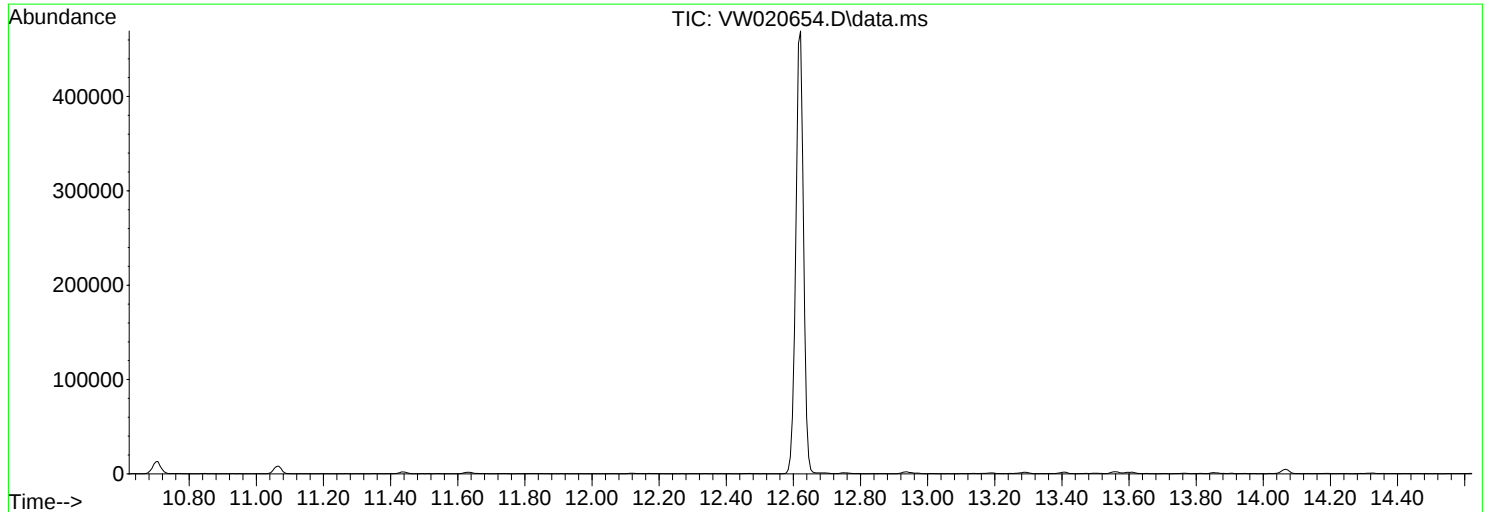

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	18421	PASS
75	95	30	80	53.5	45317	PASS
95	95	100	100	100.0	84741	PASS
96	95	5	9	6.1	5203	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.2	58683	PASS
175	174	5	9	8.6	5029	PASS
176	174	95	105	104.3	61229	PASS
177	176	5	10	6.6	4026	PASS

Scan 1749 (12.566 min): VW020654.D\data.ms
BFB457

m/z	Abundance
40.00	110.0
44.00	153.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

m/z	Abundance
36.00	1182.0
37.10	6257.0
38.00	5511.0
39.00	2227.0
40.10	200.0
41.10	90.0
43.00	100.0
44.00	756.0
45.00	1038.0
46.10	194.0
47.00	1354.0
48.00	739.0
49.10	4873.0
50.00	20816.0
51.00	6206.0
52.00	282.0
52.90	141.0
55.00	294.0
56.00	1773.0
57.00	2833.0
58.10	113.0
58.90	83.0
60.10	982.0
61.00	5498.0
62.10	5524.0
63.00	4345.0
64.10	632.0
65.00	871.0
65.90	81.0
66.90	259.0
68.00	10351.0
69.00	10413.0
70.00	812.0
72.00	529.0
73.00	4687.0
74.00	17920.0
75.10	50928.0
76.10	4380.0
77.00	672.0
77.90	448.0
79.00	3811.0
80.00	1027.0
81.00	3797.0
82.00	804.0
83.00	71.0
87.00	3886.0
88.00	3453.0
91.00	351.0
92.00	2830.0
93.00	4202.0
94.10	11226.0
95.10	92568.0
96.10	5453.0
97.10	180.0
103.00	126.0
104.00	389.0
104.90	155.0
105.90	450.0
106.80	141.0
110.00	74.0
110.90	104.0
111.90	76.0
112.90	84.0
114.90	116.0
116.00	384.0
116.90	641.0
117.90	331.0
118.90	626.0
124.90	170.0
125.90	57.0
128.00	316.0
129.00	149.0
130.00	327.0
131.00	150.0
133.00	279.0
133.90	69.0
135.00	263.0
136.90	154.0
139.80	70.0
141.00	881.0
141.90	151.0
142.90	1031.0
143.90	131.0
145.00	396.0
145.80	131.0
146.90	108.0
148.00	208.0
149.00	70.0
149.90	65.0
153.00	57.0
154.00	61.0
155.00	156.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

157.00	105.0
159.00	111.0
160.90	127.0
171.00	212.0
171.90	1045.0
173.90	60920.0
175.00	4838.0
175.90	58816.0
177.00	4247.0
178.00	153.0
178.90	75.0
190.90	304.0
192.00	100.0
193.10	336.0
194.00	60.0
207.10	182.0
249.00	149.0
249.90	55.0
251.00	133.0
265.00	330.0
266.10	90.0
267.00	106.0
281.10	2708.0
282.10	895.0
283.00	717.0
284.00	121.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

m/z	Abundance
36.00	1013.0
37.10	5858.0
38.10	5185.0
39.10	2112.0
40.10	168.0
43.00	80.0
44.00	723.0
45.10	934.0
46.00	160.0
47.00	1441.0
48.00	671.0
49.10	4721.0
50.10	20712.0
51.10	6408.0
52.10	350.0
53.10	102.0
55.00	308.0
56.00	1688.0
57.00	2983.0
58.10	98.0
58.90	57.0
60.00	1034.0
61.00	5073.0
62.00	4952.0
63.00	4168.0
64.00	511.0
65.00	715.0
65.90	93.0
67.00	318.0
68.00	10157.0
69.00	10693.0
70.10	853.0
72.00	570.0
73.10	4874.0
74.00	17688.0
75.10	50592.0
76.00	4358.0
77.00	659.0
77.90	362.0
78.90	3540.0
80.00	985.0
81.00	3625.0
82.00	732.0
83.00	97.0
86.00	137.0
87.00	3987.0
88.00	3461.0
91.00	394.0
92.10	2745.0
93.00	4401.0
94.00	12295.0
95.00	95184.0
96.10	5959.0
97.10	154.0
102.80	93.0
103.90	520.0
105.00	119.0
106.00	395.0
106.90	123.0
110.10	116.0
111.00	104.0
111.90	54.0
112.80	87.0
115.00	162.0
115.90	352.0
116.90	625.0
118.00	351.0
118.90	522.0
124.00	88.0
125.90	67.0
127.90	377.0
129.00	149.0
129.90	324.0
131.00	101.0
133.10	186.0
133.90	60.0
135.00	165.0
137.00	233.0
140.90	806.0
143.00	1262.0
144.00	100.0
145.00	263.0
145.90	131.0
146.80	105.0
147.90	264.0
149.00	63.0
149.90	68.0
153.00	63.0
154.00	65.0
155.00	206.0
156.90	138.0
158.90	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

m/z	Abundance
36.00	692.0
37.00	3837.0
38.00	3471.0
39.10	1398.0
39.90	147.0
44.00	490.0
45.00	613.0
46.00	102.0
47.00	992.0
48.00	427.0
49.00	3103.0
50.10	13734.0
51.10	4317.0
52.10	161.0
53.20	63.0
55.00	216.0
56.00	1105.0
57.00	1809.0
58.00	81.0
60.10	759.0
61.10	3328.0
62.00	3307.0
63.10	2790.0
64.00	311.0
65.00	357.0
67.00	223.0
68.00	7150.0
69.00	7027.0
70.00	566.0
72.00	439.0
73.00	3252.0
74.00	11885.0
75.00	34432.0
76.10	2915.0
76.90	345.0
77.90	299.0
78.90	2510.0
80.00	540.0
80.90	2387.0
82.00	579.0
83.00	64.0
86.00	74.0
87.00	2661.0
87.90	2534.0
91.00	295.0
92.00	1957.0
93.00	3035.0
94.00	8234.0
95.10	66472.0
96.00	4196.0
97.00	90.0
102.90	58.0
103.90	257.0
105.00	113.0
105.90	305.0
106.80	68.0
110.90	70.0
113.00	76.0
114.90	87.0
115.90	248.0
116.90	522.0
117.80	283.0
118.90	455.0
125.20	51.0
127.90	242.0
128.80	105.0
129.80	258.0
130.90	144.0
133.10	59.0
134.90	155.0
136.90	145.0
140.00	61.0
140.90	749.0
143.00	866.0
145.00	167.0
145.90	132.0
146.90	57.0
147.90	201.0
150.00	75.0
153.00	76.0
154.90	151.0
157.00	105.0
159.00	62.0
160.90	108.0
171.10	122.0
171.90	543.0
174.00	54048.0
175.00	4579.0
176.00	51992.0
177.00	3584.0
178.00	73.0
192.90	94.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

207.10	89.0
249.00	80.0
265.10	86.0
281.10	933.0
282.00	275.0
283.00	154.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457

160.90	114.0
170.90	182.0
172.00	808.0
174.00	61080.0
175.10	5671.0
176.00	72880.0
177.00	4248.0
178.00	143.0
179.10	53.0
191.00	151.0
193.00	244.0
207.00	142.0
249.00	145.0
265.00	256.0
266.10	80.0
267.20	64.0
281.10	2063.0
282.10	539.0
283.00	348.0
284.00	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB457