

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102218\
 Data File : VW006282.D
 Acq On : 23 Oct 2018 06:38
 Operator : VA/AP
 Sample : J5621-05
 Misc : 4.95G/5ML/MSVOA W/SOIL
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SA-SB-01A

Quant Time: Oct 24 08:52:53 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 18 17:01:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	237771	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	326347	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	246514	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	95151	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	68643	34.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	69.64%	
35) Dibromofluoromethane	7.88	113	68523	35.53	ug/l	0.00
Spiked Amount 50.000			Recovery	=	71.06%	
50) Toluene-d8	10.32	98	207699	28.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	56.62%	
62) 4-Bromofluorobenzene	12.62	95	60877	22.09	ug/l	0.00
Spiked Amount 50.000			Recovery	=	44.18%	
Target Compounds						
20) Methylene Chloride	4.91	84	13297	4.907	ug/l	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102218\
Data File : VW006282.D
Acq On : 23 Oct 2018 06:38
Operator : VA/AP
Sample : J5621-05
Misc : 4.95G/5ML/MSVOA W/SOIL
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SA-SB-01A

Quant Time: Oct 24 08:52:53 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W101518S.M
Quant Title : SW846 8260
QLast Update : Thu Oct 18 17:01:24 2018
Response via : Initial Calibration

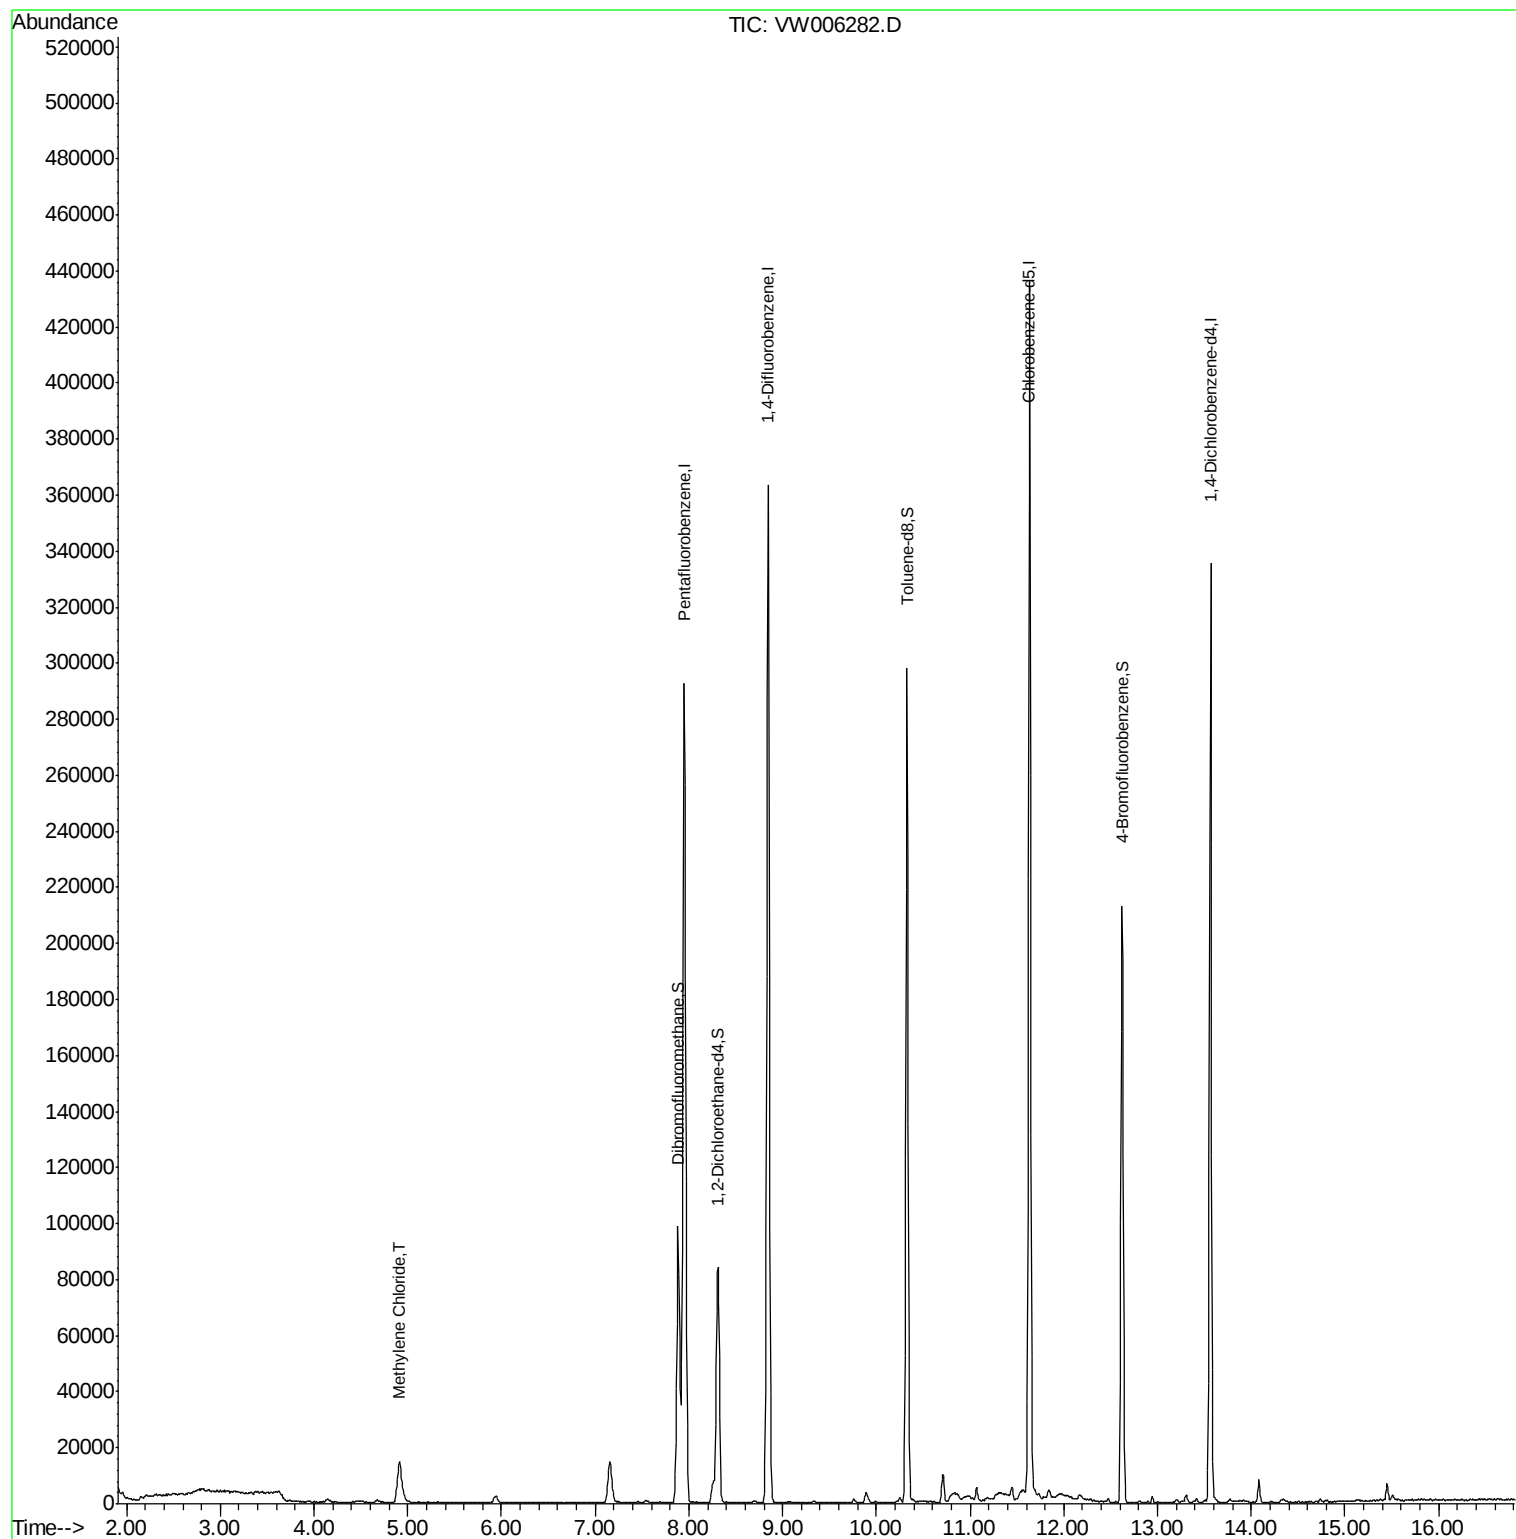



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW006282.D

Acq: 23 Oct 2018 06:38

Instrument :

MSVOA_W

ClientSampleId :


SA-SB-01A

Tot Ion:168 Resp: 237771

Ion Ratio Lower Upper

168 100

99 48.9 39.9 59.9

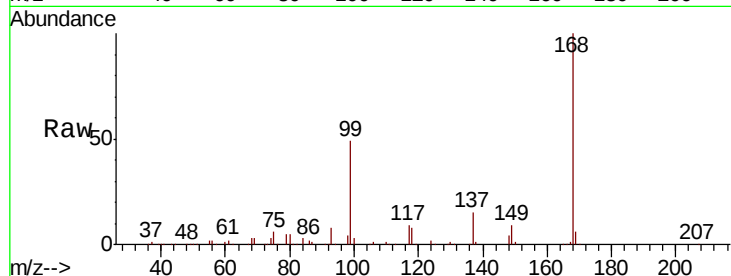

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

120000

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00 8.10

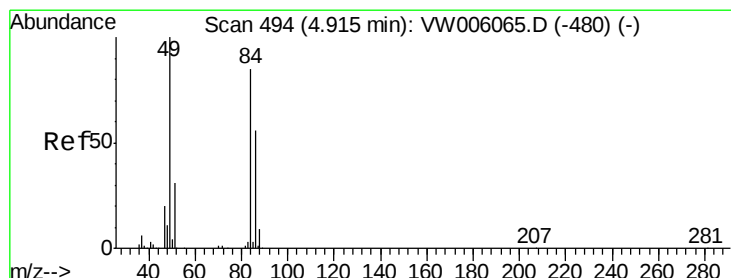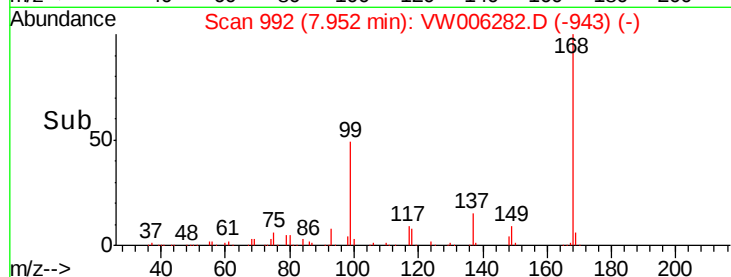

#20

Methylene Chloride

Concen: 4.907 ug/l

RT: 4.91 min Scan# 493

Delta R.T. -0.01 min

Lab File: VW006282.D

Acq: 23 Oct 2018 06:38

Tgt Ion: 84 Resp: 13297


Ion Ratio Lower Upper

84 100

49 113.8 93.6 140.4

51 34.9 29.0 43.4

86 59.5 52.6 79.0

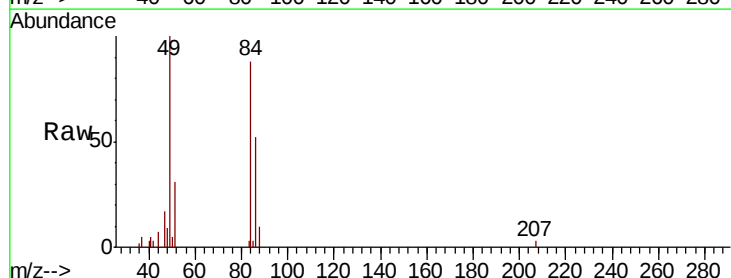

Abundance Ion 83.90 (83.60 to 84.60): VW

Ion 48.90 (48.60 to 49.60): VW

Ion 50.90 (50.60 to 51.60): VW

Ion 85.90 (85.60 to 86.60): VW

4.91


6000


4000

2000

0

Time--> 4.80 4.90 5.00




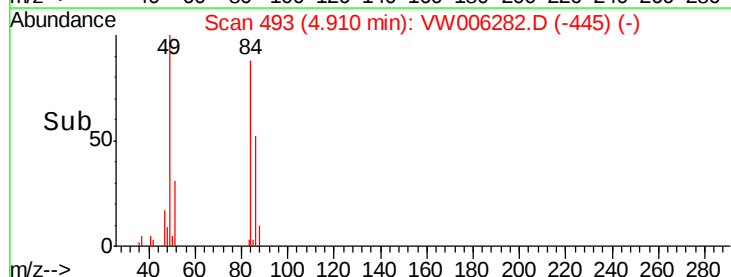


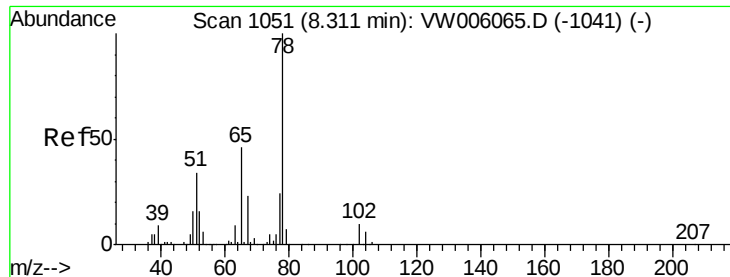

#33
 1,2-Dichloroethane-d4
 Concen: 34.822 ug/l
 RT: 8.31 min Scan# 1051
 Delta R.T. 0.00 min
 Lab File: VW006282.D
 Acq: 23 Oct 2018 06:38




Instrument :
 MSVOA_W
 ClientSampleId :
 SA-SB-01A

Tot Ion: 65 Resp: 68643
 Ion Ratio Lower Upper
 65 100
 67 50.7 0.0 101.0

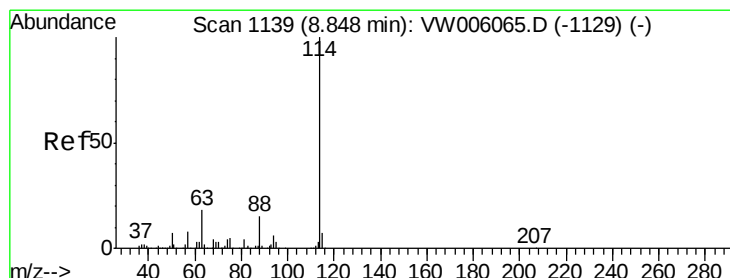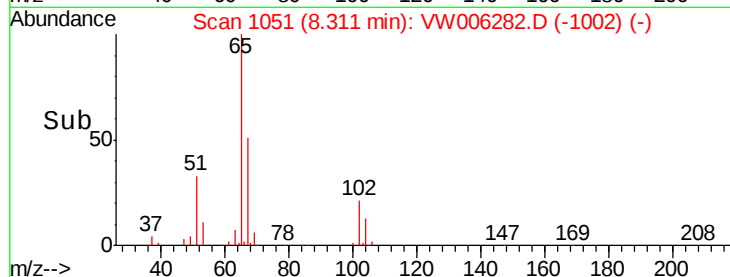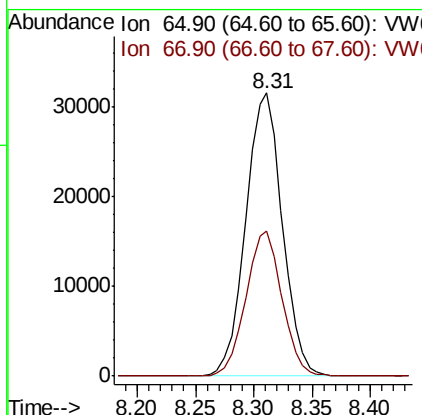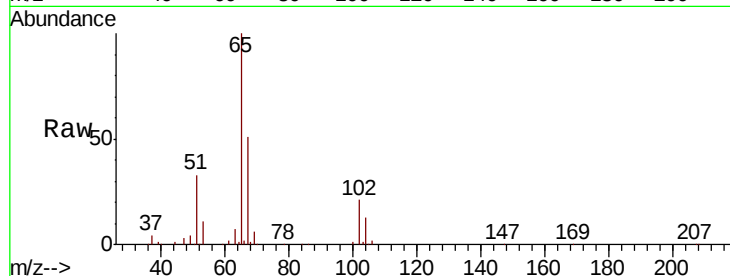

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. 0.00 min
 Lab File: VW006282.D
 Acq: 23 Oct 2018 06:38

Tgt Ion: 114 Resp: 326347
 Ion Ratio Lower Upper
 114 100
 63 17.5 0.0 36.8
 88 14.6 0.0 29.0


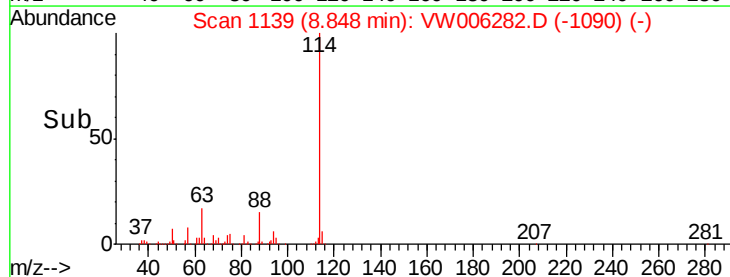
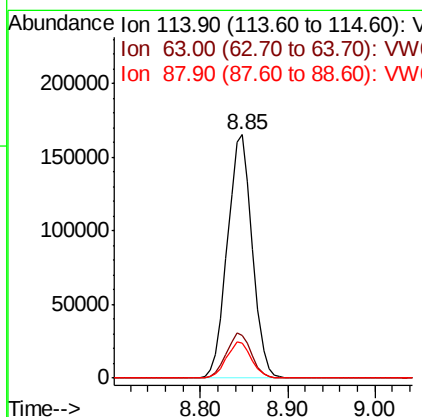
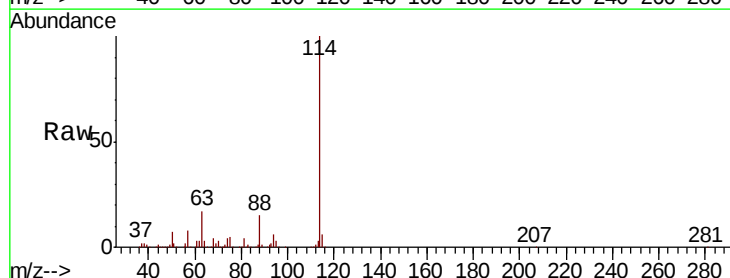




#35
 Dibromofluoromethane
 Concen: 35.534 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.01 min
 Lab File: VW006282.D
 Acq: 23 Oct 2018 06:38




Instrument :
 MSVOA_W
 ClientSampleId :
 SA-SB-01A

Tot Ion:113 Resp: 68523
 Ion Ratio Lower Upper
 113 100
 111 102.0 81.4 122.0
 192 23.1 18.7 28.1

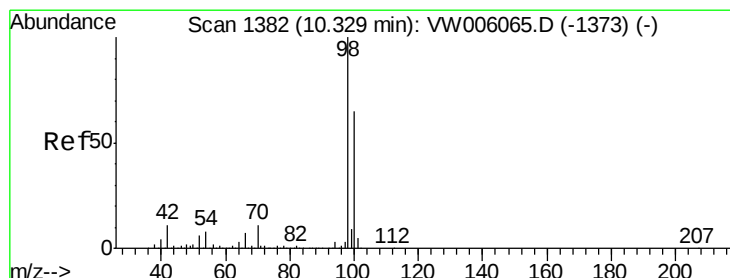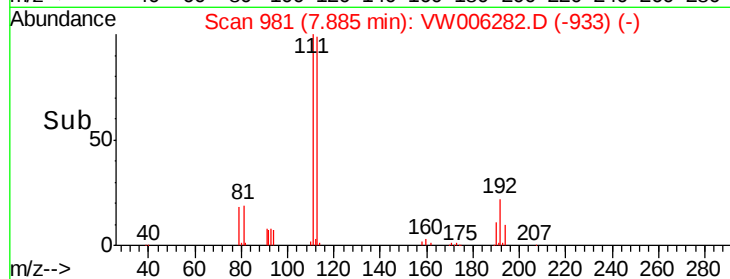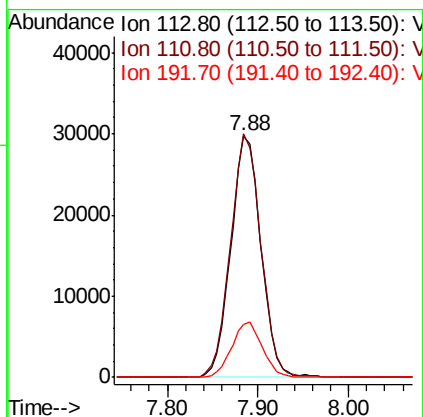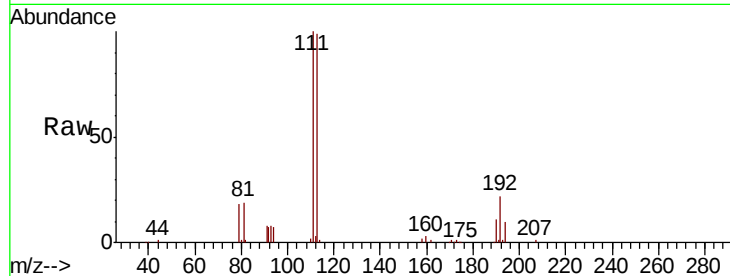

#50
 Toluene-d8
 Concen: 28.310 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. -0.01 min
 Lab File: VW006282.D
 Acq: 23 Oct 2018 06:38

Tgt Ion: 98 Resp: 207699
 Ion Ratio Lower Upper
 98 100
 100 64.4 51.6 77.4


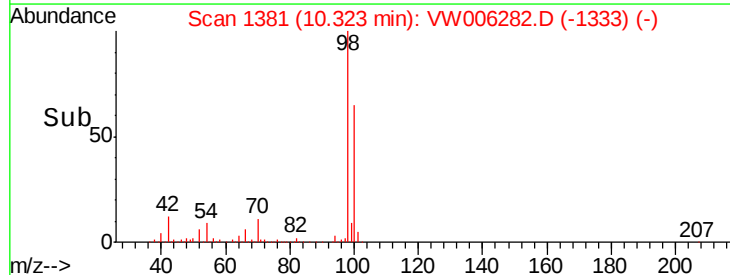
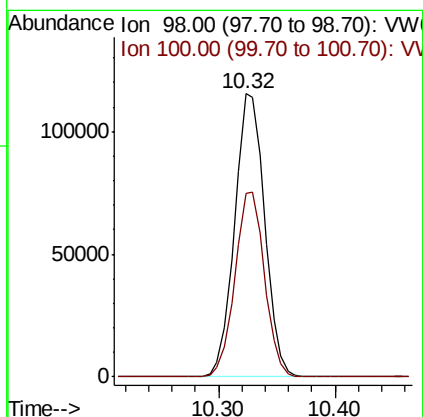
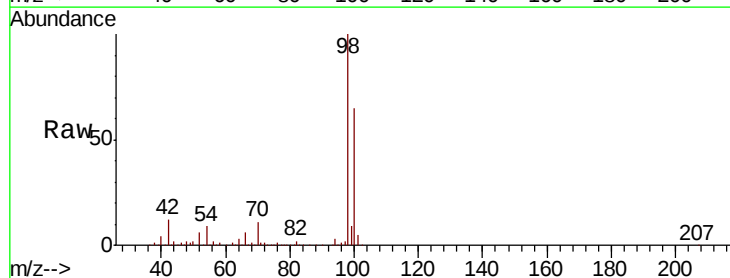




#62
4-Bromofluorobenzene
Concen: 22.093 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. 0.00 min
Lab File: VW006282.D
Acq: 23 Oct 2018 06:38




Instrument :
MSVOA_W
ClientSampleId :
SA-SB-01A


Tot Ion	95	Resp	60877
Ion Ratio	Lower	Upper	
95	100		
174	95.7	0.0	186.0
176	89.6	0.0	181.6

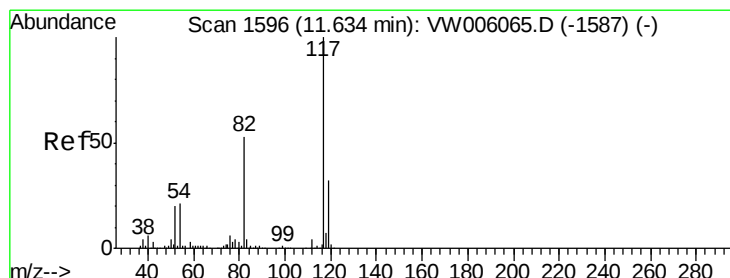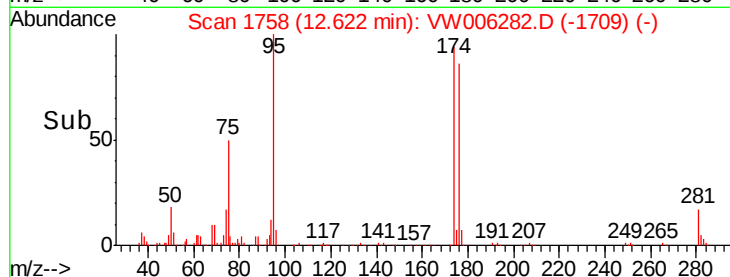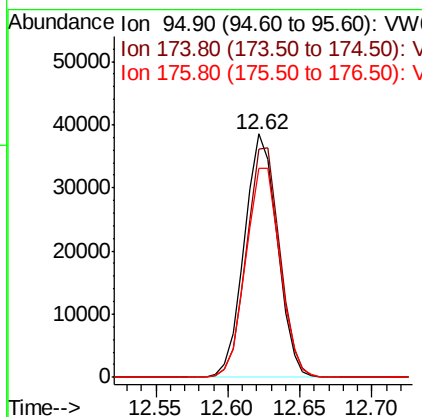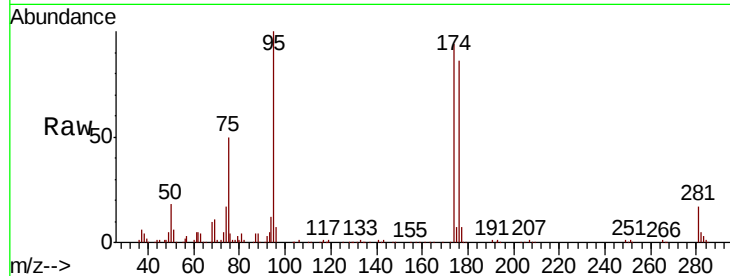

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW006282.D
Acq: 23 Oct 2018 06:38

Tgt Ion	117	Resp	246514
Ion Ratio	Lower	Upper	
117	100		
82	54.6	42.1	63.1
119	32.4	25.8	38.6

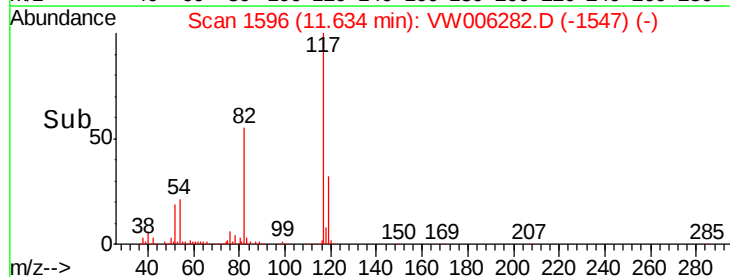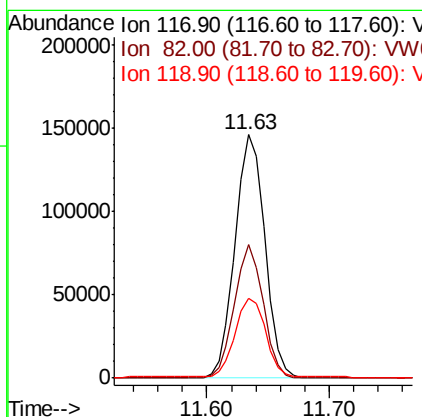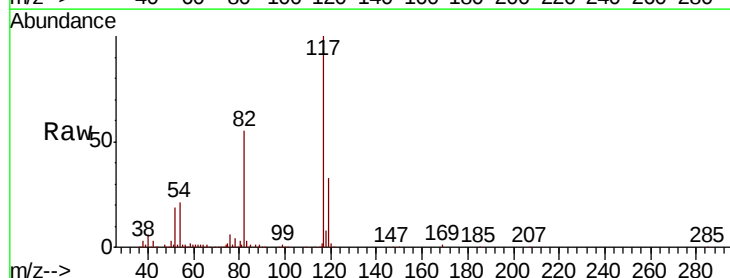

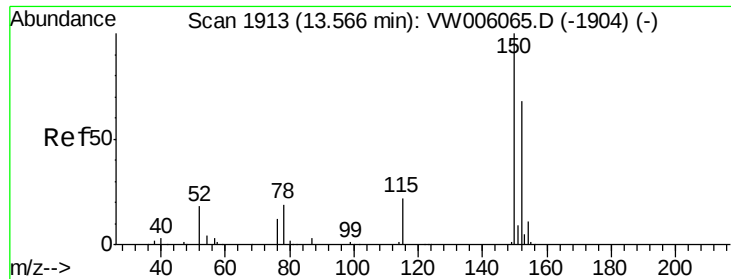

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.57 min Scan# 1913

Delta R.T. 0.00 min

Lab File: VW006282.D

Acq: 23 Oct 2018 06:38

Instrument :

MSVOA_W

ClientSampleId :

SA-SB-01A


Tot Ion:152 Resp: 95151

Ion Ratio Lower Upper

152 100

115 55.0 27.8 83.3

150 153.7 0.0 349.2

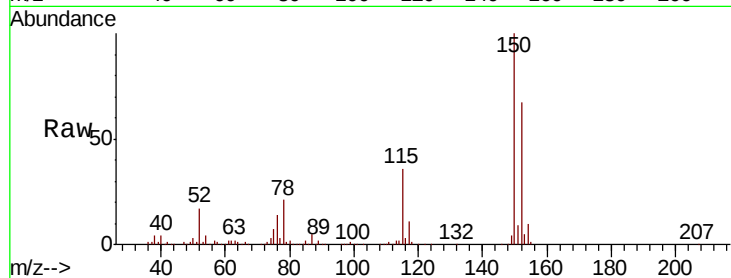

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

