



Dichlorodifluoromethane

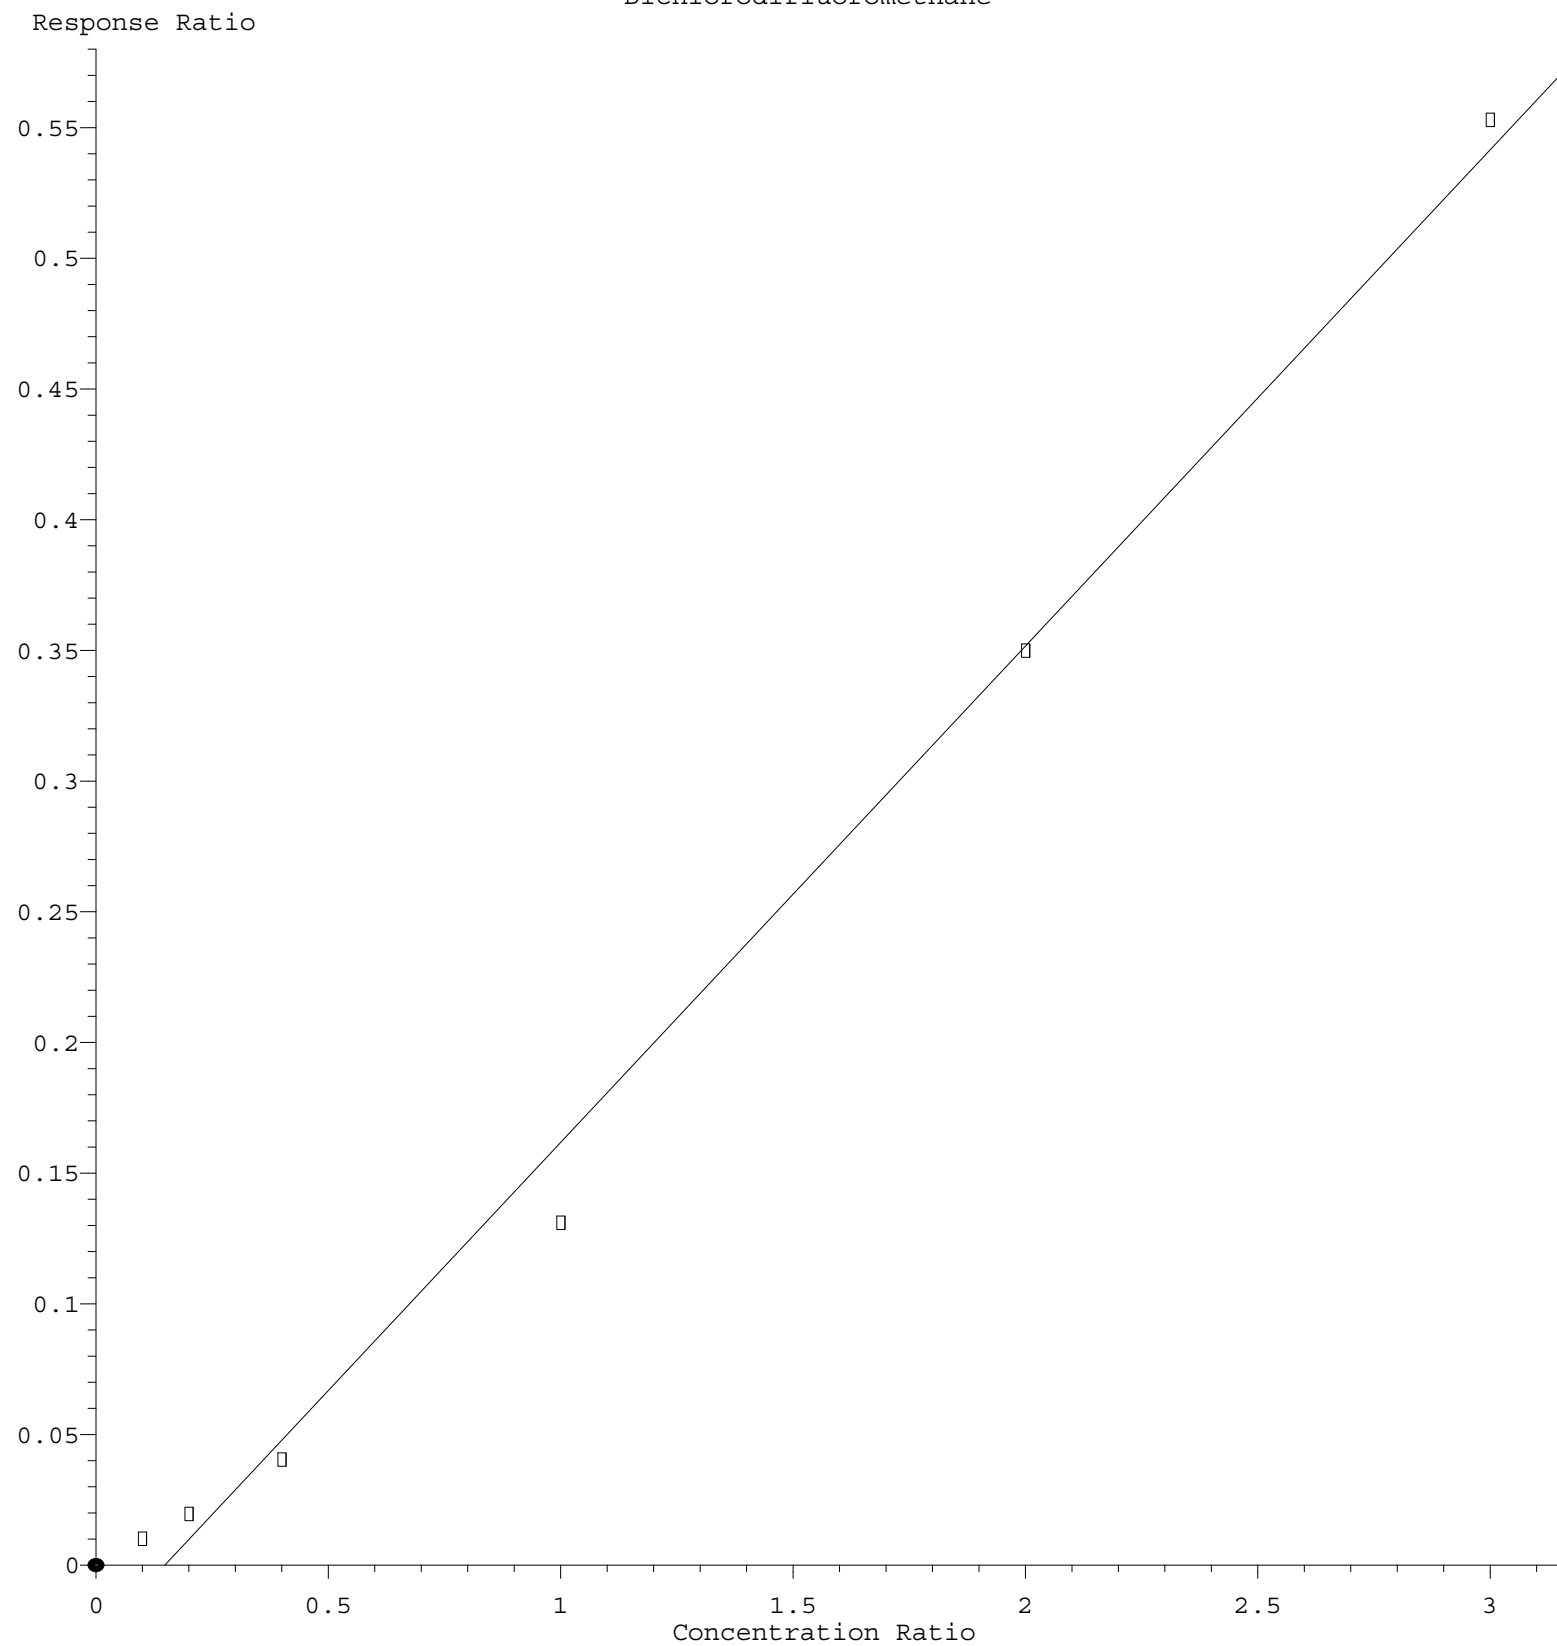

$\text{Response} = 1.899\text{e-}001 * \text{Amt} - 2.810\text{e-}002$
 Coef of Det (r^2) = 0.993448 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W102221S.M
 Calibration Table Last Updated: Sat Oct 23 05:58:59 2021

Methylene Chloride

Response Ratio

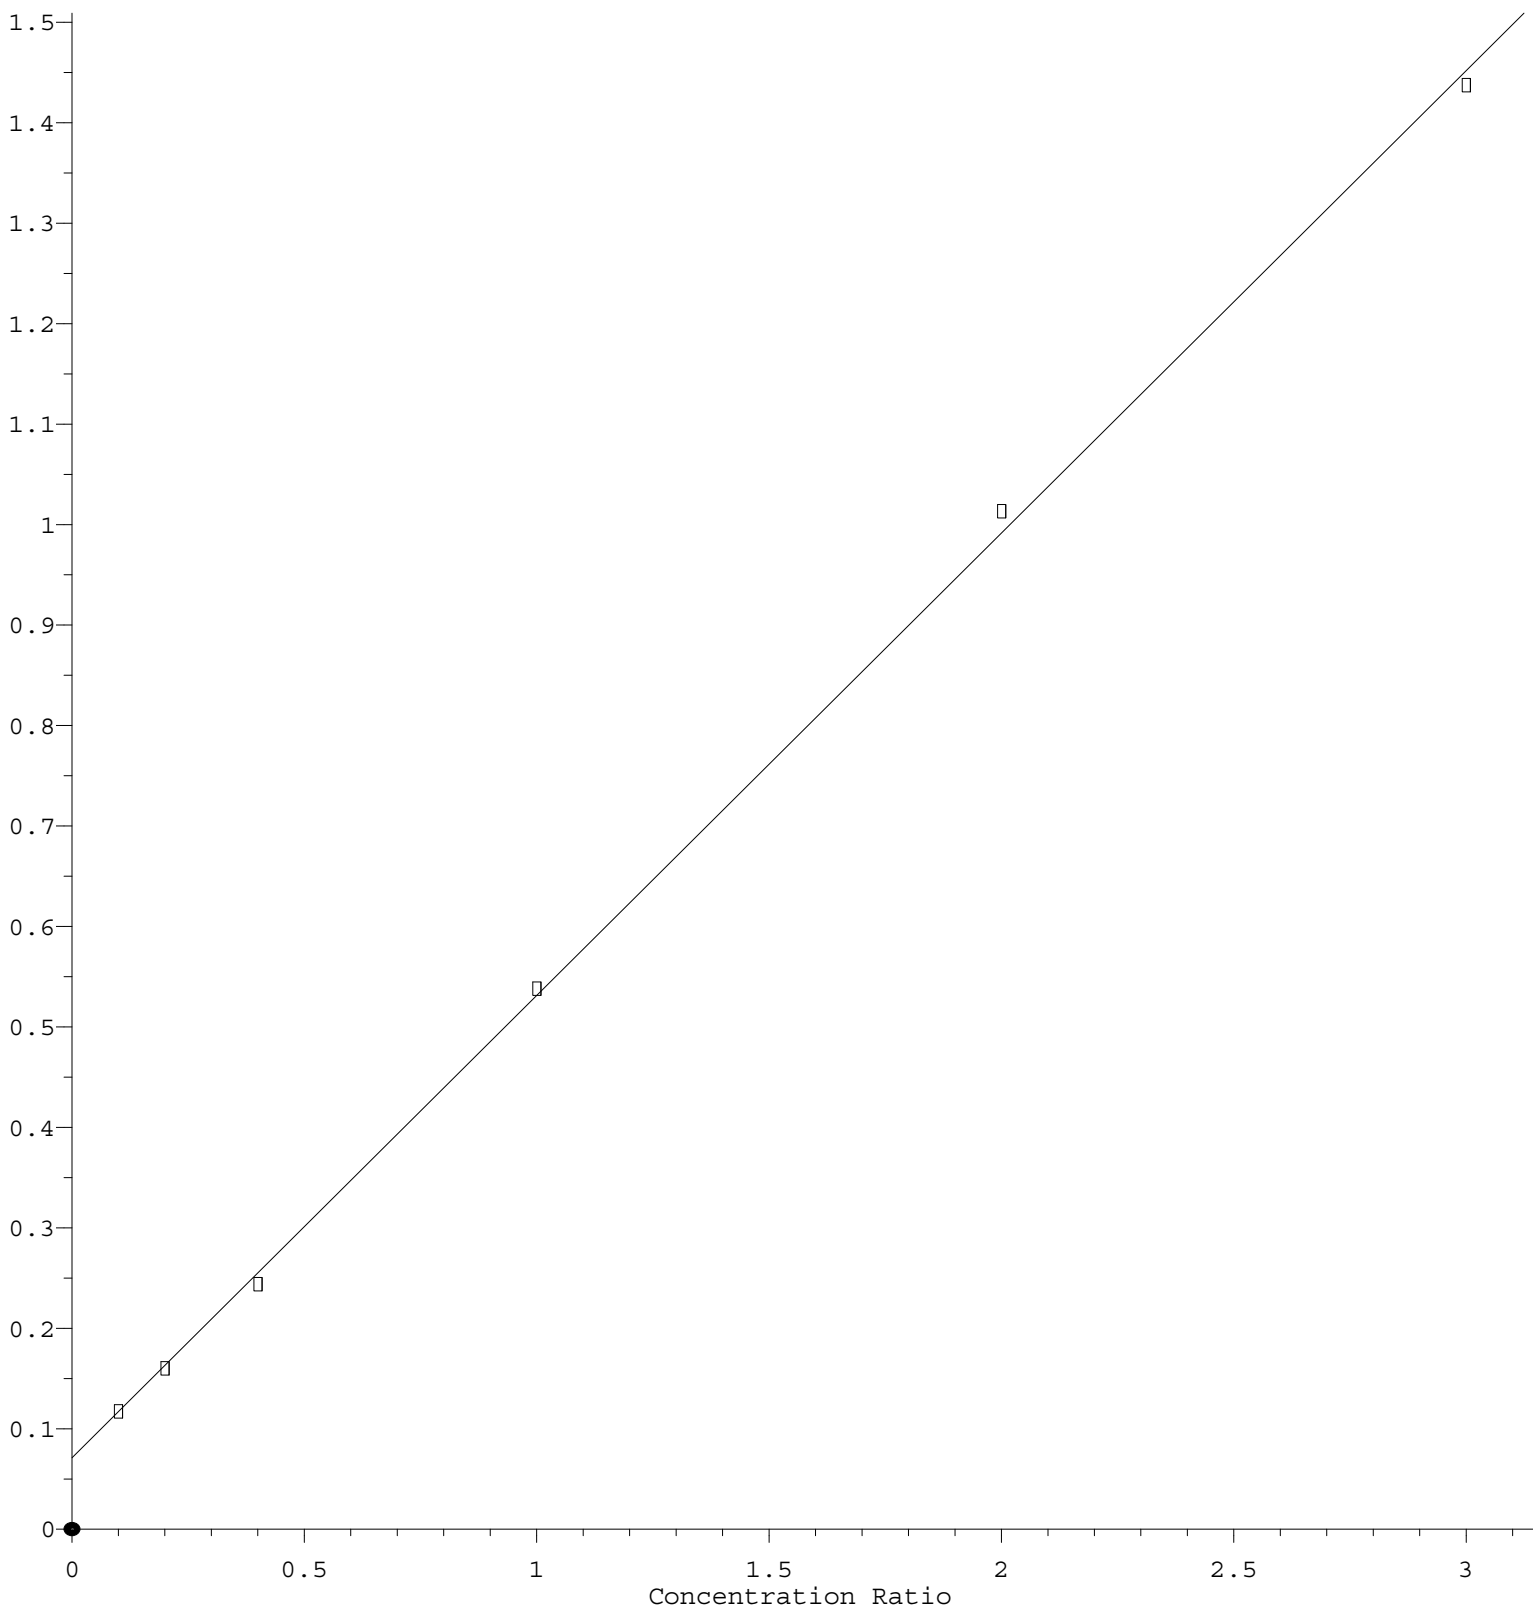

$$\text{Response} = 4.605\text{e-}001 * \text{Amt} + 7.067\text{e-}002$$

Coef of Det (r^2) = 0.999397 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W102221S.M

Calibration Table Last Updated: Sat Oct 23 05:58:59 2021