
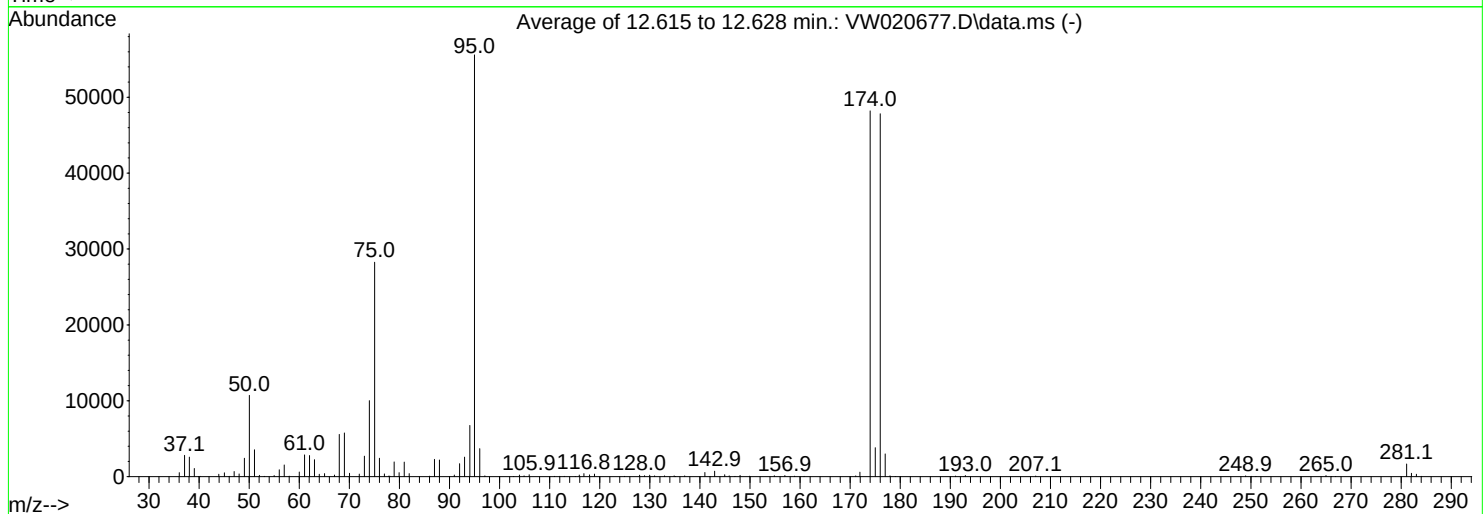


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102221\
Data File : VW020677.D
Acq On : 22 Oct 2021 10:26
Operator : SY/VA
Sample : BFB
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W102221S.M
Title : SW846 8260
Last Update : Sat Oct 23 05:58:59 2021

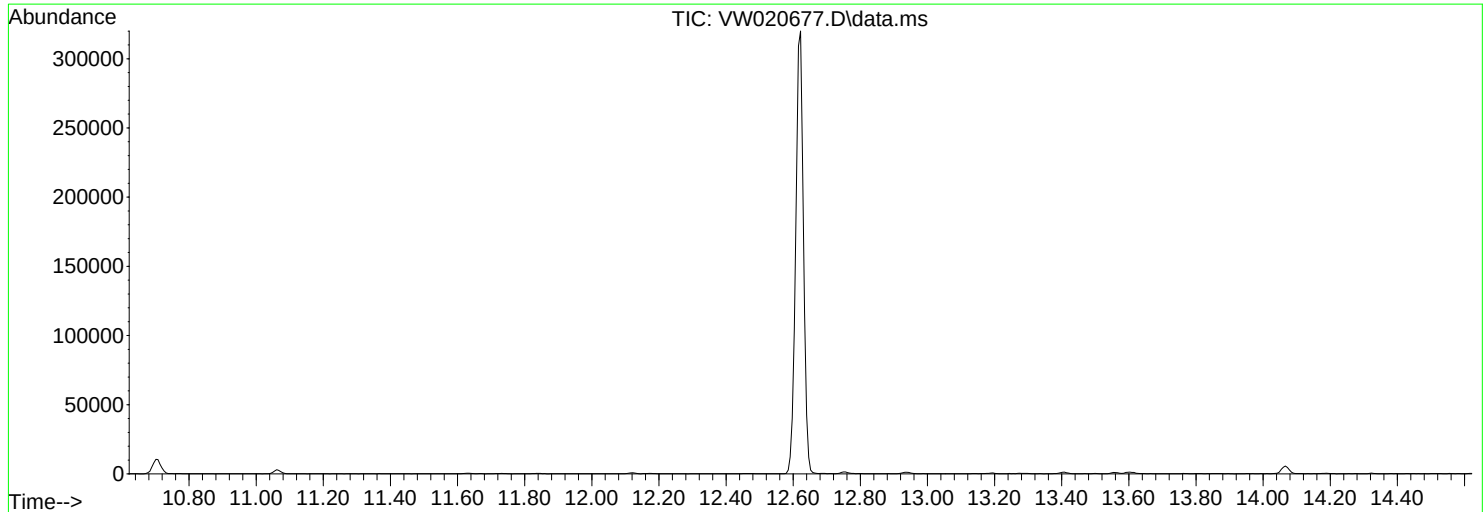

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	10709	PASS
75	95	30	60	50.8	28251	PASS
95	95	100	100	100.0	55595	PASS
96	95	5	9	6.6	3683	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.7	48205	PASS
175	174	5	9	7.9	3815	PASS
176	174	95	101	99.2	47827	PASS
177	176	5	9	6.3	3000	PASS