

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW102318\
 Data File : VW006293.D
 Acq On : 23 Oct 2018 13:32
 Operator : SY/AP
 Sample : VW1023SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK91

Quant Time: Oct 24 02:11:38 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 24 01:59:01 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	399806	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	375071	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	195738	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	97818	21.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.76%
7) Chloroethane-d5	2.90	69	91457	23.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.28%
10) 1,1-Dichloroethene-d2	4.01	63	157646	18.21	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	72.84%
20) 2-Butanone-d5	7.09	46	57851	38.71	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.42%
24) Chloroform-d	7.65	84	220318	25.44	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.76%
26) 1,2-Dichloroethane-d4	8.31	65	124027	25.89	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.56%
29) Benzene-d6	8.27	84	450873	26.48	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.92%
33) 1,2-Dichloropropane-d6	9.28	67	128660	25.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.12%
37) Toluene-d8	10.33	98	446312	26.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.84%
38) trans-1,3-Dichloropropene-	10.58	79	53003	21.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.88%
39) 2-Hexanone-d5	10.93	63	48831	39.32	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	78.64%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	113571	22.73	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.92%
61) 1,2-Dichlorobenzene-d4	13.86	152	183718	27.38	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.52%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Methylene chloride	4.91	84	7764	1.504	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW102318\
Data File : VW006293.D
Acq On : 23 Oct 2018 13:32
Operator : SY/AP
Sample : VW1023SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK91

Quant Time: Oct 24 02:11:38 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM100918S.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 24 01:59:01 2018
Response via : Initial Calibration

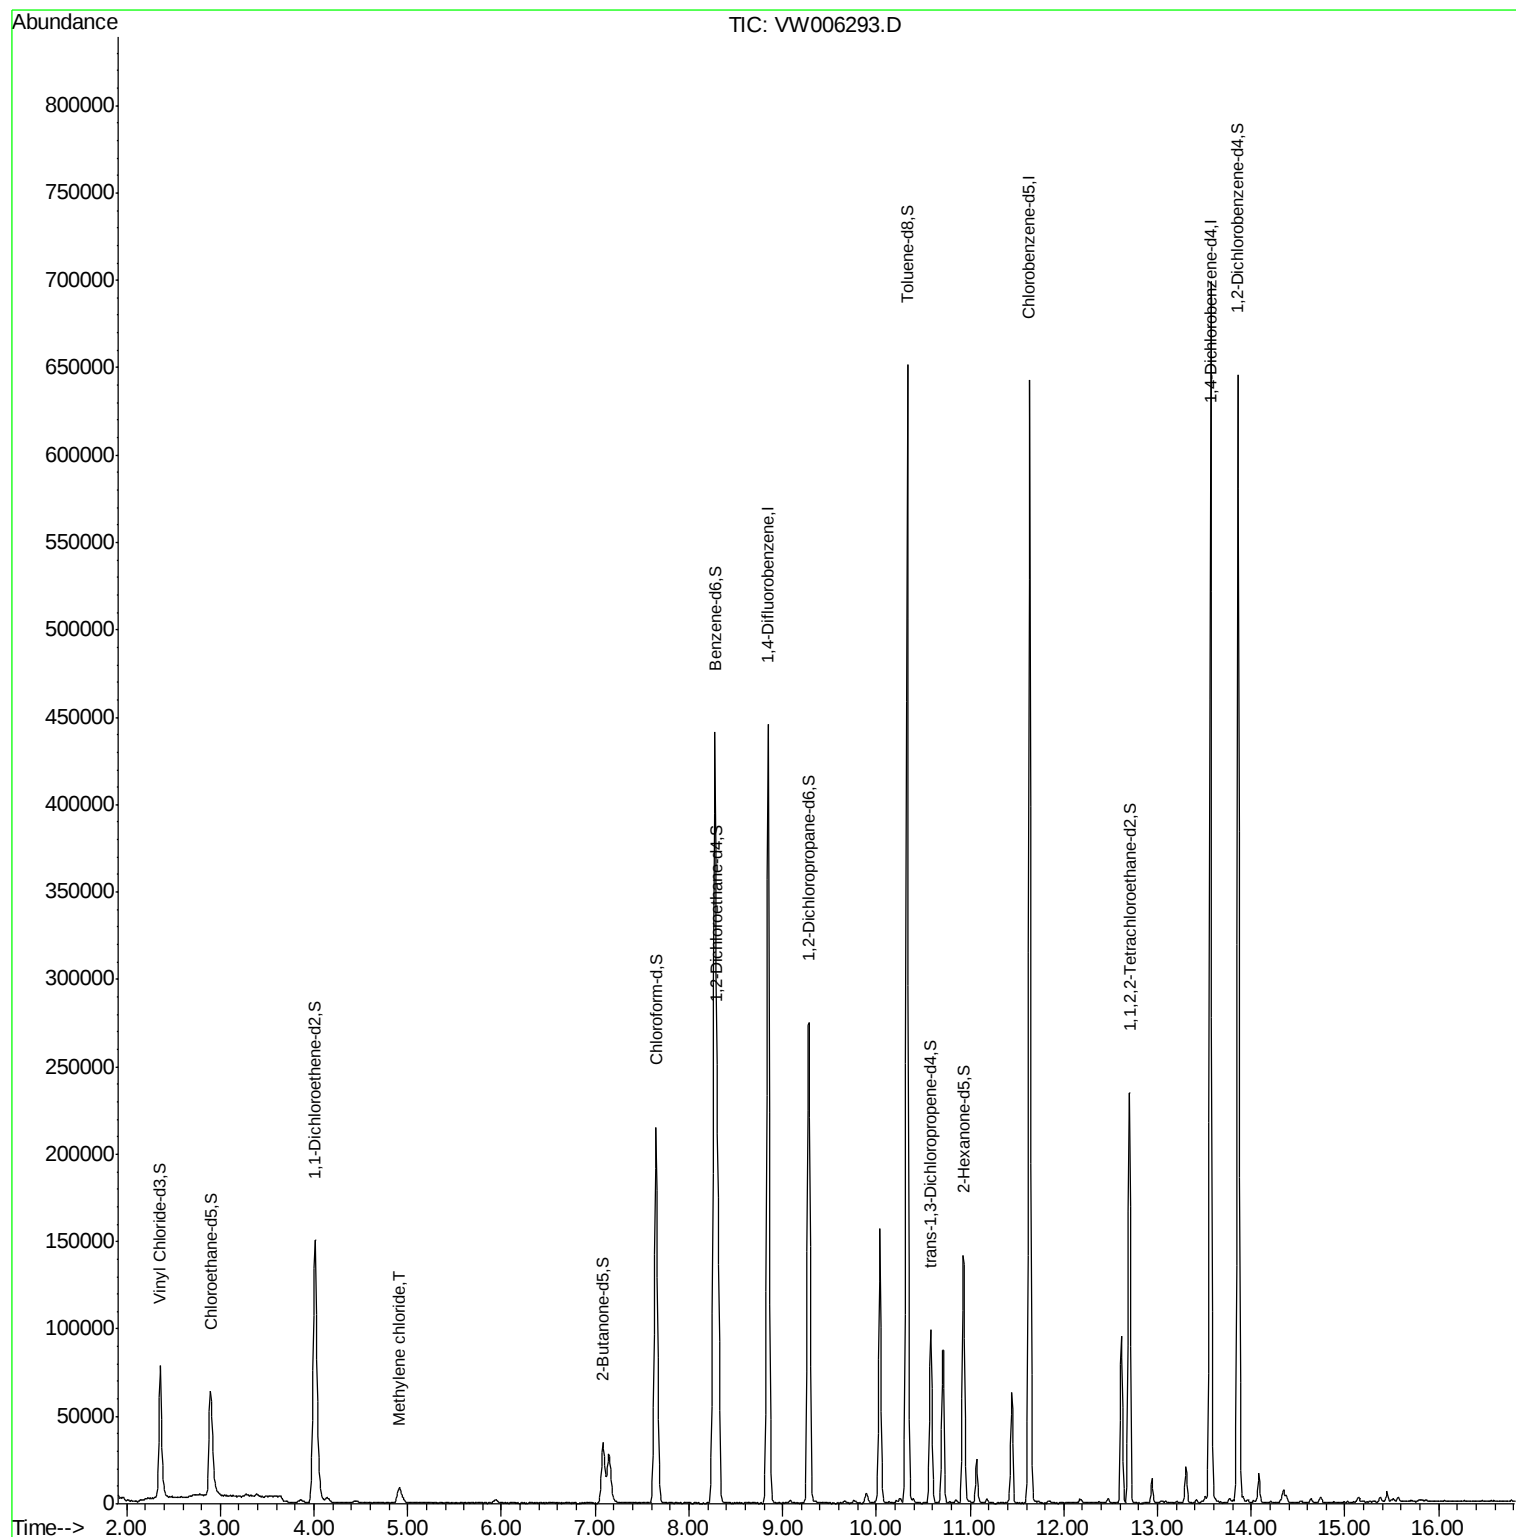

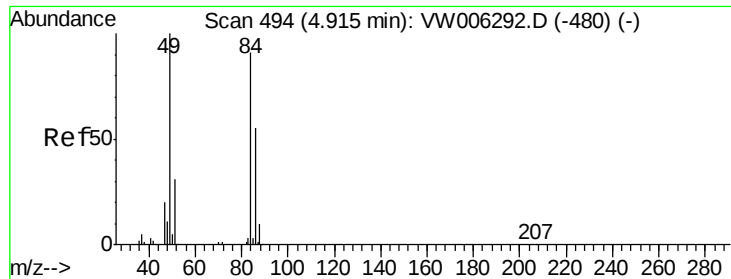

#16
Methylene chloride
Concen: 1.504 ug/L
RT: 4.91 min Scan# 493
Delta R.T. -0.01 min
Lab File: VW006293.D
Acq: 23 Oct 2018 13:32

Instrument :
MSVOA_W
ClientSampleId :
VBLK91

Tgt Ion: 84 Resp: 7764
Ion Ratio Lower Upper
84 100
49 111.7 83.5 155.1
86 58.7 44.9 83.5

