

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102319\
 Data File : VW013672.D
 Acq On : 23 Oct 2019 17:32
 Operator : SY/VA
 Sample : K5501-10
 Misc : 6.26G/5ML/MSVOA W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 185-56-(2.2)

Quant Time: Oct 24 08:00:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W102319S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 23 14:11:46 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	67282	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	95557	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	78566	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	27378	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	27510	54.50	ug/l	0.00
Spiked Amount 50.000			Recovery	=	109.00%	
35) Dibromofluoromethane	7.88	113	28602	53.87	ug/l	0.00
Spiked Amount 50.000			Recovery	=	107.74%	
50) Toluene-d8	10.32	98	108507	50.15	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.30%	
62) 4-Bromofluorobenzene	12.62	95	29598	40.40	ug/l	0.00
Spiked Amount 50.000			Recovery	=	80.80%	
Target Compounds						
16) Acetone	4.12	43	2684	25.080	ug/l	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102319\
Data File : VW013672.D
Acq On : 23 Oct 2019 17:32
Operator : SY/VA
Sample : K5501-10
Misc : 6.26G/5ML/MSVOA W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
185-56-(2.2)

Quant Time: Oct 24 08:00:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W102319S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 23 14:11:46 2019
Response via : Initial Calibration

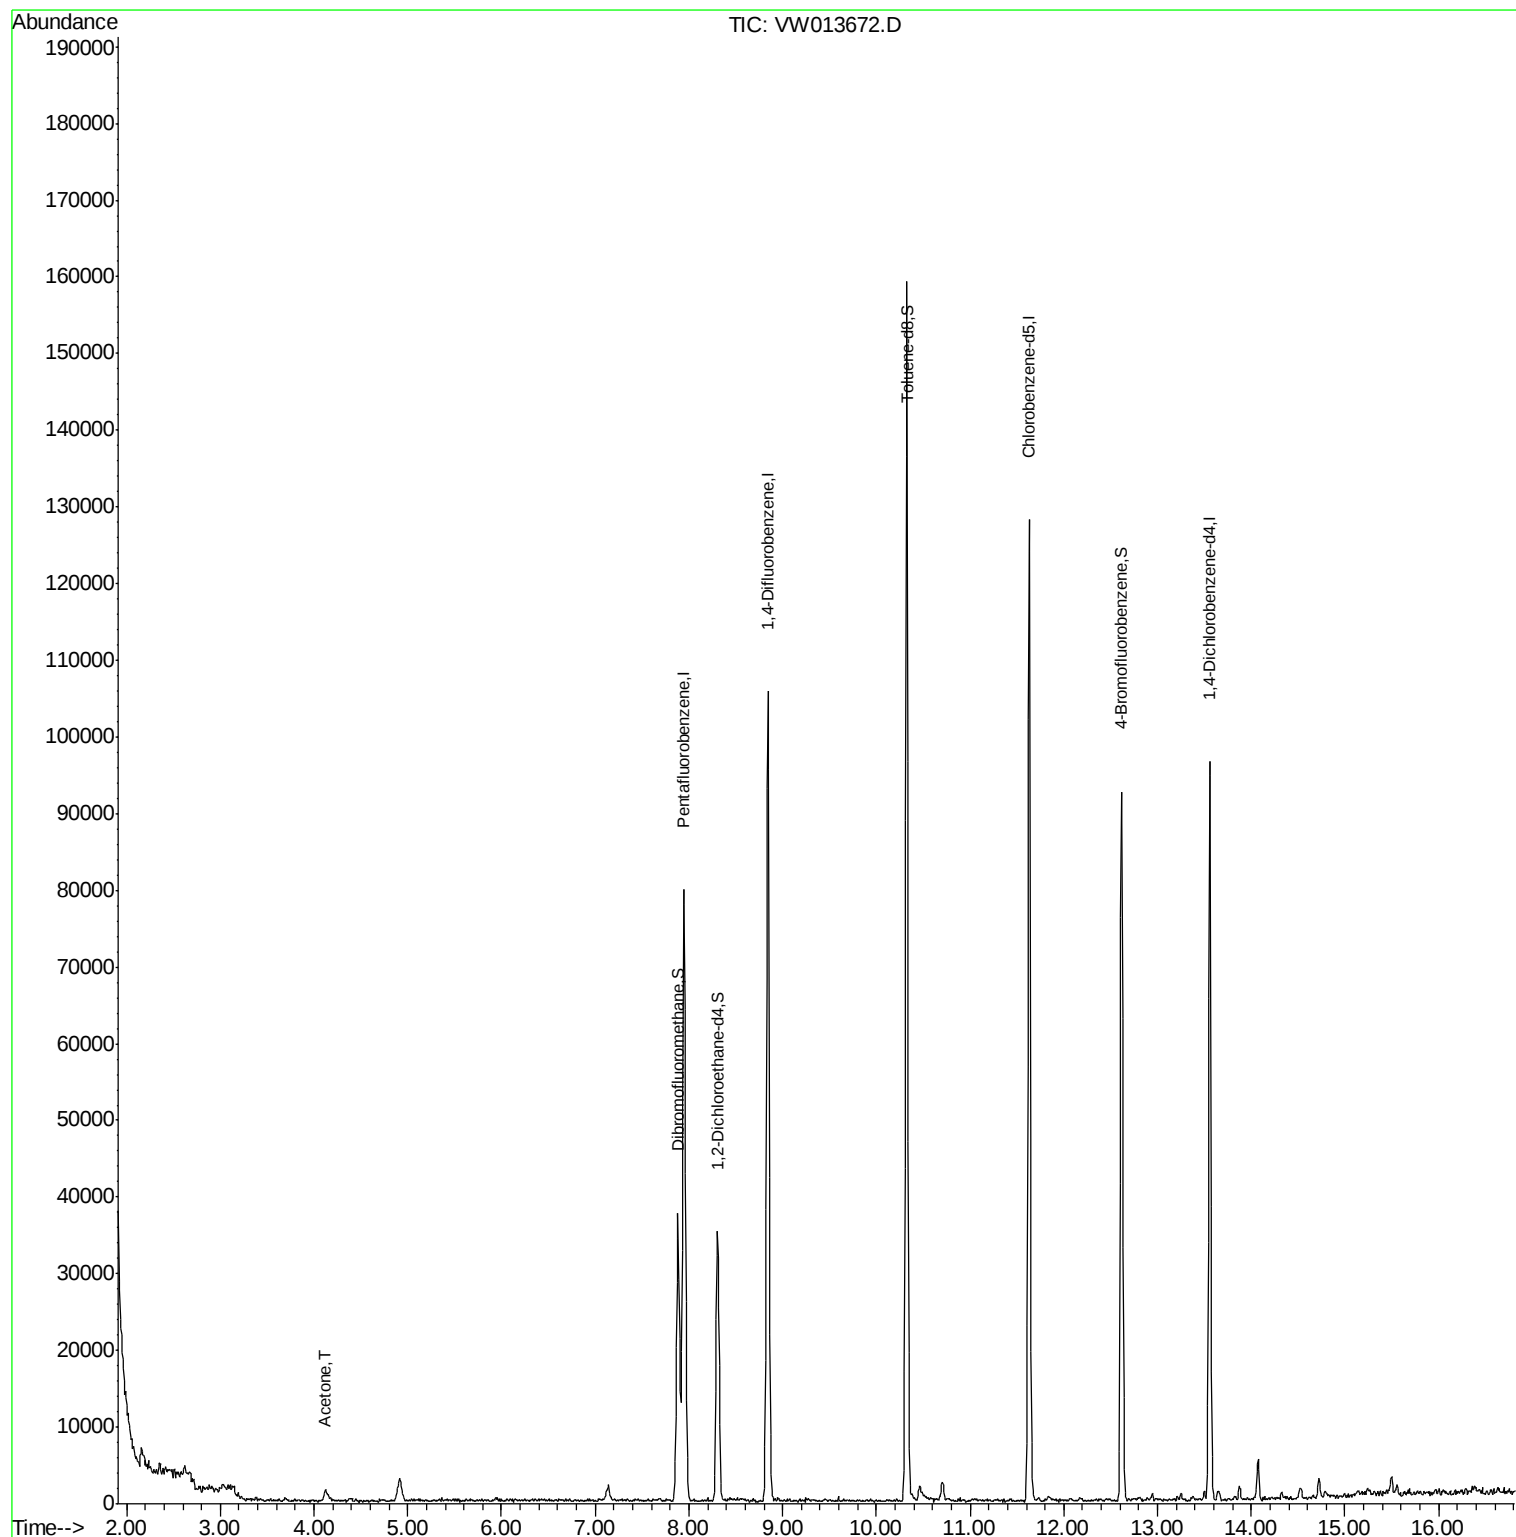

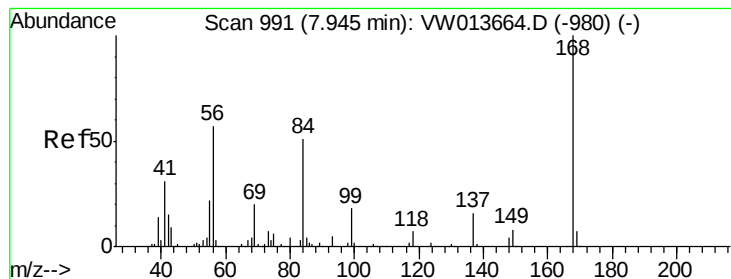

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW013672.D

Acq: 23 Oct 2019 17:32

Instrument :

MSVOA_W

ClientSampleId :


185-56-(2.2)

Tot Ion:168 Resp: 67282

Ion Ratio Lower Upper




168 100

99 47.1 39.0 58.6

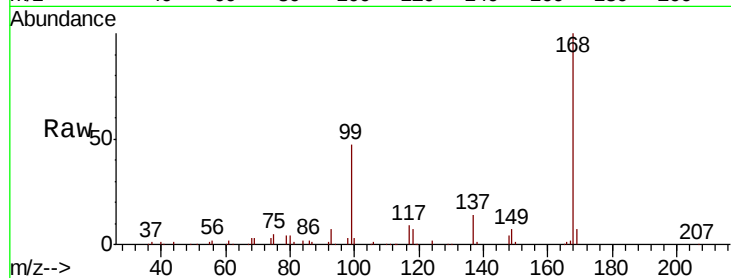

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

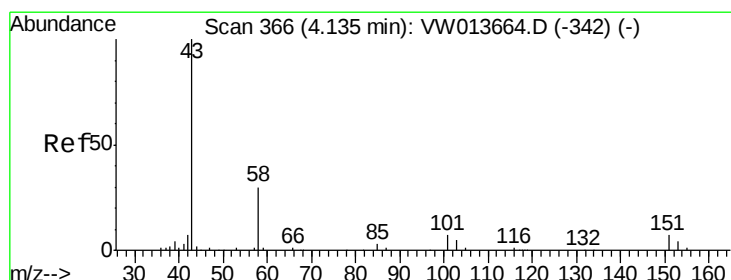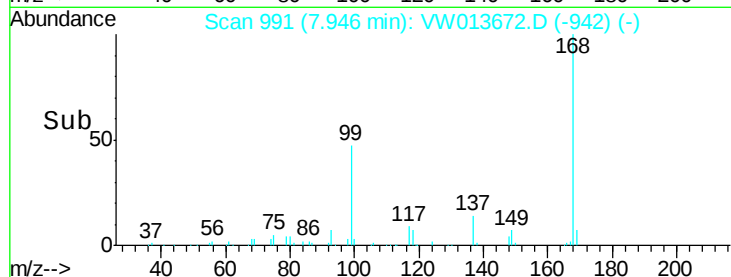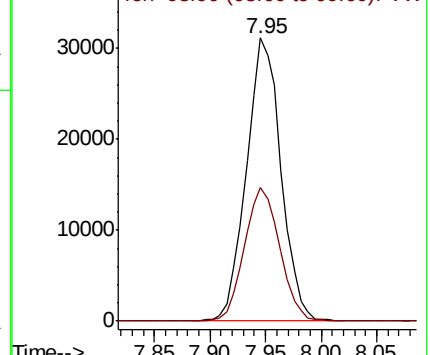

#16

Acetone

Concen: 25.080 ug/l

RT: 4.12 min Scan# 364

Delta R.T. -0.01 min

Lab File: VW013672.D


Acq: 23 Oct 2019 17:32

Tgt Ion: 43 Resp: 2684

Ion Ratio Lower Upper



43 100


58 26.1 24.1 36.1

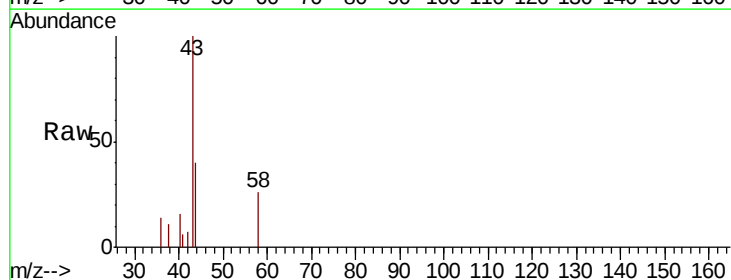

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW



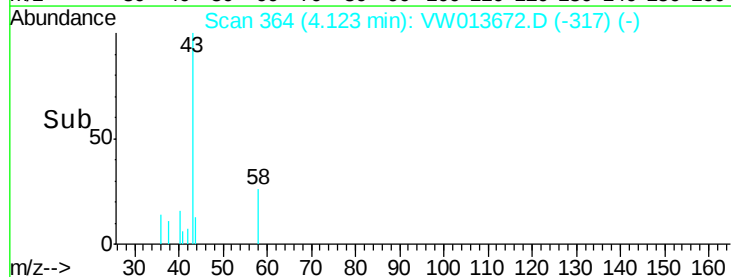
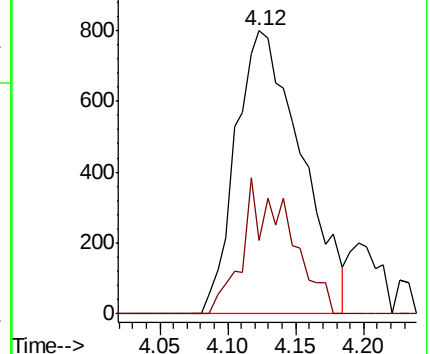


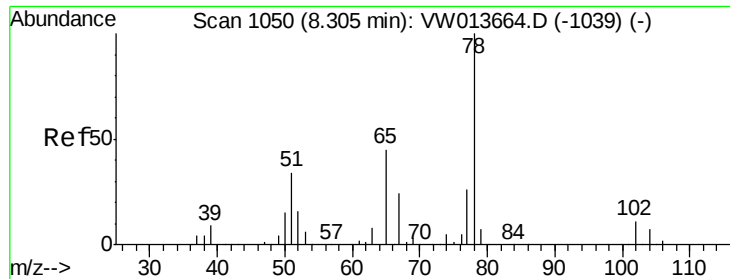

#33
 1,2-Dichloroethane-d4
 Concen: 54.505 ug/l
 RT: 8.31 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: VW013672.D
 Acq: 23 Oct 2019 17:32




Instrument :
 MSVOA_W
 ClientSampleId :
 185-56-(2.2)


Tot Ion: 65 Resp: 27510
 Ion Ratio Lower Upper
 65 100
 67 52.8 0.0 109.4

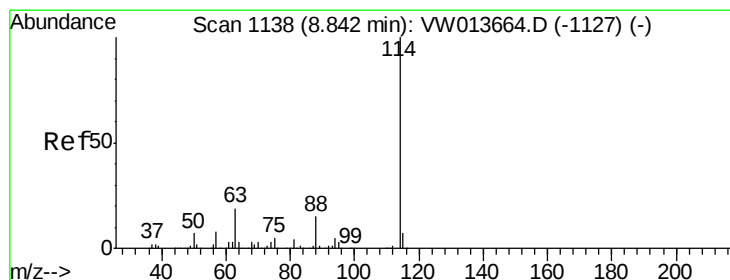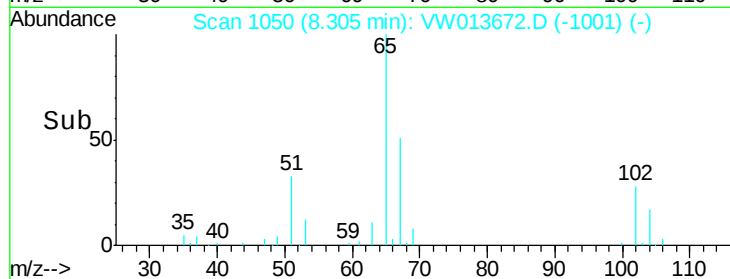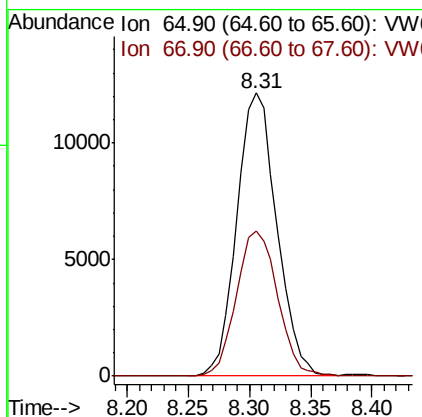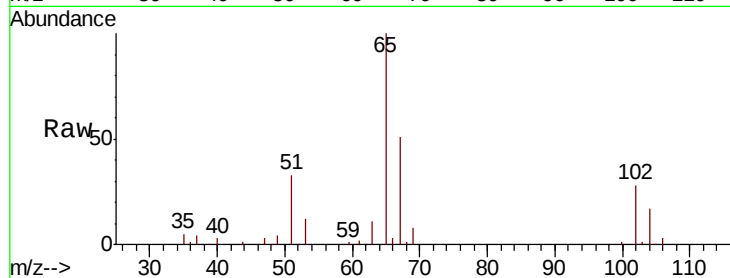

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW013672.D
 Acq: 23 Oct 2019 17:32

Tgt Ion: 114 Resp: 95557
 Ion Ratio Lower Upper
 114 100
 63 21.0 0.0 37.6
 88 14.9 0.0 30.2


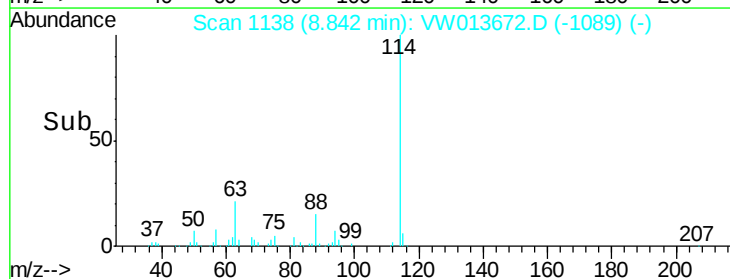
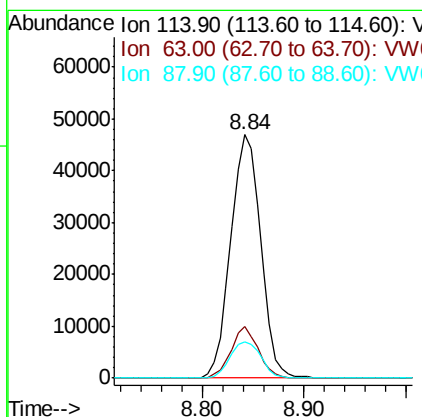
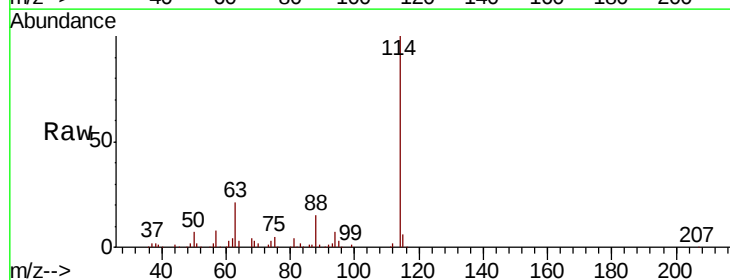


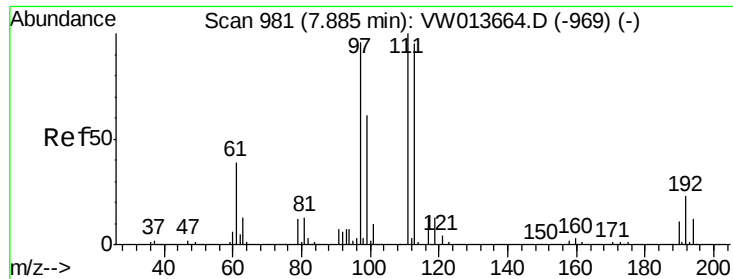

#35
 Dibromofluoromethane
 Concen: 53.868 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. 0.00 min
 Lab File: VW013672.D
 Acq: 23 Oct 2019 17:32




Instrument :
 MSVOA_W
 ClientSampleId :
 185-56-(2.2)


Tot Ion:113 Resp: 28602
 Ion Ratio Lower Upper
 113 100
 111 100.2 83.0 124.6
 192 24.1 19.4 29.2

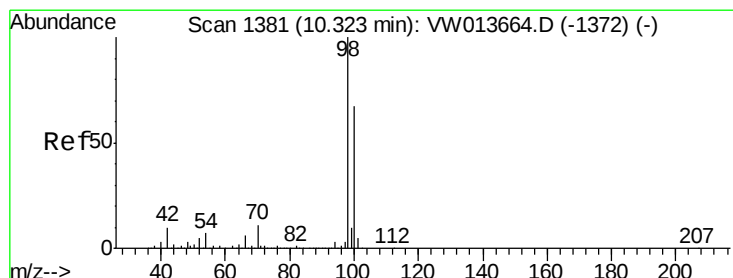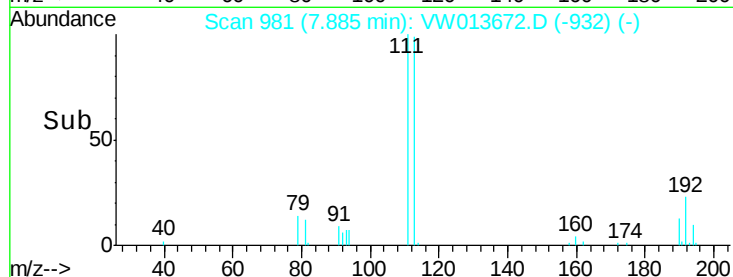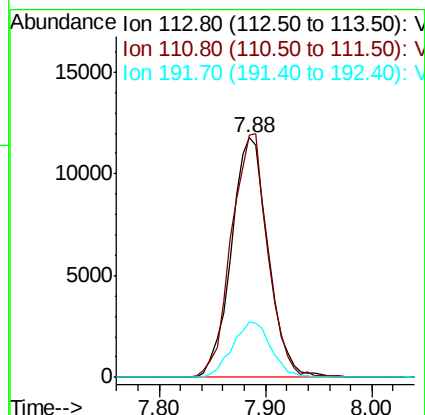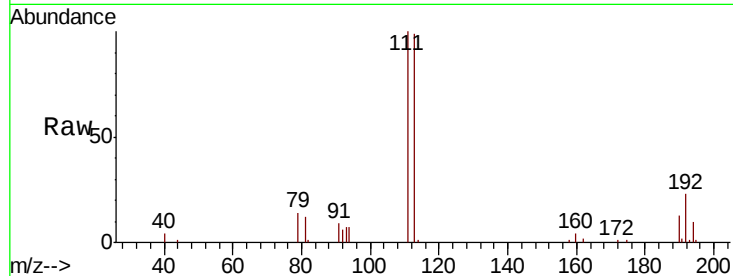

#50
 Toluene-d8
 Concen: 50.152 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. 0.00 min
 Lab File: VW013672.D
 Acq: 23 Oct 2019 17:32

Tgt Ion: 98 Resp: 108507
 Ion Ratio Lower Upper
 98 100
 100 65.1 53.4 80.0


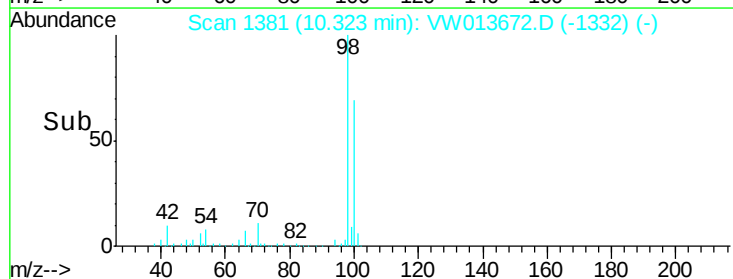
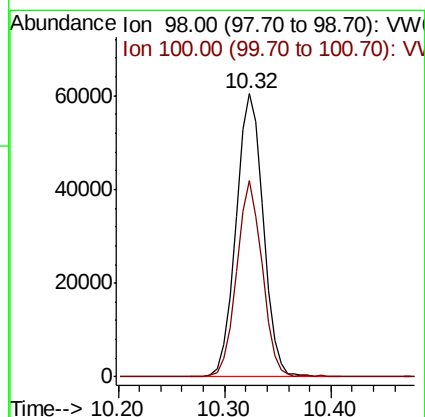
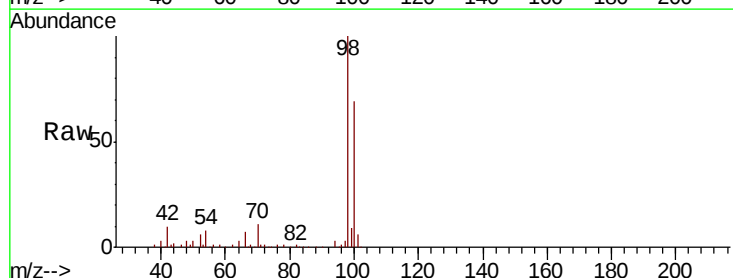


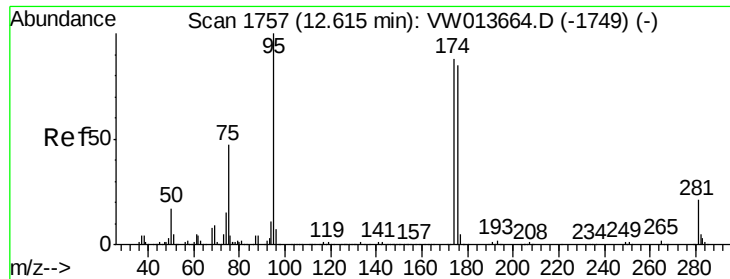

#62
4-Bromofluorobenzene
Concen: 40.402 ug/l
RT: 12.62 min Scan# 1757
Delta R.T. 0.00 min
Lab File: VW013672.D
Acq: 23 Oct 2019 17:32




Instrument :
MSVOA_W
ClientSampleId :
185-56-(2.2)


Tot Ion: 95 Resp: 29598
Ion Ratio Lower Upper
95 100
174 95.6 0.0 183.6
176 91.1 0.0 178.0

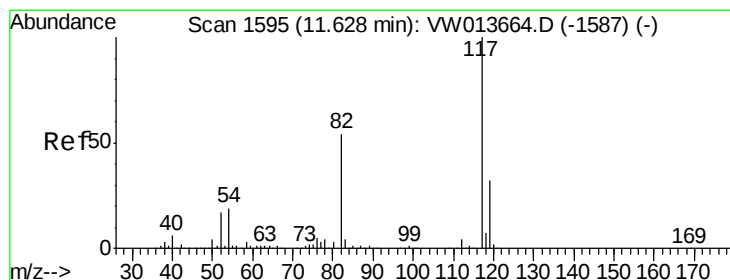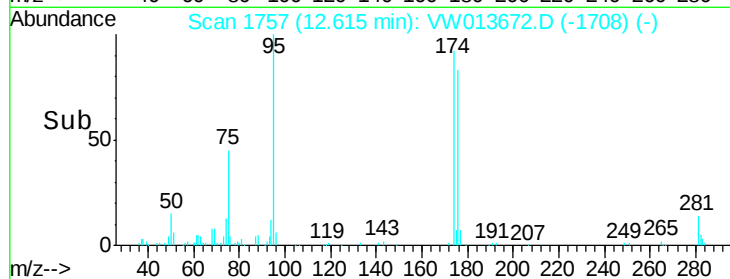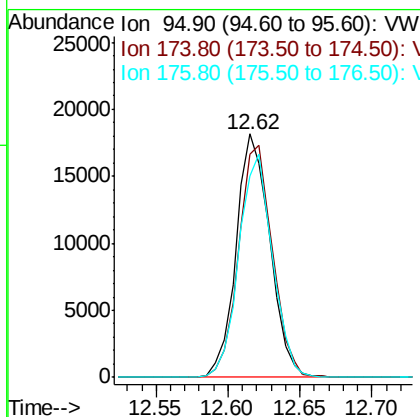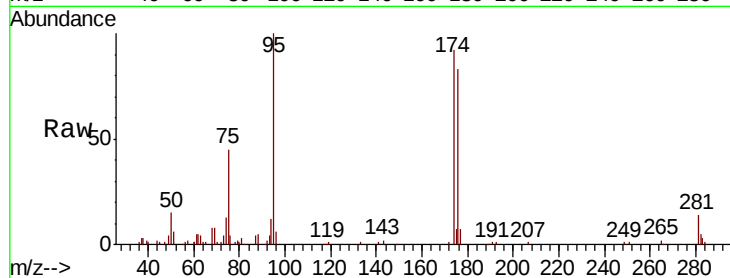

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1595
Delta R.T. 0.00 min
Lab File: VW013672.D
Acq: 23 Oct 2019 17:32

Tgt Ion: 117 Resp: 78566
Ion Ratio Lower Upper
117 100
82 54.3 43.6 65.4
119 33.2 25.4 38.2

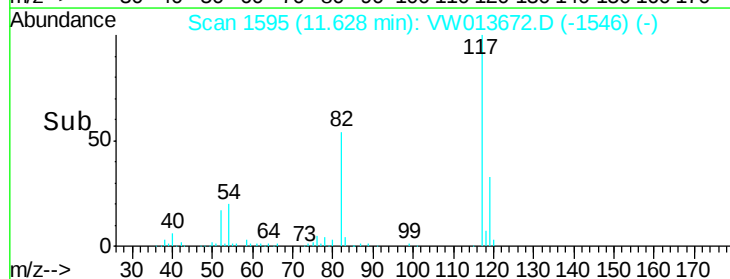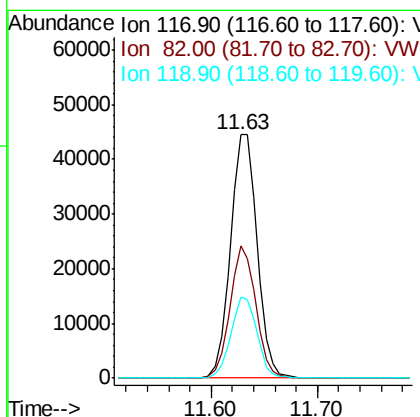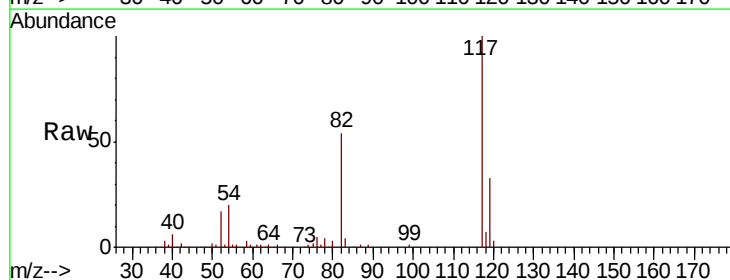

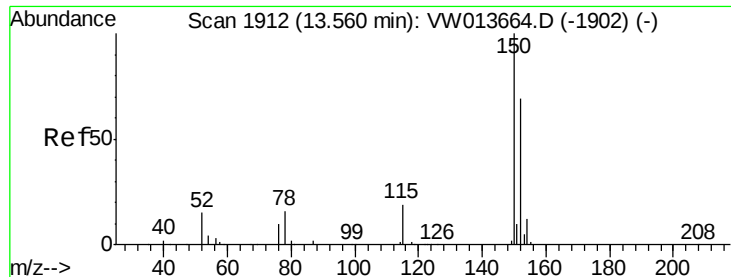

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW013672.D

Acq: 23 Oct 2019 17:32

Instrument :

MSVOA_W

ClientSampleId :

185-56-(2.2)


Tot Ion:152 Resp: 27378

Ion Ratio Lower Upper

152 100

115 56.5 27.4 82.2

150 160.7 0.0 345.4

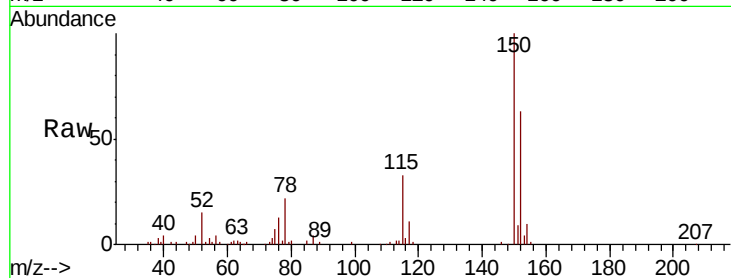

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

