

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102319\
 Data File : VW013679.D
 Acq On : 23 Oct 2019 20:34
 Operator : SY/VA
 Sample : K5485-02
 Misc : 3.63G/5ML/MSVOA W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 TP-24B-S2

Quant Time: Oct 24 08:18:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W102319S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 23 14:11:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	279360	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	423813	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	353022	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	147819	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	121886	58.16	ug/l	0.00
Spiked Amount						
			Recovery	=	116.32%	
35) Dibromofluoromethane	7.88	113	124935	53.05	ug/l	0.00
Spiked Amount						
			Recovery	=	106.10%	
50) Toluene-d8	10.32	98	483875	50.43	ug/l	0.00
Spiked Amount						
			Recovery	=	100.86%	
62) 4-Bromofluorobenzene	12.62	95	146997	45.24	ug/l	0.00
Spiked Amount						
			Recovery	=	90.48%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102319\
Data File : VW013679.D
Acq On : 23 Oct 2019 20:34
Operator : SY/VA
Sample : K5485-02
Misc : 3.63G/5ML/MSVOA W/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
TP-24B-S2

Quant Time: Oct 24 08:18:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W102319S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 23 14:11:46 2019
Response via : Initial Calibration

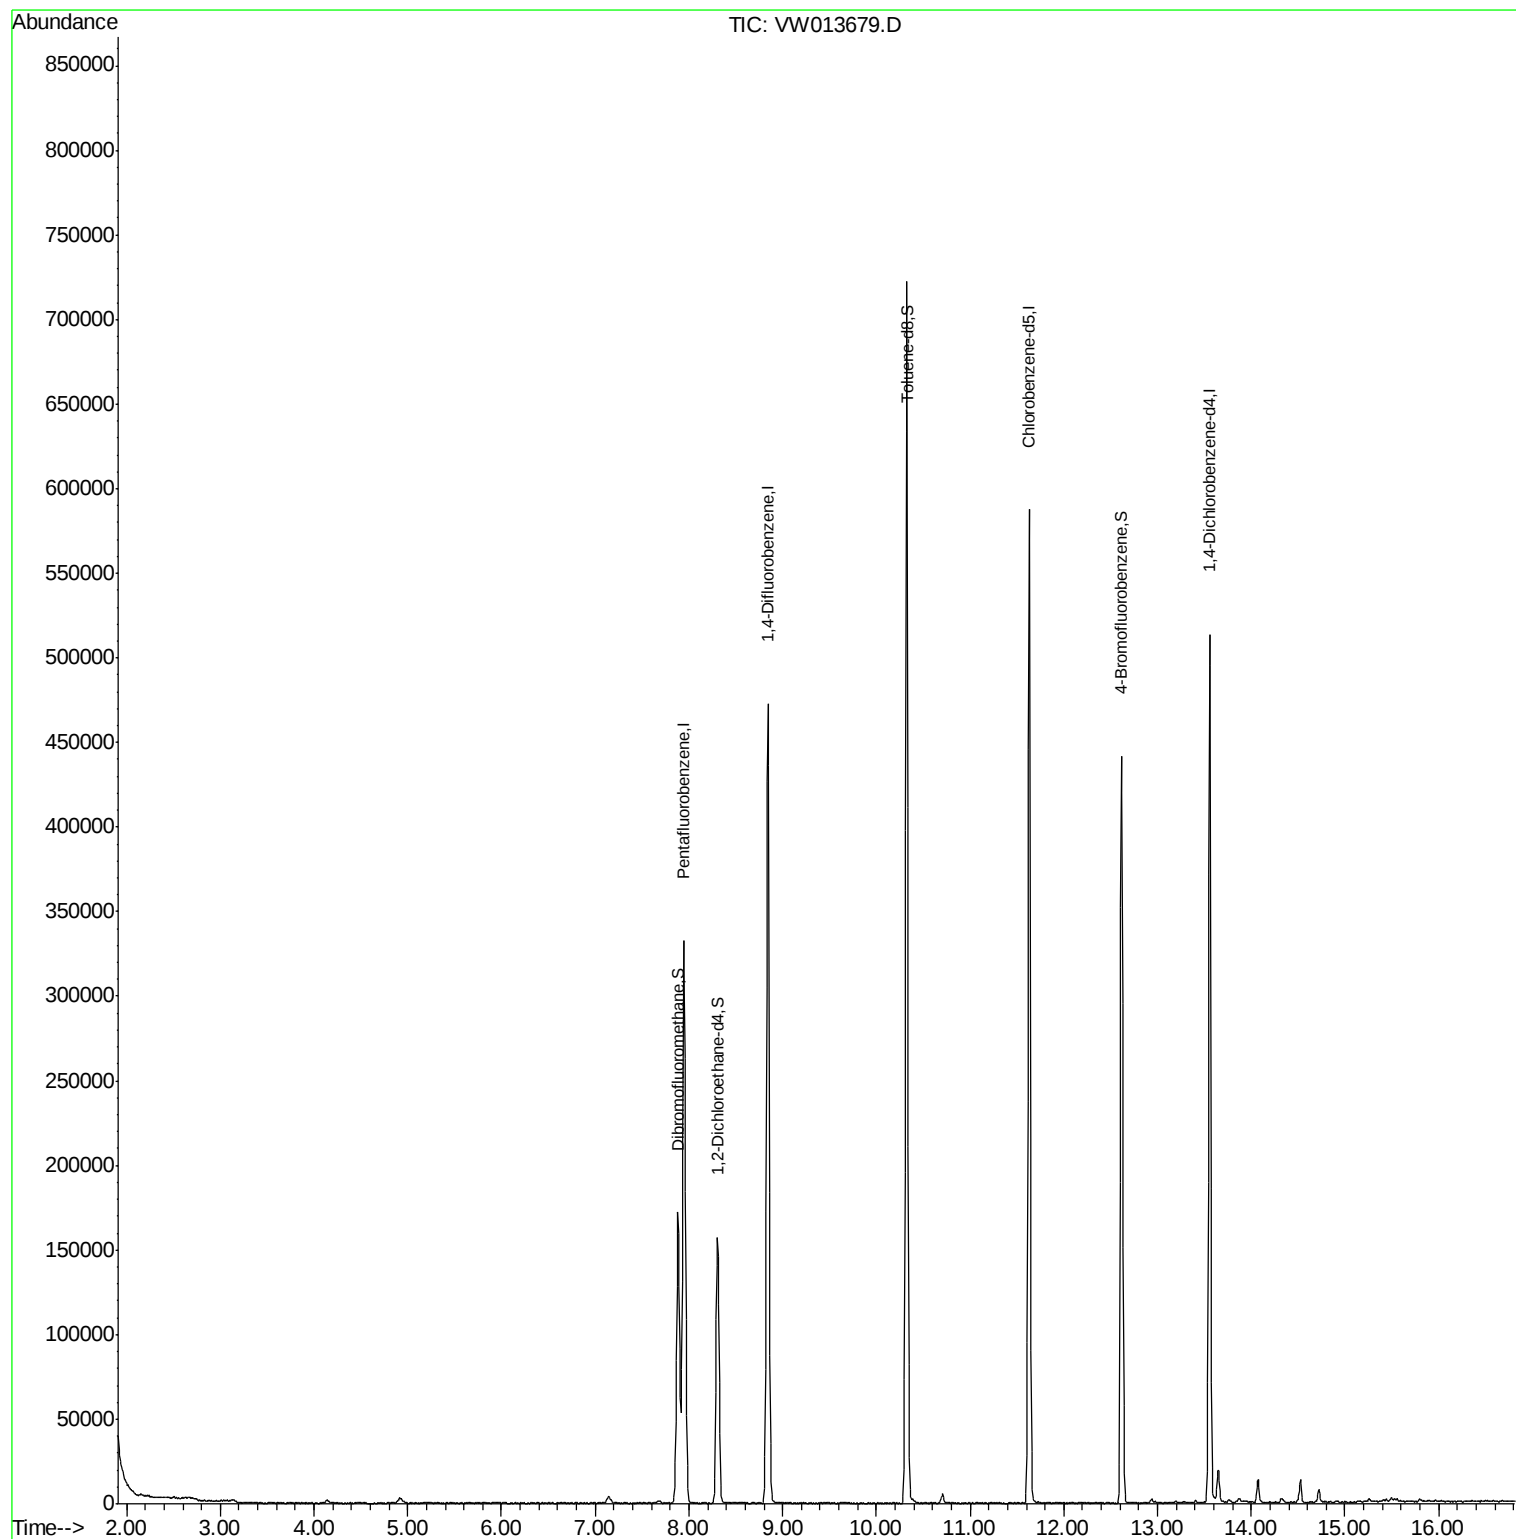

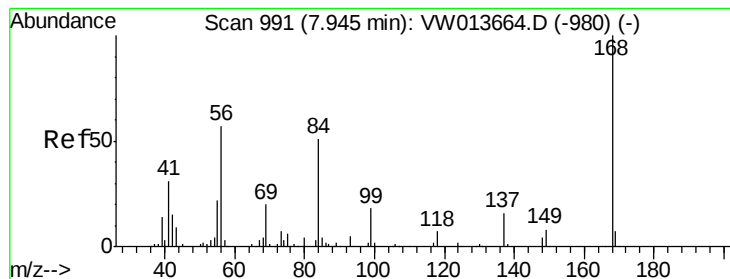

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW013679.D

Acq: 23 Oct 2019 20:34

Instrument :

MSVOA_W

ClientSampleId :


TP-24B-S2

Tot Ion:168 Resp: 279360

Ion Ratio Lower Upper

168 100

99 51.9 39.0 58.6

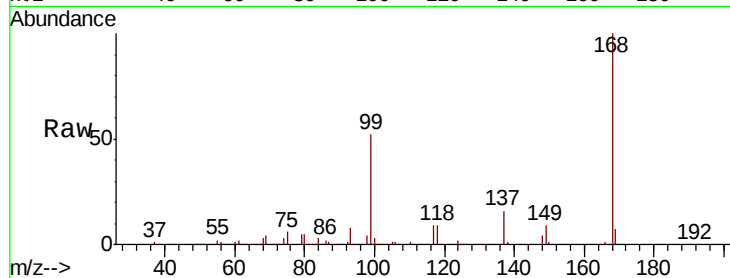

Abundance Ion 167.90 (167.60 to 168.60): VW

Ion 98.90 (98.60 to 99.60): VW



7.95

100000

50000

0

Time-->

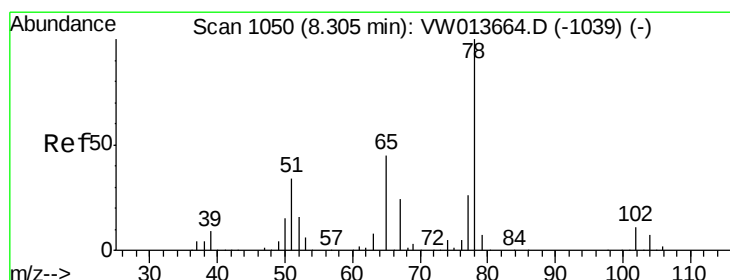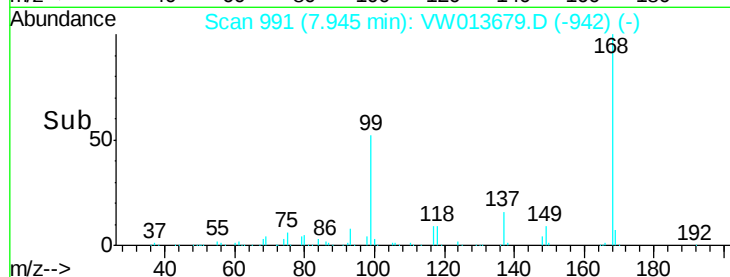

#33

1,2-Dichloroethane-d4

Concen: 58.161 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW013679.D


Acq: 23 Oct 2019 20:34

Tgt Ion: 65 Resp: 121886

Ion Ratio Lower Upper

65 100

67 53.2 0.0 109.4

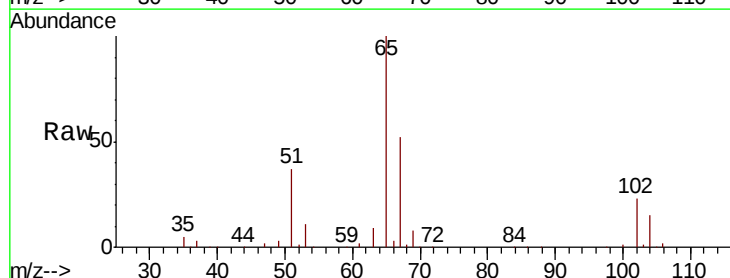

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31

60000

50000

40000


30000


20000

10000

0

Time-->

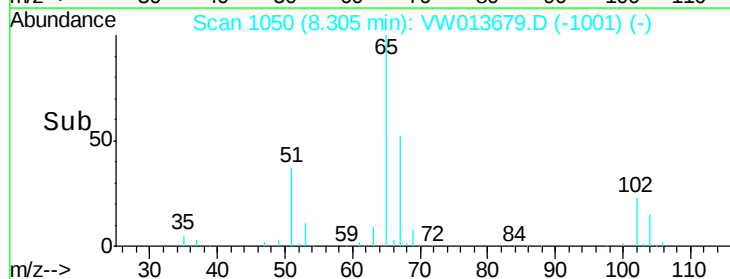


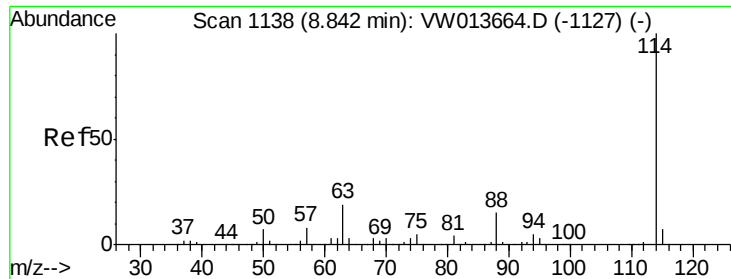




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.84 min Scan# 1138
Delta R.T. -0.00 min
Lab File: VW013679.D
Acq: 23 Oct 2019 20:34

Instrument :
MSVOA_W
ClientSampleId :
TP-24B-S2

Tot Ion:114 Resp: 423813
Ion Ratio Lower Upper
114 100
63 20.0 0.0 37.6
88 15.8 0.0 30.2

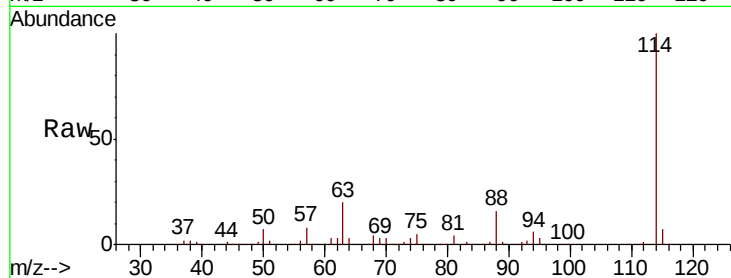


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VW
Ion 87.90 (87.60 to 88.60): VW

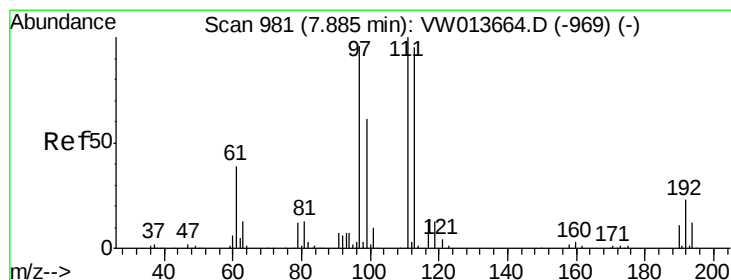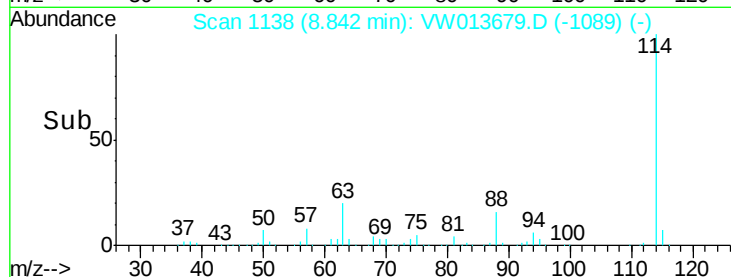
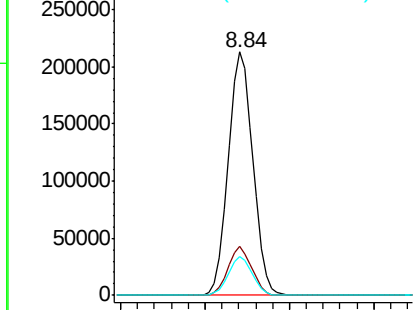


#35
Dibromofluoromethane
Concen: 53.052 ug/l
RT: 7.88 min Scan# 981
Delta R.T. -0.00 min
Lab File: VW013679.D
Acq: 23 Oct 2019 20:34

Tgt Ion:113 Resp: 124935
Ion Ratio Lower Upper
113 100
111 102.8 83.0 124.6
192 23.5 19.4 29.2

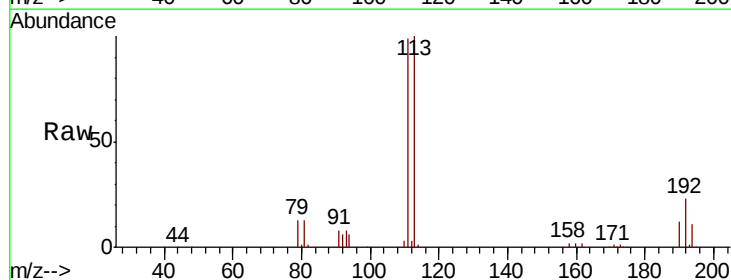

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

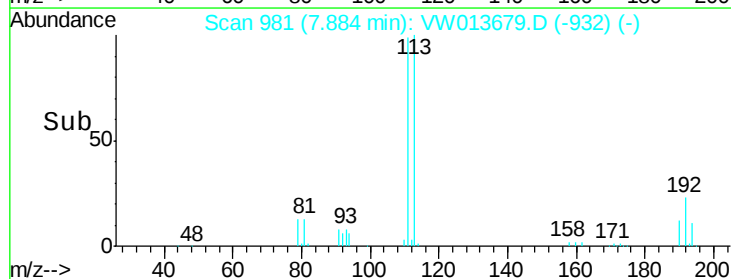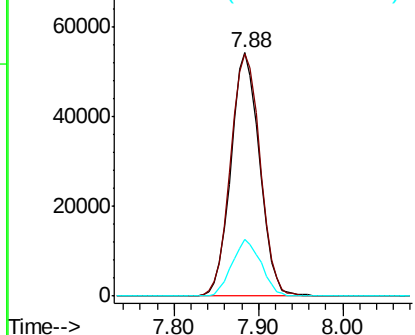



#50

Toluene-d8

Concen: 50.426 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW013679.D

Acq: 23 Oct 2019 20:34

Instrument :

MSVOA_W

ClientSampleId :





TP-24B-S2

Tot Ion: 98 Resp: 483875

Ion Ratio Lower Upper

98 100

100 66.7 53.4 80.0

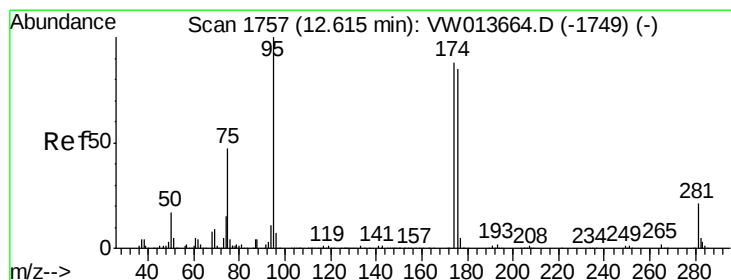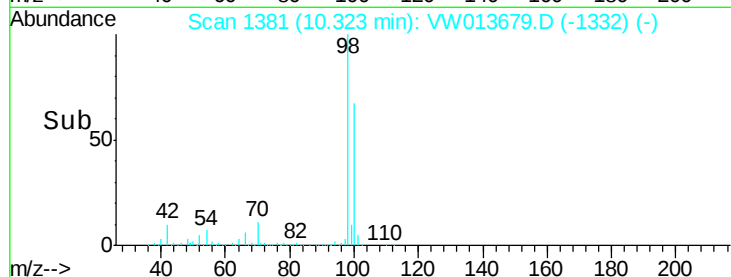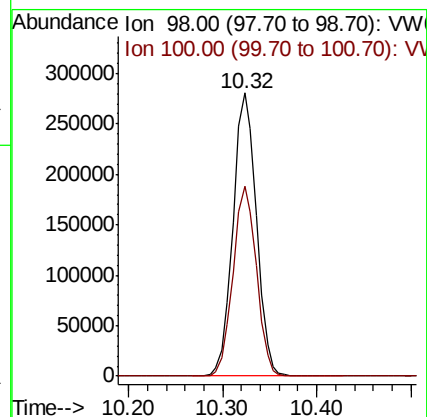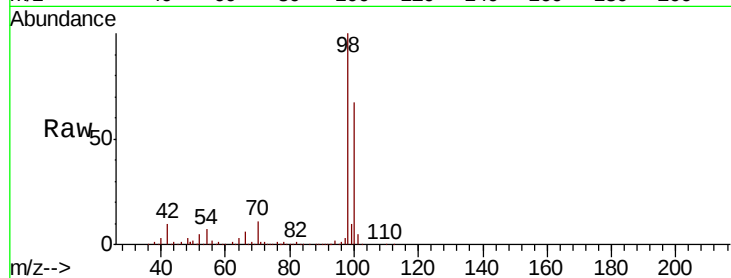

#62

4-Bromofluorobenzene

Concen: 45.242 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. -0.00 min

Lab File: VW013679.D

Acq: 23 Oct 2019 20:34




Tgt Ion: 95 Resp: 146997

Ion Ratio Lower Upper

95 100

174 92.6 0.0 183.6

176 88.0 0.0 178.0

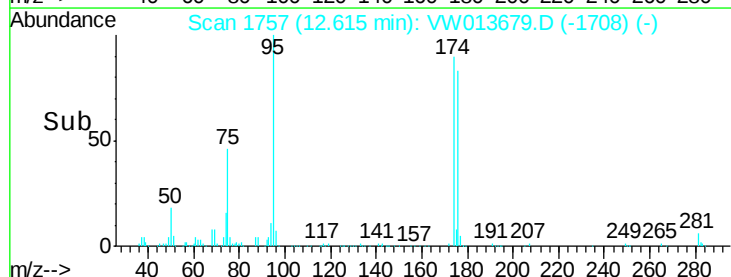
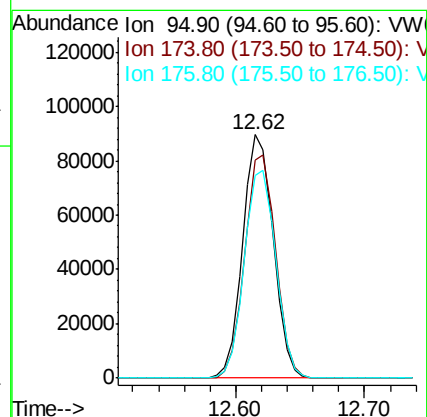
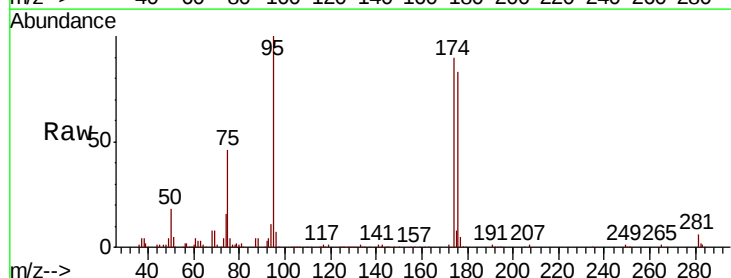




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.01 min
Lab File: VW013679.D
Acq: 23 Oct 2019 20:34

Instrument :
MSVOA_W
ClientSampled :
TP-24B-S2

Tot Ion:117 Resp: 353022
Ion Ratio Lower Upper
117 100
82 51.4 43.6 65.4
119 31.8 25.4 38.2

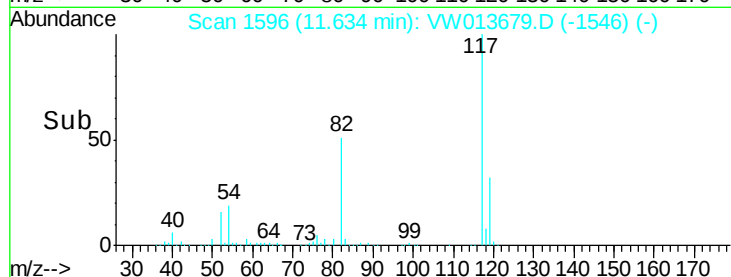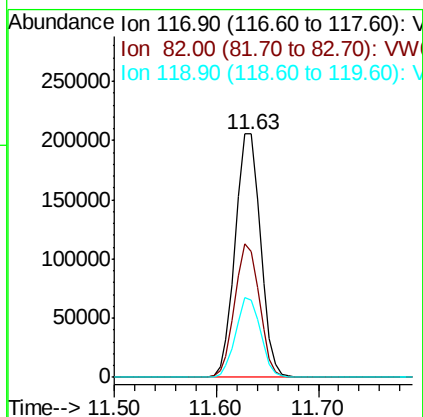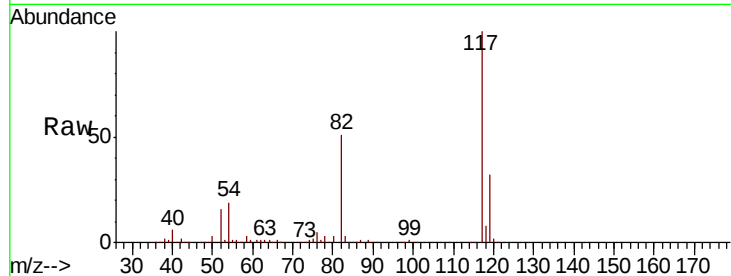

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW013679.D
Acq: 23 Oct 2019 20:34

Tgt Ion:152 Resp: 147819
Ion Ratio Lower Upper
152 100
115 54.5 27.4 82.2
150 157.3 0.0 345.4

