

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW102319\
 Data File : VW013700.D
 Acq On : 24 Oct 2019 07:01
 Operator : SY/VA
 Sample : K5503-06
 Misc : 5.53G/5ML/MSVOA W/SOIL
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 175-12-(2)

Quant Time: Oct 24 08:20:59 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W102319S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 23 14:11:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.95
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.84
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.63
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.56

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	0.00	65	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
35) Dibromofluoromethane	0.00	113	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
50) Toluene-d8	0.00	98	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene	0.00	95	0	0.00	ug/l	
Spiked Amount 50.000			Recovery	=	0.00%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW102319\
Data File : VW013700.D
Acq On : 24 Oct 2019 07:01
Operator : SY/VA
Sample : K5503-06
Misc : 5.53G/5ML/MSVOA W/SOIL
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
175-12-(2)

Quant Time: Oct 24 08:20:59 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W102319S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 23 14:11:46 2019
Response via : Initial Calibration

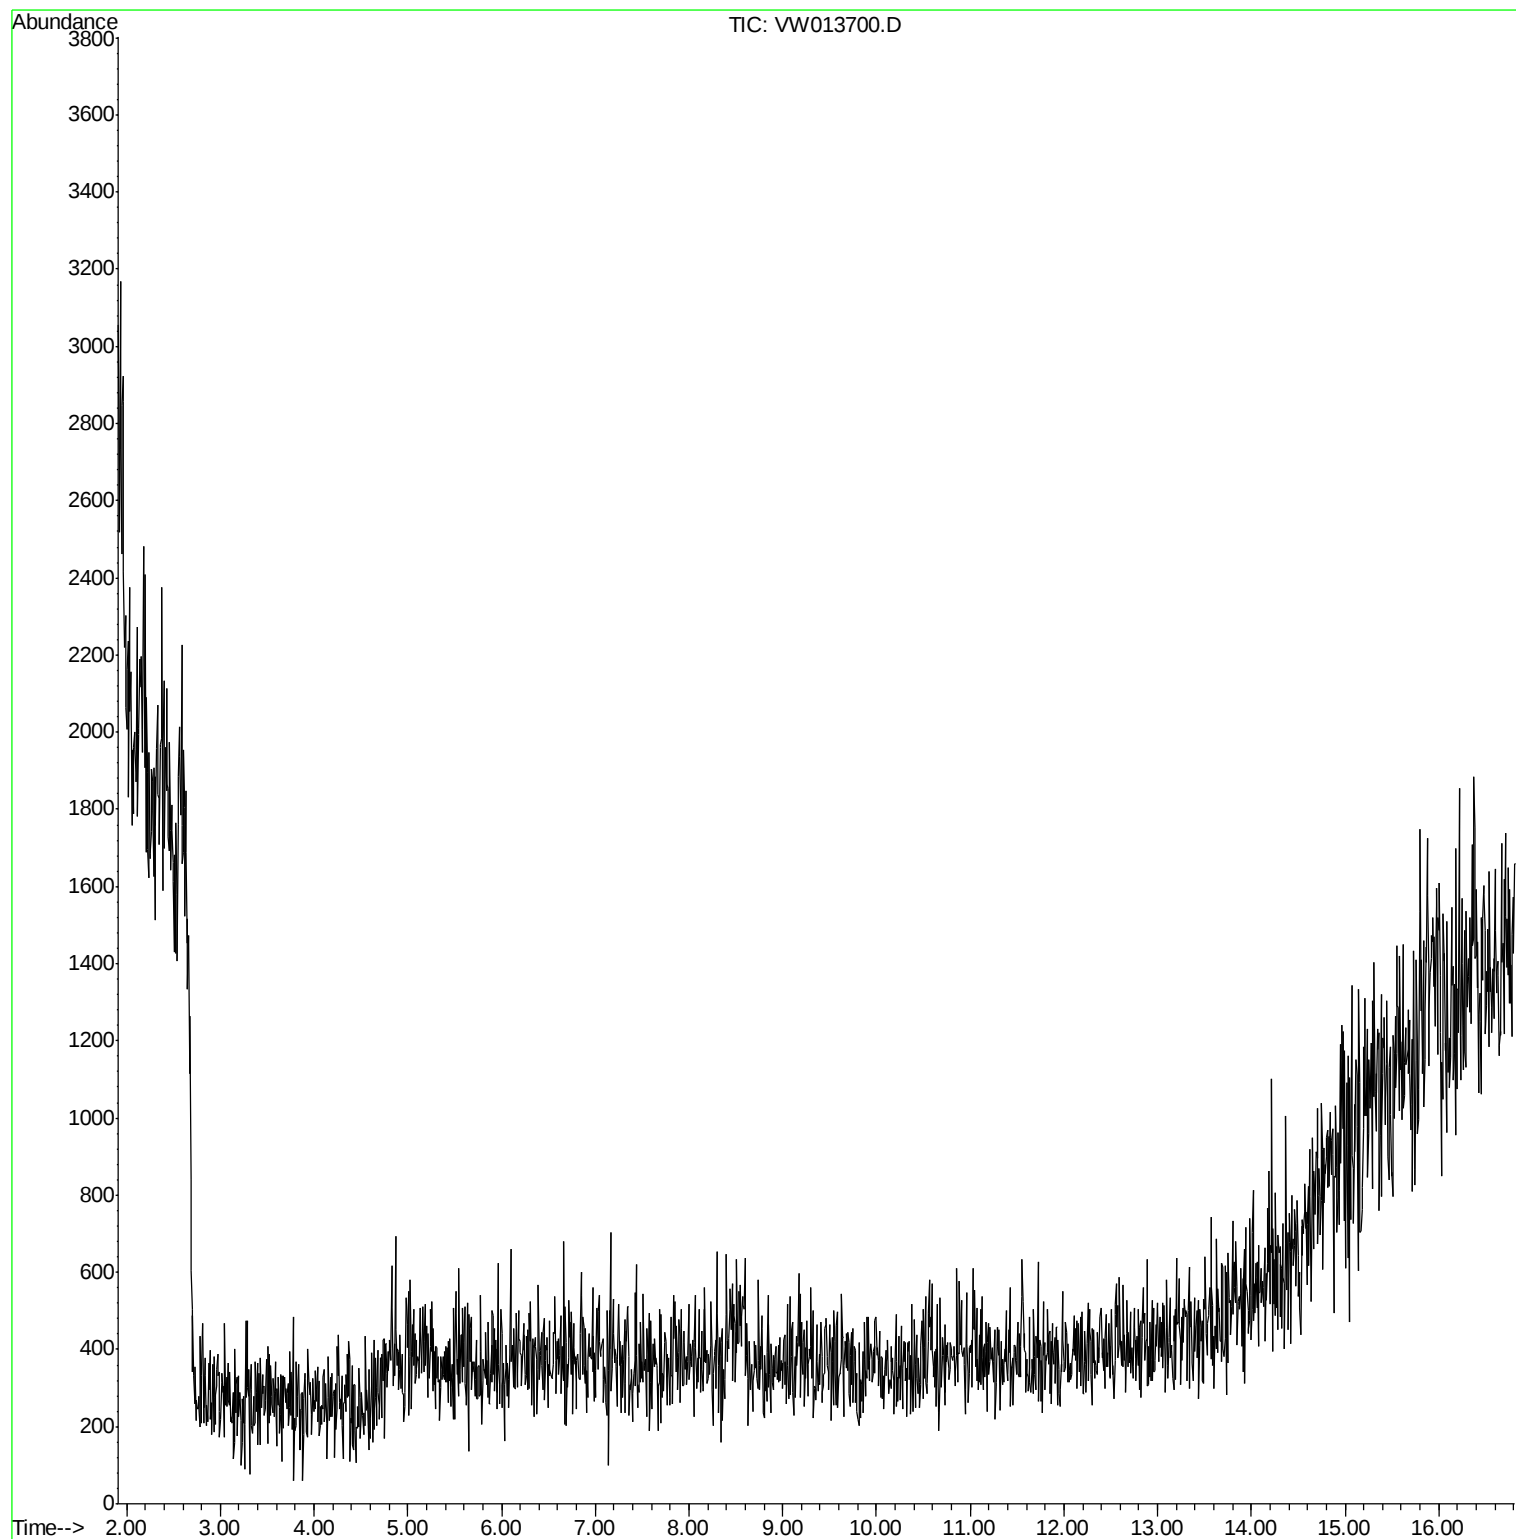


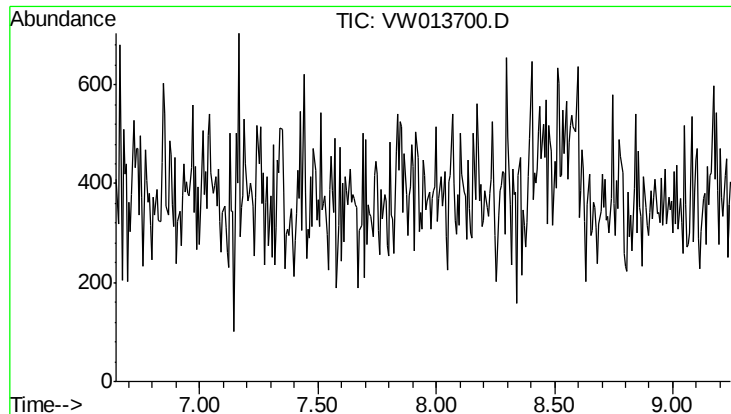


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.95 min

Lab File: VW013700.D
Acq: 24 Oct 2019 07:01

Instrument :
MSVOA_W
ClientSampleId :
175-12-(2)


Tot Ion: 168
Sig Exp Ratio
168 100
99 48.8

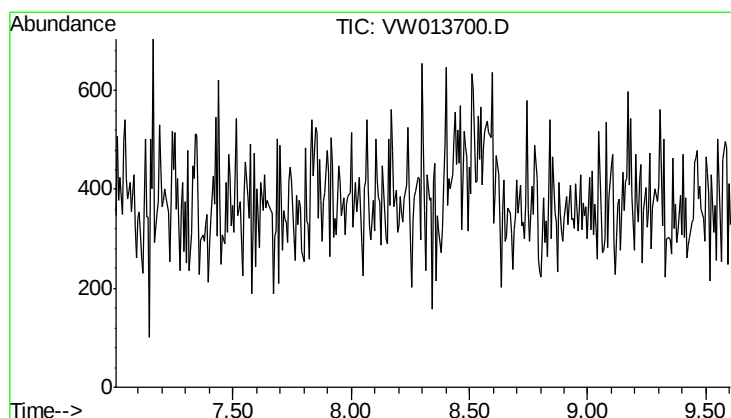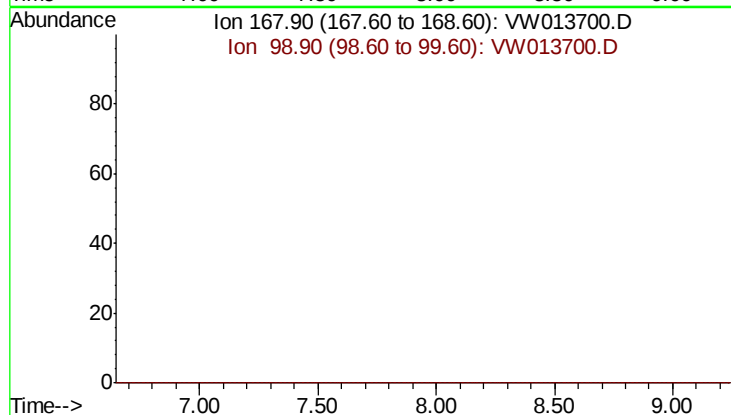


#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
Expected RT: 8.31 min

Lab File: VW013700.D
Acq: 24 Oct 2019 07:01

Tgt Ion: 65
Sig Exp Ratio
65 100
67 54.7


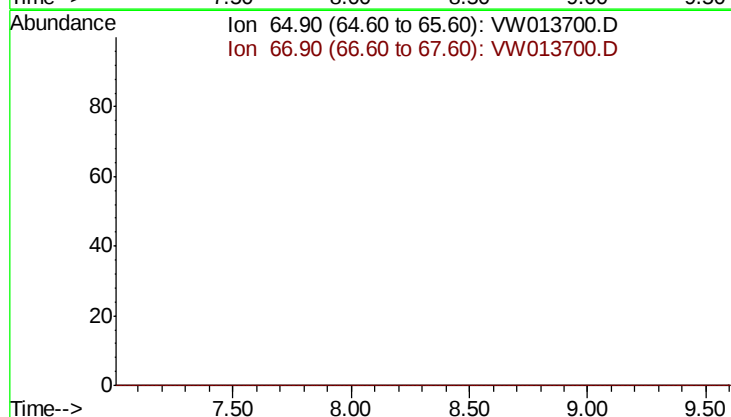


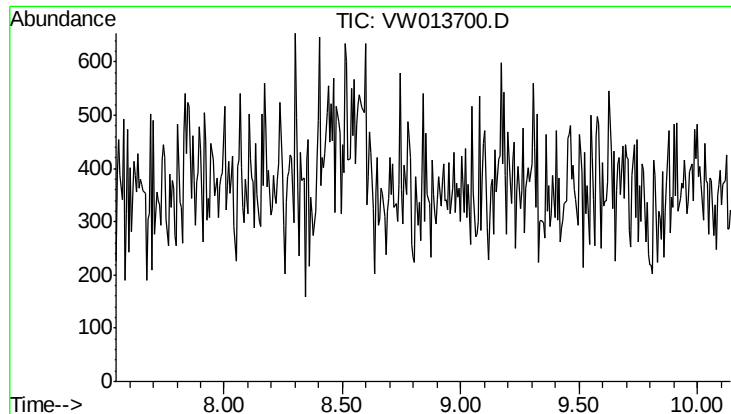

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.84 min
 Lab File: VW013700.D
 Acq: 24 Oct 2019 07:01


Instrument :
 MSVOA_W
 ClientSampleId :
 175-12-(2)


Tot Ion	114
Sig	Exp Ratio
114	100
63	18.8
88	15.1

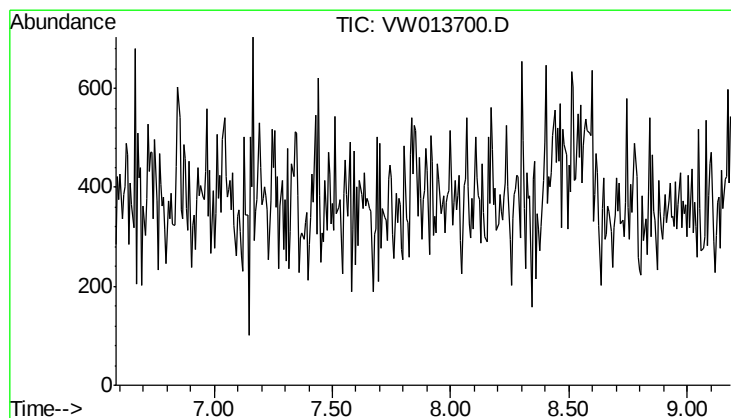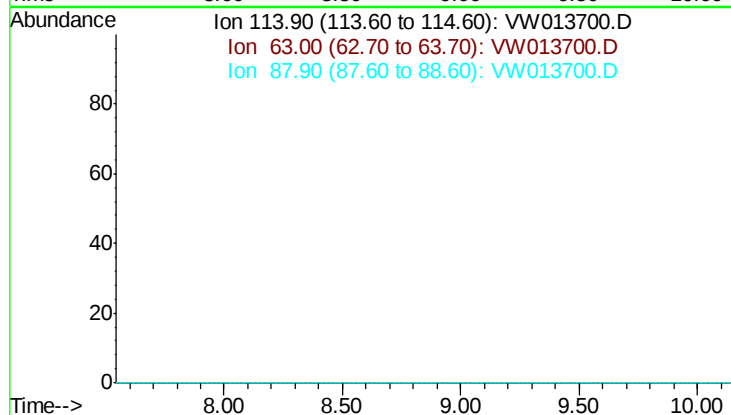

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.88 min
 Lab File: VW013700.D
 Acq: 24 Oct 2019 07:01

Tgt Ion	113
Sig	Exp Ratio
113	100
111	103.8
192	24.3

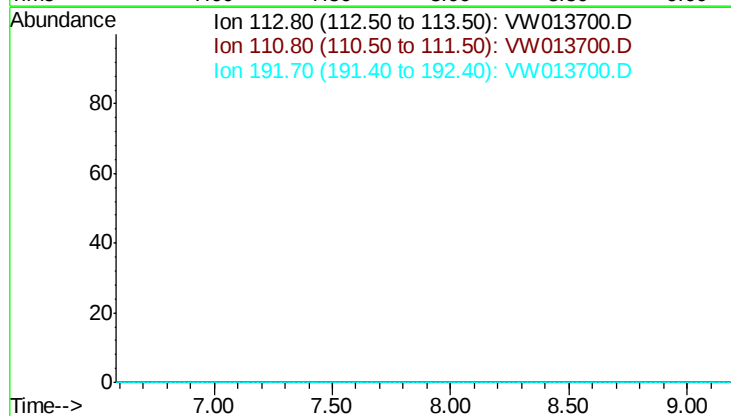


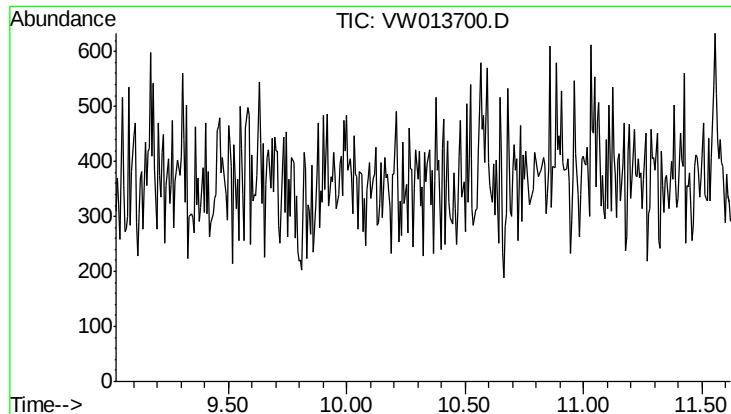


#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.32 min

Lab File: VW013700.D
Acq: 24 Oct 2019 07:01

Instrument :
MSVOA_W
ClientSampleId :
175-12-(2)


Tot Ion:	98
Sig	Exp Ratio
98	100
100	66.7

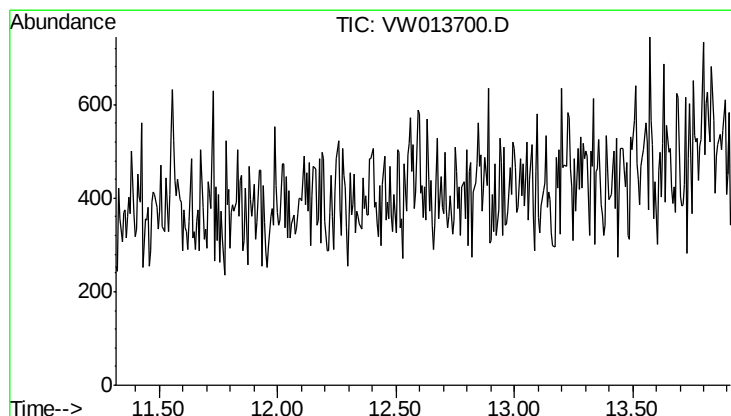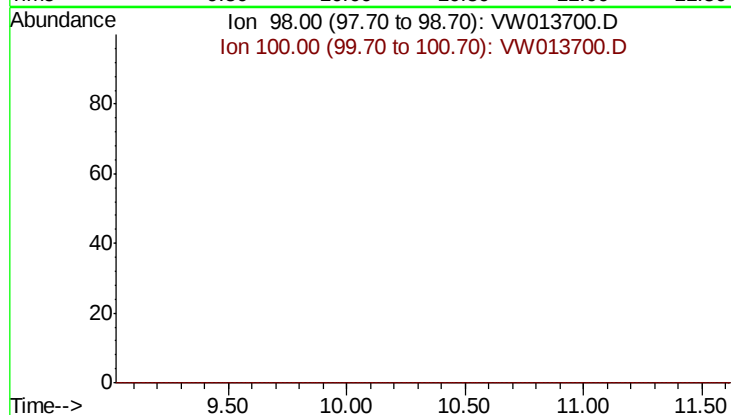


#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.62 min

Lab File: VW013700.D
Acq: 24 Oct 2019 07:01

Tgt Ion:	95
Sig	Exp Ratio
95	100
174	91.8
176	89.0

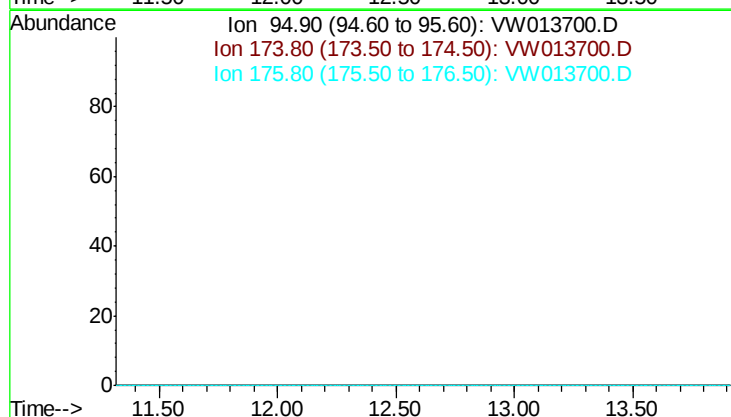


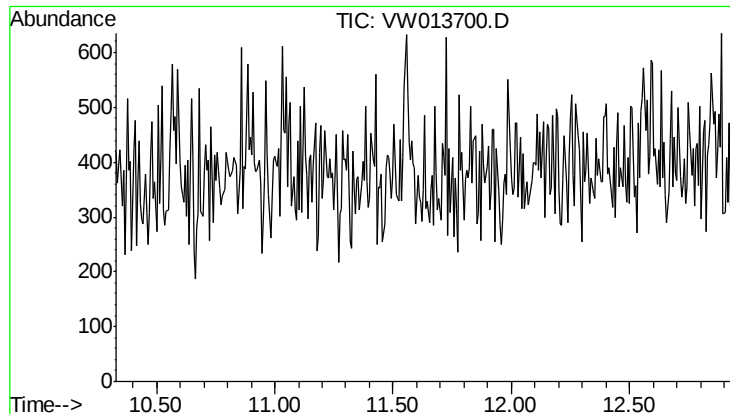


#63
Chlorobenzene-d5
Concen: 0.000 ug/l
Expected RT: 11.63 min

Lab File: VW013700.D
Acq: 24 Oct 2019 07:01

Instrument :
MSVOA_W
ClientSampleId :
175-12-(2)

Tot Ion	117
Sig	Exp Ratio
117	100
82	54.5
119	31.8

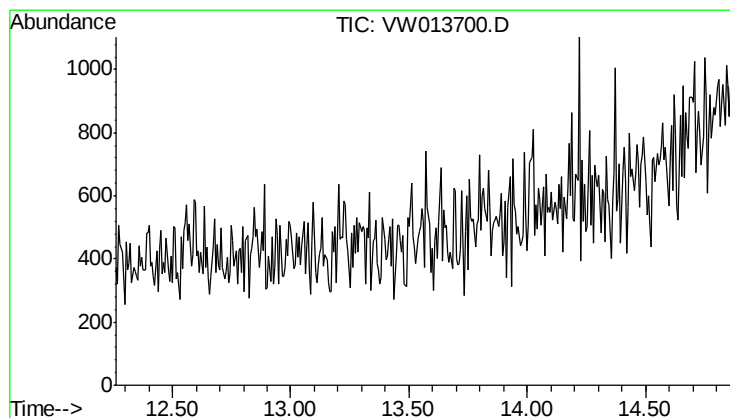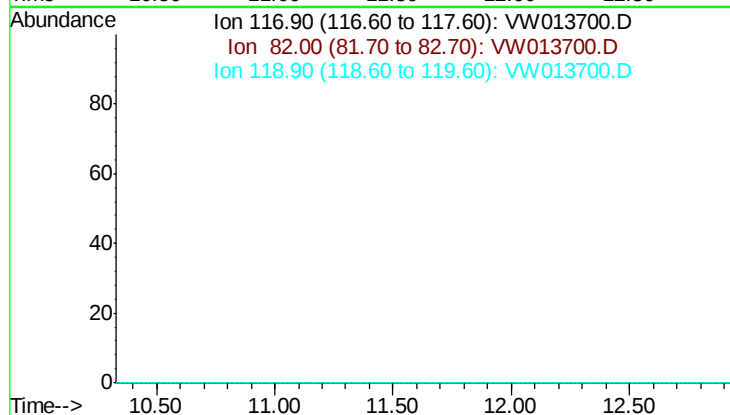

#72
1,4-Dichlorobenzene-d4
Concen: 0.000 ug/l
Expected RT: 13.56 min

Lab File: VW013700.D
Acq: 24 Oct 2019 07:01

Tgt Ion	152
Sig	Exp Ratio
152	100
115	54.8
150	172.7

