

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102324\
 Data File : VW030724.D
 Acq On : 23 Oct 2024 14:53
 Operator : SY/MD
 Sample : P4415-20
 Misc : 5.62g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Oct 24 01:37:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Oct 24 01:34:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.849	114	234610	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	231342	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	96443	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	59953	16.257	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.040%
7) Chloroethane-d5	2.905	69	57698	20.670	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.680%
11) 1,1-Dichloroethene-d2	4.027	65	25933	16.908	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.640%
21) 2-Butanone-d5	7.081	46	34311	51.700	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.400%
24) Chloroform-d	7.648	84	152810	22.776	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.120%
26) 1,2-Dichloroethane-d4	8.307	65	84275	24.155	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.640%
32) Benzene-d6	8.276	84	261458	19.472	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.880%
36) 1,2-Dichloropropane-d6	9.276	67	87065	22.092	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.360%
41) Toluene-d8	10.325	98	235186	19.187	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.760%
43) trans-1,3-Dichloroprop...	10.581	79	31543	19.114	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.440%
47) 2-Hexanone-d5	10.922	63	25541	50.318	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.640%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	74192	25.634	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.520%
66) 1,2-Dichlorobenzene-d4	13.848	152	80833	24.771	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.080%
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	2973	0.524	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW102324\
Data File : VW030724.D
Acq On : 23 Oct 2024 14:53
Operator : SY/MD
Sample : P4415-20
Misc : 5.62g/10mL/MSVOA_W/SOIL/B
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Oct 24 01:37:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM100924SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Oct 24 01:34:36 2024
Response via : Initial Calibration

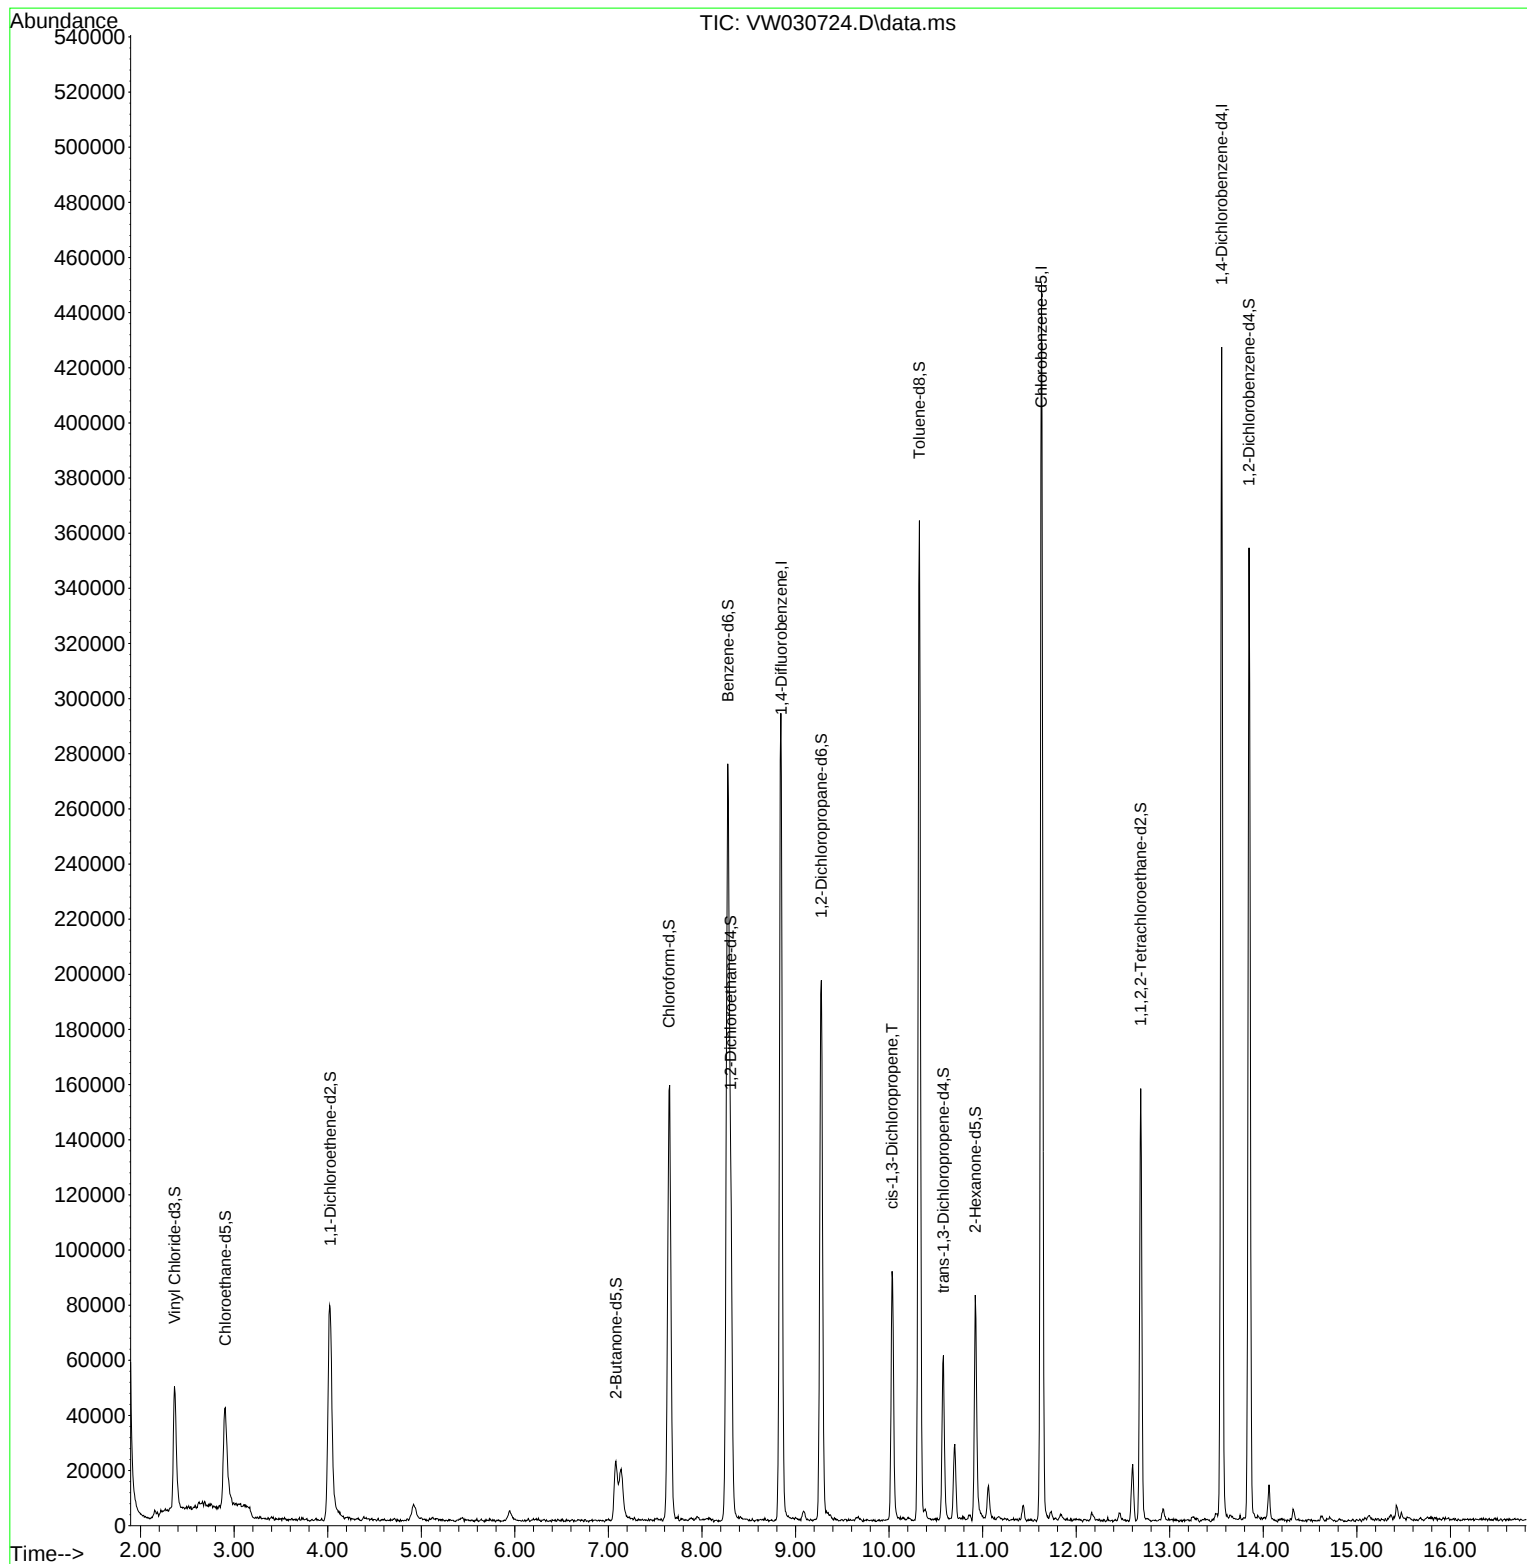

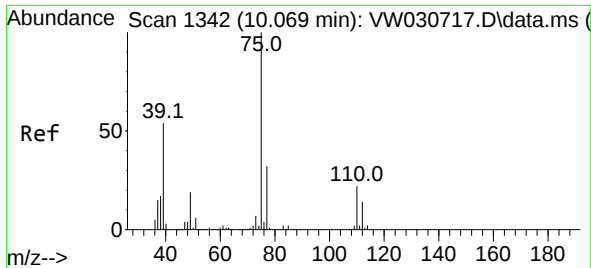

#39
cis-1,3-Dichloropropene
Concen: 0.524 ug/L
RT: 10.032 min Scan# 11
Delta R.T. -0.037 min
Lab File: VW030724.D
Acq: 23 Oct 2024 14:53

Instrument :
MSVOA_W
ClientSampleId :

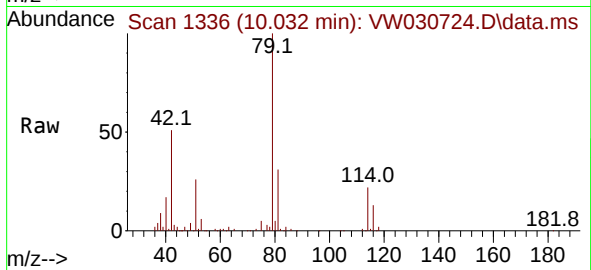

Tgt Ion: 75 Resp: 2973
Ion Ratio Lower Upper
75 100
77 48.3 21.1 39.1#

